
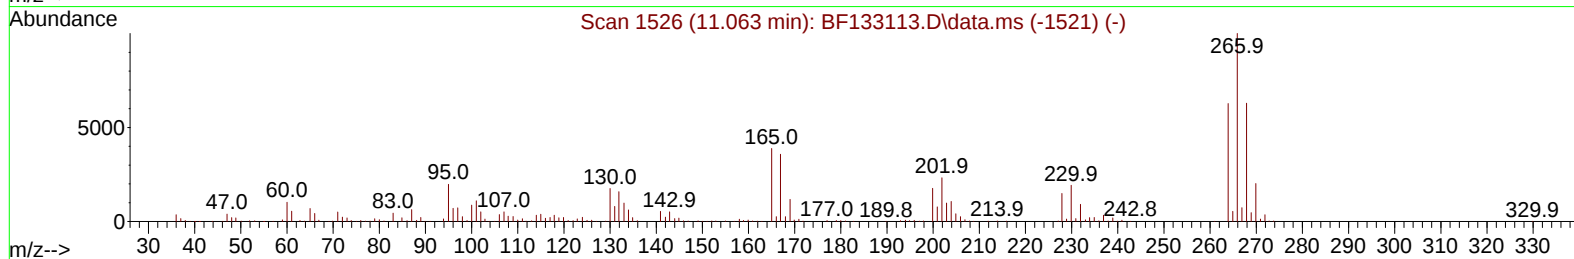
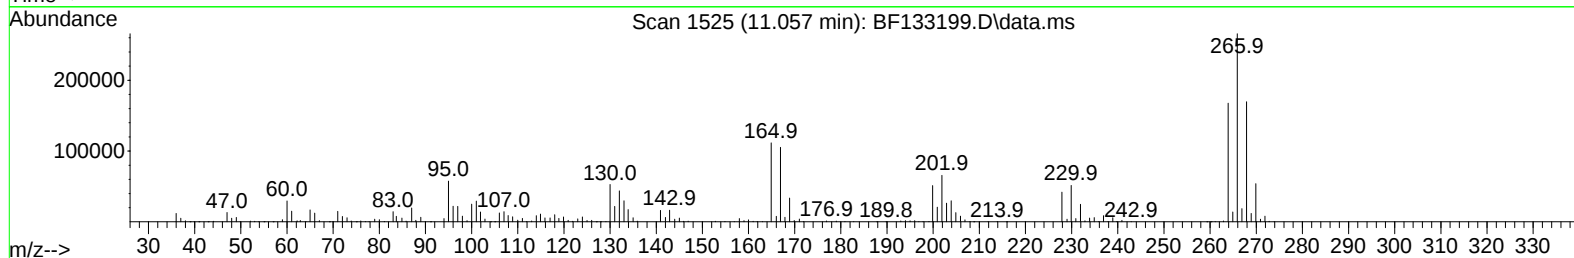


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050323\
Data File : BF133199.D
Acq On : 03 May 2023 10:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 12:12:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 12:00:39 2023
Response via : Initial Calibration

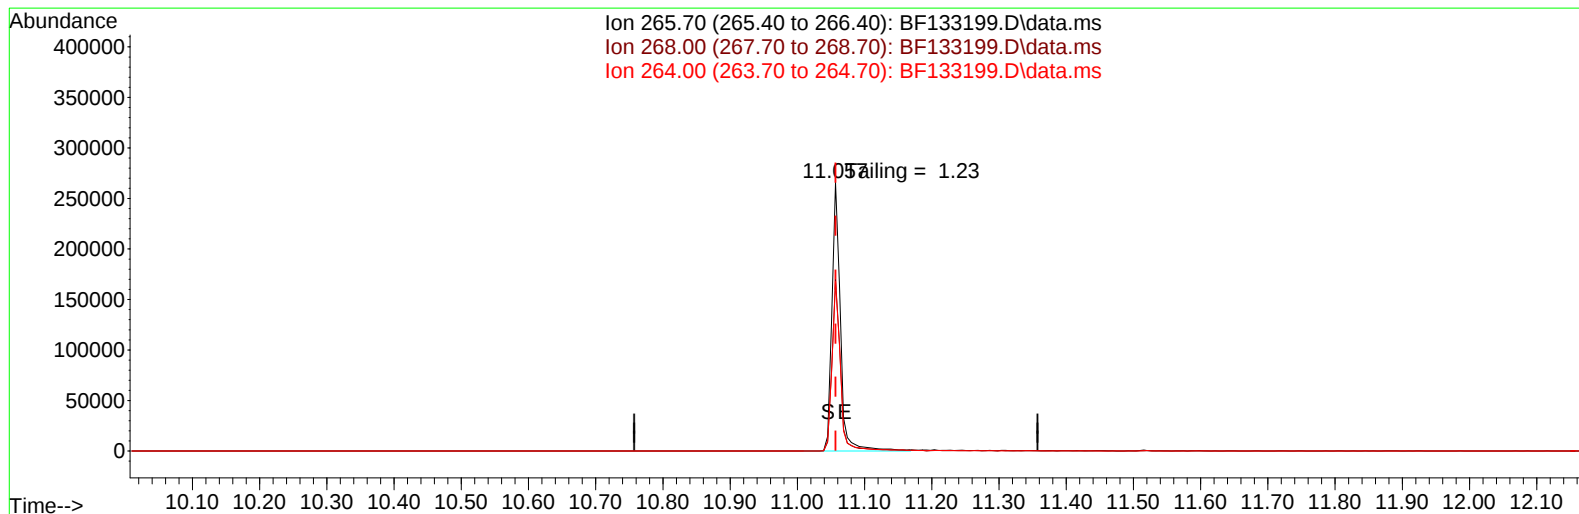

TIC: BF133199.D\data.ms

(70) Pentachlorophenol (C)




11.057min (-0.000) 103694.51 ng

response 233907

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.82
264.00	63.30	63.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050323\
Data File : BF133199.D
Acq On : 03 May 2023 10:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 12:12:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 12:00:39 2023
Response via : Initial Calibration

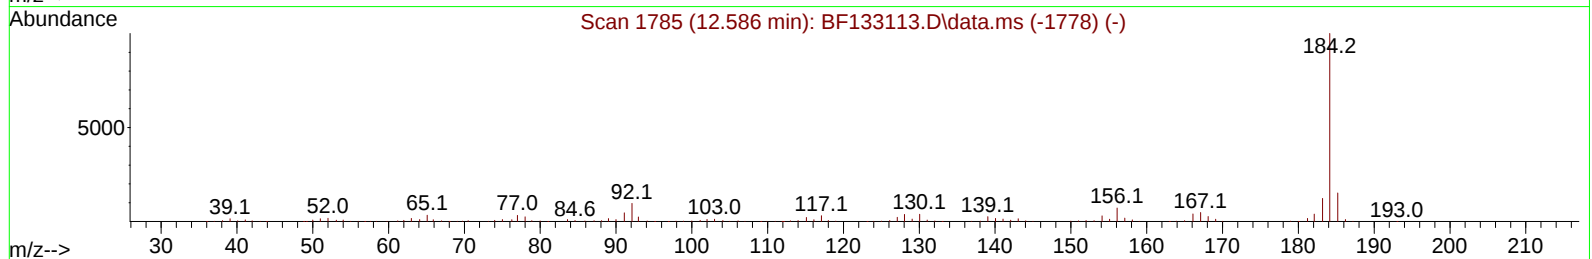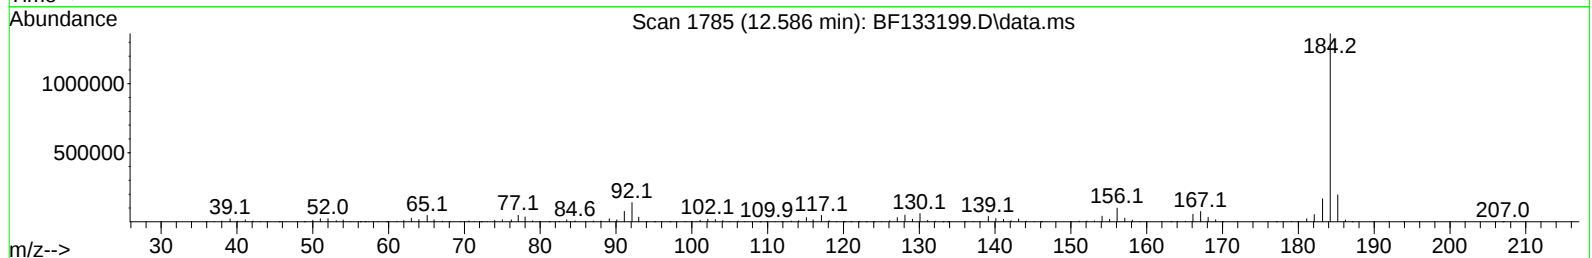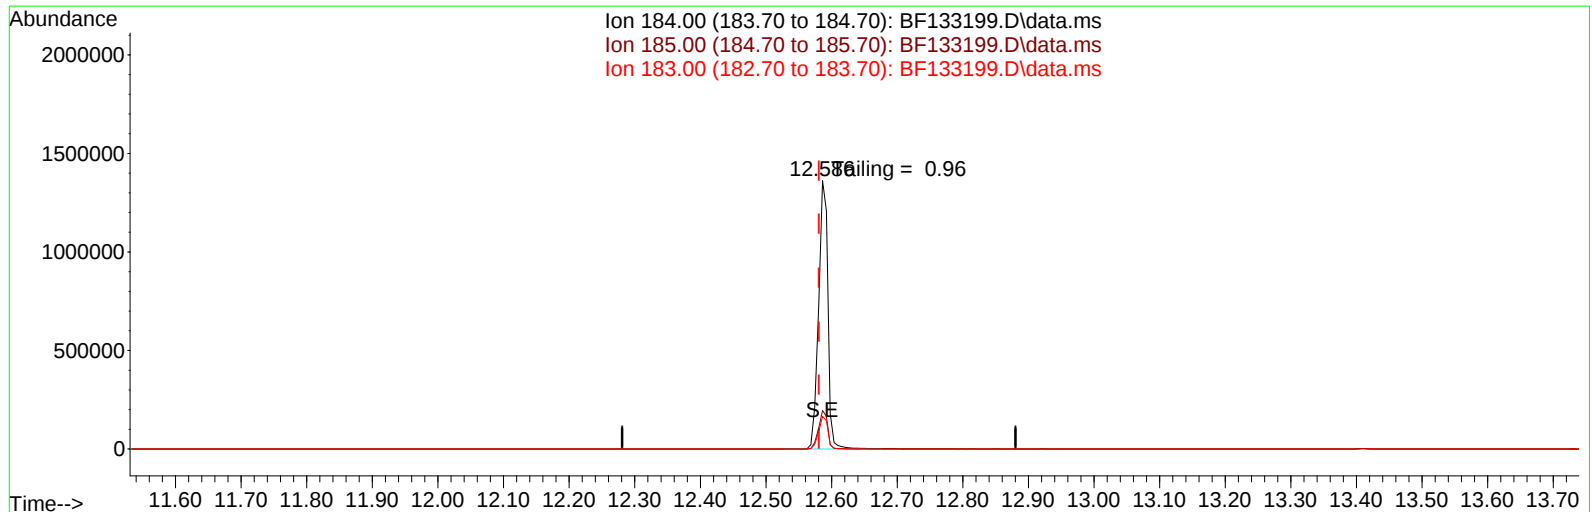

TIC: BF133199.D\data.ms

(77) Benzidine

12.586min (+ 0.005) 343223.01 ng

response 1352351

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.30#
183.00	11.70	12.17
0.00	0.00	0.00