


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050323\
 Data File : BF133199.D
 Acq On : 03 May 2023 10:54
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 04 12:22:53 2023

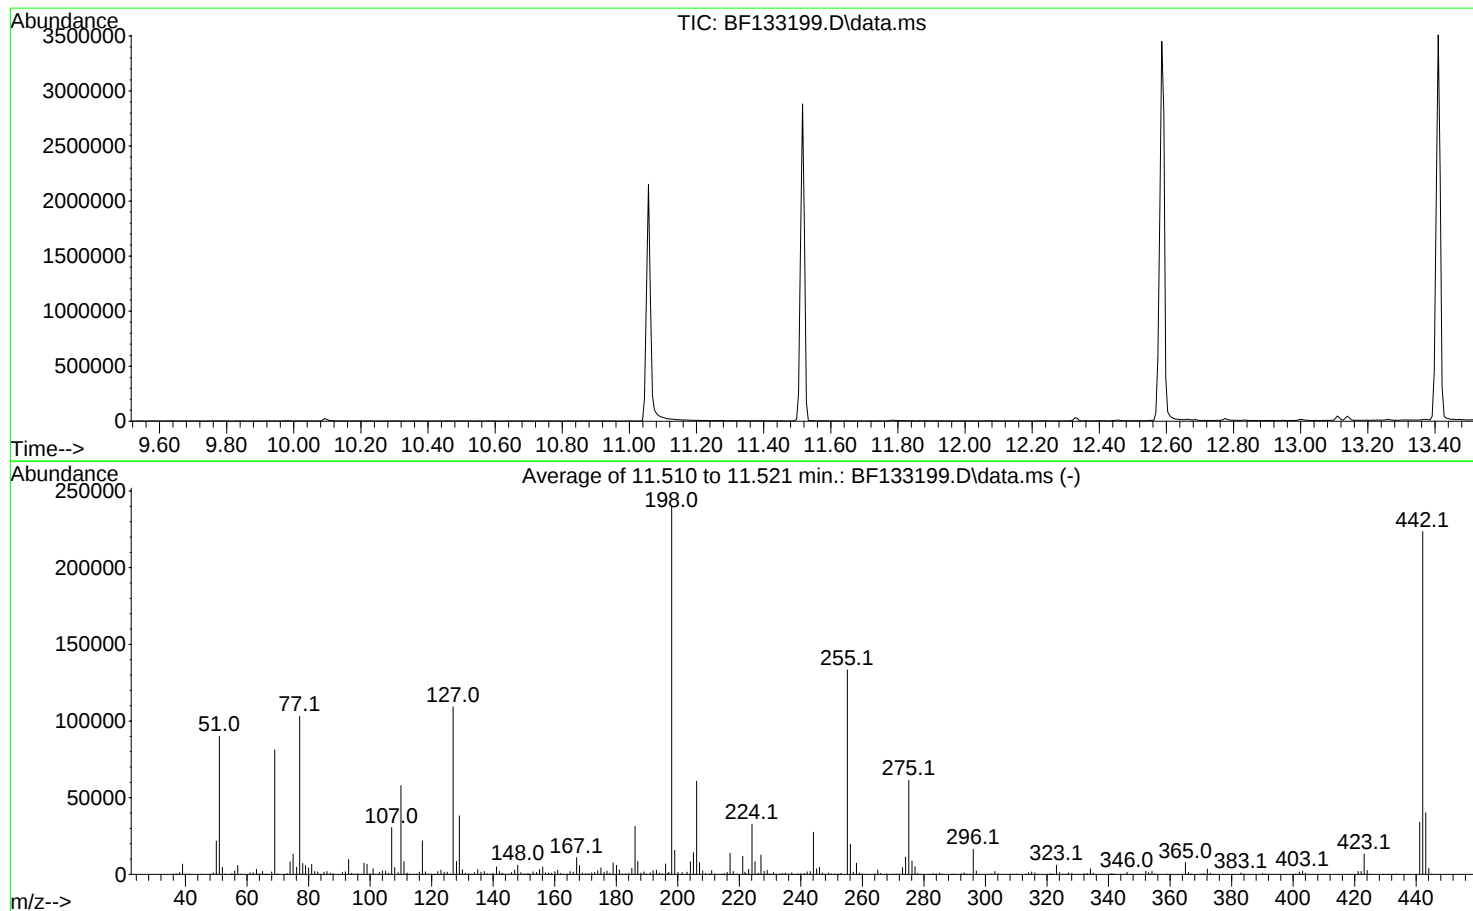

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	90088	PASS
68	69	0.00	2	1.9	1549	PASS
69	198	0.00	100	33.8	81205	PASS
70	69	0.00	2	0.4	345	PASS
127	198	10	80	45.5	109224	PASS
197	198	0.00	2	0.6	1355	PASS
198	198	100	100	100.0	239915	PASS
199	198	5	9	6.5	15698	PASS
275	198	10	60	25.5	61259	PASS
365	198	1	100	3.2	7683	PASS
441	198	0.01	100	14.1	33932	PASS
442	442	50	100	100.0	223576	PASS
443	442	15	24	18.0	40219	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/3/2023	BNA_F	<u>BF133199.D</u>
Compound Name	Response	Retention Time
DDT	600825	13.41
DDD	12746	13.11
DDE	3559	12.774
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16305	617130	2.64

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050323\
Data File : BF133199.D
Acq On : 03 May 2023 10:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 03 12:12:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 12:00:39 2023
Response via : Initial Calibration

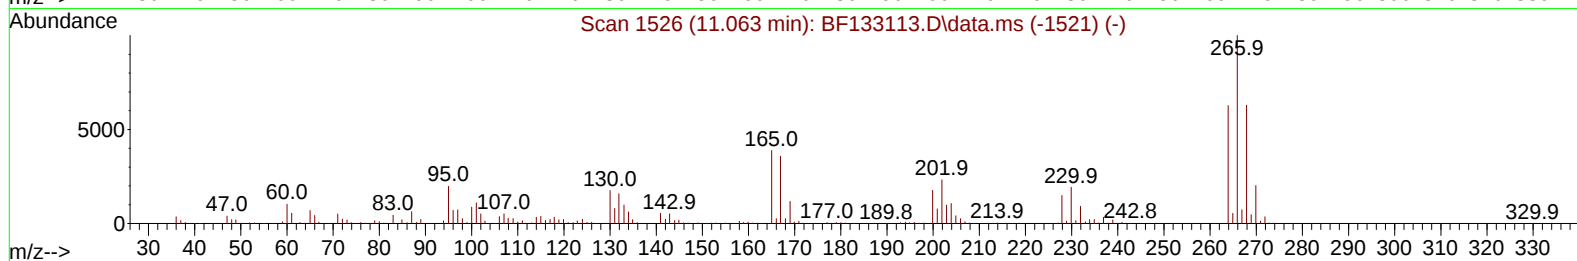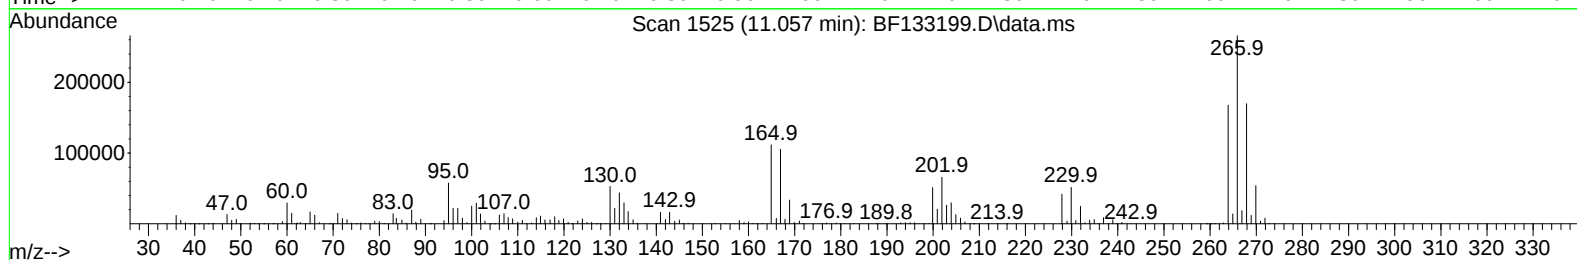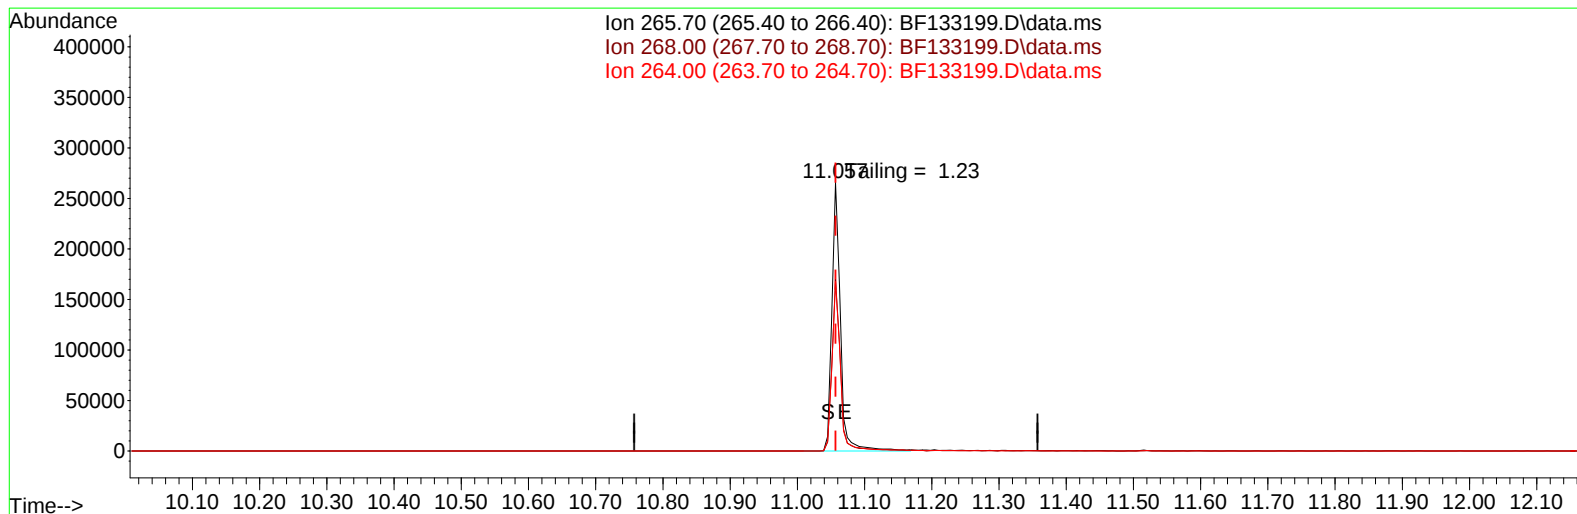

TIC: BF133199.D\data.ms

(70) Pentachlorophenol (C)

11.057min (-0.000) 103694.51 ng




response 233907

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.82
264.00	63.30	63.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050323\
Data File : BF133199.D
Acq On : 03 May 2023 10:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 03 12:12:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 12:00:39 2023
Response via : Initial Calibration

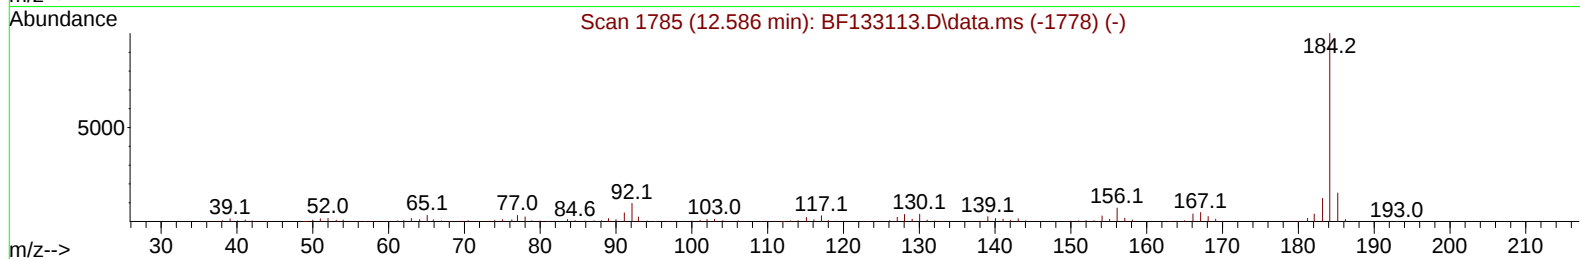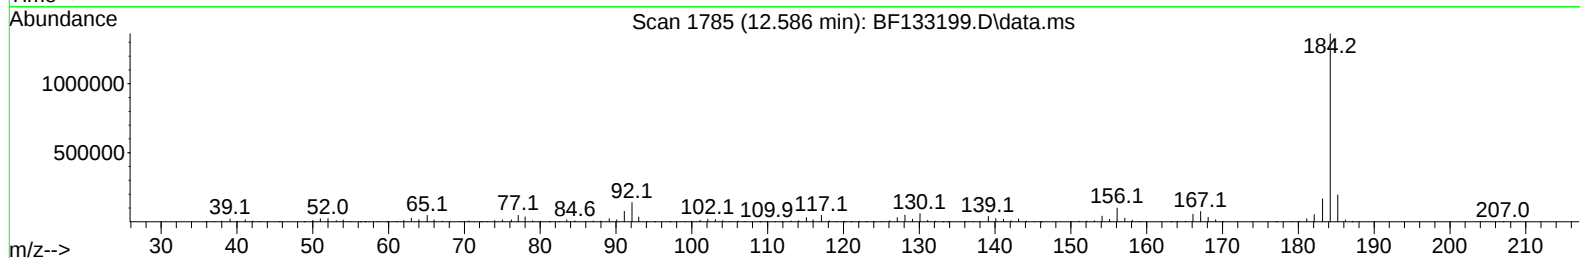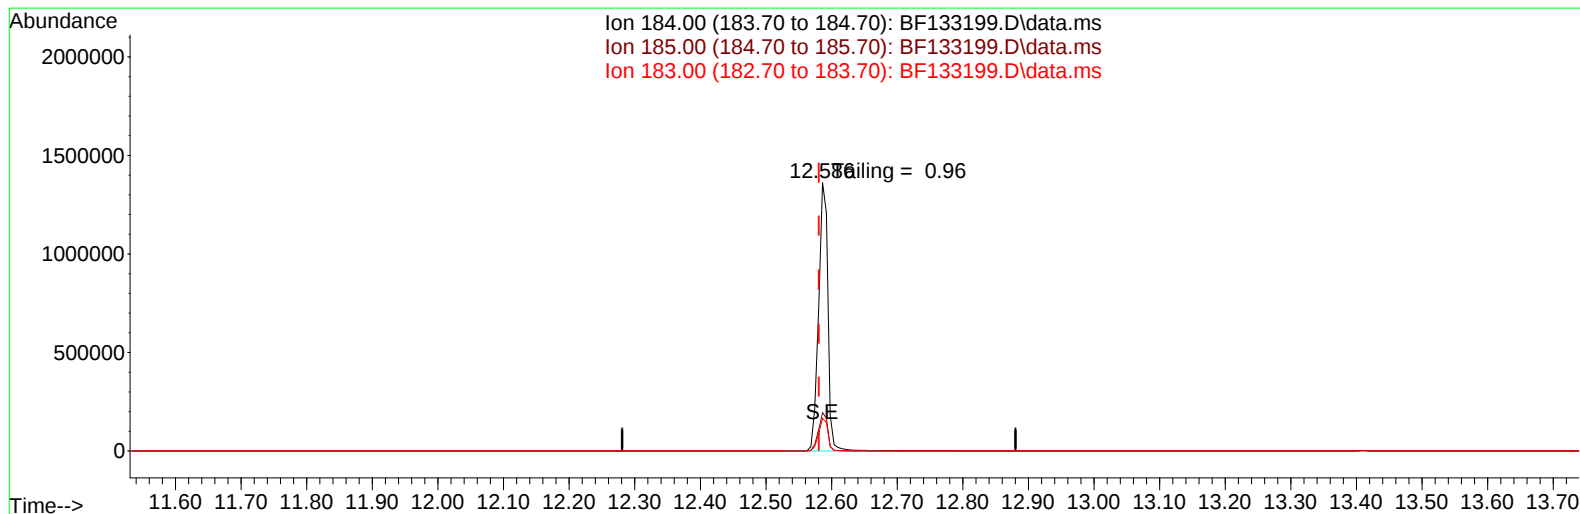

TIC: BF133199.D\data.ms

(77) Benzidine

12.586min (+ 0.005) 343223.01 ng

response 1352351

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.30#
183.00	11.70	12.17
0.00	0.00	0.00