
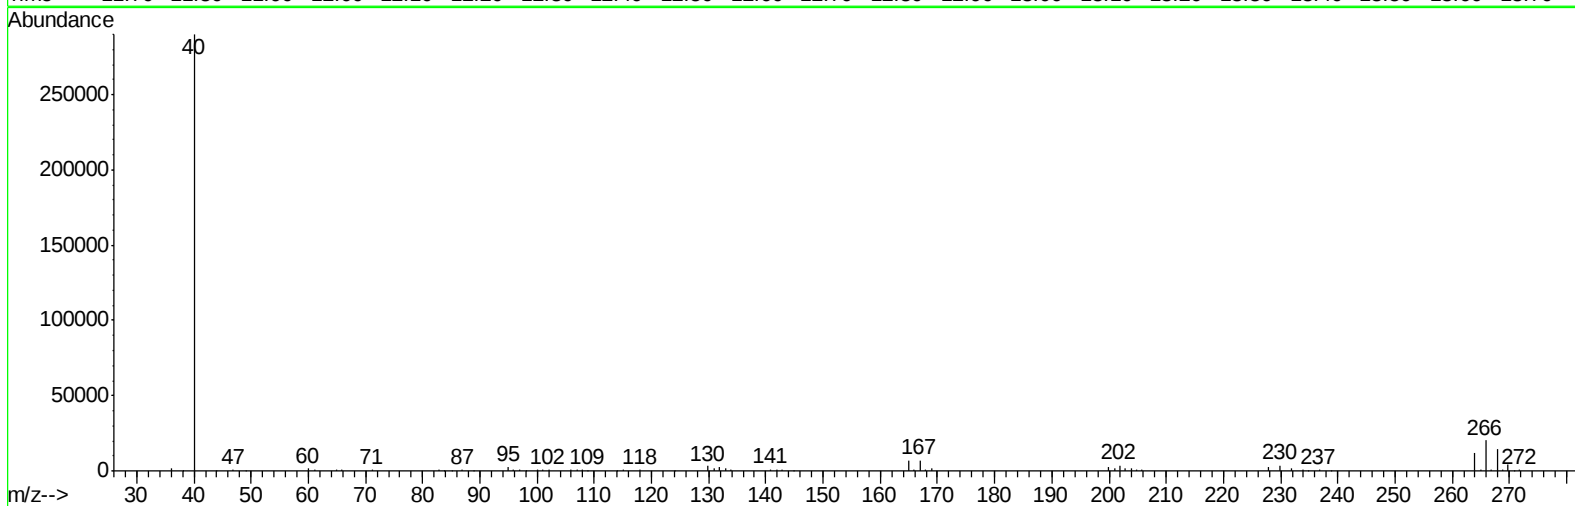


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050415\
Data File : BF078907.D
Acq On : 4 May 2015 8:57
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 05 05:50:01 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 05 00:58:01 2015
Response via : Initial Calibration

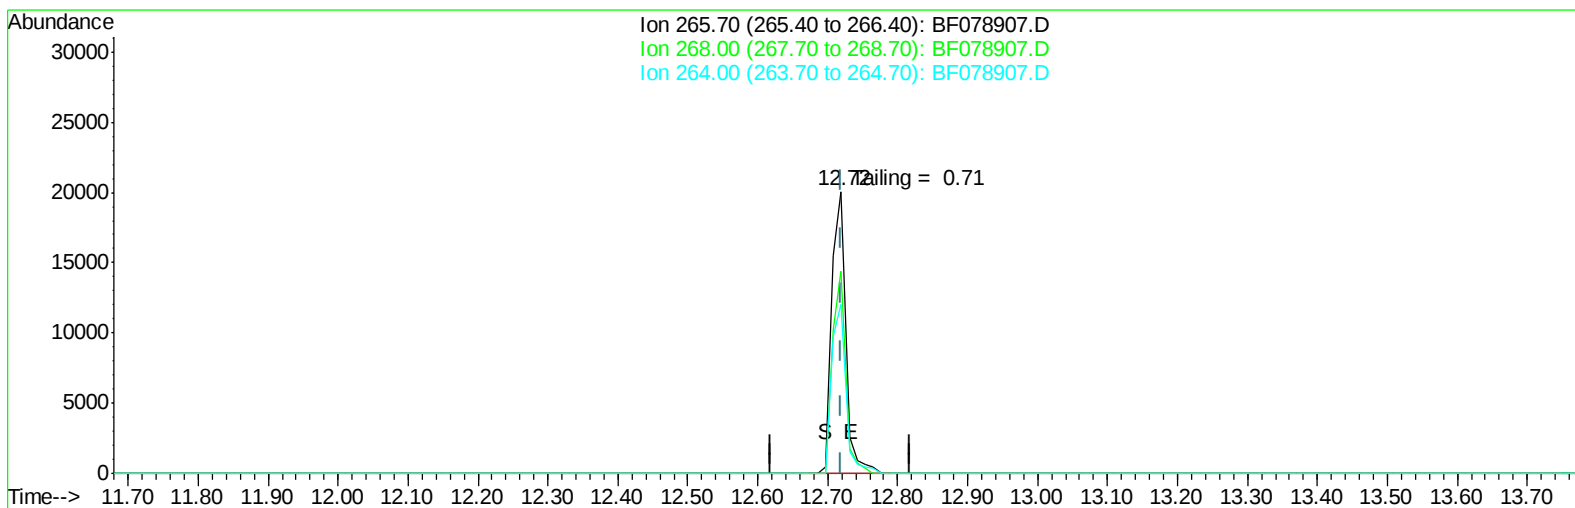

TIC: BF078907.D

(69) Pentachlorophenol (C)



12.720min (+0.000) 0.00ng

response 27890

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	71.74
264.00	60.20	60.24
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050415\
Data File : BF078907.D
Acq On : 4 May 2015 8:57
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 05 05:50:01 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 05 00:58:01 2015
Response via : Initial Calibration

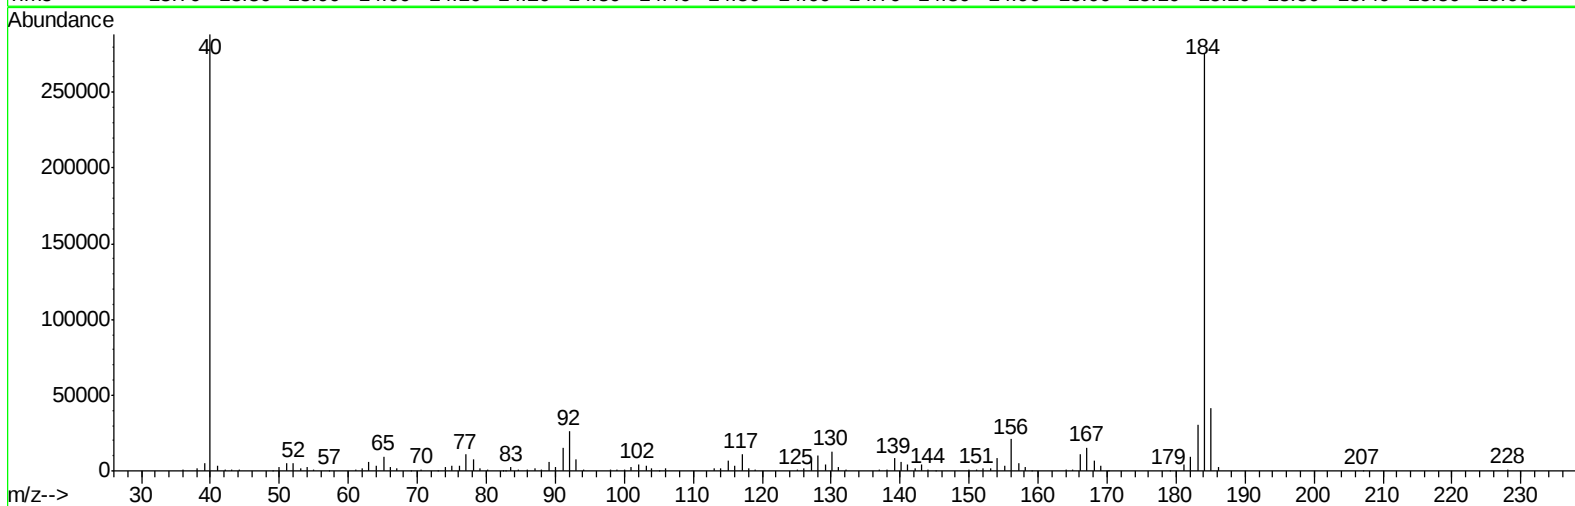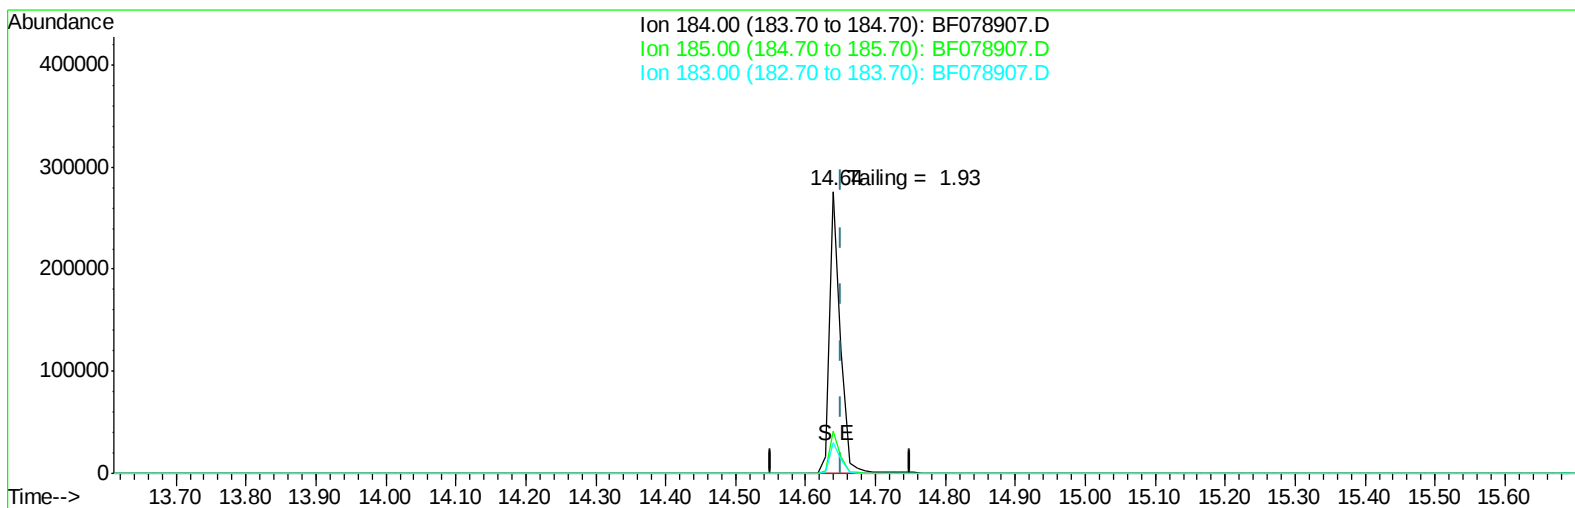

TIC: BF078907.D

(76) Benzidine

14.640min (-0.011) 0.00ng

response 298070

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	15.03
183.00	10.50	11.08
0.00	0.00	0.00