


Data Path : Z:\HPCHEM1\BNA_F\Data\BF050415\
 Data File : BF078907.D
 Acq On : 4 May 2015 8:57
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 30 19:07:47 2015

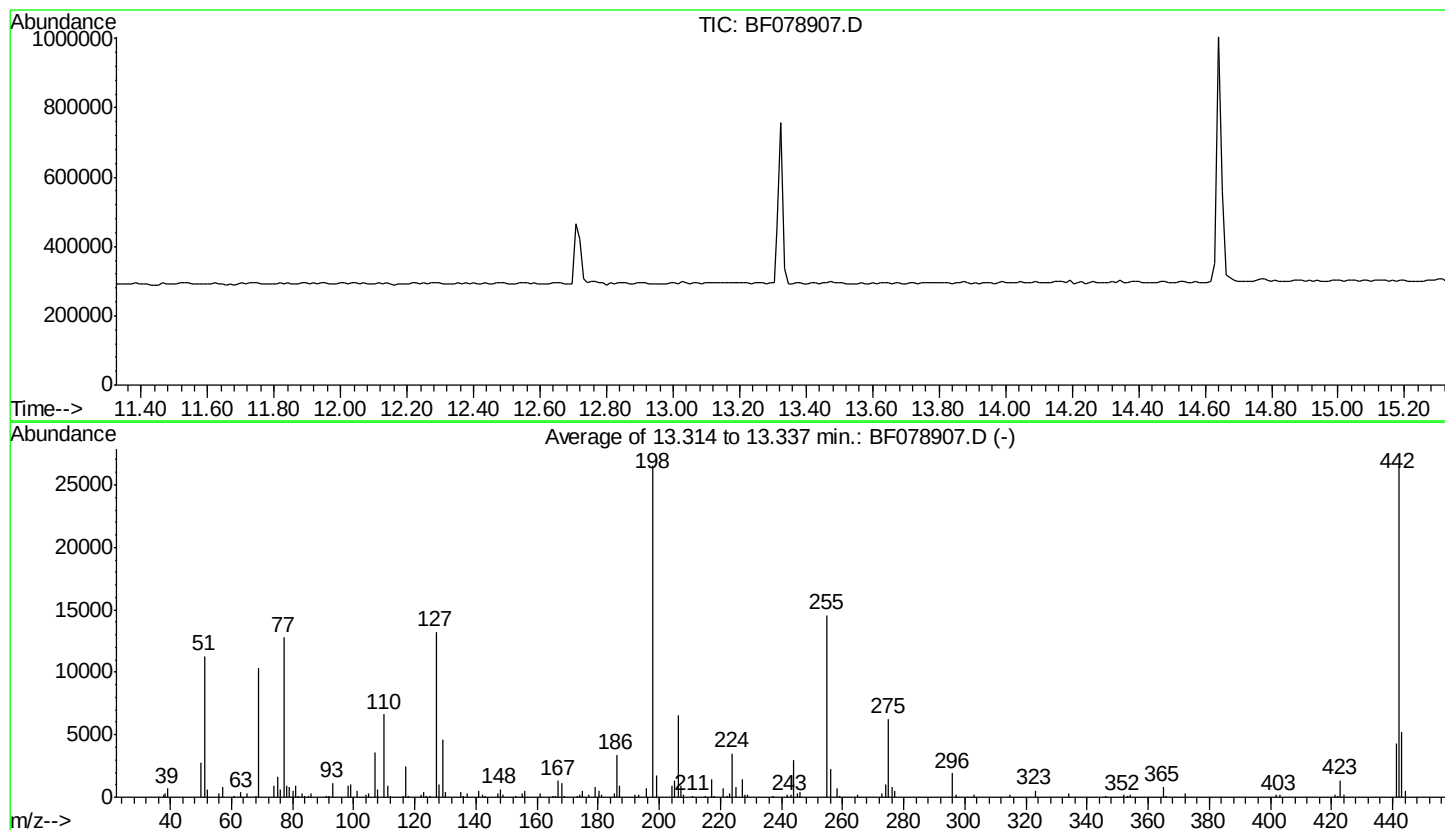

AutoFind: Scans 1061, 1062, 1063; Background Corrected with Scan 1058

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	11279	PASS
68	69	0.00	2	1.1	114	PASS
69	198	0.00	100	39.0	10344	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.9	13247	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26538	PASS
199	198	5	9	6.7	1784	PASS
275	198	10	60	23.7	6299	PASS
365	198	1	100	3.2	847	PASS
441	442	0.01	24	16.2	4290	PASS
442	198	50	100	99.9	26523	PASS
443	442	15	24	19.8	5263	PASS