
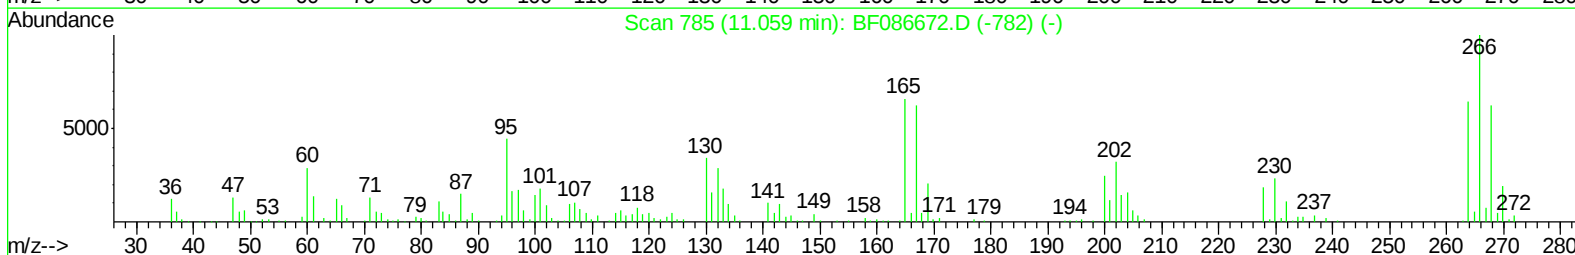
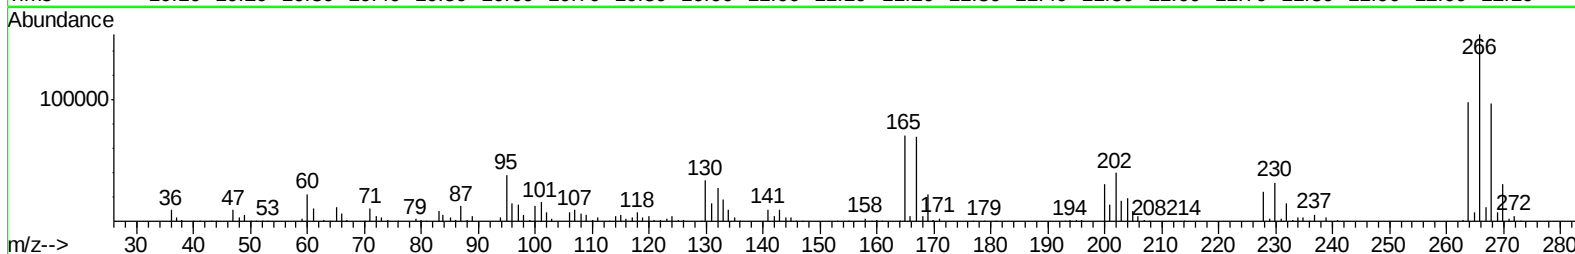


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF050416\  
Data File : BF086679.D  
Acq On : 4 May 2016 16:22  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 05 05:54:29 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050416.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed May 04 15:12:53 2016  
Response via : Initial Calibration

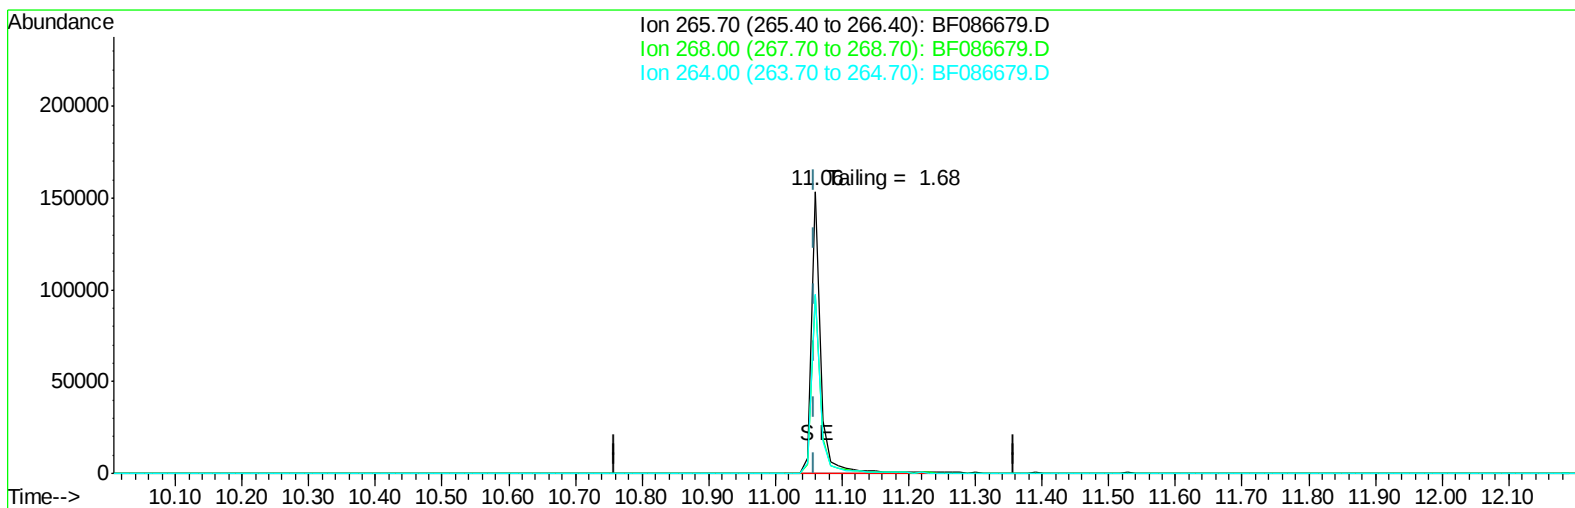

TIC: BF086679.D

(69) Pentachlorophenol (C)




11.059min (+0.000) 48901.28ng

response 147001

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 64.40 | 63.09 |
| 264.00 | 66.10 | 63.55 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF050416\  
Data File : BF086679.D  
Acq On : 4 May 2016 16:22  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 05 05:54:29 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050416.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed May 04 15:12:53 2016  
Response via : Initial Calibration

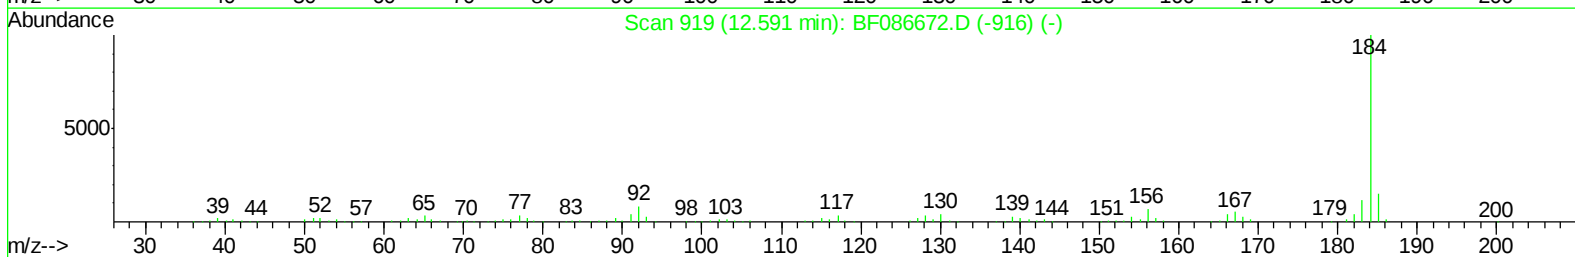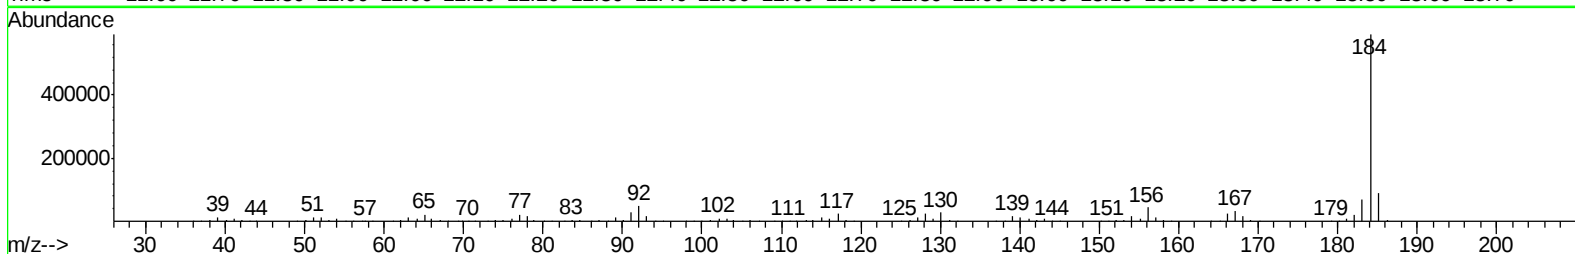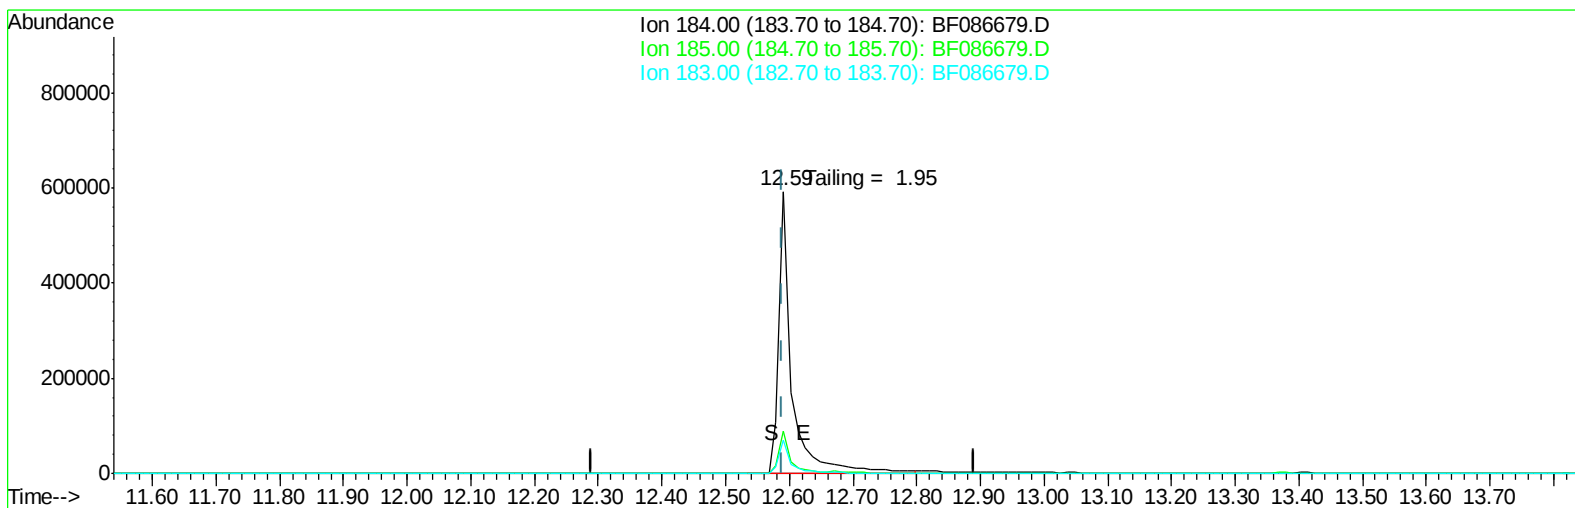

TIC: BF086679.D

(76) Benzidine

12.591min (+0.001) 56227.07ng

response 838529

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 17.00 | 14.97 |
| 183.00 | 12.20 | 11.90 |
| 0.00   | 0.00  | 0.00  |