


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050416\
 Data File : BF086667.D
 Acq On : 4 May 2016 10:23
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 04 15:12:53 2016

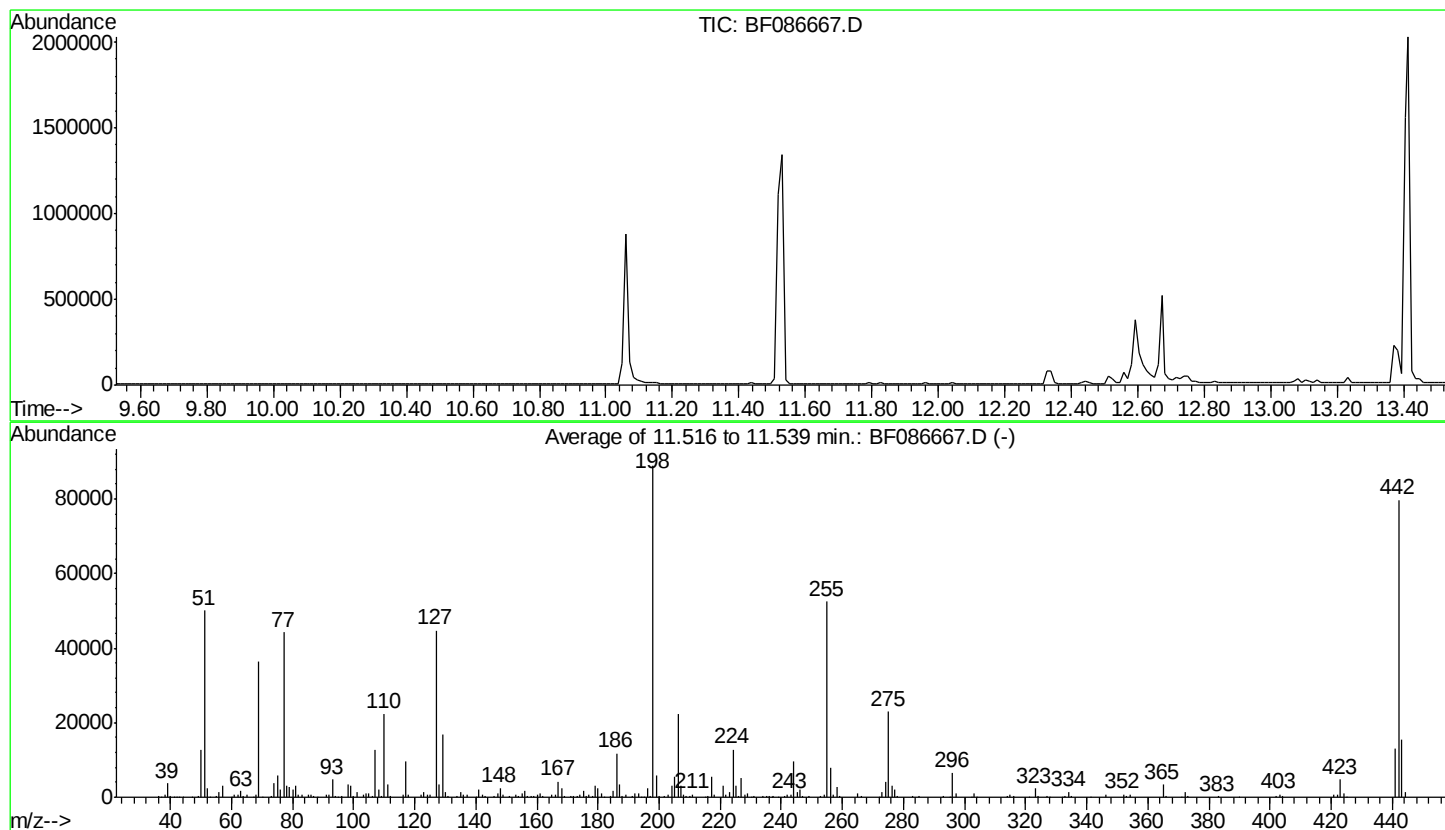

AutoFind: Scans 825, 826, 827; Background Corrected with Scan 821

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.3	50124	PASS
68	69	0.00	2	1.9	673	PASS
69	198	0.00	100	40.8	36283	PASS
70	69	0.00	2	0.5	171	PASS
127	198	10	80	50.4	44821	PASS
197	198	0.00	2	0.3	309	PASS
198	198	100	100	100.0	88963	PASS
199	198	5	9	6.7	5944	PASS
275	198	10	60	25.7	22859	PASS
365	198	1	100	3.8	3363	PASS
441	442	0.01	24	16.2	12959	PASS
442	198	50	100	89.7	79834	PASS
443	442	15	24	19.3	15395	PASS