


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050416\
 Data File : BF086679.D
 Acq On : 4 May 2016 16:22
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 04 15:12:53 2016

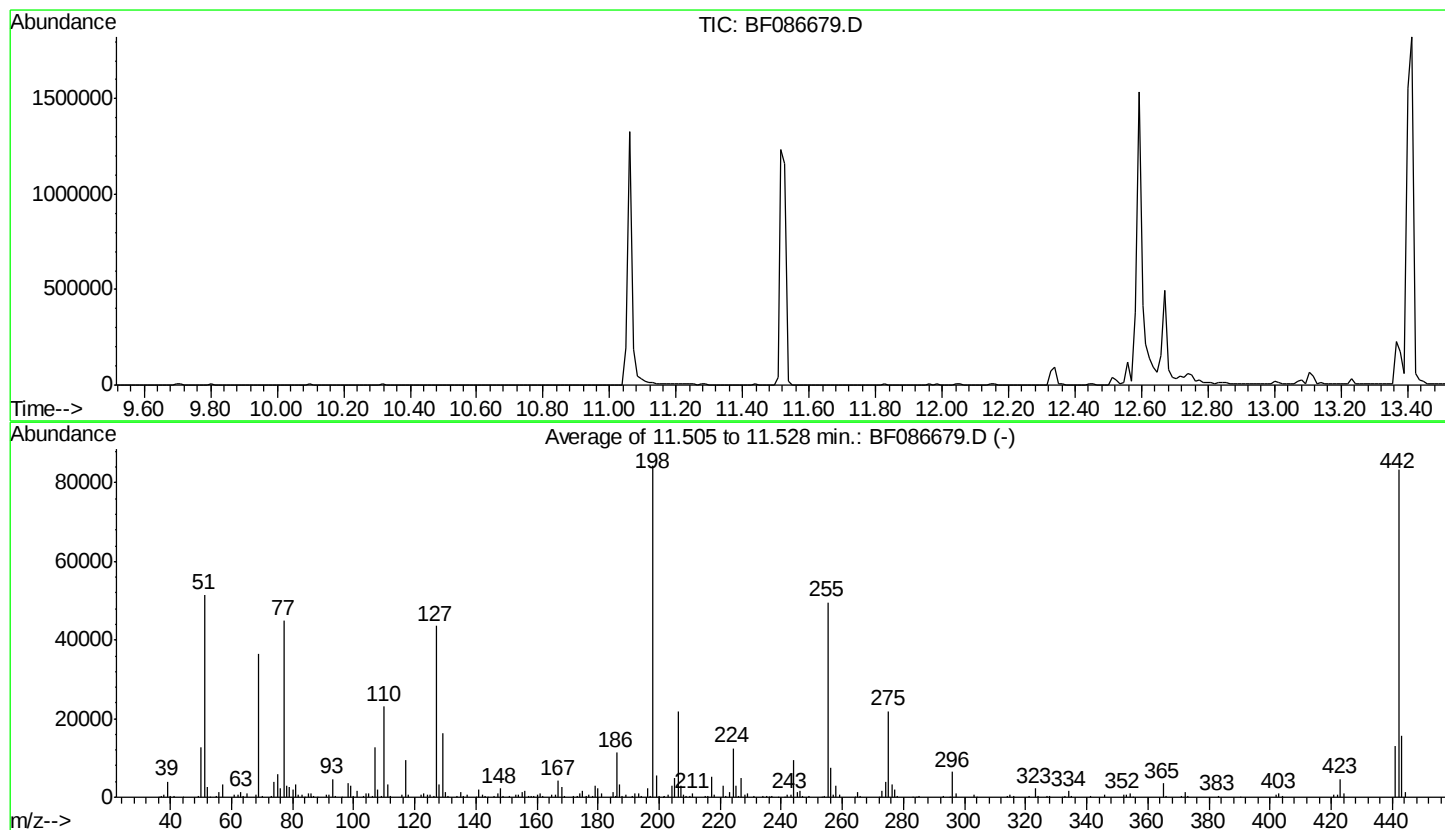

AutoFind: Scans 824, 825, 826; Background Corrected with Scan 821

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.0	51480	PASS
68	69	0.00	2	1.8	647	PASS
69	198	0.00	100	43.3	36540	PASS
70	69	0.00	2	0.6	215	PASS
127	198	10	80	51.7	43638	PASS
197	198	0.00	2	0.4	365	PASS
198	198	100	100	100.0	84391	PASS
199	198	5	9	6.4	5429	PASS
275	198	10	60	26.0	21943	PASS
365	198	1	100	4.2	3529	PASS
441	442	0.01	24	15.5	12883	PASS
442	198	50	100	98.7	83253	PASS
443	442	15	24	18.9	15739	PASS