

Data Path : Z:\HPCHEM1\BNA_F\Data\BF050417\
 Data File : BF094877.D
 Acq On : 4 May 2017 16:54
 Operator : SJ/MA
 Sample : I2936-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP3-COMP(0.5-4.5FT)

Quant Time: May 04 17:26:50 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 03 17:24:51 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	80364	20.00	ng	0.00
21) Naphthalene-d8	9.74	136	324591	20.00	ng	-0.01
38) Acenaphthene-d10	12.57	164	150426	20.00	ng	-0.01
63) Phenanthrene-d10	14.97	188	288047	20.00	ng	-0.01
75) Chrysene-d12	18.64	240	277512	20.00	ng	-0.02
86) Perylene-d12	20.30	264	222656	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.68	112	618540	128.32	ng	0.00
7) Phenol-d6	7.27	99	677974	117.22	ng	-0.01
23) Nitrobenzene-d5	8.62	82	482268	93.69	ng	-0.02
41) 2,4,6-Tribromophenol	13.87	330	189110	153.51	ng	-0.02
44) 2-Fluorobiphenyl	11.52	172	941965	90.13	ng	-0.01
78) Terphenyl-d14	17.30	244	969631	76.96	ng	-0.01
Target Compounds						
19) n-Nitroso-di-n-propylamine	8.62	70	62150	15.89	ng	# 76
50) 2,6-Dinitrotoluene	12.57	165	15496	6.15	ng	# 31
76) Benzidine	16.98	184	23155	9.25	ng	# 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\Data\BF050417\
Data File : BF094877.D
Acq On : 4 May 2017 16:54
Operator : SJ/MA
Sample : I2936-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP3-COMP(0.5-4.5FT)

Quant Time: May 04 17:26:50 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

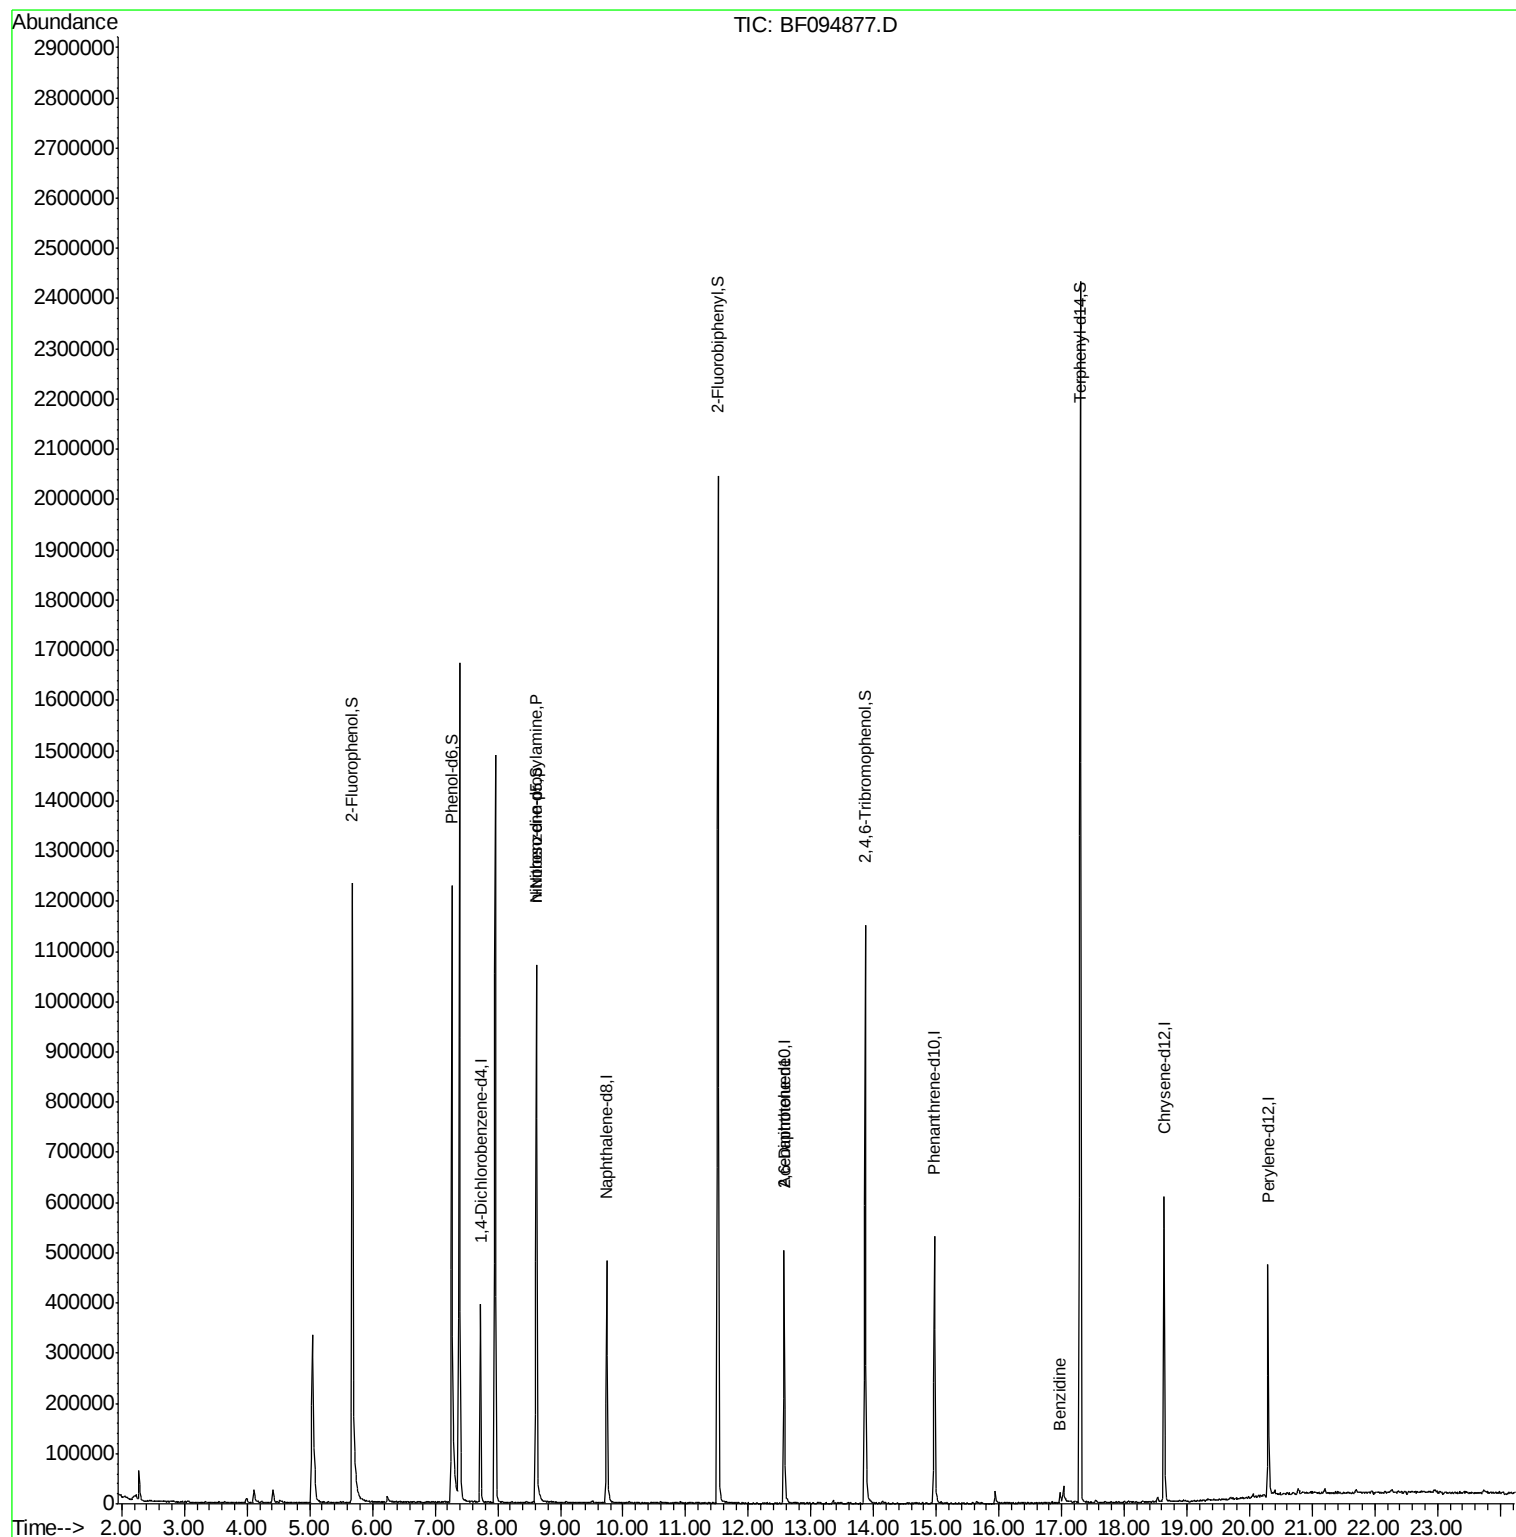

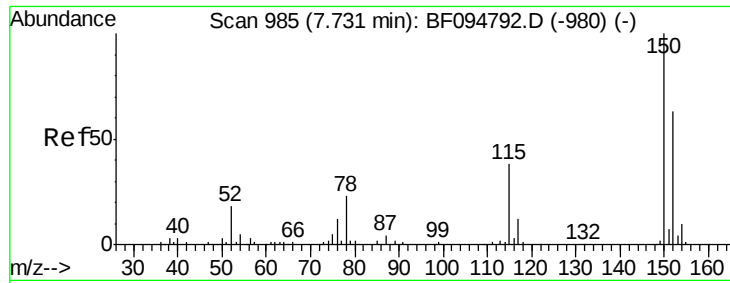


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.72 min Scan# 984
Delta R.T. -0.01 min
Lab File: BF094877.D
Acq: 4 May 2017 16:54

Instrument :
BNA_F
ClientSampleId :
TP3-COMP(0.5-4.5FT)

Tgt Ion:152 Resp: 80364
Ion Ratio Lower Upper
152 100
150 162.3 126.2 189.2
115 60.7 52.2 78.2

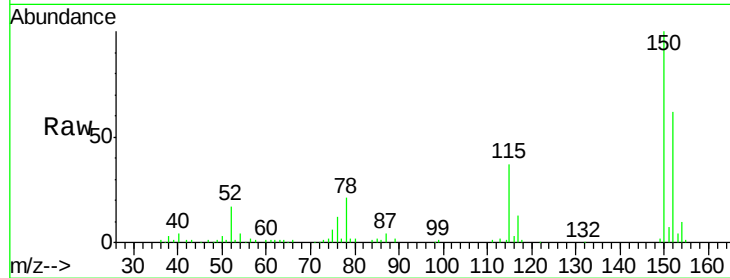


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

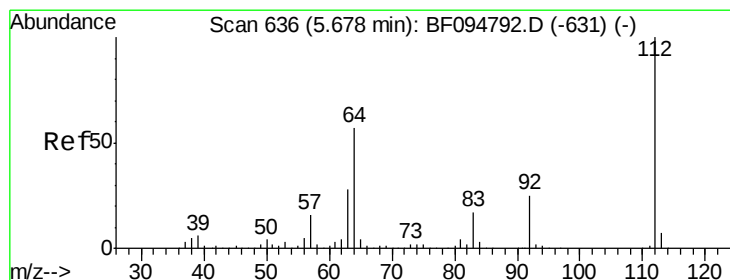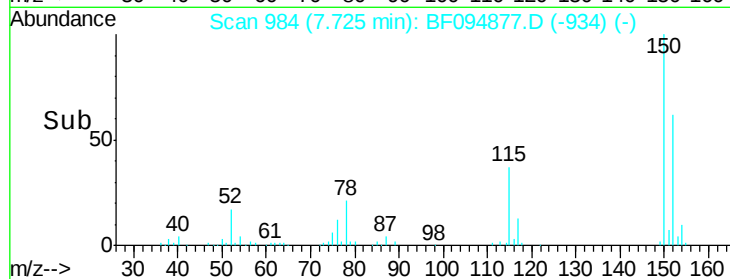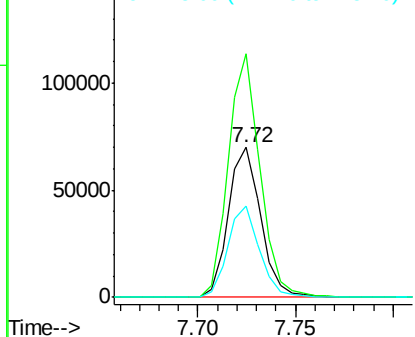



#5


2-Fluorophenol
Concen: 128.32 ng
RT: 5.68 min Scan# 637
Delta R.T. 0.01 min
Lab File: BF094877.D
Acq: 4 May 2017 16:54

Tgt Ion:112 Resp: 618540
Ion Ratio Lower Upper
112 100
64 54.2 46.0 69.0
63 26.5 23.4 35.0

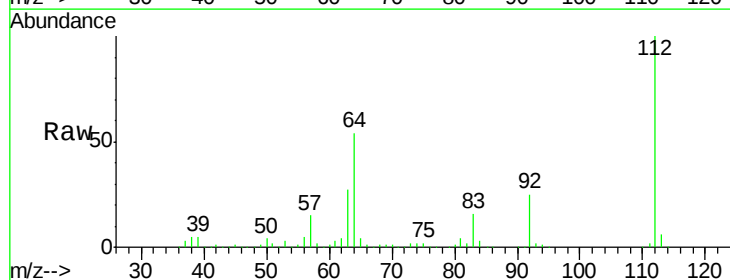

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

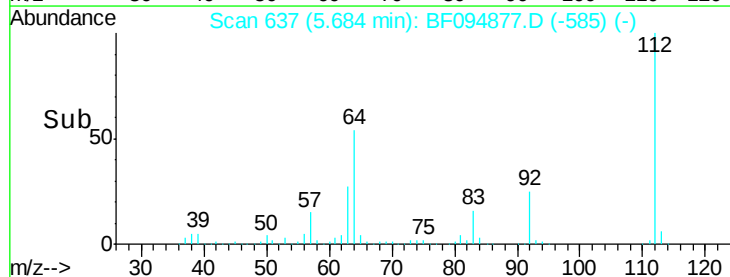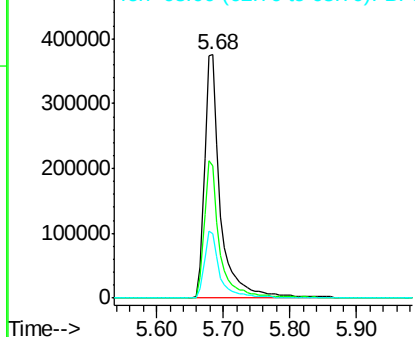

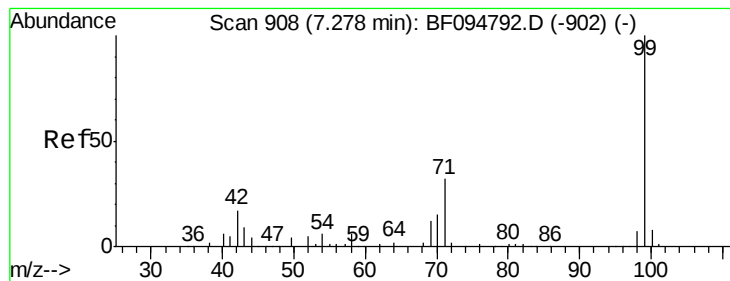

#7

Phenol-d6

Concen: 117.22 ng

RT: 7.27 min Scan# 906

Delta R.T. -0.01 min

Lab File: BF094877.D

Acq: 4 May 2017 16:54

Instrument :

BNA_F

ClientSampleId :

TP3-COMP(0.5-4.5FT)


Tgt Ion: 99 Resp: 677974

Ion Ratio Lower Upper

99 100

42 16.9 13.5 20.3




71 32.1 24.5 36.7

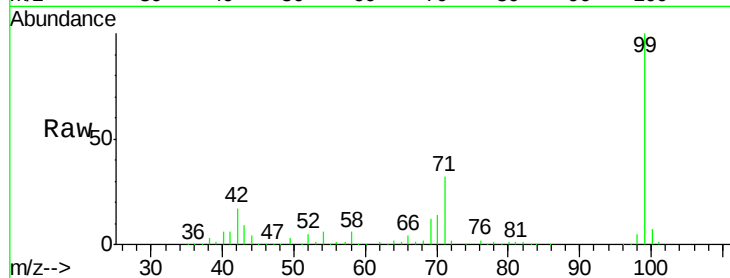

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

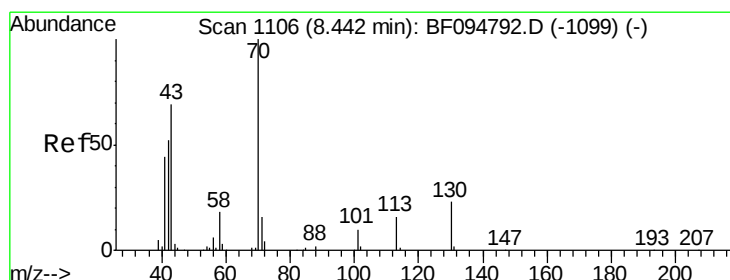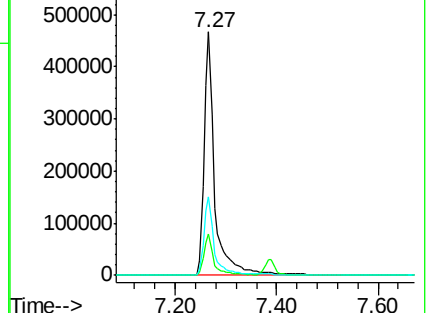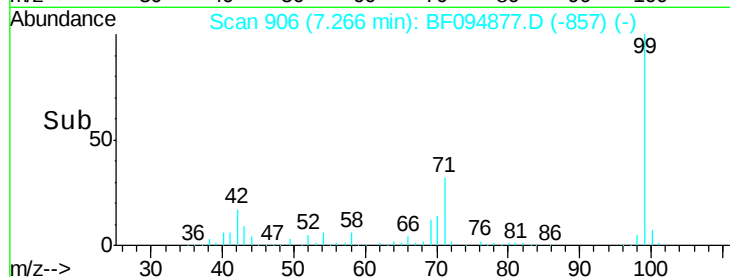

#19

n-Nitroso-di-n-propylamine

Concen: 15.89 ng

RT: 8.62 min Scan# 1136

Delta R.T. 0.18 min

Lab File: BF094877.D

Acq: 4 May 2017 16:54

Tgt Ion: 70 Resp: 62150


Ion Ratio Lower Upper

70 100

42 44.3 47.2 70.8#

101 0.0 7.2 10.8#

130 2.6 15.9 23.9#


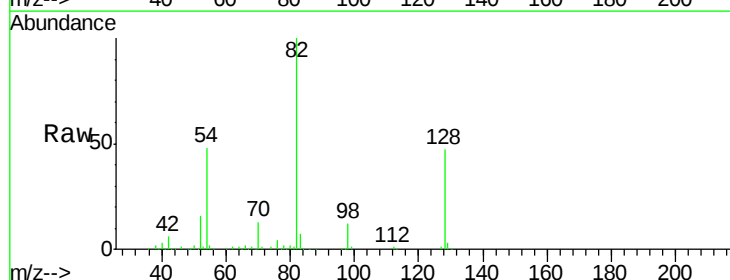



Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

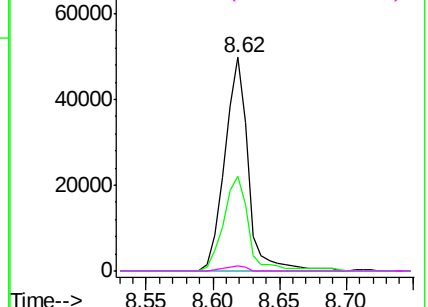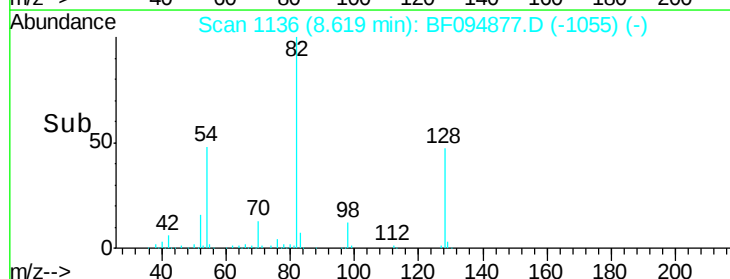

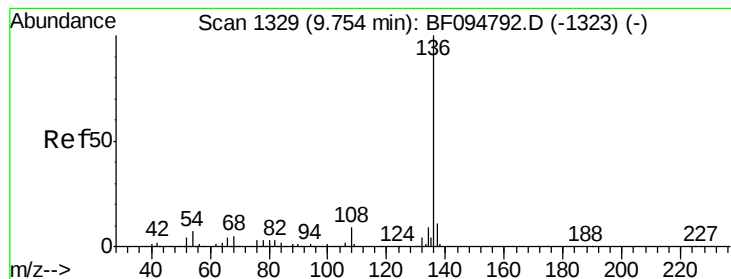

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.74 min Scan# 1327

Delta R.T. -0.01 min

Lab File: BF094877.D

Acq: 4 May 2017 16:54

Instrument :

BNA_F

ClientSampleId :

TP3-COMP(0.5-4.5FT)

Tgt Ion:136 Resp: 324591



Ion Ratio Lower Upper

136 100

137 11.2 8.5 12.7

54 6.6 4.9 7.3

68 5.9 4.1 6.1

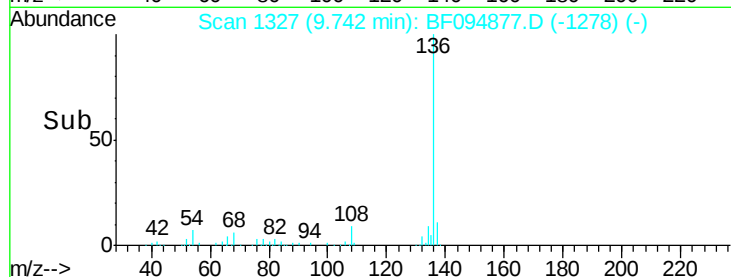
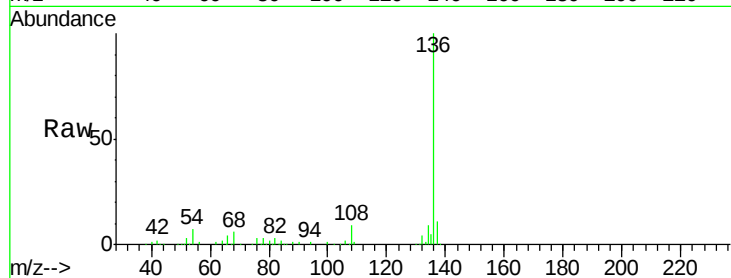


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

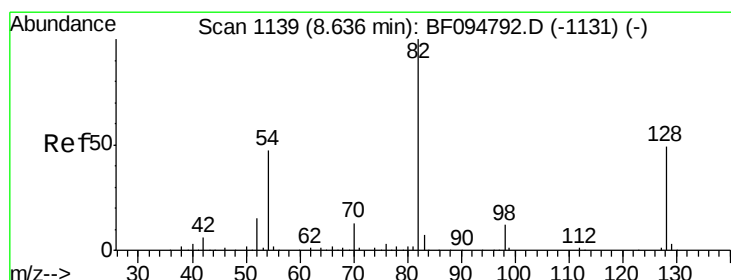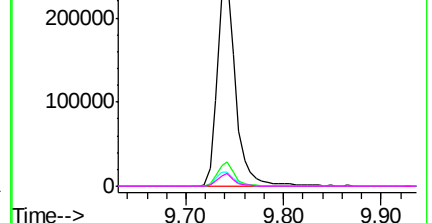

#23

Nitrobenzene-d5

Concen: 93.69 ng

RT: 8.62 min Scan# 1136

Delta R.T. -0.02 min

Lab File: BF094877.D

Acq: 4 May 2017 16:54



Tgt Ion: 82 Resp: 482268

Ion Ratio Lower Upper

82 100

128 47.2 34.0 51.0


54 48.1 42.2 63.2

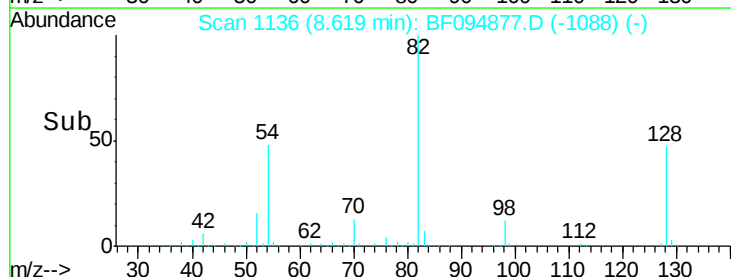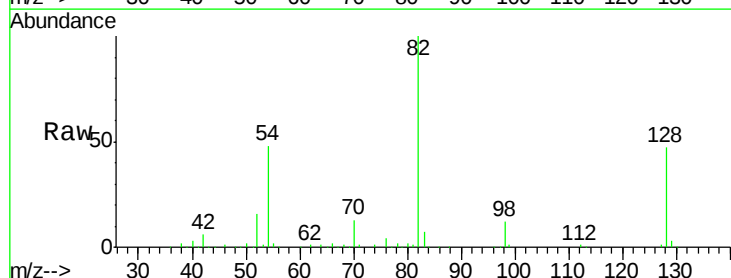


Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

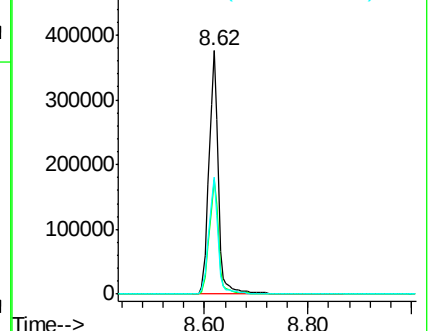

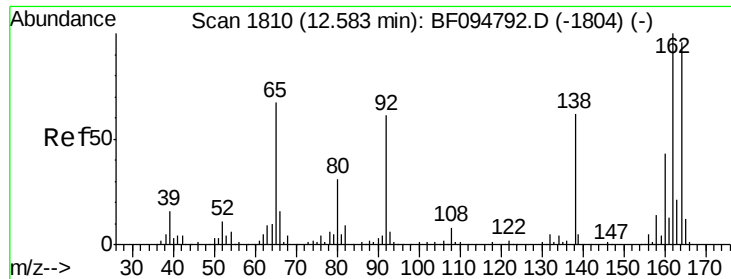

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 12.57 min Scan# 1808

Delta R.T. -0.01 min

Lab File: BF094877.D

Acq: 4 May 2017 16:54

Instrument :

BNA_F

ClientSampleId :

TP3-COMP(0.5-4.5FT)


Tgt Ion:164 Resp: 150426

Ion Ratio Lower Upper

164 100

162 106.3 82.6 123.8




160 45.8 36.2 54.2

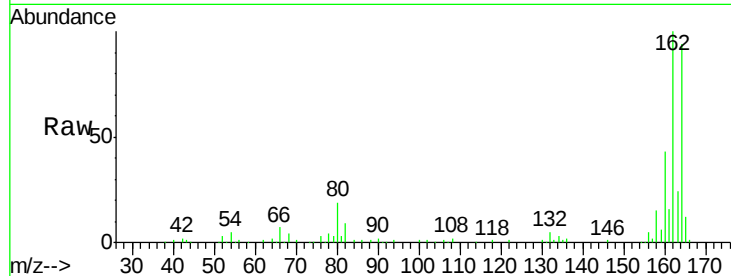

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

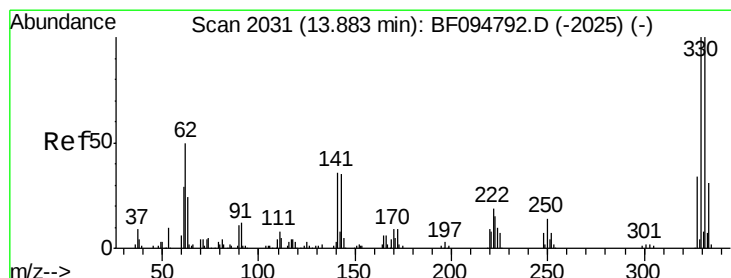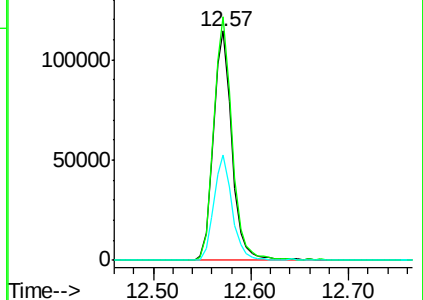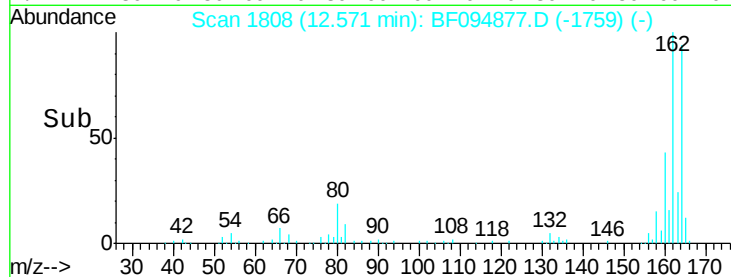

#41

2,4,6-Tribromophenol

Concen: 153.51 ng

RT: 13.87 min Scan# 2028

Delta R.T. -0.02 min

Lab File: BF094877.D

Acq: 4 May 2017 16:54


Tgt Ion:330 Resp: 189110

Ion Ratio Lower Upper

330 100

332 95.1 76.6 115.0



141 38.1 31.4 47.2

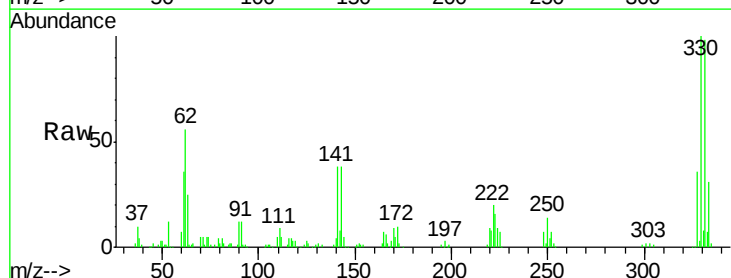


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



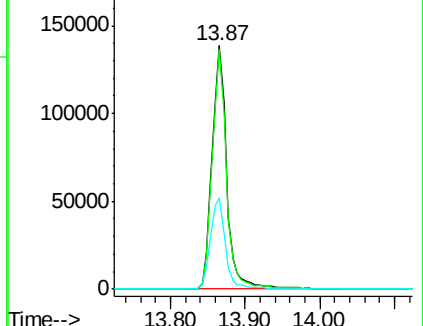
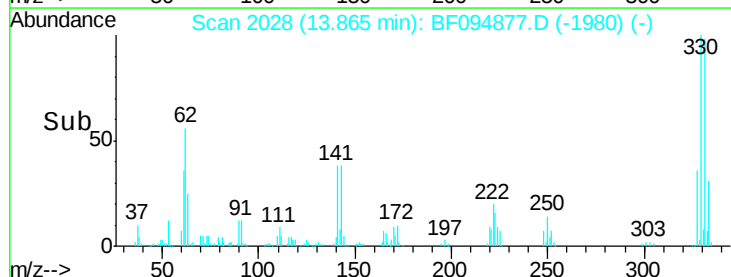


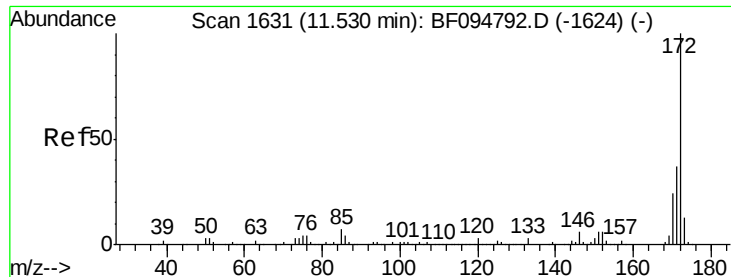

#44
 2-Fluorobiphenyl
 Concen: 90.13 ng
 RT: 11.52 min Scan# 1629
 Delta R.T. -0.01 min
 Lab File: BF094877.D
 Acq: 4 May 2017 16:54




Instrument :
 BNA_F
 ClientSampleId :
 TP3-COMP(0.5-4.5FT)


Tgt Ion:172 Resp: 941965
 Ion Ratio Lower Upper
 172 100
 171 35.4 29.6 44.4
 170 23.4 19.8 29.8

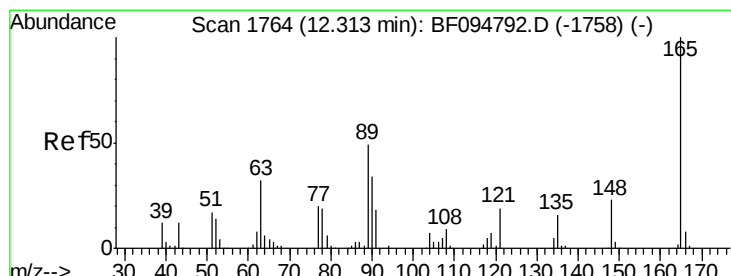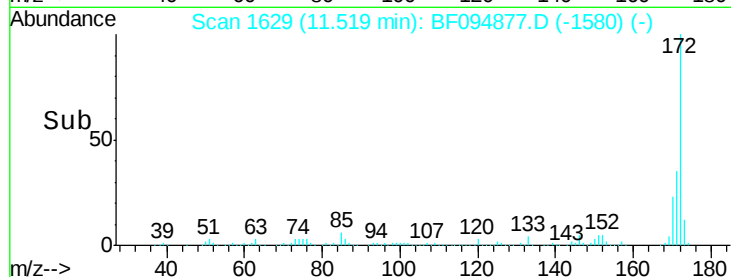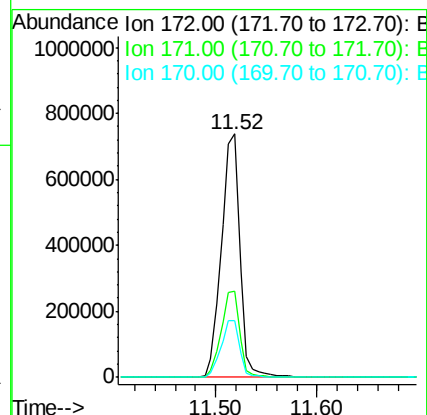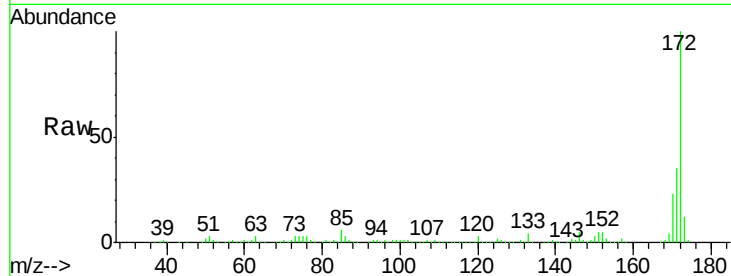

#50
 2,6-Dinitrotoluene
 Concen: 6.15 ng
 RT: 12.57 min Scan# 1808
 Delta R.T. 0.26 min
 Lab File: BF094877.D
 Acq: 4 May 2017 16:54

Tgt Ion:165 Resp: 15496
 Ion Ratio Lower Upper
 165 100
 63 0.0 34.3 51.5#
 89 0.0 37.1 55.7#


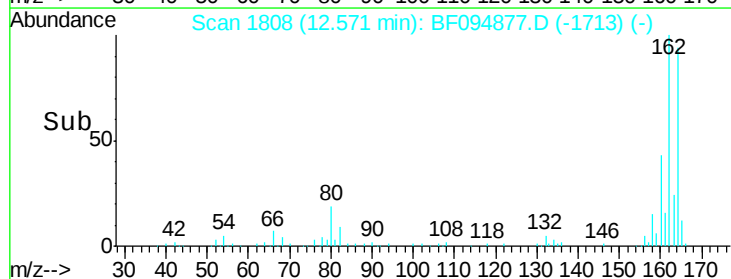
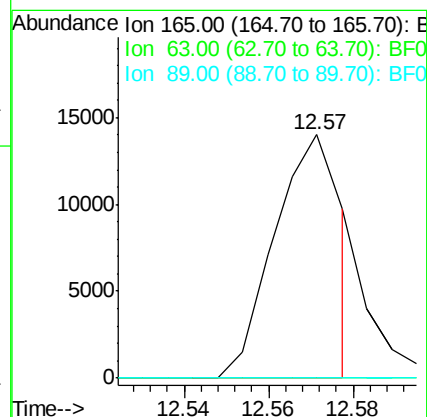
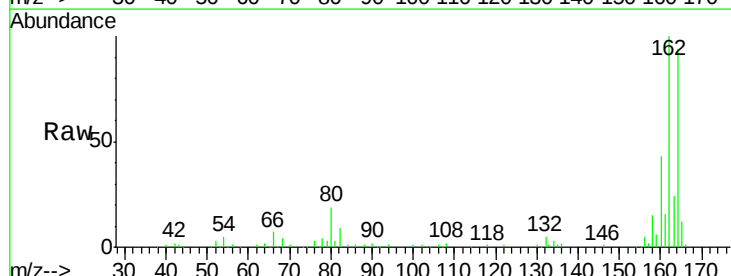


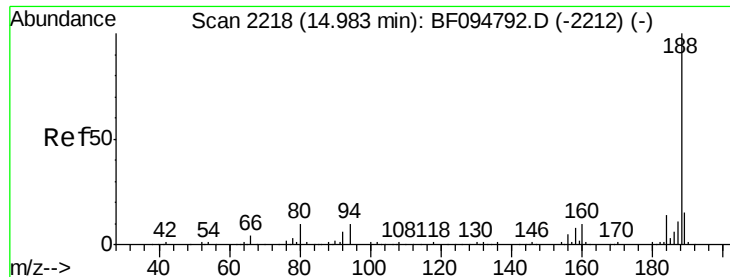

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 14.97 min Scan# 2216
Delta R.T. -0.01 min
Lab File: BF094877.D
Acq: 4 May 2017 16:54




Instrument :
BNA_F
ClientSampleId :
TP3-COMP(0.5-4.5FT)


Tgt Ion:188 Resp: 288047
Ion Ratio Lower Upper
188 100
94 9.7 9.4 14.2
80 11.1 10.2 15.2

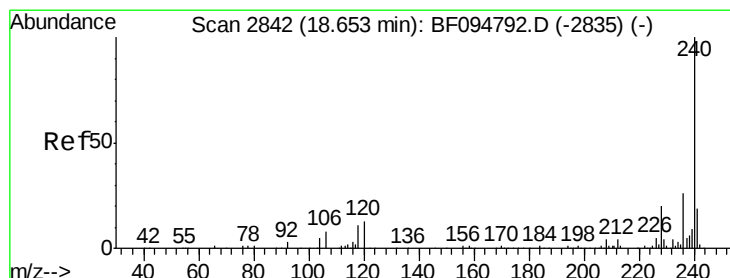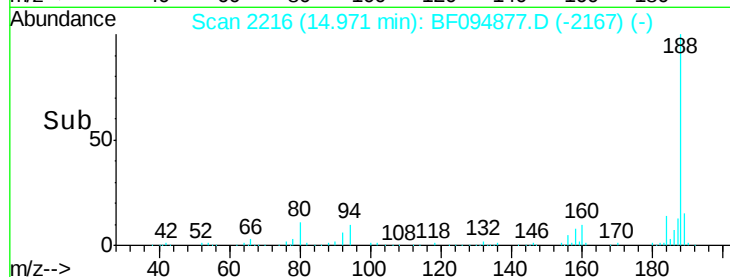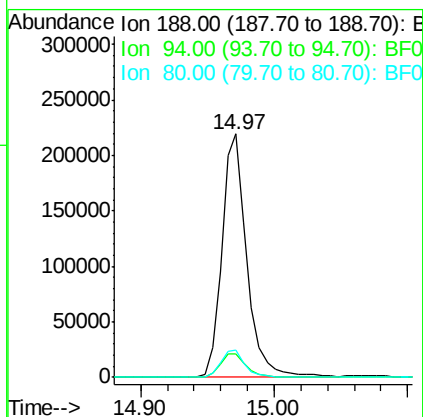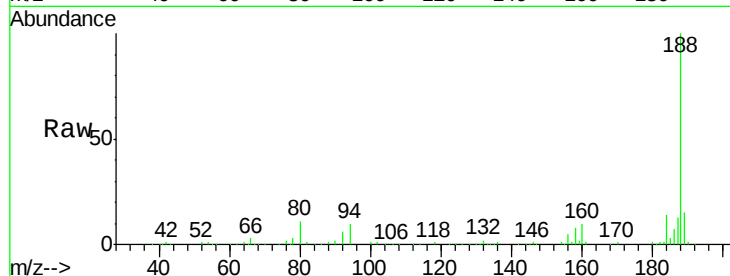

#75
Chrysene-d12
Concen: 20.00 ng
RT: 18.64 min Scan# 2839
Delta R.T. -0.02 min
Lab File: BF094877.D
Acq: 4 May 2017 16:54

Tgt Ion:240 Resp: 277512
Ion Ratio Lower Upper
240 100
120 13.3 5.8 8.8#
236 24.3 20.5 30.7

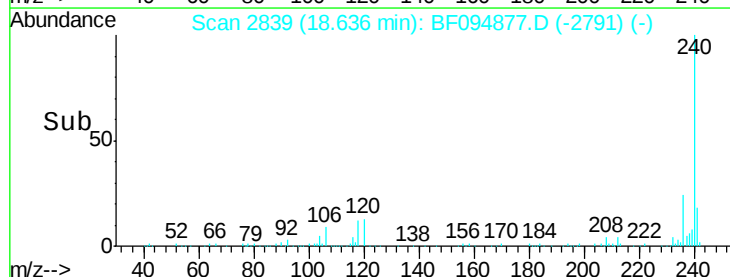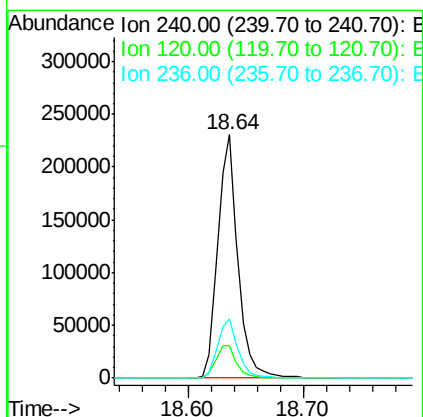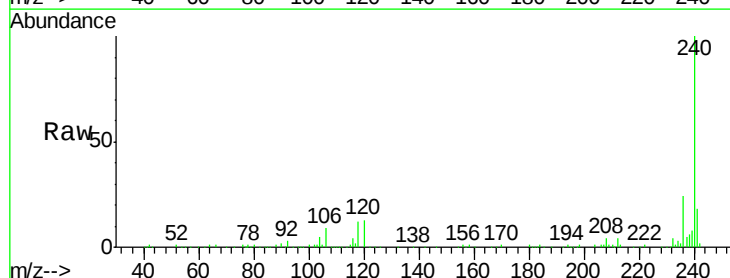


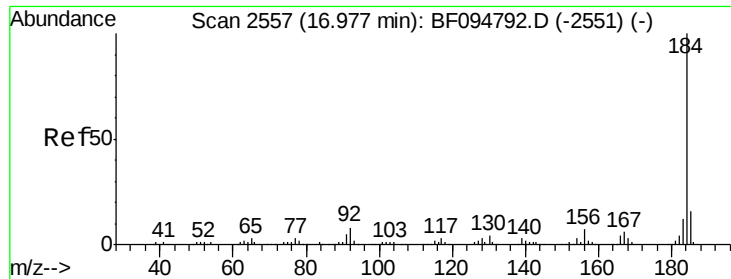




#76
Benzidine
Concen: 9.25 ng
RT: 16.98 min Scan# 2557
Delta R.T. 0.00 min
Lab File: BF094877.D
Acq: 4 May 2017 16:54

Instrument :
BNA_F
ClientSampleId :
TP3-COMP(0.5-4.5FT)

Tgt Ion:184 Resp: 23155
Ion Ratio Lower Upper
184 100
185 14.6 15.5 23.3#
183 13.1 9.8 14.6

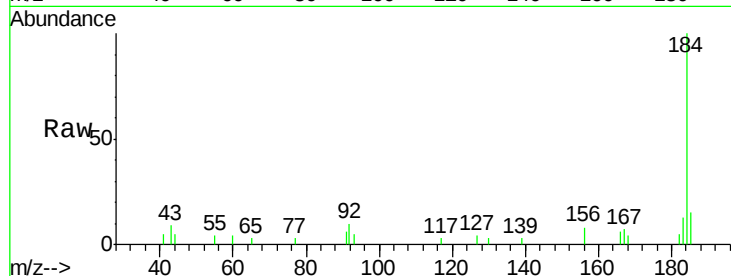


Abundance Ion 184.00 (183.70 to 184.70): E
Ion 185.00 (184.70 to 185.70): E
Ion 183.00 (182.70 to 183.70): E

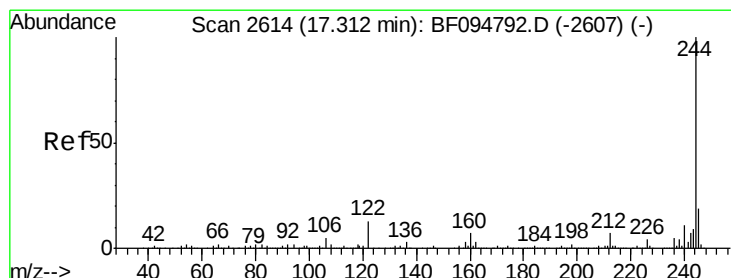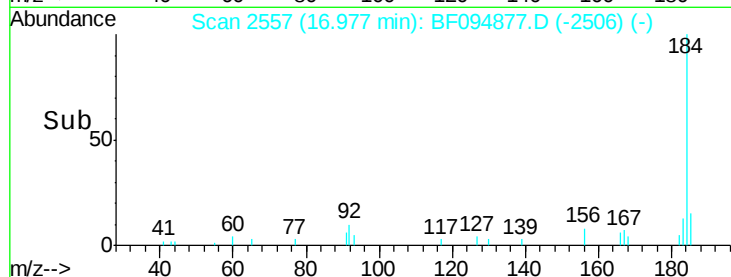
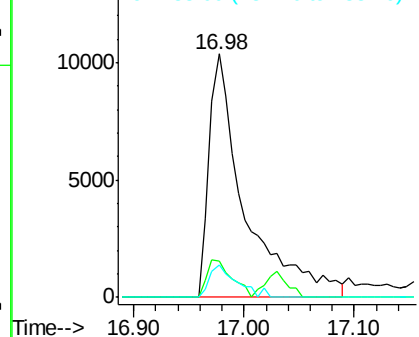



#78
Terphenyl-d14
Concen: 76.96 ng
RT: 17.30 min Scan# 2612
Delta R.T. -0.01 min
Lab File: BF094877.D
Acq: 4 May 2017 16:54

Tgt Ion:244 Resp: 969631
Ion Ratio Lower Upper
244 100
212 7.2 6.0 9.0
122 13.9 10.3 15.5

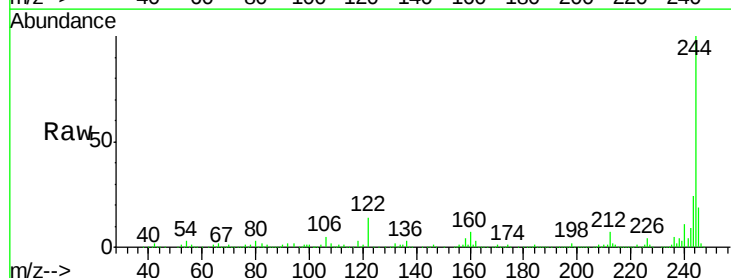

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

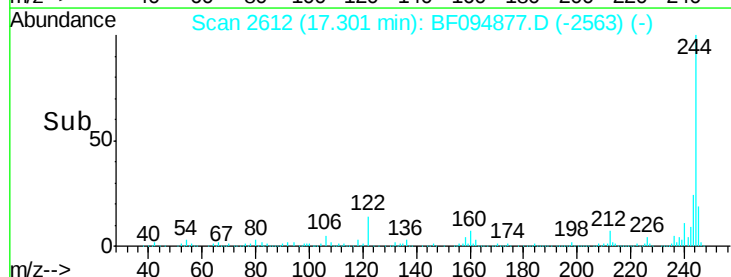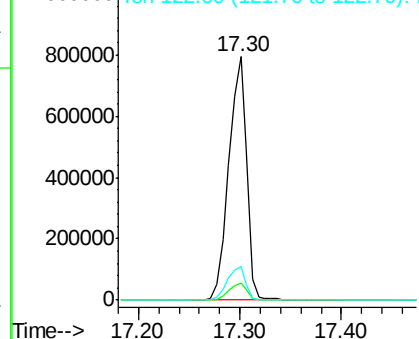


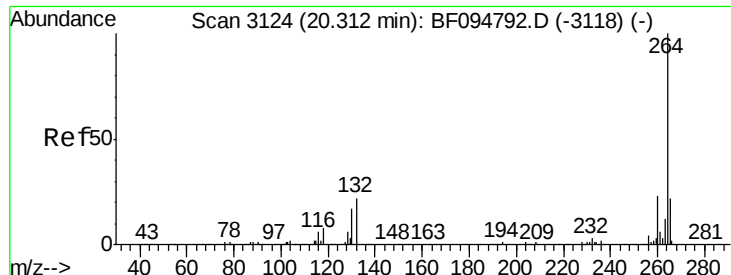

#86
Perylene-d12
Concen: 20.00 ng
RT: 20.30 min Scan# 3122
Delta R.T. -0.01 min
Lab File: BF094877.D
Acq: 4 May 2017 16:54

Instrument :
BNA_F
ClientSampleId :
TP3-COMP(0.5-4.5FT)

Tgt Ion	Ratio	Lower	Upper
264	100		
260	22.3	19.5	29.3
265	20.6	17.2	25.8

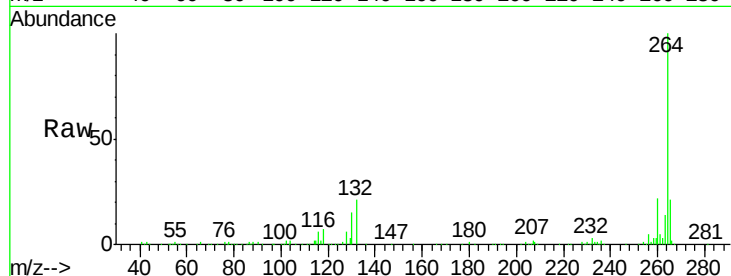

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

