

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050417\
 Data File : BF094884.D
 Acq On : 4 May 2017 20:38
 Operator : SJ/MA
 Sample : I2916-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: May 05 01:25:24 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 03 17:24:51 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	82022	20.00	ng	-0.01
21) Naphthalene-d8	9.74	136	326225	20.00	ng	-0.02
38) Acenaphthene-d10	12.57	164	155372	20.00	ng	-0.02
63) Phenanthrene-d10	14.97	188	309531	20.00	ng	-0.02
75) Chrysene-d12	18.64	240	266141	20.00	ng	-0.02
86) Perylene-d12	20.30	264	193675	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.67	112	720335	146.42	ng	-0.01
7) Phenol-d6	7.27	99	908863	153.97	ng	-0.01
23) Nitrobenzene-d5	8.62	82	514999	99.55	ng	-0.02
41) 2,4,6-Tribromophenol	13.87	330	169324	133.07	ng	-0.02
44) 2-Fluorobiphenyl	11.51	172	738741	68.44	ng	-0.02
78) Terphenyl-d14	17.29	244	583058	48.25	ng	-0.02
Target Compounds						
15) Benzyl Alcohol	7.96	79	10753	2.83	ng	# 79
19) n-Nitroso-di-n-propylamine	8.62	70	67168	16.82	ng	# 76
49) Dimethylphthalate	12.21	163	130756	10.25	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050417\
Data File : BF094884.D
Acq On : 4 May 2017 20:38
Operator : SJ/MA
Sample : I2916-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: May 05 01:25:24 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

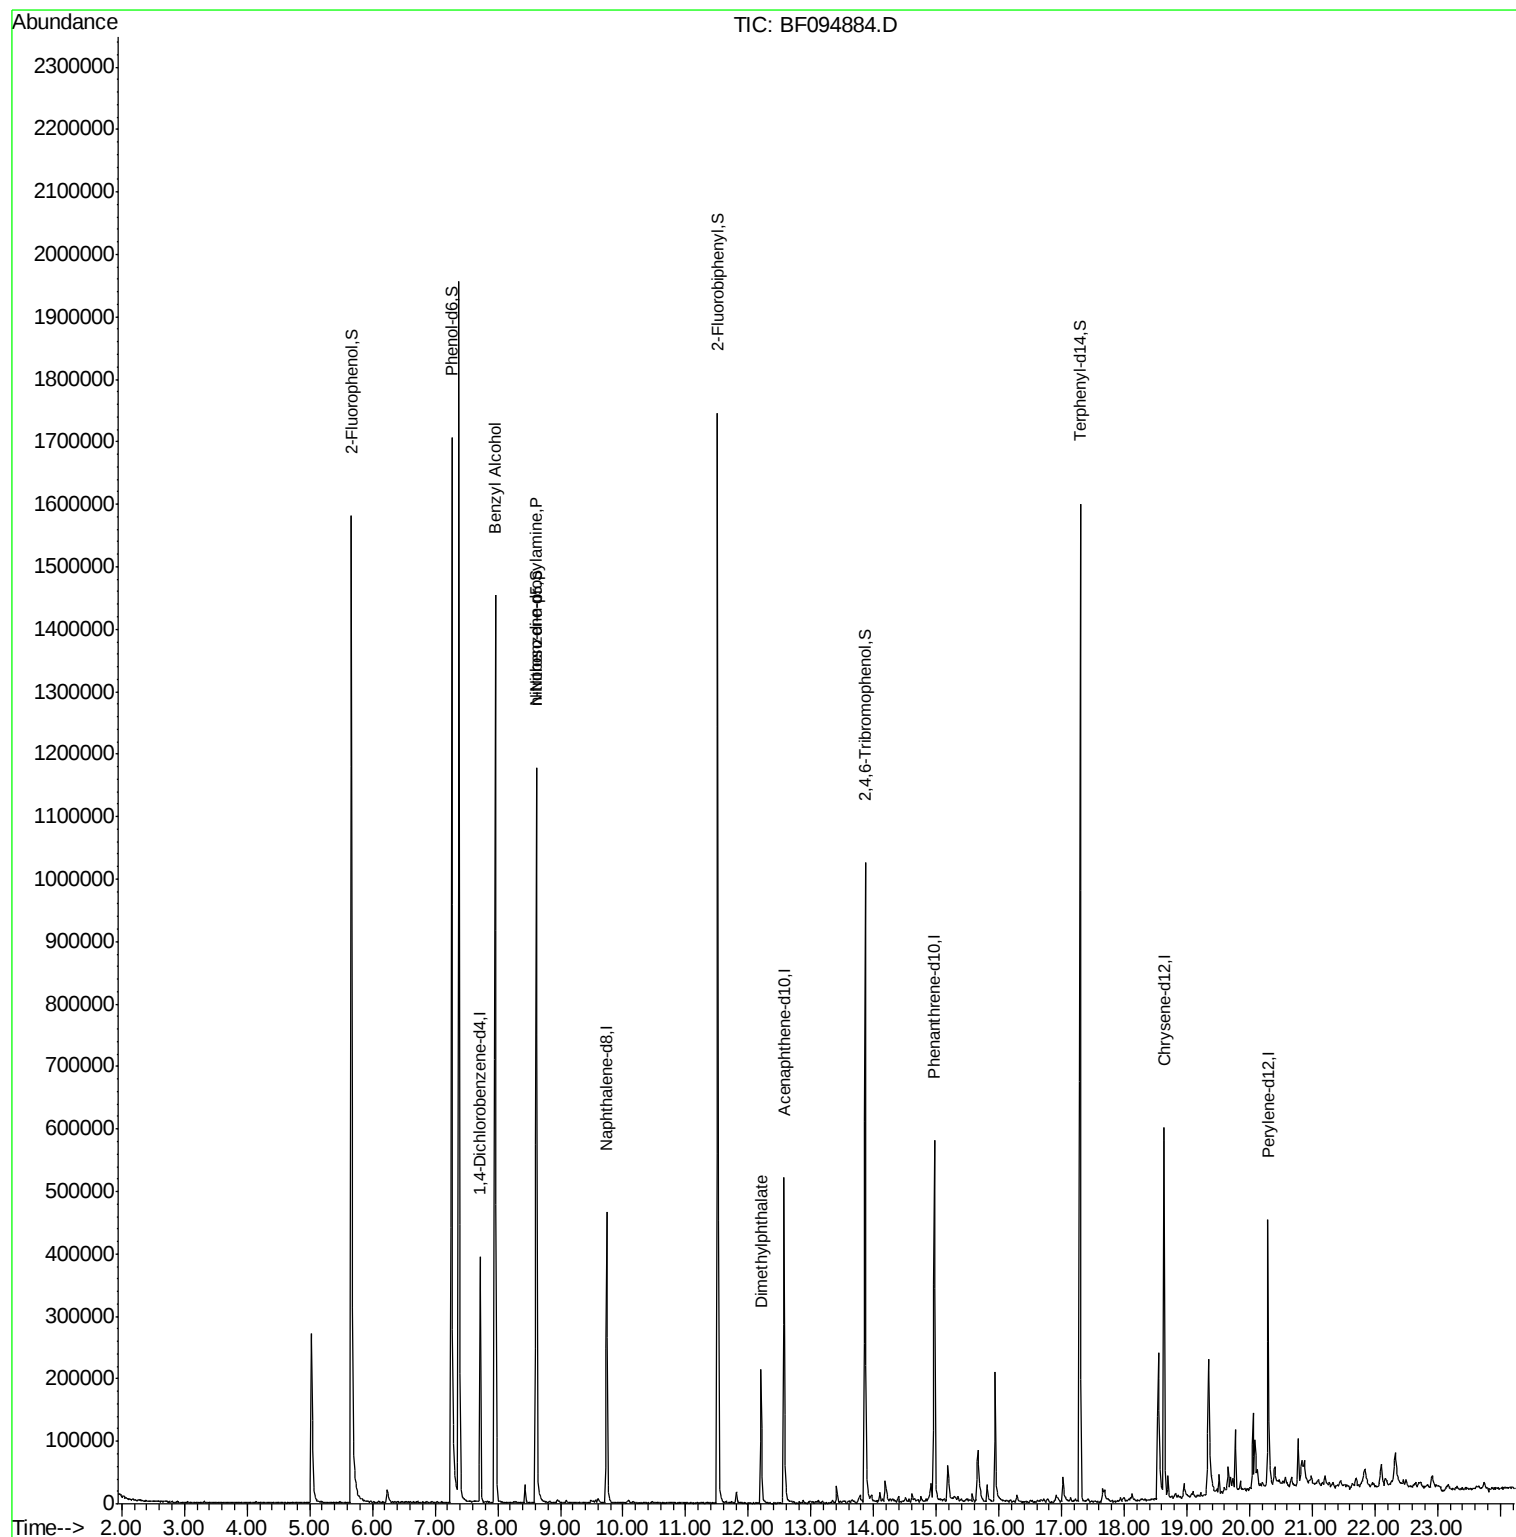

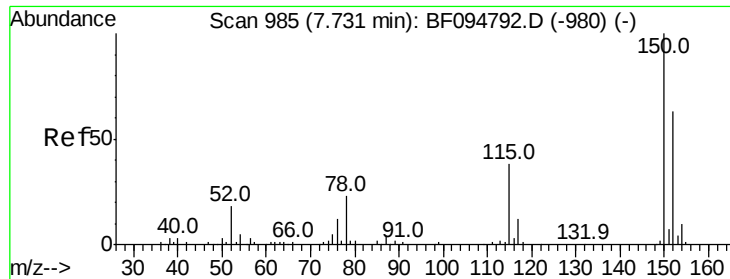


#1



1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.72 min Scan# 983
Delta R.T. -0.01 min
Lab File: BF094884.D
Acq: 4 May 2017 20:38

Instrument :
BNA_F
ClientSampled :

Tot Ion:152 Resp: 82022
Ion Ratio Lower Upper
152 100
150 161.3 126.2 189.2
115 62.2 52.2 78.2

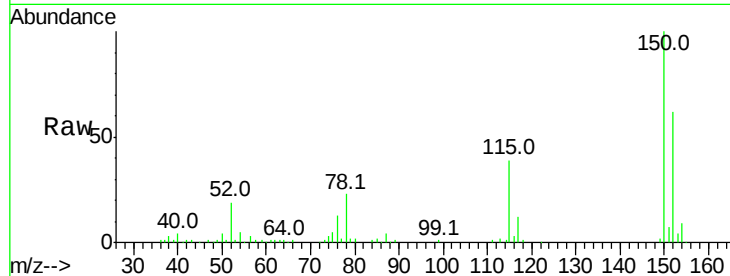


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

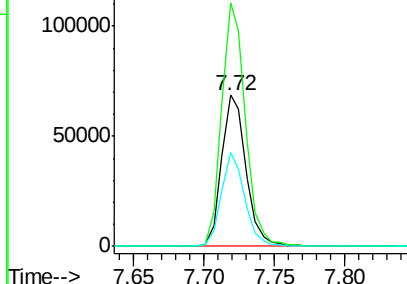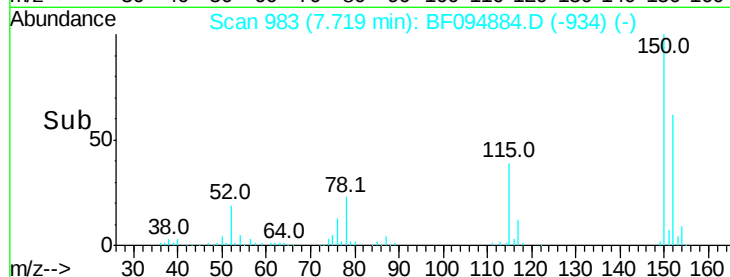



#5

2-Fluorophenol
Concen: 146.42 ng
RT: 5.67 min Scan# 634
Delta R.T. -0.01 min
Lab File: BF094884.D
Acq: 4 May 2017 20:38

Tgt Ion:112 Resp: 720335
Ion Ratio Lower Upper
112 100
64 56.4 46.0 69.0
63 28.5 23.4 35.0

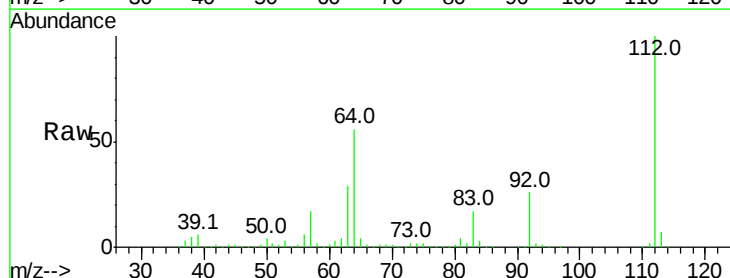

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

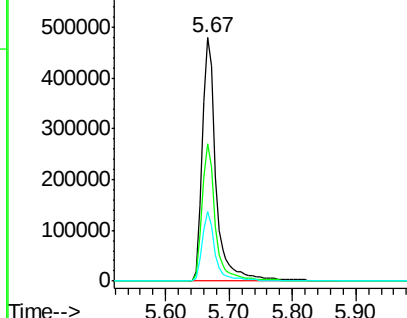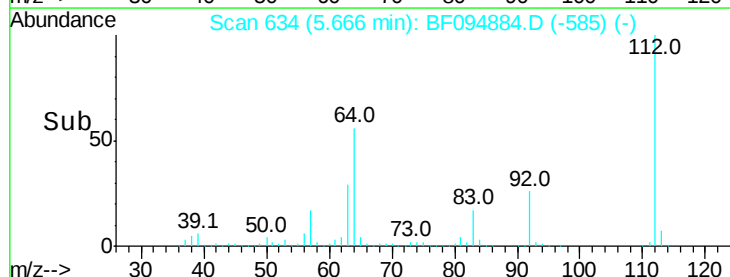



#7

Phenol-d6

Concen: 153.97 ng

RT: 7.27 min Scan# 906

Delta R.T. -0.01 min

Lab File: BF094884.D

Acq: 4 May 2017 20:38

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 908863

Ion Ratio Lower Upper

99 100

42 16.9 13.5 20.3




71 32.4 24.5 36.7

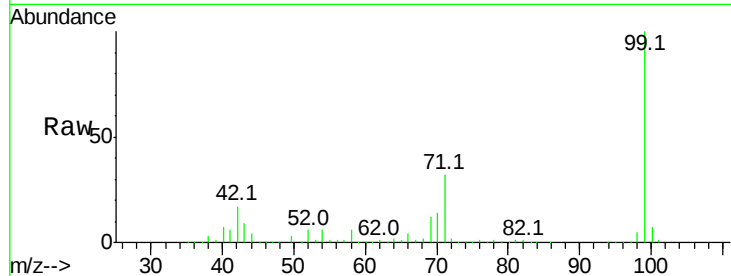

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

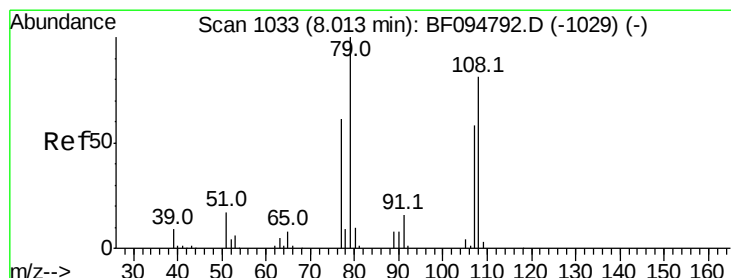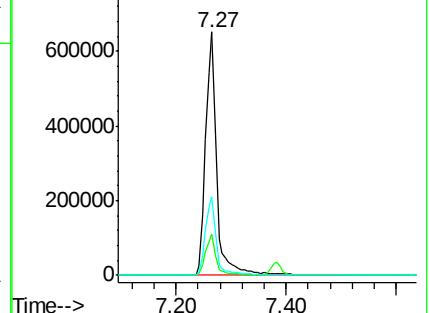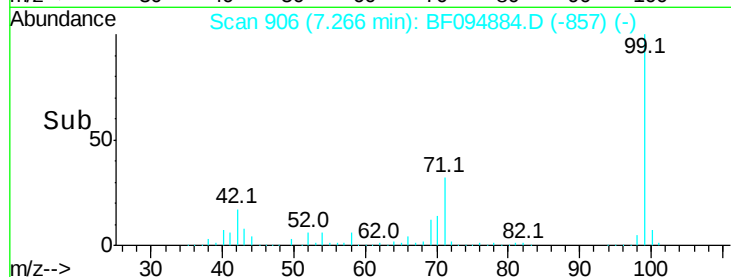

#15

Benzyl Alcohol

Concen: 2.83 ng

RT: 7.96 min Scan# 1024

Delta R.T. -0.05 min

Lab File: BF094884.D

Acq: 4 May 2017 20:38


Tgt Ion: 79 Resp: 10753

Ion Ratio Lower Upper

79 100

108 75.7 63.4 95.0



77 95.0 49.2 73.8#

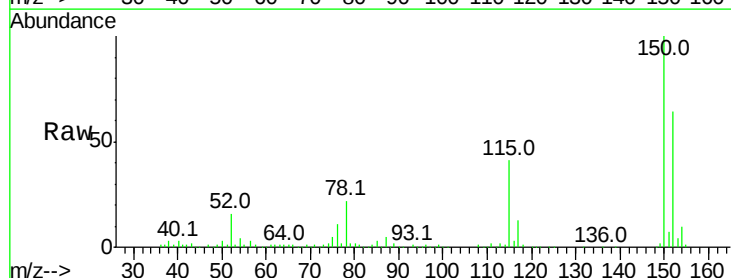

Abundance Ion 79.00 (78.70 to 79.70): BF0

Ion 108.00 (107.70 to 108.70): BF0

Ion 77.00 (76.70 to 77.70): BF0



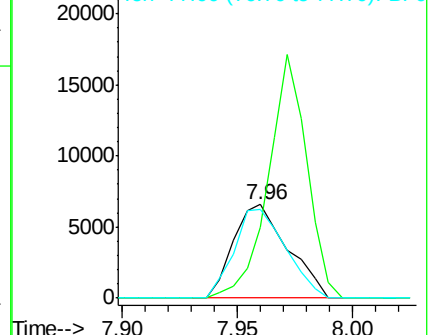
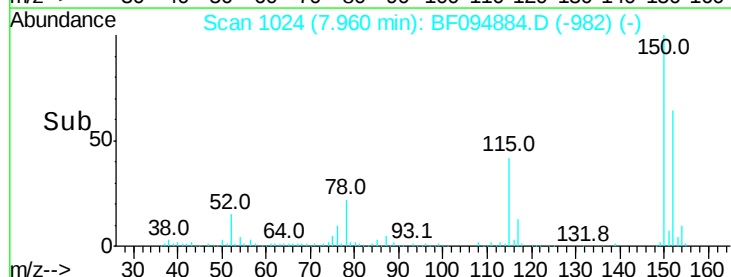




#19
n-Nitroso-di-n-propylamine
Concen: 16.82 ng
RT: 8.62 min Scan# 1136
Delta R.T. 0.18 min
Lab File: BF094884.D
Acq: 4 May 2017 20:38




Instrument :
BNA_F
ClientSampleId :

Tot Ion: 70 Resp: 67168
Ion Ratio Lower Upper
70 100
42 44.3 47.2 70.8#
101 0.0 7.2 10.8#
130 2.7 15.9 23.9#

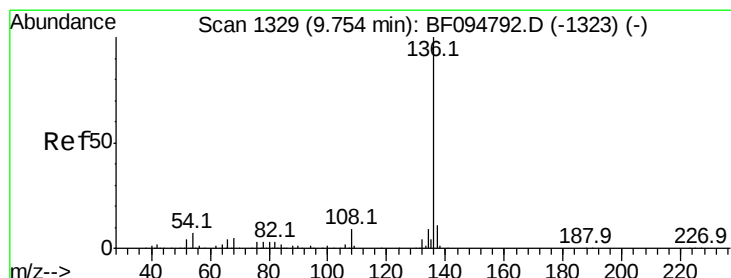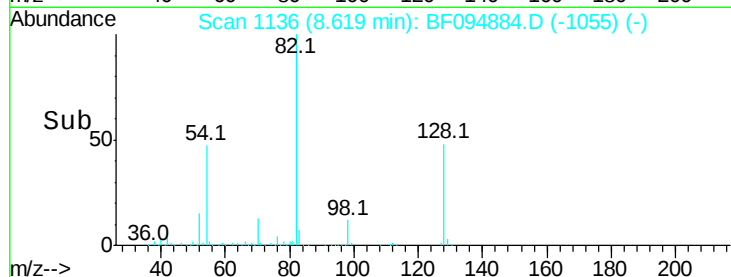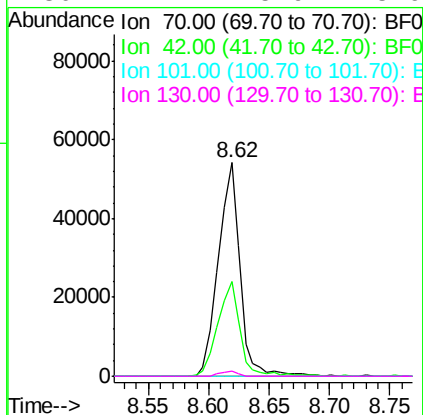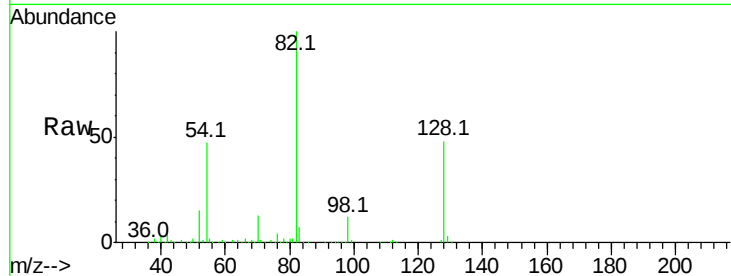

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 9.74 min Scan# 1326
Delta R.T. -0.02 min
Lab File: BF094884.D
Acq: 4 May 2017 20:38

Tgt Ion: 136 Resp: 326225
Ion Ratio Lower Upper
136 100
137 10.7 8.5 12.7
54 7.2 4.9 7.3
68 5.5 4.1 6.1


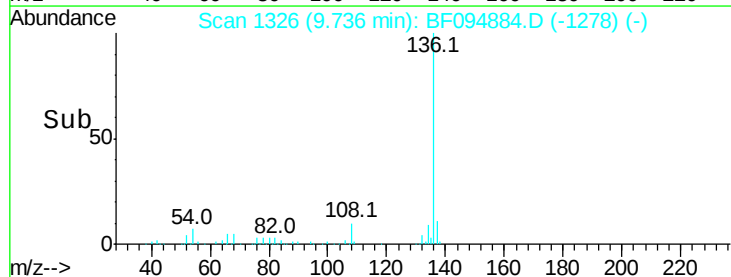
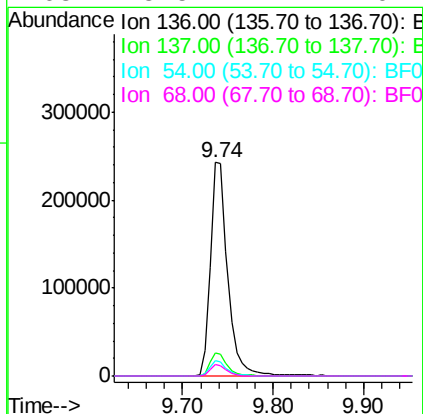
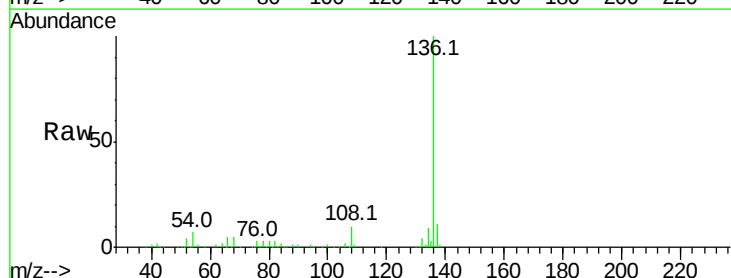




#23
 Nitrobenzene-d5
 Concen: 99.55 ng
 RT: 8.62 min Scan# 1136
 Delta R.T. -0.02 min
 Lab File: BF094884.D
 Acq: 4 May 2017 20:38




Instrument :
 BNA_F
 ClientSampleId :

Tot Ion: 82 Resp: 514999
 Ion Ratio Lower Upper
 82 100
 128 47.9 34.0 51.0
 54 46.8 42.2 63.2

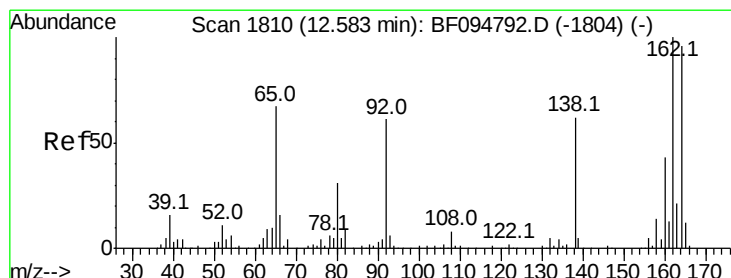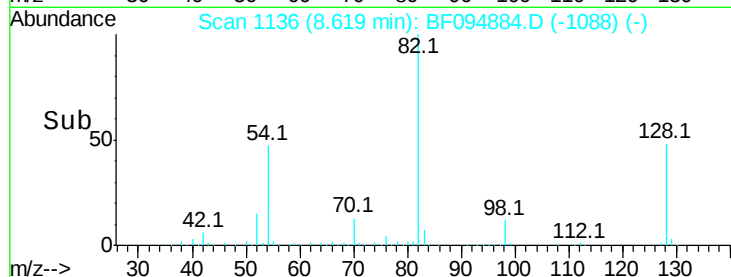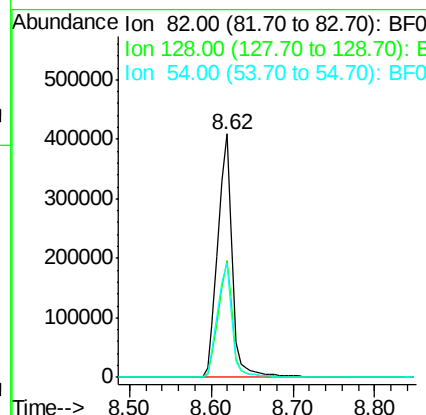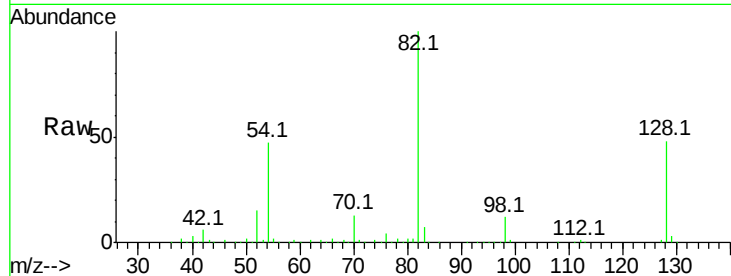

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 12.57 min Scan# 1807
 Delta R.T. -0.02 min
 Lab File: BF094884.D
 Acq: 4 May 2017 20:38

Tgt Ion:164 Resp: 155372
 Ion Ratio Lower Upper
 164 100
 162 103.1 82.6 123.8
 160 44.5 36.2 54.2

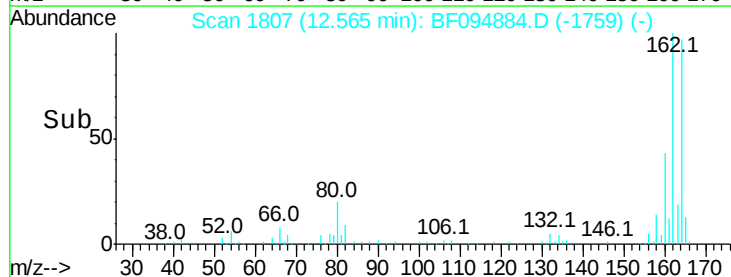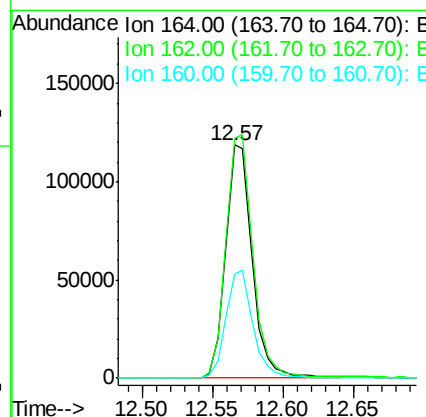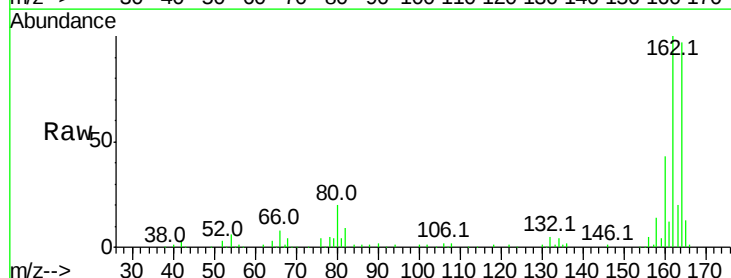







#41
 2,4,6-Tribromophenol
 Concen: 133.07 ng
 RT: 13.87 min Scan# 2028
 Delta R.T. -0.02 min
 Lab File: BF094884.D
 Acq: 4 May 2017 20:38

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:330 Resp: 169324
 Ion Ratio Lower Upper
 330 100
 332 96.1 76.6 115.0
 141 39.6 31.4 47.2

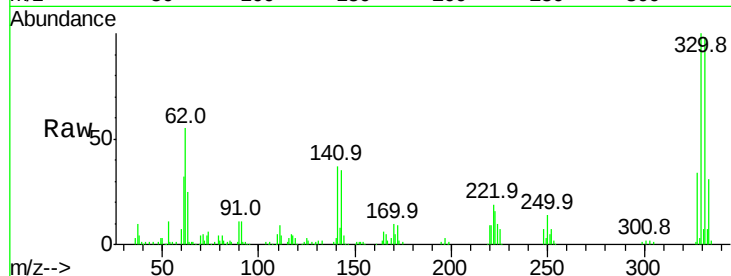


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

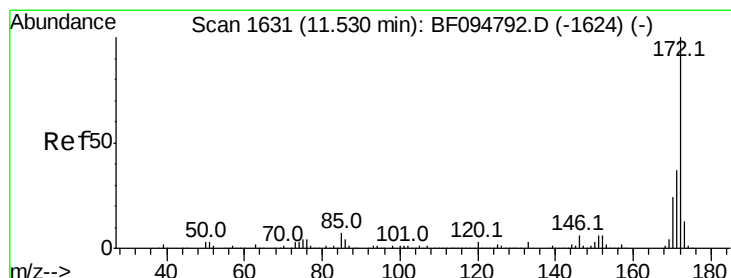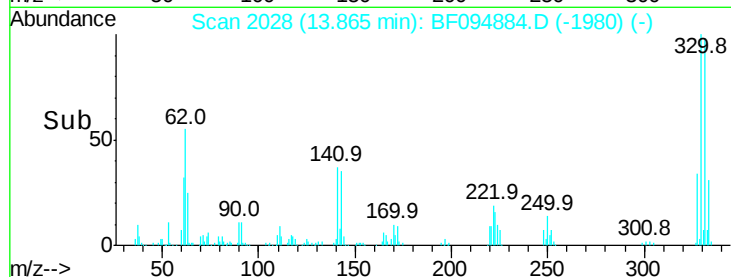
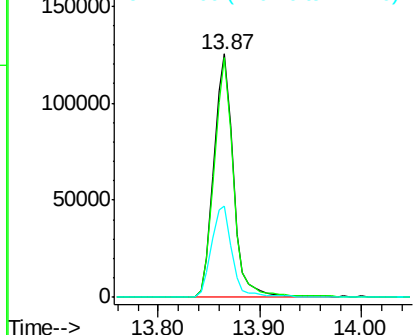


#44
 2-Fluorobiphenyl
 Concen: 68.44 ng
 RT: 11.51 min Scan# 1628
 Delta R.T. -0.02 min
 Lab File: BF094884.D
 Acq: 4 May 2017 20:38

Tgt Ion:172 Resp: 738741
 Ion Ratio Lower Upper
 172 100
 171 35.1 29.6 44.4
 170 24.0 19.8 29.8

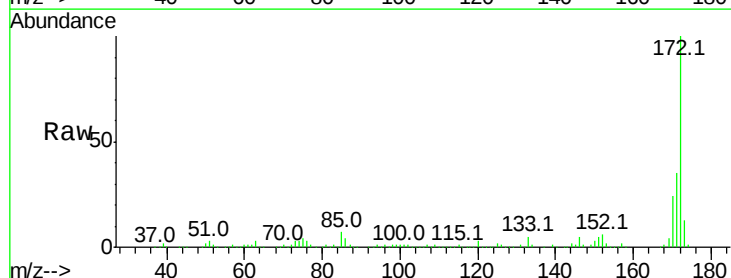

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

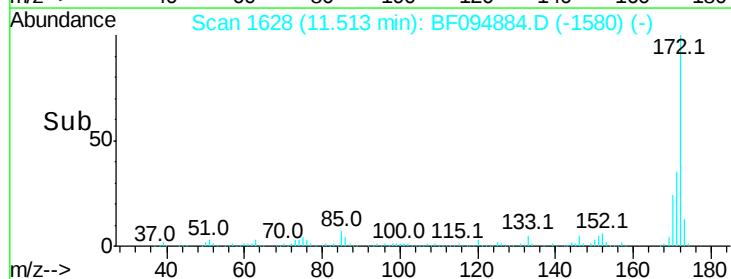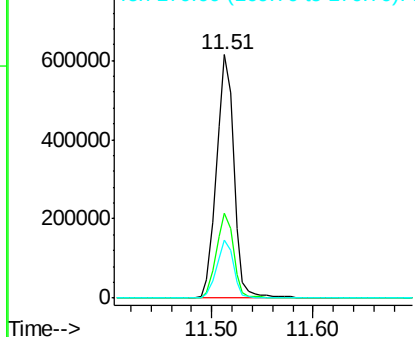



#49

Dimethylphthalate

Concen: 10.25 ng

RT: 12.21 min Scan# 1746

Delta R.T. -0.02 min

Lab File: BF094884.D

Acq: 4 May 2017 20:38

Instrument :

BNA_F

ClientSampled :


Tot Ion:163 Resp: 130756

Ion Ratio Lower Upper

163 100

194 3.5 2.6 4.0




164 9.7 8.4 12.6

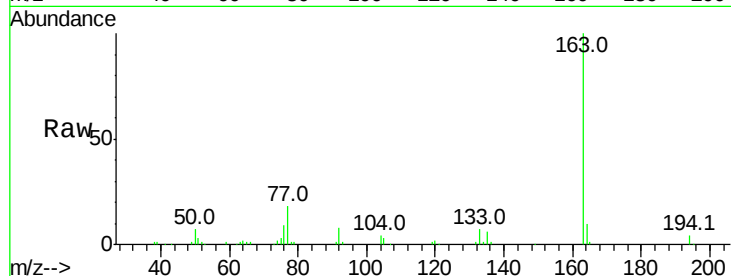

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

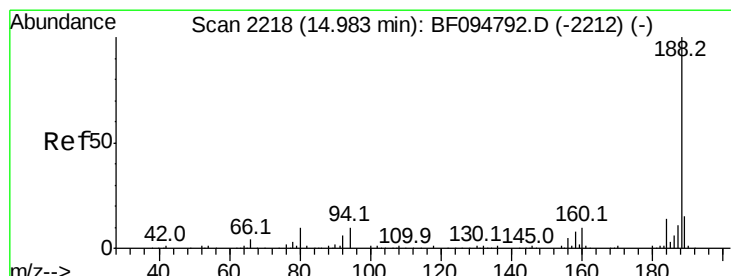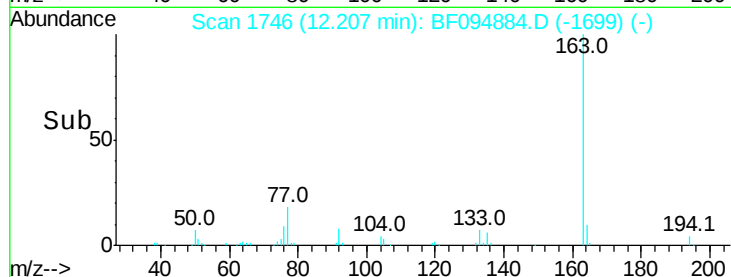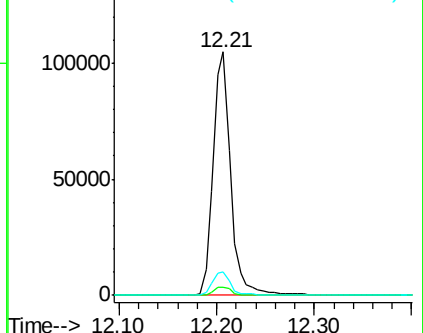

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 14.97 min Scan# 2215

Delta R.T. -0.02 min

Lab File: BF094884.D

Acq: 4 May 2017 20:38


Tgt Ion:188 Resp: 309531

Ion Ratio Lower Upper

188 100

94 10.4 9.4 14.2



80 11.0 10.2 15.2

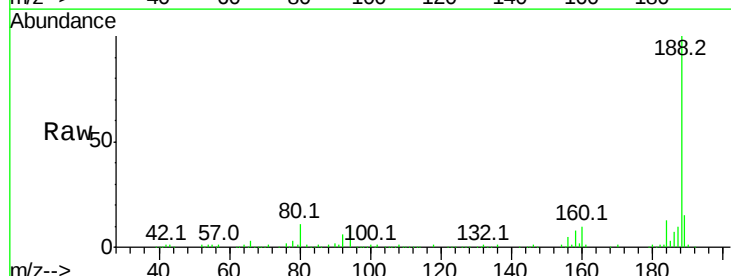

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0



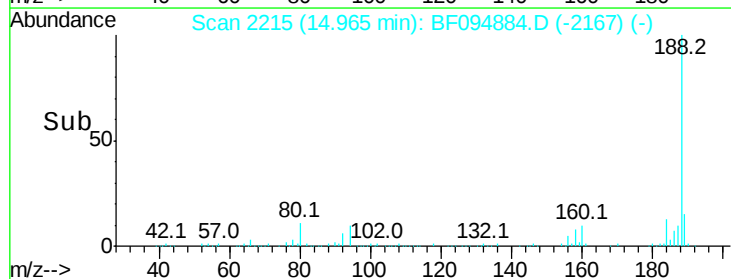
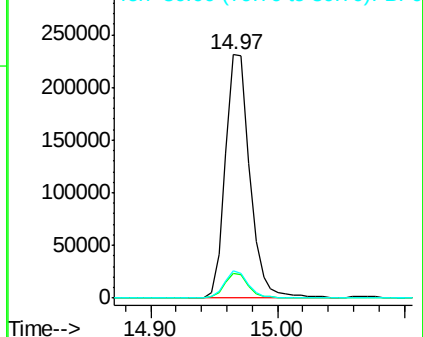




#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 18.64 min Scan# 2839
 Delta R.T. -0.02 min
 Lab File: BF094884.D
 Acq: 4 May 2017 20:38




Instrument :
 BNA_F
 ClientSampled :

Tot Ion:240 Resp: 266141
 Ion Ratio Lower Upper
 240 100
 120 12.9 5.8 8.8#
 236 25.8 20.5 30.7

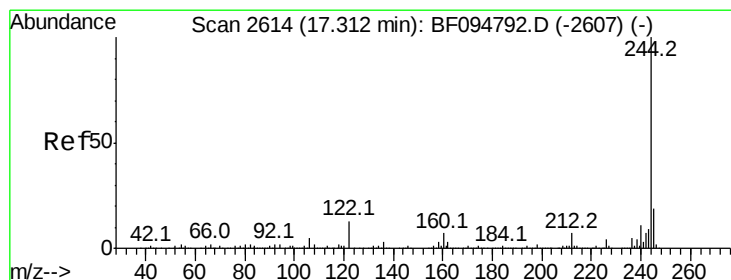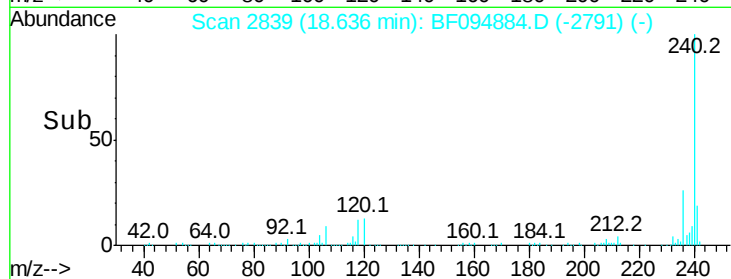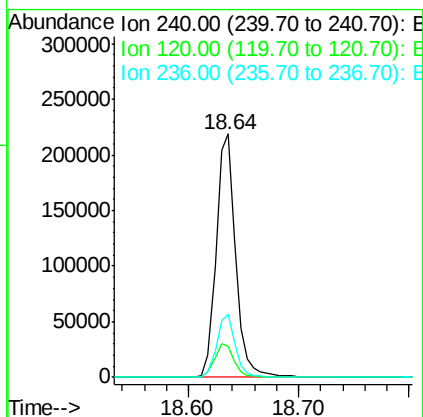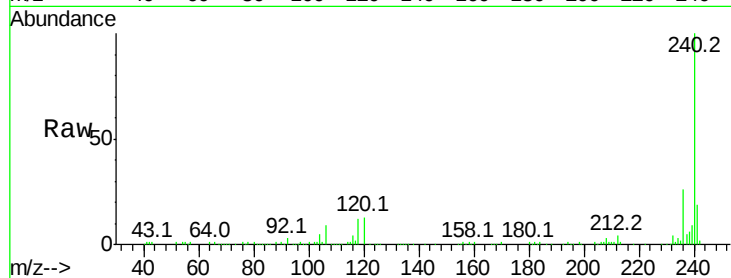

#78
 Terphenyl-d14
 Concen: 48.25 ng
 RT: 17.29 min Scan# 2611
 Delta R.T. -0.02 min
 Lab File: BF094884.D
 Acq: 4 May 2017 20:38

Tgt Ion:244 Resp: 583058
 Ion Ratio Lower Upper
 244 100
 212 7.2 6.0 9.0
 122 13.7 10.3 15.5

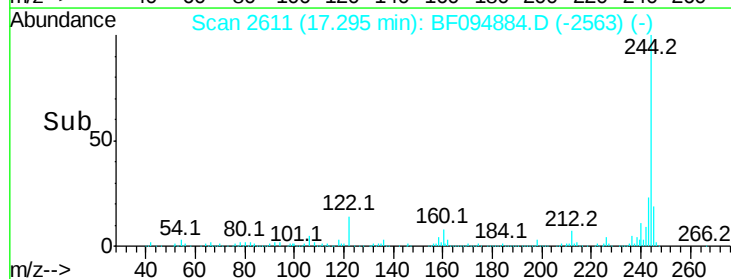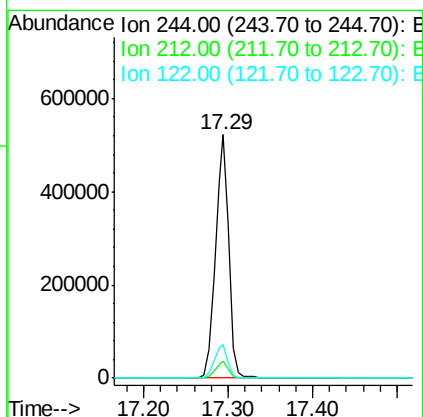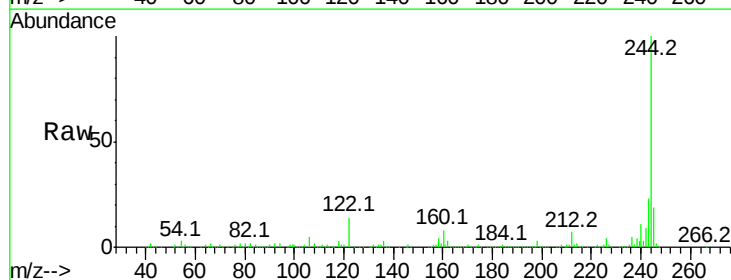




#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 20.30 min Scan# 3122
 Delta R.T. -0.01 min
 Lab File: BF094884.D
 Acq: 4 May 2017 20:38

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.9	19.5	29.3
265	21.8	17.2	25.8

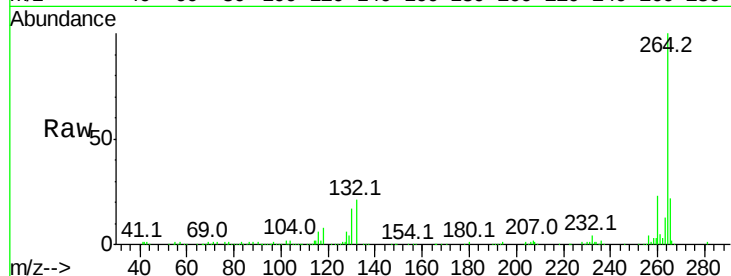

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

