

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050417\
 Data File : BF094882.D
 Acq On : 4 May 2017 19:34
 Operator : SJ/MA
 Sample : I2949-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TWP-07

Quant Time: May 05 02:07:32 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 03 17:24:51 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	83784	20.00	ng	-0.01
21) Naphthalene-d8	9.74	136	346064	20.00	ng	-0.01
38) Acenaphthene-d10	12.57	164	158407	20.00	ng	-0.01
63) Phenanthrene-d10	14.97	188	298109	20.00	ng	-0.01
75) Chrysene-d12	18.64	240	278069	20.00	ng	-0.02
86) Perylene-d12	20.30	264	240312	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.67	112	478641	95.24	ng	-0.01
7) Phenol-d6	7.25	99	404350	67.06	ng	-0.02
23) Nitrobenzene-d5	8.62	82	536909	97.83	ng	-0.02
41) 2,4,6-Tribromophenol	13.87	330	201855	155.60	ng	-0.02
44) 2-Fluorobiphenyl	11.52	172	1026959	93.31	ng	-0.01
78) Terphenyl-d14	17.30	244	879176	69.64	ng	-0.01


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050417\
Data File : BF094882.D
Acq On : 4 May 2017 19:34
Operator : SJ/MA
Sample : I2949-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP-07

Quant Time: May 05 02:07:32 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

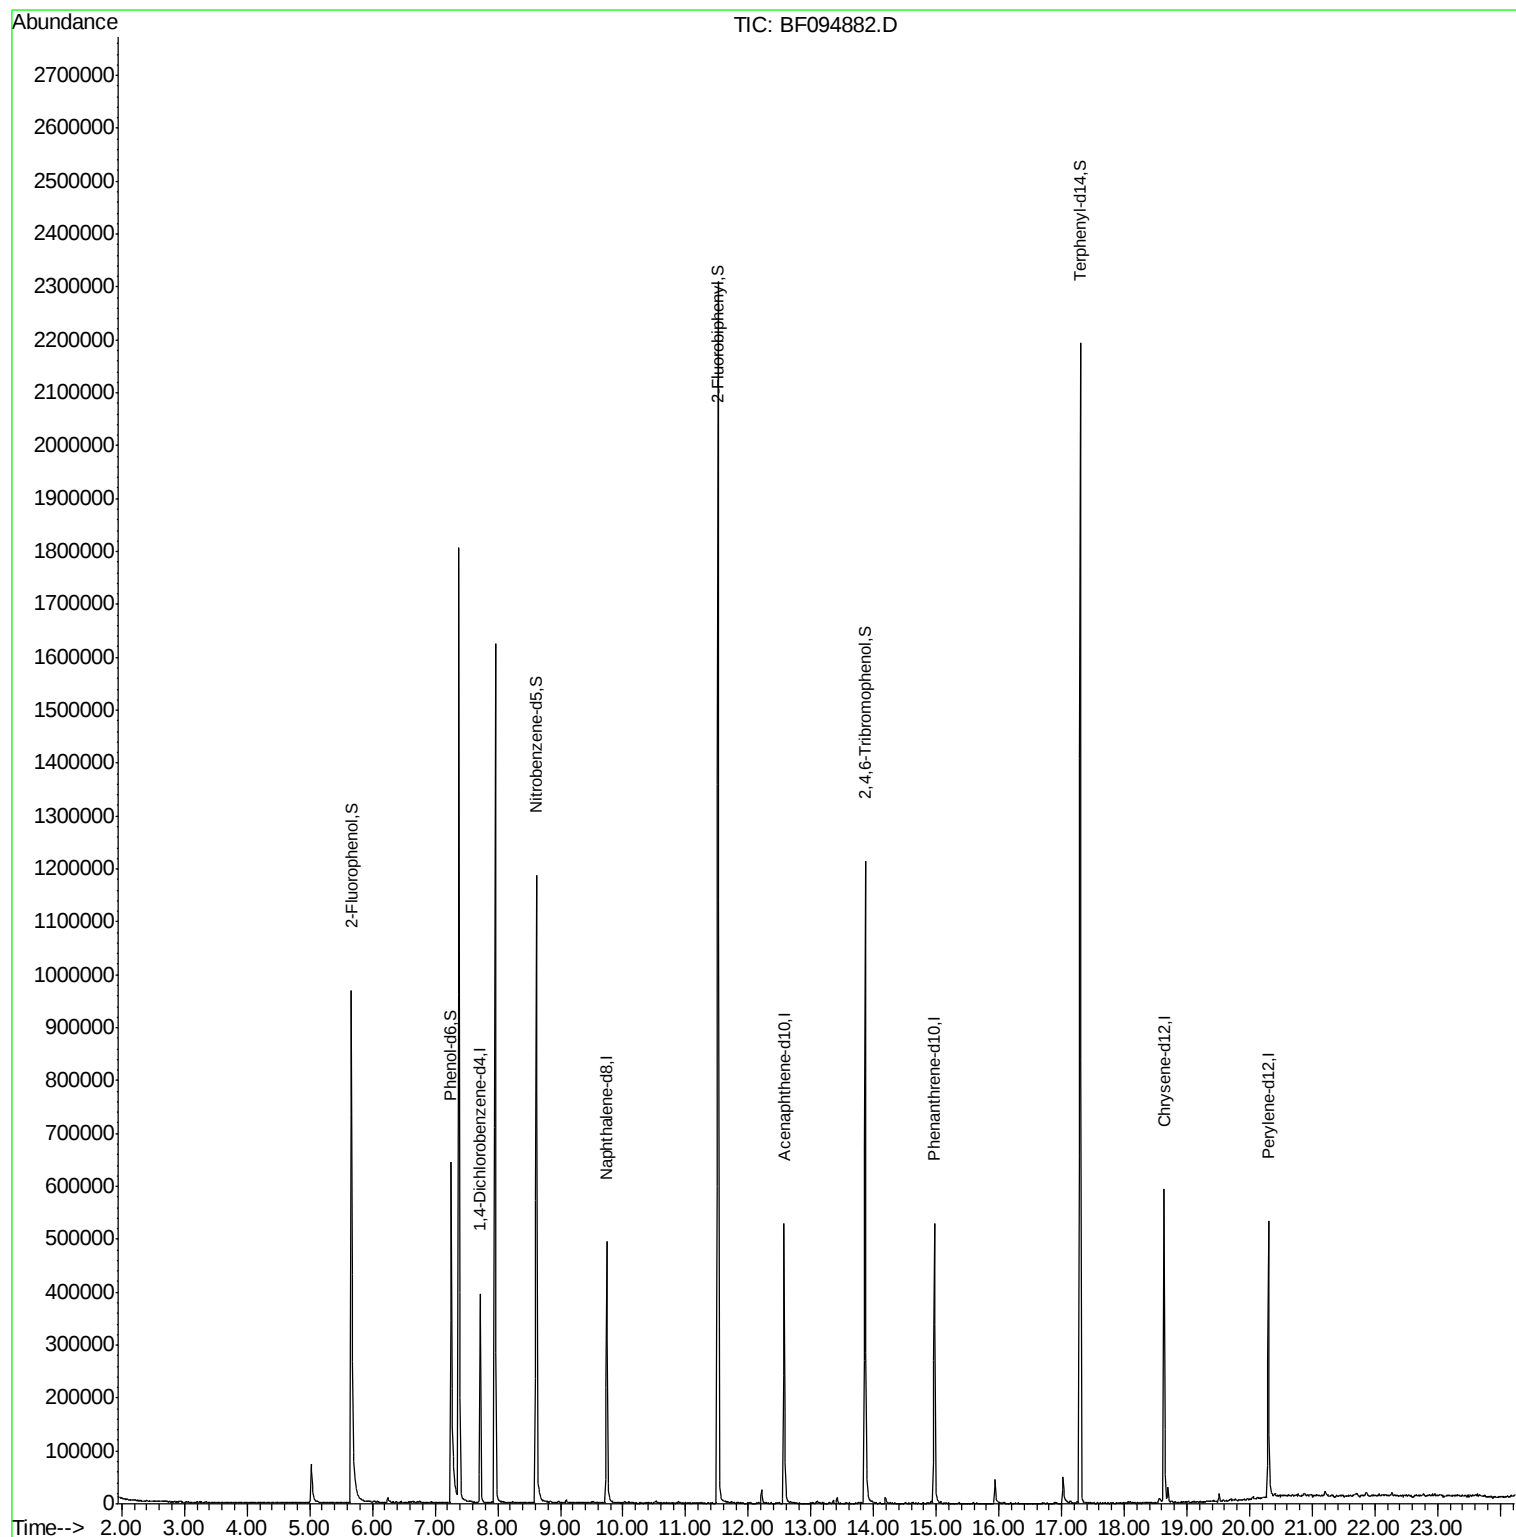




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.72 min Scan# 983
Delta R.T. -0.01 min
Lab File: BF094882.D
Acq: 4 May 2017 19:34

Instrument :
BNA_F
ClientSampled :
TWP-07

Tgt Ion:152 Resp: 83784
Ion Ratio Lower Upper
152 100
150 151.8 126.2 189.2
115 59.9 52.2 78.2

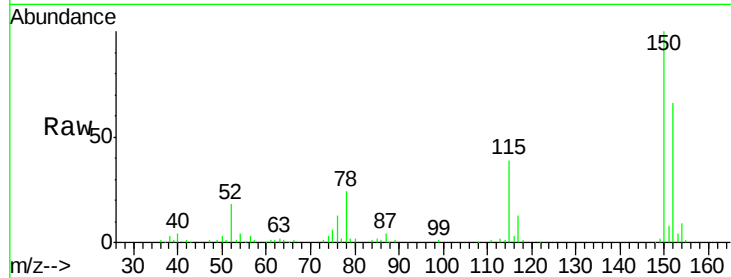


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

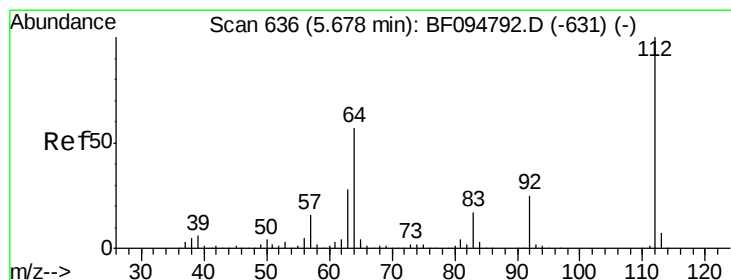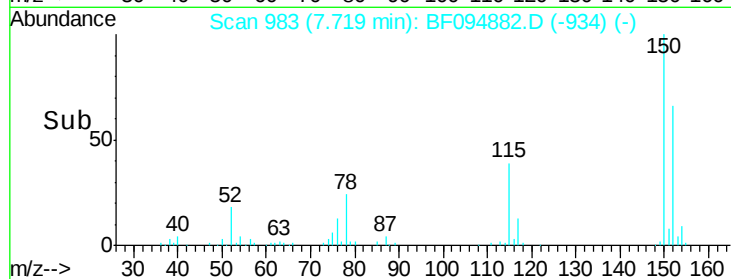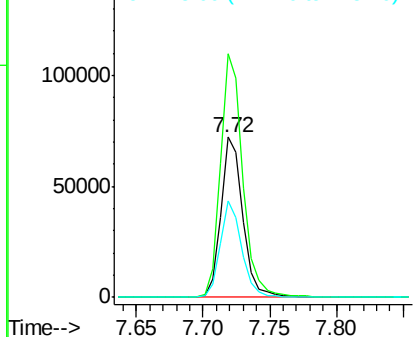



#5


2-Fluorophenol
Concen: 95.24 ng
RT: 5.67 min Scan# 634
Delta R.T. -0.01 min
Lab File: BF094882.D
Acq: 4 May 2017 19:34

Tgt Ion:112 Resp: 478641
Ion Ratio Lower Upper
112 100
64 54.4 46.0 69.0
63 27.1 23.4 35.0

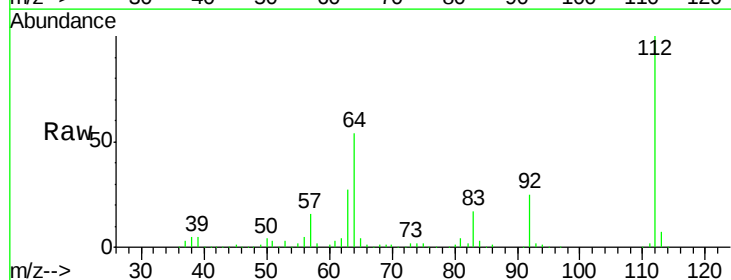

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

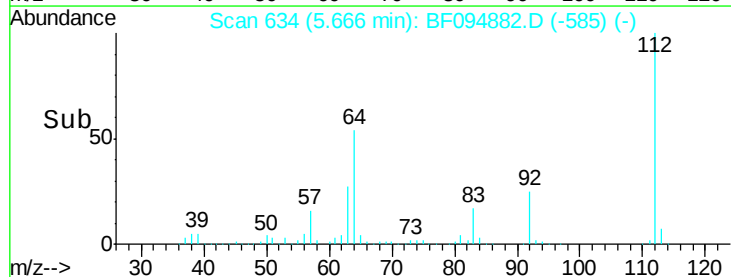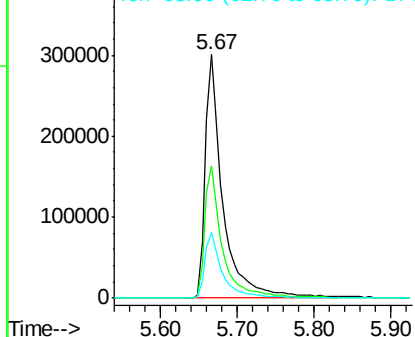

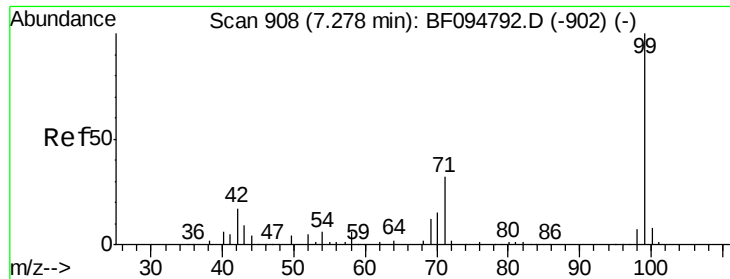

#7

Phenol-d6

Concen: 67.06 ng

RT: 7.25 min Scan# 904

Delta R.T. -0.02 min

Lab File: BF094882.D

Acq: 4 May 2017 19:34

Instrument :

BNA_F

ClientSampleId :

TWP-07


Tgt Ion: 99 Resp: 404350

Ion Ratio Lower Upper

99 100

42 16.6 13.5 20.3




71 32.1 24.5 36.7

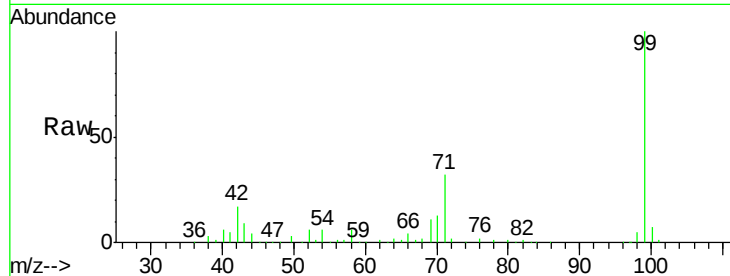

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

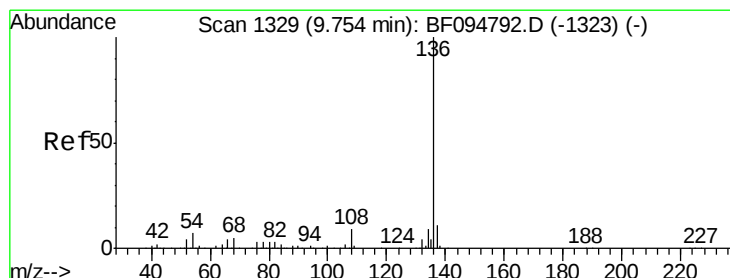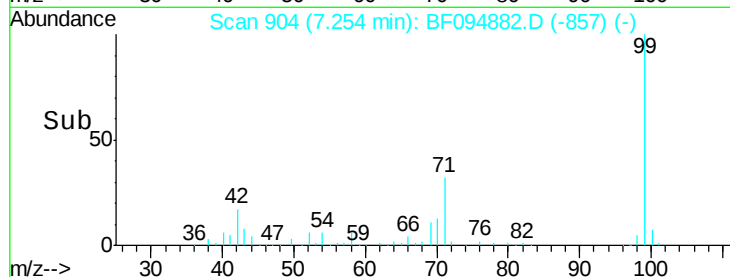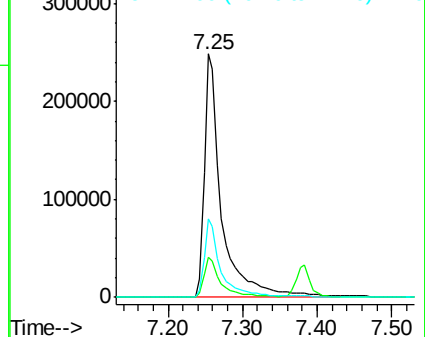

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.74 min Scan# 1327

Delta R.T. -0.01 min

Lab File: BF094882.D

Acq: 4 May 2017 19:34

Tgt Ion: 136 Resp: 346064


Ion Ratio Lower Upper

136 100

137 11.0 8.5 12.7

54 6.8 4.9 7.3

68 5.5 4.1 6.1


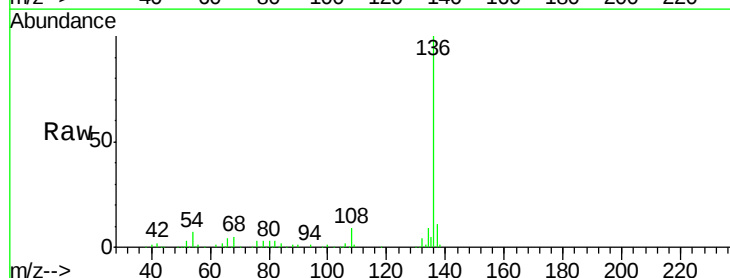


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



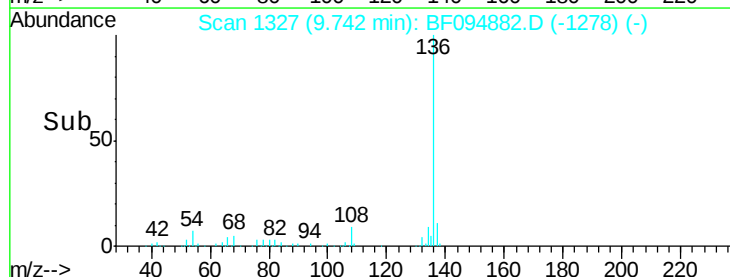
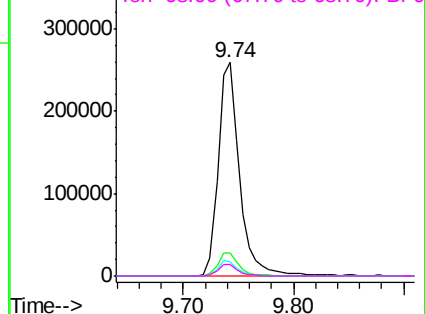




#23
 Nitrobenzene-d5
 Concen: 97.83 ng
 RT: 8.62 min Scan# 1136
 Delta R.T. -0.02 min
 Lab File: BF094882.D
 Acq: 4 May 2017 19:34




Instrument :
 BNA_F
 ClientSampleId :
 TWP-07

Tgt Ion: 82 Resp: 536909
 Ion Ratio Lower Upper
 82 100
 128 46.9 34.0 51.0
 54 48.3 42.2 63.2

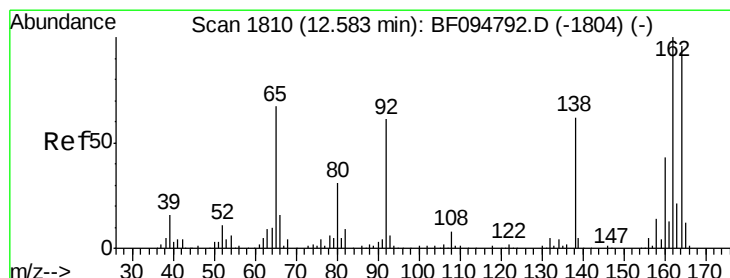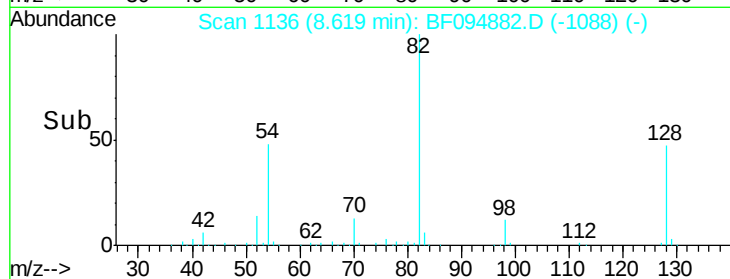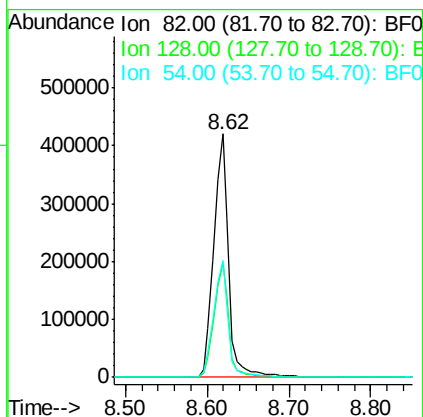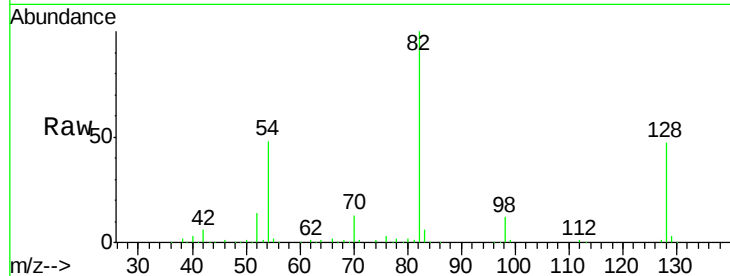

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 12.57 min Scan# 1808
 Delta R.T. -0.01 min
 Lab File: BF094882.D
 Acq: 4 May 2017 19:34

Tgt Ion: 164 Resp: 158407
 Ion Ratio Lower Upper
 164 100
 162 101.1 82.6 123.8
 160 44.8 36.2 54.2

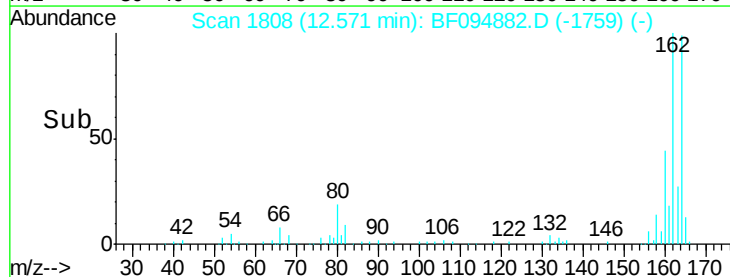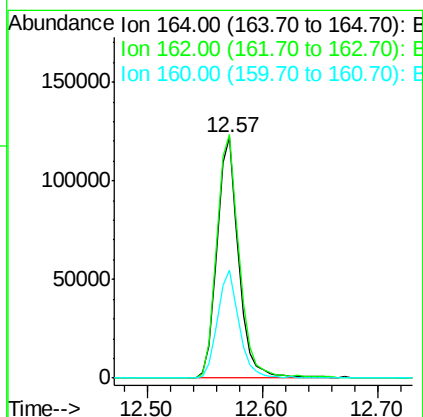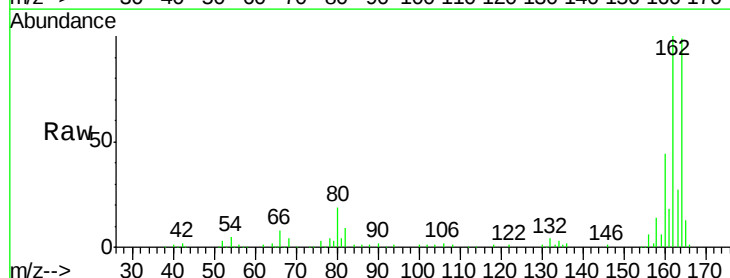







#41
 2,4,6-Tribromophenol
 Concen: 155.60 ng
 RT: 13.87 min Scan# 2028
 Delta R.T. -0.02 min
 Lab File: BF094882.D
 Acq: 4 May 2017 19:34

Instrument :
 BNA_F
 ClientSampleId :
 TWP-07

Tgt Ion: 330 Resp: 201855
 Ion Ratio Lower Upper
 330 100
 332 95.2 76.6 115.0
 141 39.5 31.4 47.2

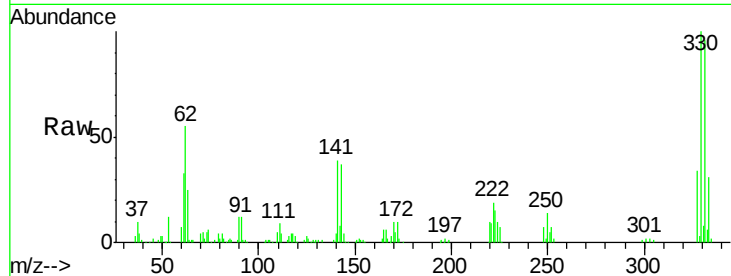


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

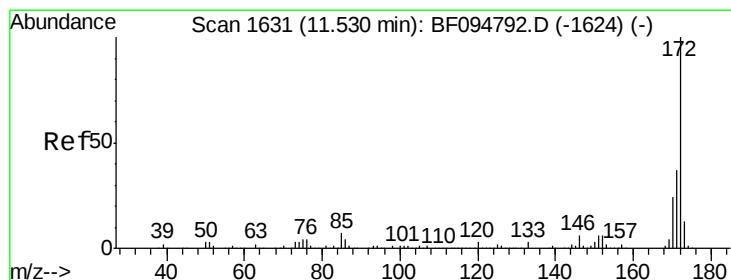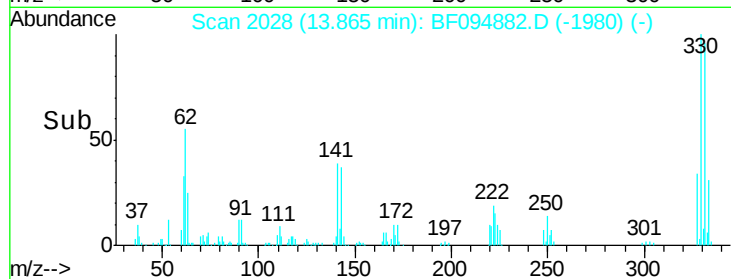
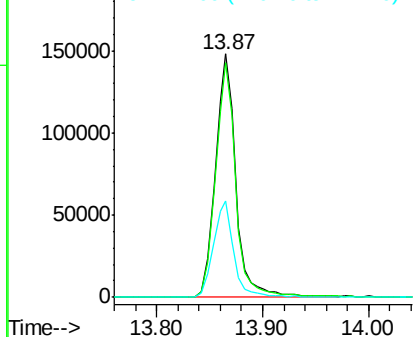



#44
 2-Fluorobiphenyl
 Concen: 93.31 ng
 RT: 11.52 min Scan# 1629
 Delta R.T. -0.01 min
 Lab File: BF094882.D
 Acq: 4 May 2017 19:34

Tgt Ion: 172 Resp: 1026959
 Ion Ratio Lower Upper
 172 100
 171 35.7 29.6 44.4
 170 23.4 19.8 29.8

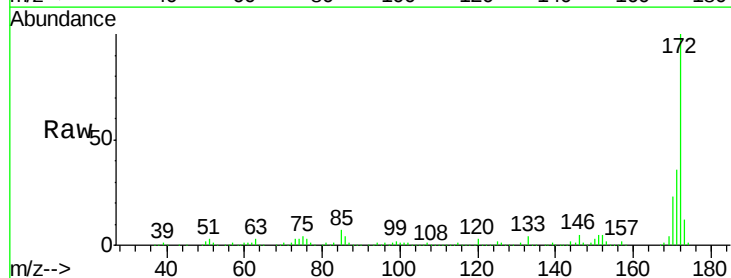

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

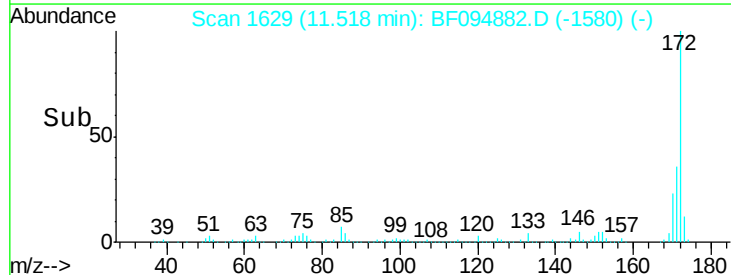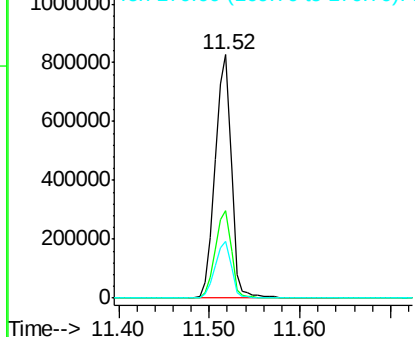


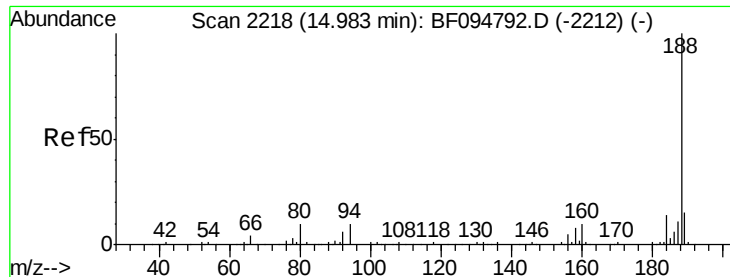




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 14.97 min Scan# 2216
Delta R.T. -0.01 min
Lab File: BF094882.D
Acq: 4 May 2017 19:34

Instrument :
BNA_F
ClientSampleId :
TWP-07

Tgt Ion:188 Resp: 298109
Ion Ratio Lower Upper
188 100
94 9.8 9.4 14.2
80 10.1 10.2 15.2#

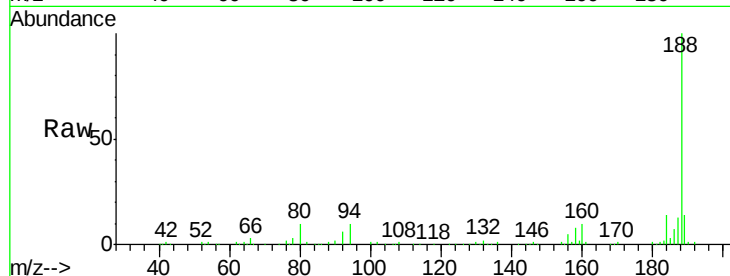


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

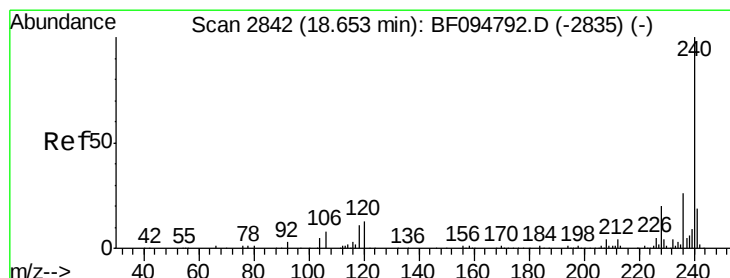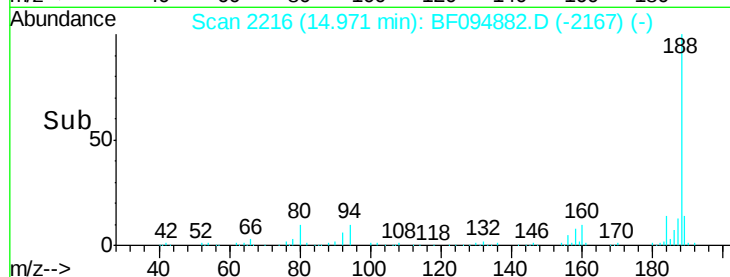
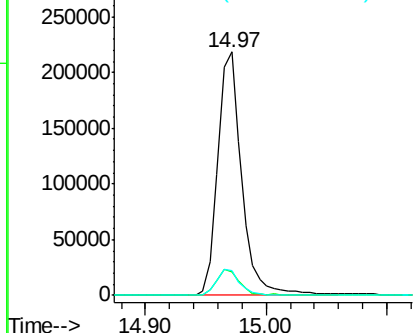


#75
Chrysene-d12
Concen: 20.00 ng
RT: 18.64 min Scan# 2839
Delta R.T. -0.02 min
Lab File: BF094882.D
Acq: 4 May 2017 19:34

Tgt Ion:240 Resp: 278069
Ion Ratio Lower Upper
240 100
120 13.1 5.8 8.8#
236 24.3 20.5 30.7

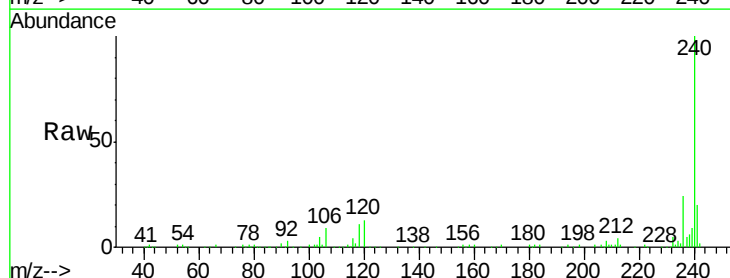

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



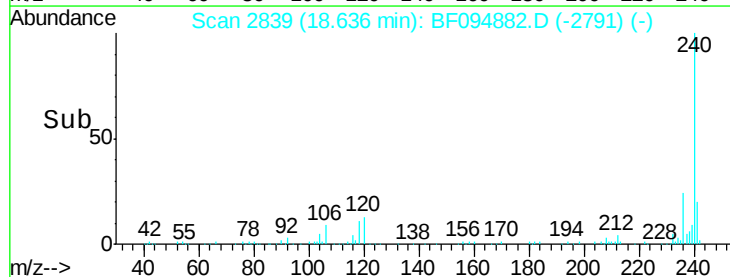
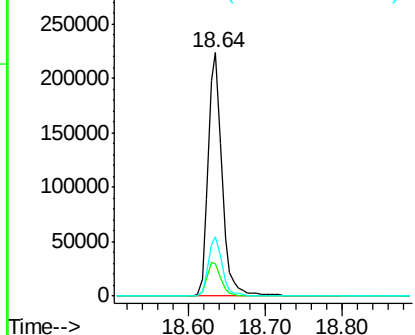




#78
 Terphenyl-d14
 Concen: 69.64 ng
 RT: 17.30 min Scan# 2612
 Delta R.T. -0.01 min
 Lab File: BF094882.D
 Acq: 4 May 2017 19:34

Instrument :
 BNA_F
 ClientSampleId :
 TWP-07

Tgt Ion:244 Resp: 879176
 Ion Ratio Lower Upper
 244 100
 212 7.1 6.0 9.0
 122 12.9 10.3 15.5

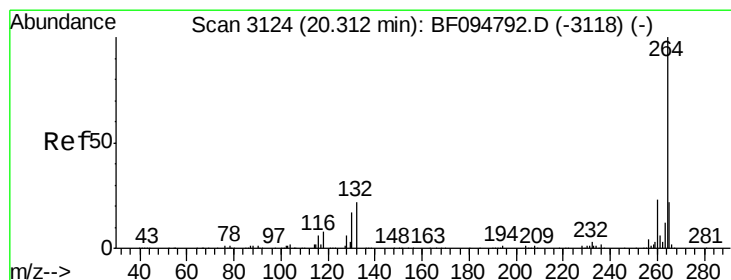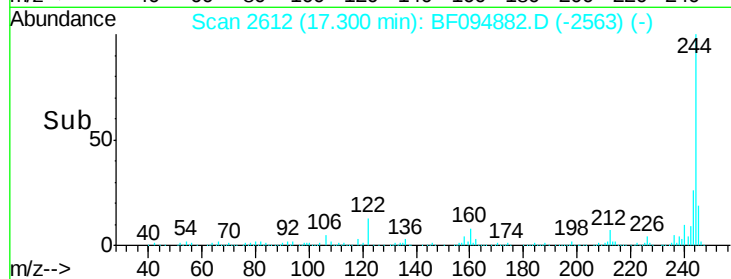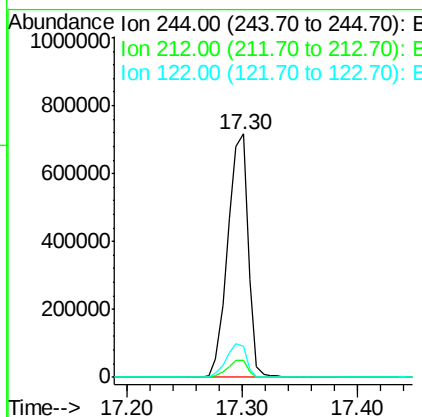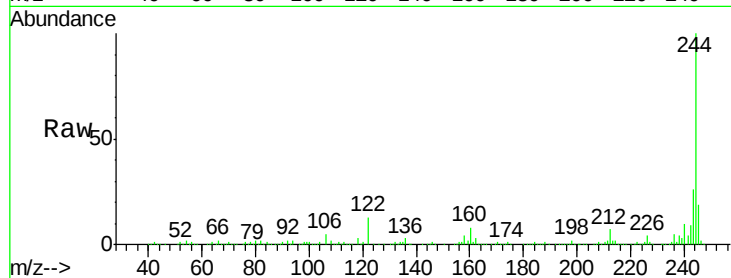

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 20.30 min Scan# 3122
 Delta R.T. -0.01 min
 Lab File: BF094882.D
 Acq: 4 May 2017 19:34

Tgt Ion:264 Resp: 240312
 Ion Ratio Lower Upper
 264 100
 260 23.1 19.5 29.3
 265 20.5 17.2 25.8

