

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050417\
 Data File : BF094885.D
 Acq On : 4 May 2017 21:10
 Operator : SJ/MA
 Sample : I2957-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RT-3025

Quant Time: May 05 02:40:10 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 03 17:24:51 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	91795	20.00	ng	-0.01
21) Naphthalene-d8	9.74	136	371492	20.00	ng	-0.01
38) Acenaphthene-d10	12.57	164	167716	20.00	ng	-0.02
63) Phenanthrene-d10	14.97	188	329175	20.00	ng	-0.01
75) Chrysene-d12	18.64	240	300847	20.00	ng	-0.02
86) Perylene-d12	20.30	264	221560	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.67	112	773680	140.52	ng	0.00
7) Phenol-d6	7.27	99	938095	142.00	ng	-0.01
23) Nitrobenzene-d5	8.62	82	569956	96.75	ng	-0.02
41) 2,4,6-Tribromophenol	13.87	330	208615	151.88	ng	-0.02
44) 2-Fluorobiphenyl	11.51	172	901662	77.38	ng	-0.02
78) Terphenyl-d14	17.29	244	567077	41.52	ng	-0.02
Target Compounds						
49) Dimethylphthalate	12.21	163	143288	10.41	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050417\
Data File : BF094885.D
Acq On : 4 May 2017 21:10
Operator : SJ/MA
Sample : I2957-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RT-3025

Quant Time: May 05 02:40:10 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

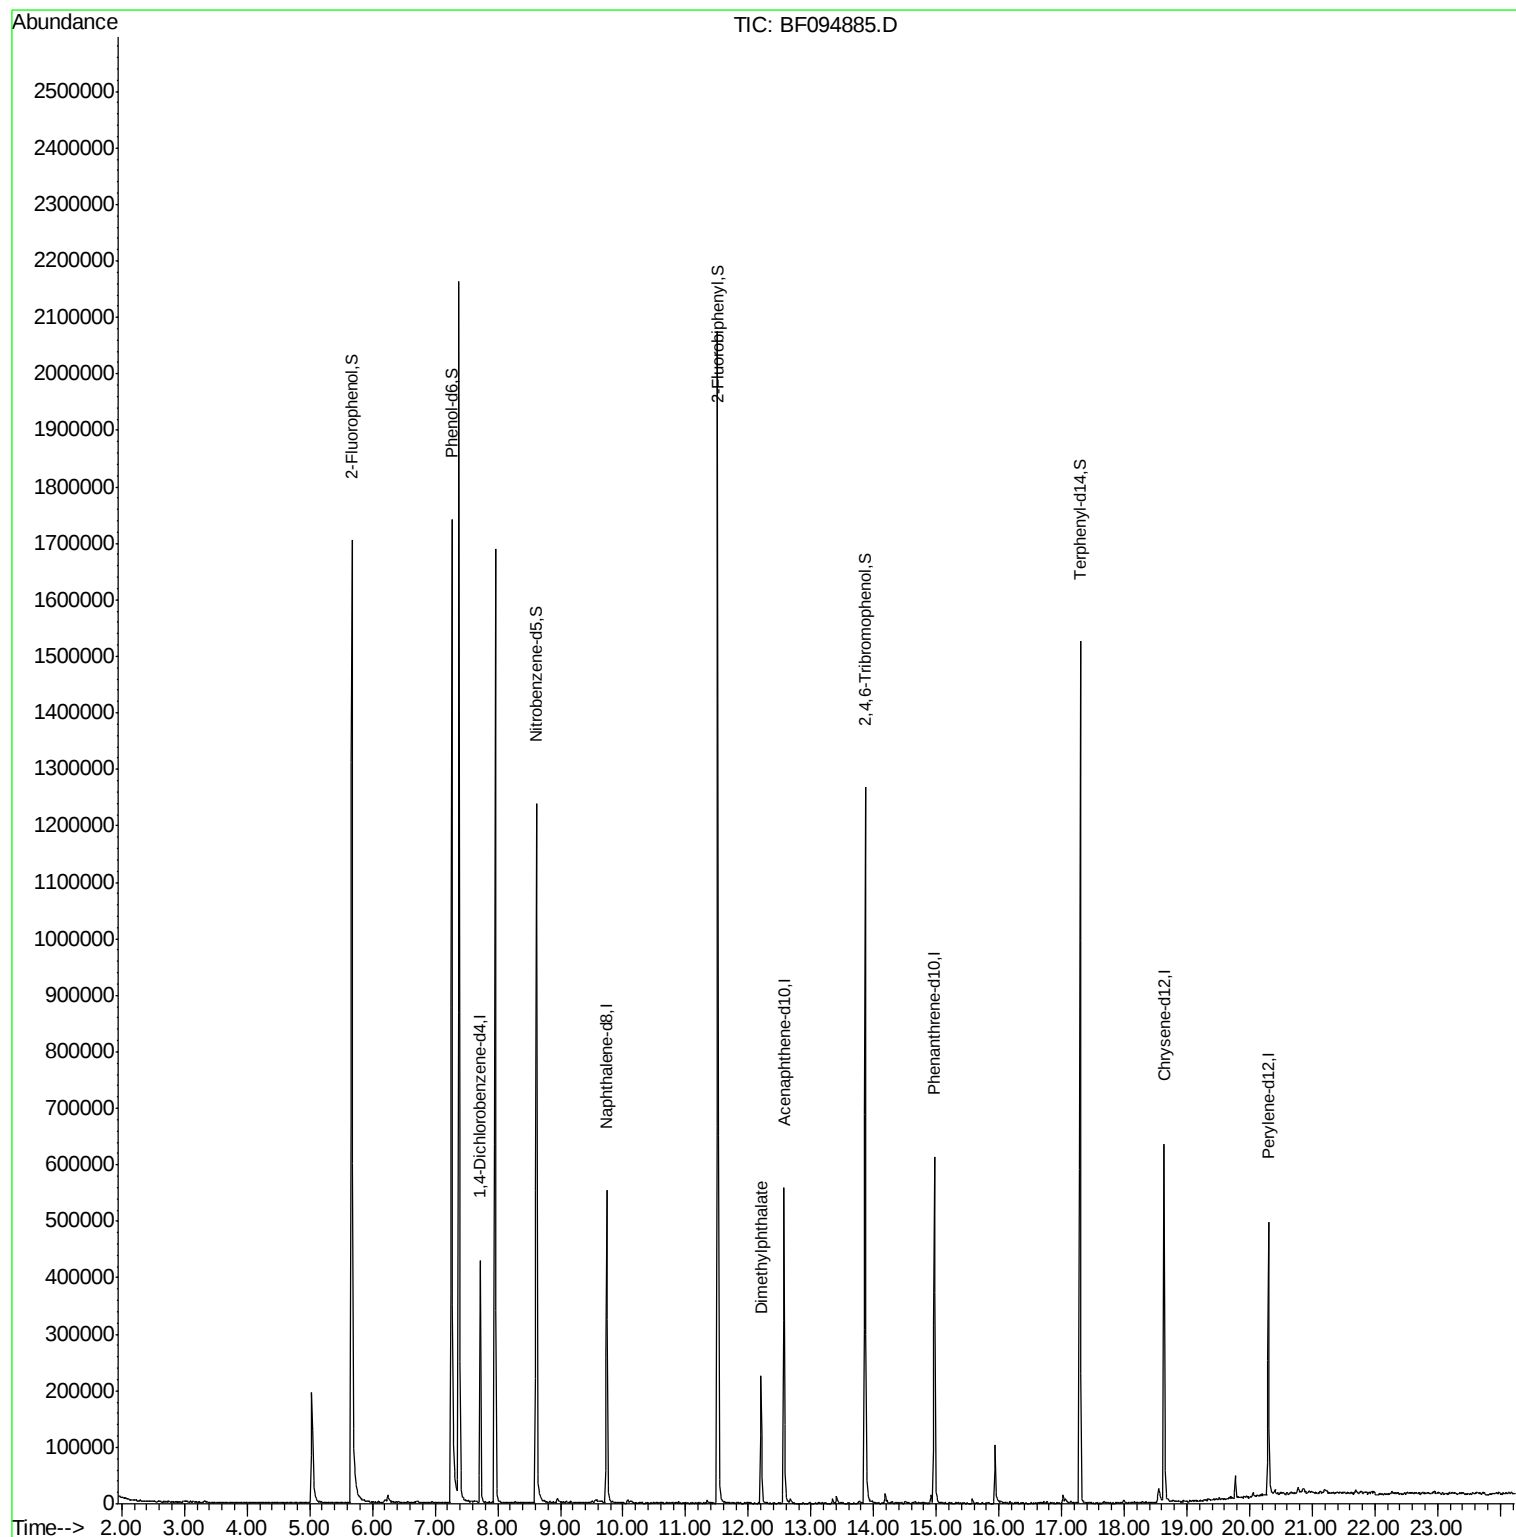

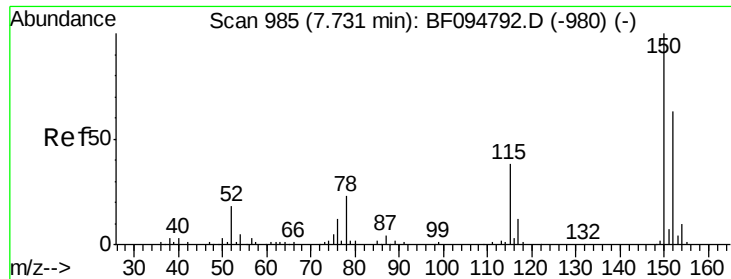


#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.72 min Scan# 983
 Delta R.T. -0.01 min
 Lab File: BF094885.D
 Acq: 4 May 2017 21:10

Instrument :
 BNA_F
 ClientSampleId :
 RT-3025

Tgt Ion:152 Resp: 91795
 Ion Ratio Lower Upper
 152 100
 150 155.0 126.2 189.2
 115 60.6 52.2 78.2

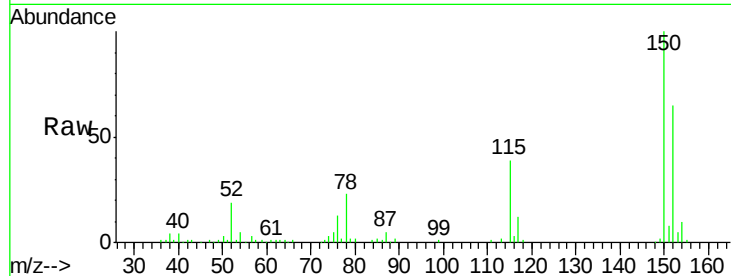


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

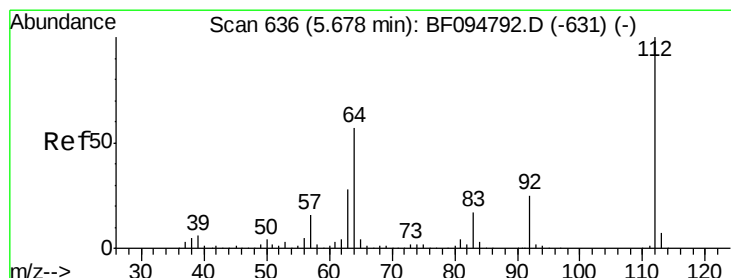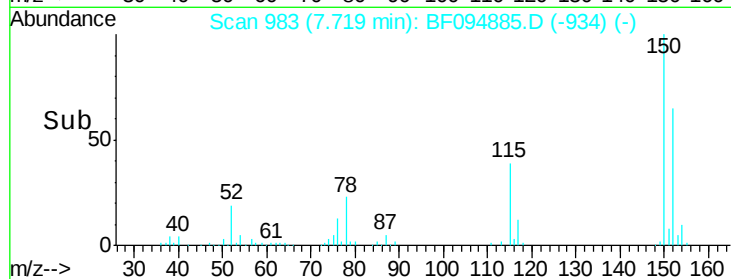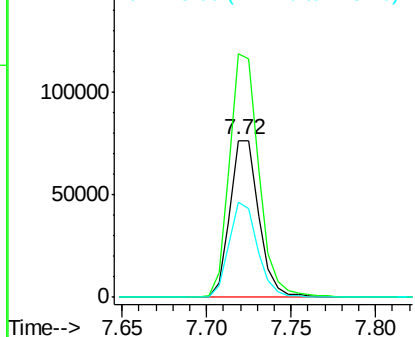



#5


2-Fluorophenol
 Concen: 140.52 ng
 RT: 5.67 min Scan# 635
 Delta R.T. -0.01 min
 Lab File: BF094885.D
 Acq: 4 May 2017 21:10

Tgt Ion:112 Resp: 773680
 Ion Ratio Lower Upper
 112 100
 64 56.9 46.0 69.0
 63 27.5 23.4 35.0



Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

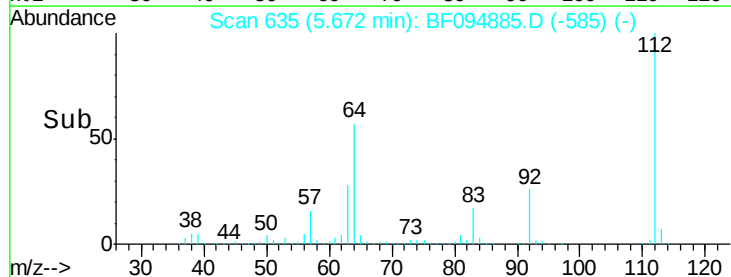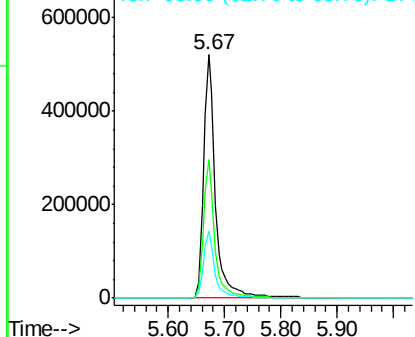

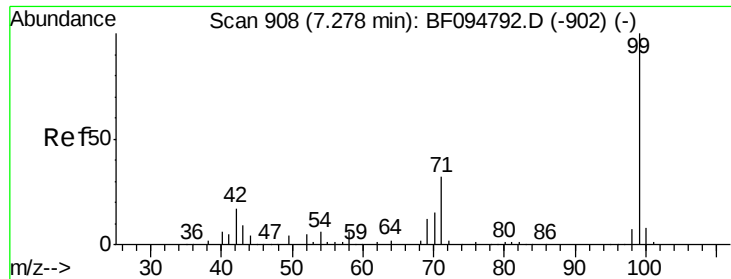

#7

Phenol-d6

Concen: 142.00 ng

RT: 7.27 min Scan# 906

Delta R.T. -0.01 min

Lab File: BF094885.D

Acq: 4 May 2017 21:10

Instrument :

BNA_F

ClientSampleId :

RT-3025


Tgt Ion: 99 Resp: 938095

Ion Ratio Lower Upper

99 100

42 16.7 13.5 20.3




71 33.3 24.5 36.7

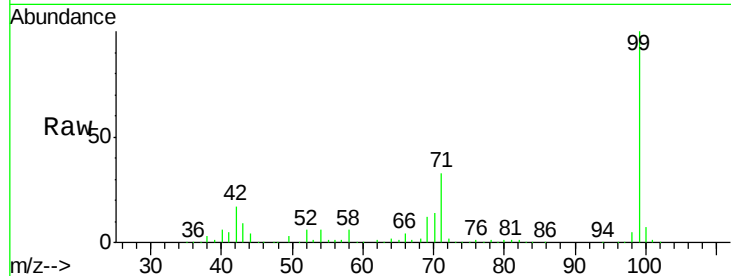

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

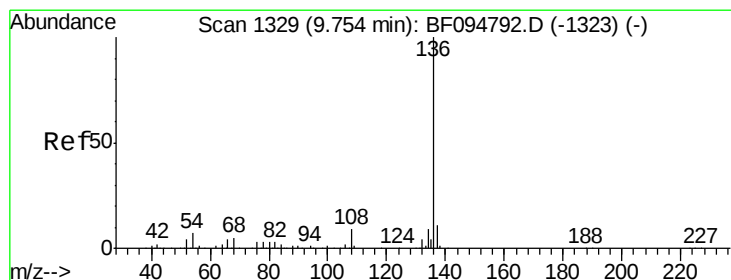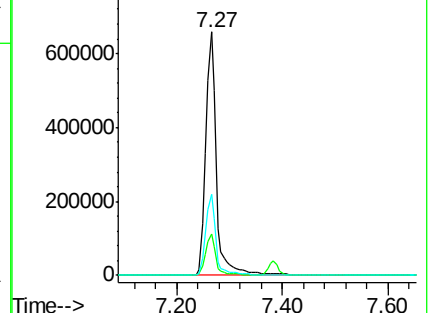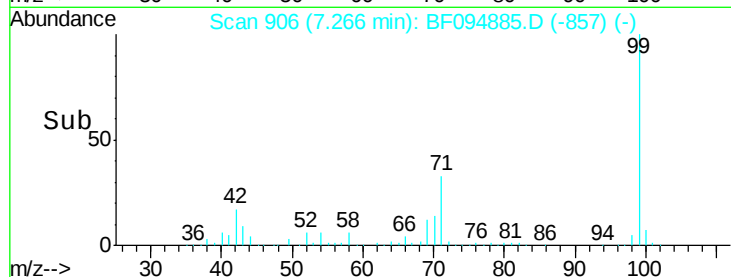

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.74 min Scan# 1327

Delta R.T. -0.01 min

Lab File: BF094885.D

Acq: 4 May 2017 21:10

Tgt Ion: 136 Resp: 371492


Ion Ratio Lower Upper

136 100

137 10.6 8.5 12.7

54 6.4 4.9 7.3

68 5.3 4.1 6.1






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



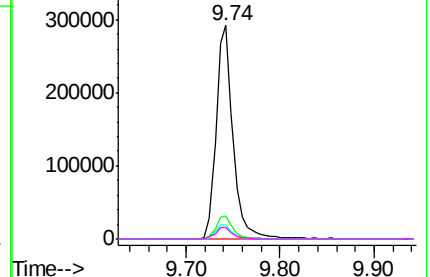
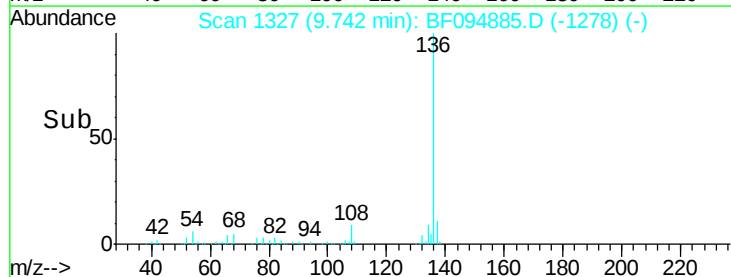


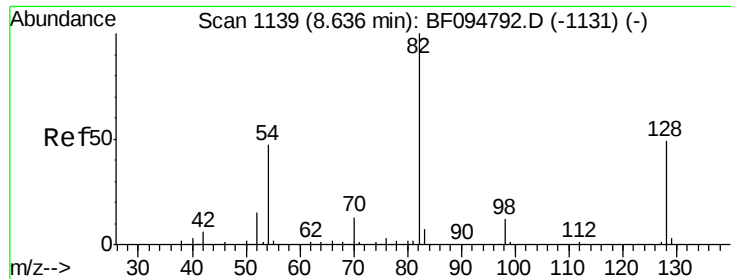

#23
 Nitrobenzene-d5
 Concen: 96.75 ng
 RT: 8.62 min Scan# 1136
 Delta R.T. -0.02 min
 Lab File: BF094885.D
 Acq: 4 May 2017 21:10




Instrument :
 BNA_F
 ClientSampleId :
 RT-3025


Tgt Ion	Ratio	Lower	Upper
82	100		
128	47.2	34.0	51.0
54	47.9	42.2	63.2

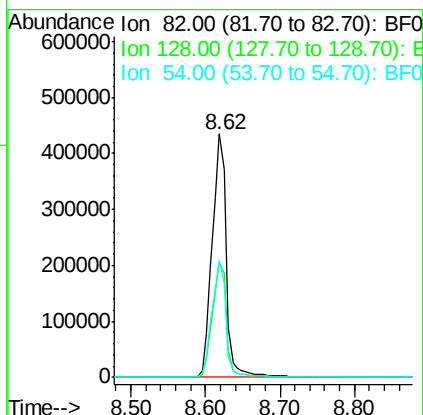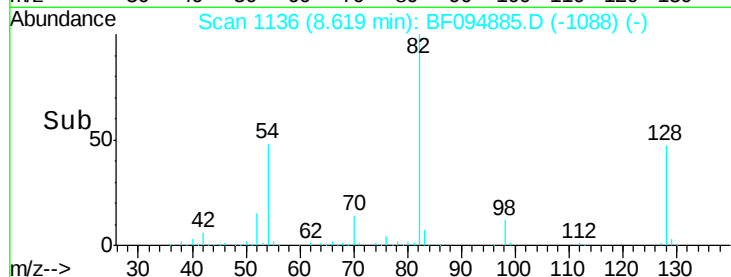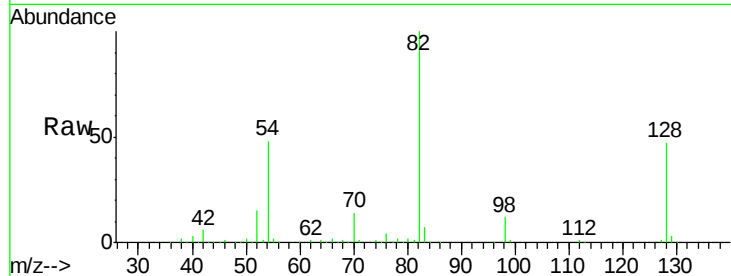

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 12.57 min Scan# 1807
 Delta R.T. -0.02 min
 Lab File: BF094885.D
 Acq: 4 May 2017 21:10

Tgt Ion	Ratio	Lower	Upper
164	100		
162	103.9	82.6	123.8
160	44.7	36.2	54.2

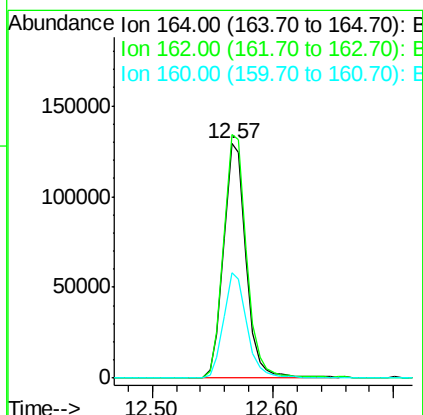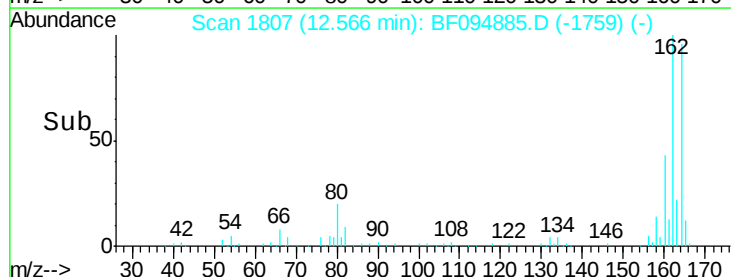


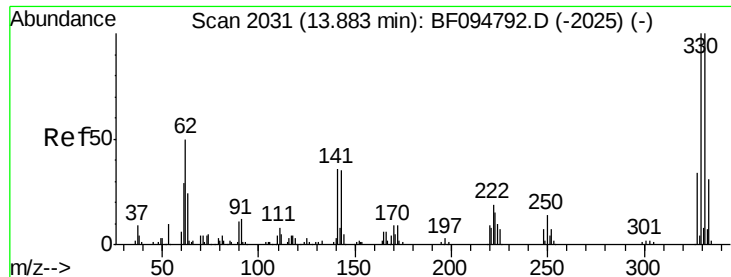




#41
 2,4,6-Tribromophenol
 Concen: 151.88 ng
 RT: 13.87 min Scan# 2028
 Delta R.T. -0.02 min
 Lab File: BF094885.D
 Acq: 4 May 2017 21:10

Instrument :
 BNA_F
 ClientSampleId :
 RT-3025

Tgt Ion	Ratio	Lower	Upper
330	100		
332	97.2	76.6	115.0
141	39.9	31.4	47.2

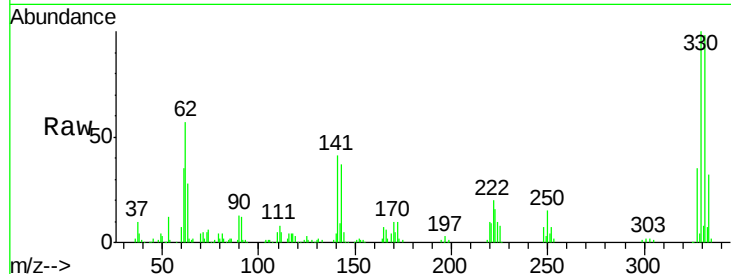


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

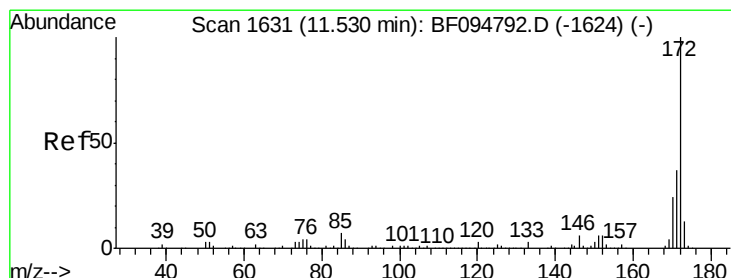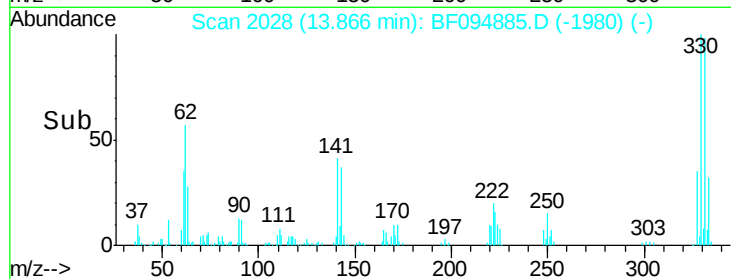
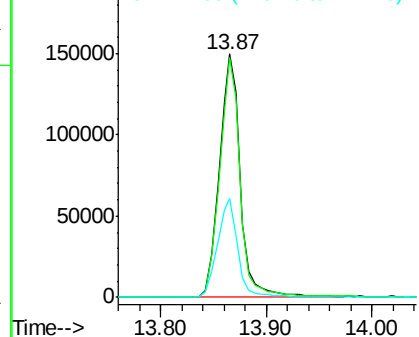



#44
 2-Fluorobiphenyl
 Concen: 77.38 ng
 RT: 11.51 min Scan# 1628
 Delta R.T. -0.02 min
 Lab File: BF094885.D
 Acq: 4 May 2017 21:10

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.4	29.6	44.4
170	23.4	19.8	29.8



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

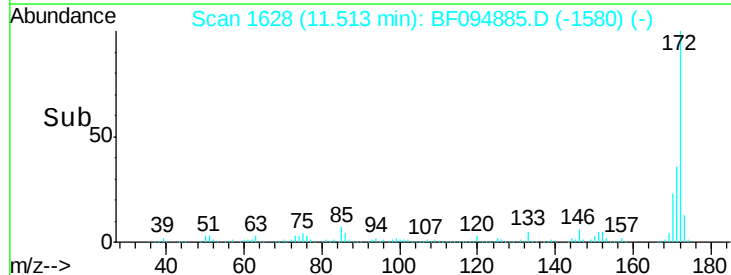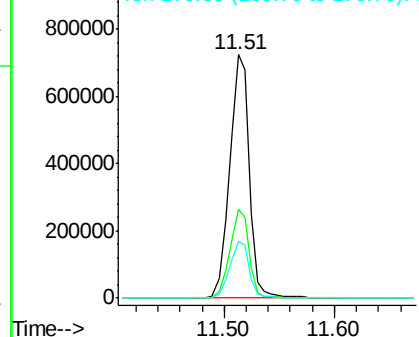

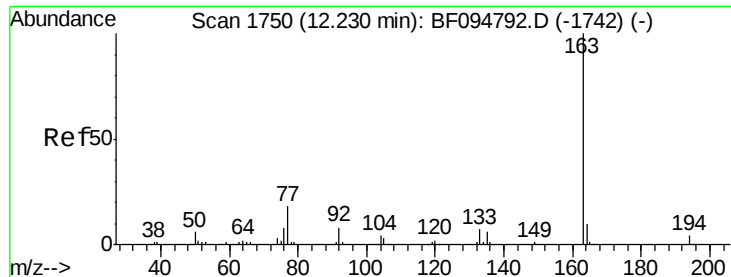

#49

Dimethylphthalate

Concen: 10.41 ng

RT: 12.21 min Scan# 1746

Delta R.T. -0.02 min

Lab File: BF094885.D

Acq: 4 May 2017 21:10

Instrument :

BNA_F

ClientSampleId :

RT-3025


Tgt Ion:163 Resp: 143288

Ion Ratio Lower Upper

163 100

194 3.9 2.6 4.0




164 10.0 8.4 12.6



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

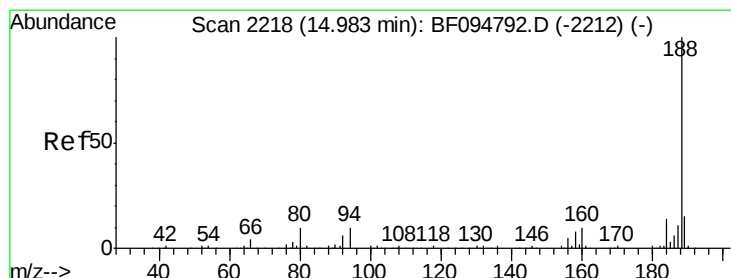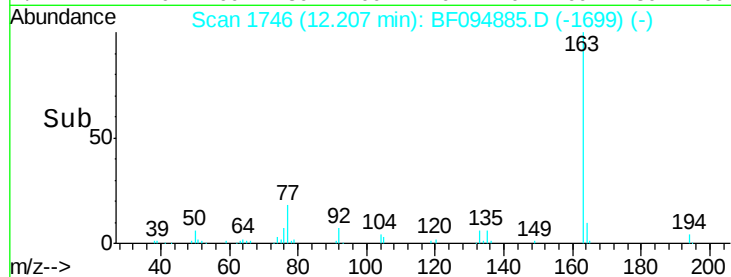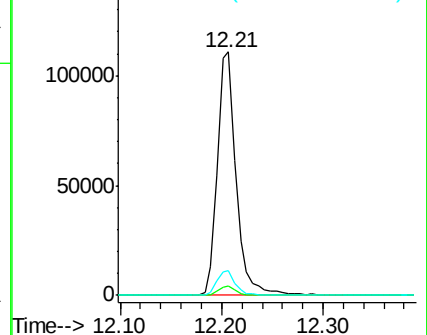

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 14.97 min Scan# 2216

Delta R.T. -0.01 min

Lab File: BF094885.D

Acq: 4 May 2017 21:10


Tgt Ion:188 Resp: 329175

Ion Ratio Lower Upper

188 100

94 10.0 9.4 14.2



80 10.5 10.2 15.2




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0



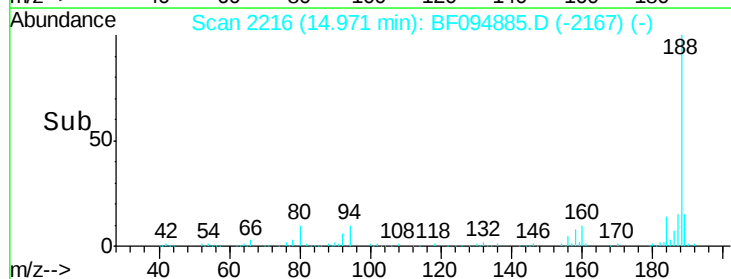
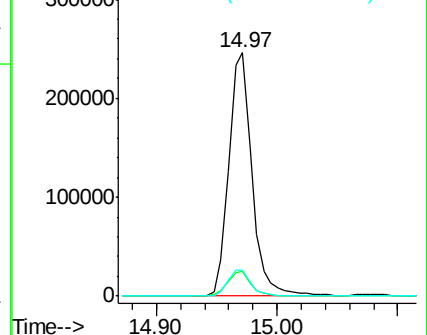


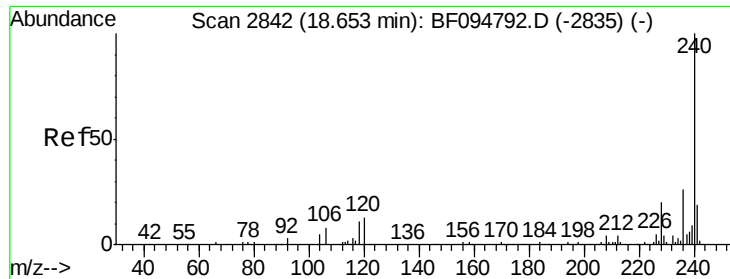

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 18.64 min Scan# 2839
 Delta R.T. -0.02 min
 Lab File: BF094885.D
 Acq: 4 May 2017 21:10




Instrument :
 BNA_F
 ClientSampleId :
 RT-3025


Tgt Ion:240 Resp: 300847
 Ion Ratio Lower Upper
 240 100
 120 13.7 5.8 8.8#
 236 25.2 20.5 30.7

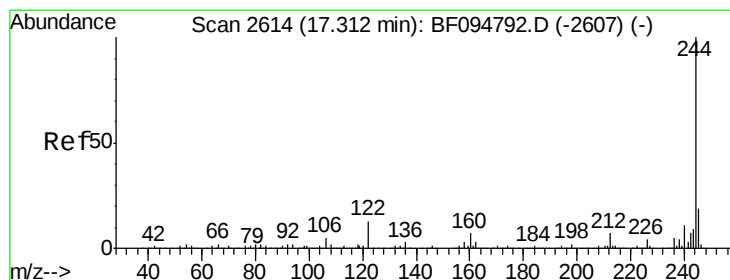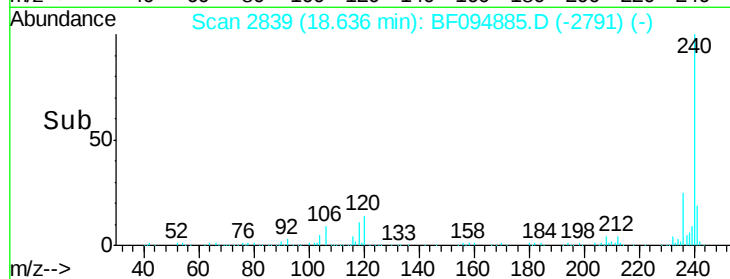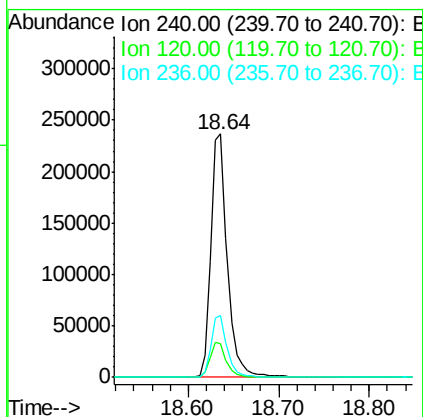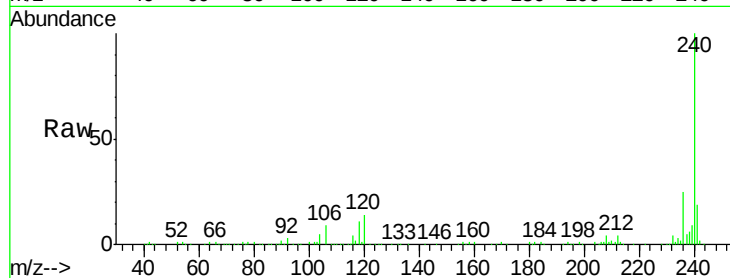

#78
 Terphenyl-d14
 Concen: 41.52 ng
 RT: 17.29 min Scan# 2611
 Delta R.T. -0.02 min
 Lab File: BF094885.D
 Acq: 4 May 2017 21:10

Tgt Ion:244 Resp: 567077
 Ion Ratio Lower Upper
 244 100
 212 6.8 6.0 9.0
 122 13.5 10.3 15.5

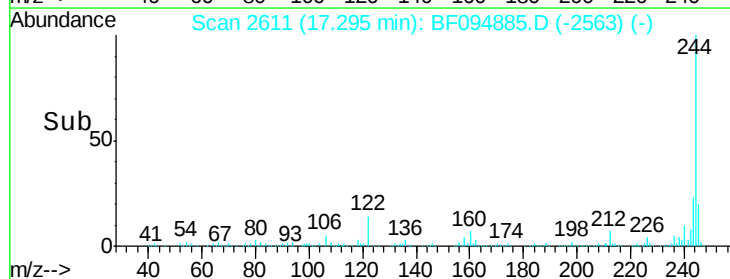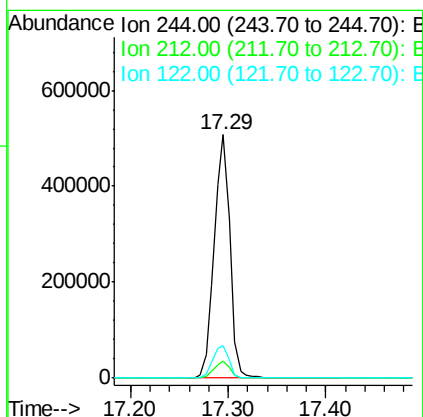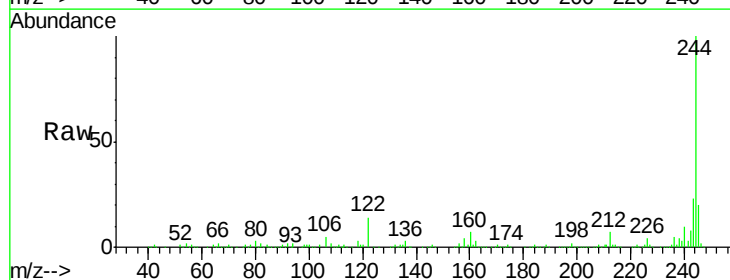


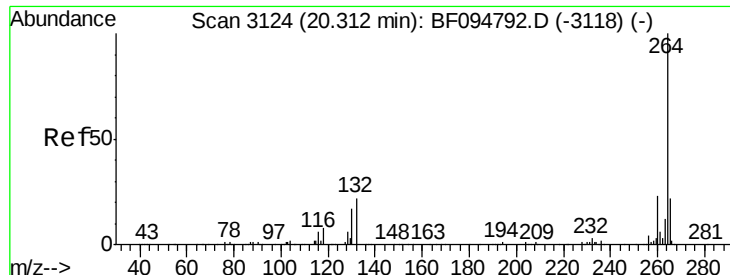

#86
Perylene-d12
Concen: 20.00 ng
RT: 20.30 min Scan# 3122
Delta R.T. -0.01 min
Lab File: BF094885.D
Acq: 4 May 2017 21:10

Instrument :
BNA_F
ClientSampleId :
RT-3025

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.5	19.5	29.3
265	21.1	17.2	25.8

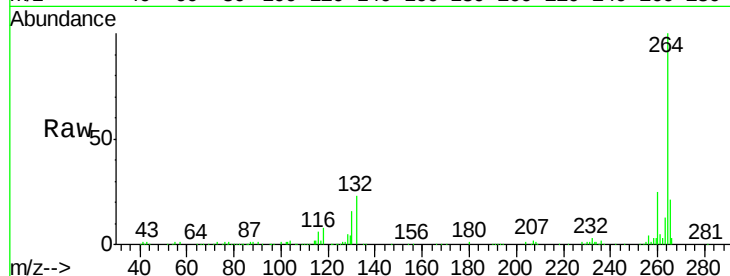

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

