

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050417\
 Data File : BF094910.D
 Acq On : 5 May 2017 11:13
 Operator : SJ/MA
 Sample : I2956-03
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 IP-TP(0-5)

Quant Time: May 05 12:02:52 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 03 17:24:51 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	87978	20.00	ng	0.00
21) Naphthalene-d8	9.74	136	359480	20.00	ng	-0.01
38) Acenaphthene-d10	12.57	164	165185	20.00	ng	-0.01
63) Phenanthrene-d10	14.97	188	292664	20.00	ng	-0.01
75) Chrysene-d12	18.64	240	199650	20.00	ng	-0.02
86) Perylene-d12	20.30	264	174866	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.68	112	578469	109.62	ng	0.00
7) Phenol-d6	7.26	99	629999	99.50	ng	-0.02
23) Nitrobenzene-d5	8.62	82	445422	78.13	ng	-0.02
41) 2,4,6-Tribromophenol	13.87	330	161744	119.56	ng	-0.02
44) 2-Fluorobiphenyl	11.51	172	913729	79.62	ng	-0.02
78) Terphenyl-d14	17.29	244	718711	79.29	ng	-0.02


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050417\
Data File : BF094910.D
Acq On : 5 May 2017 11:13
Operator : SJ/MA
Sample : I2956-03
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
IP-TP(0-5)

Quant Time: May 05 12:02:52 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

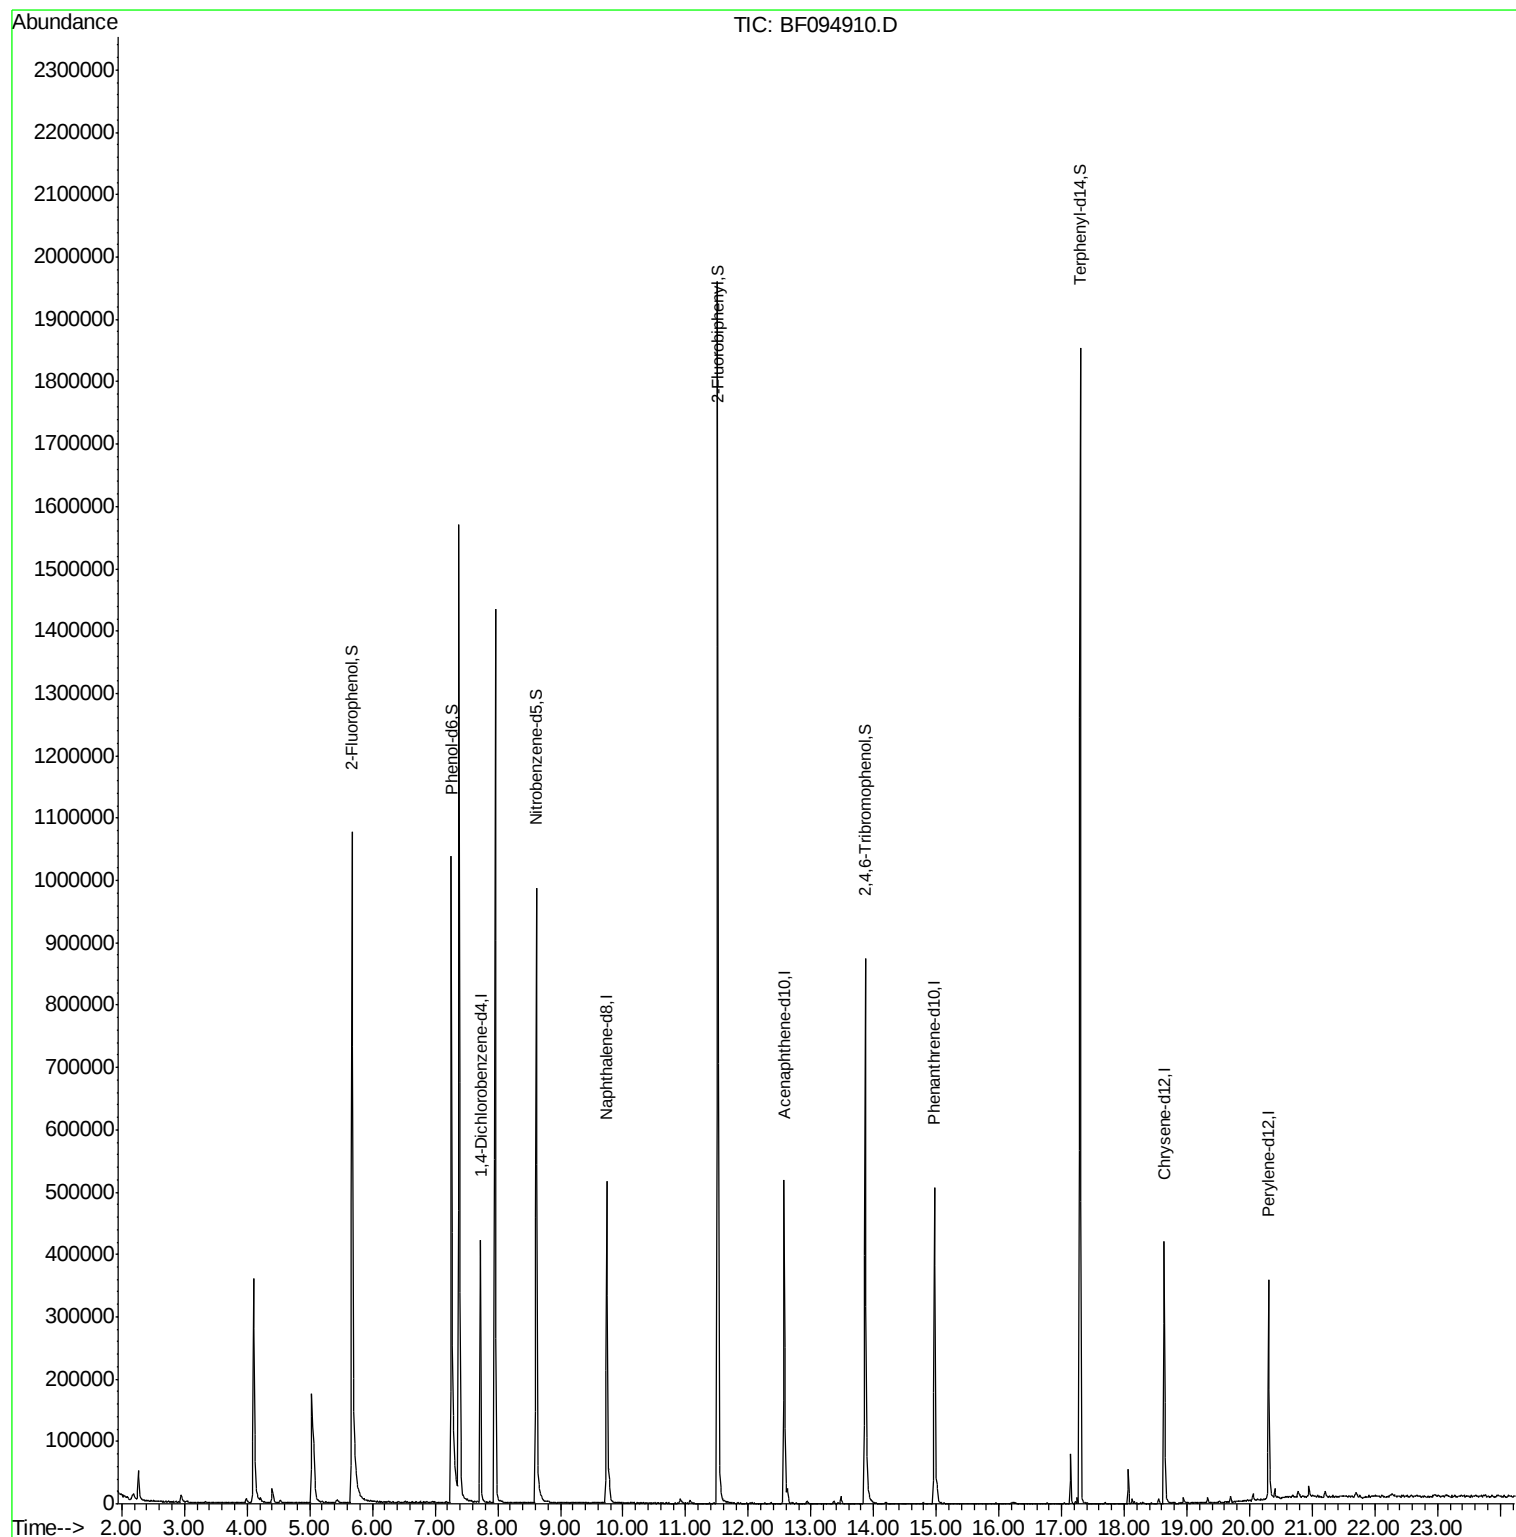




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.72 min Scan# 984
Delta R.T. -0.01 min
Lab File: BF094910.D
Acq: 5 May 2017 11:13

Instrument :
BNA_F
ClientSampleId :
IP-TP(0-5)

Tgt Ion:152 Resp: 87978
Ion Ratio Lower Upper
152 100
150 167.4 126.2 189.2
115 60.1 52.2 78.2

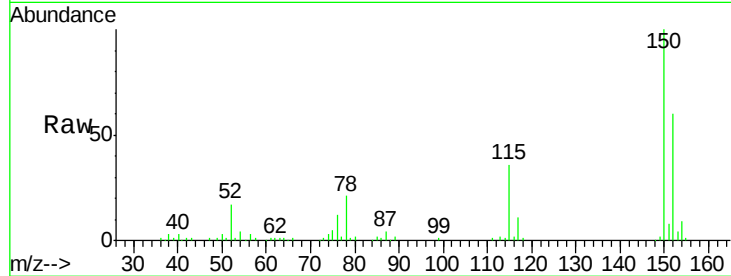


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

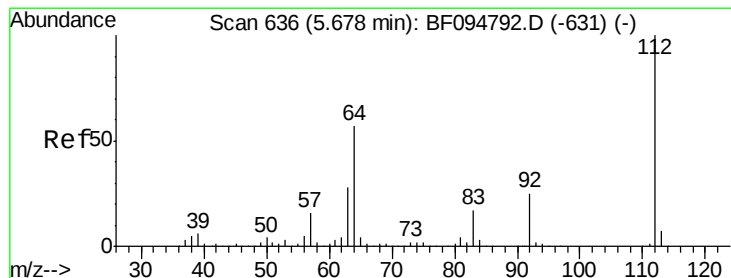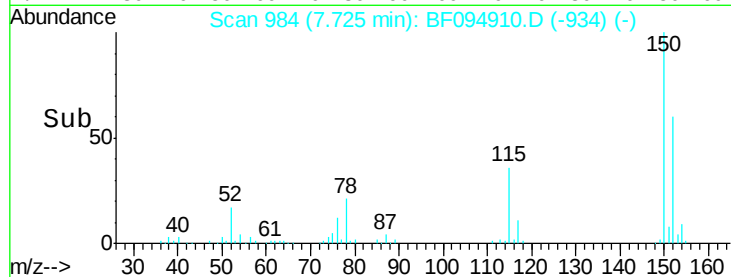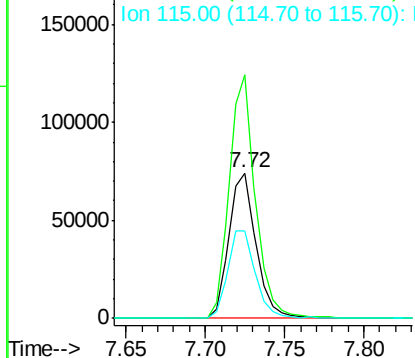



#5


2-Fluorophenol
Concen: 109.62 ng
RT: 5.68 min Scan# 636
Delta R.T. 0.00 min
Lab File: BF094910.D
Acq: 5 May 2017 11:13

Tgt Ion:112 Resp: 578469
Ion Ratio Lower Upper
112 100
64 53.9 46.0 69.0
63 26.4 23.4 35.0

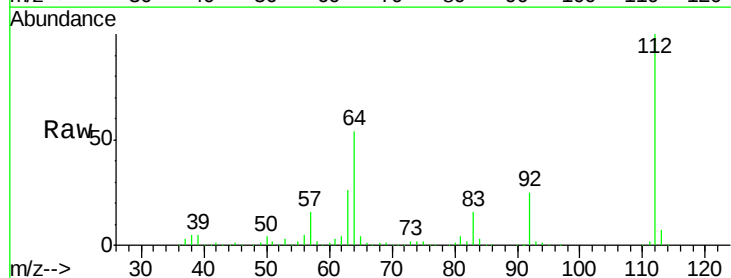

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

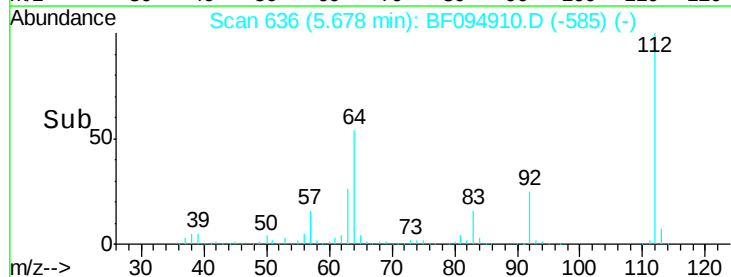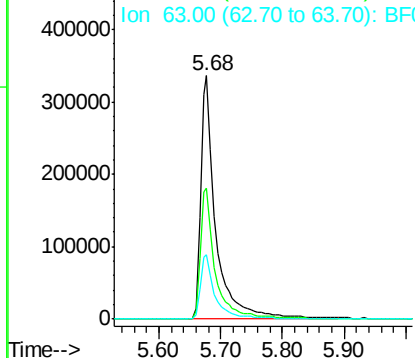

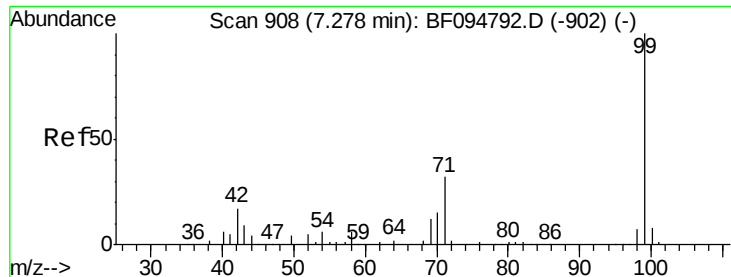

#7

Phenol-d6

Concen: 99.50 ng

RT: 7.26 min Scan# 905

Delta R.T. -0.02 min

Lab File: BF094910.D

Acq: 5 May 2017 11:13

Instrument :

BNA_F

ClientSampleId :

IP-TP(0-5)


Tgt Ion: 99 Resp: 629999

Ion Ratio Lower Upper

99 100

42 16.6 13.5 20.3




71 32.3 24.5 36.7

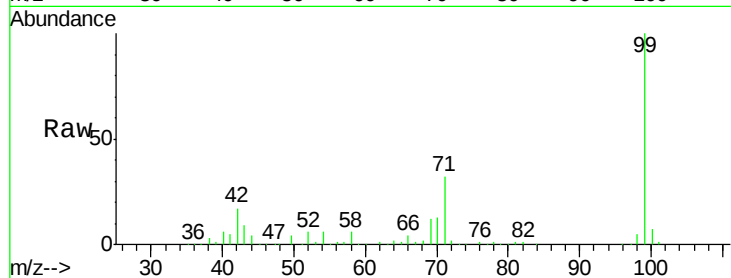

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

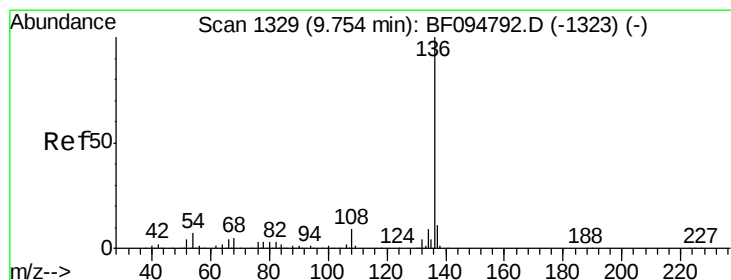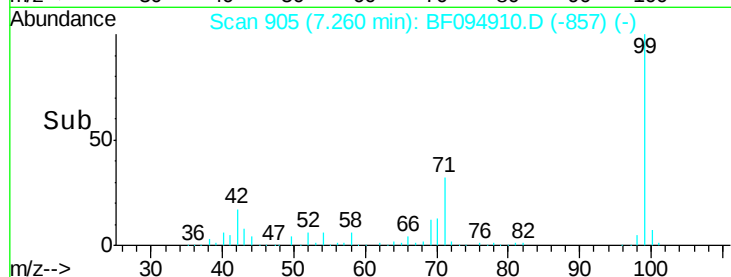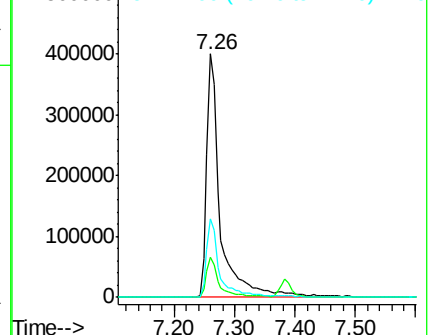

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.74 min Scan# 1327

Delta R.T. -0.01 min

Lab File: BF094910.D

Acq: 5 May 2017 11:13

Tgt Ion: 136 Resp: 359480


Ion Ratio Lower Upper

136 100

137 10.9 8.5 12.7

54 6.7 4.9 7.3

68 5.5 4.1 6.1


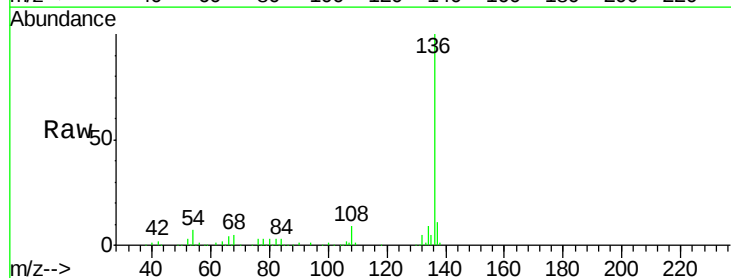


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

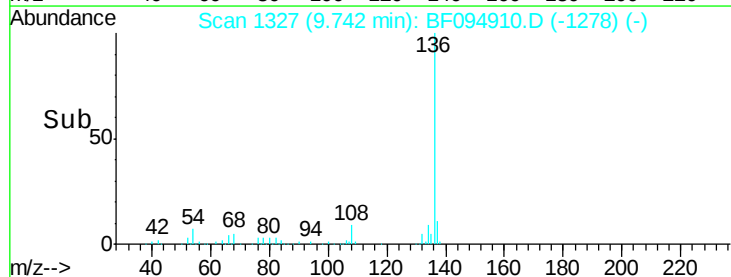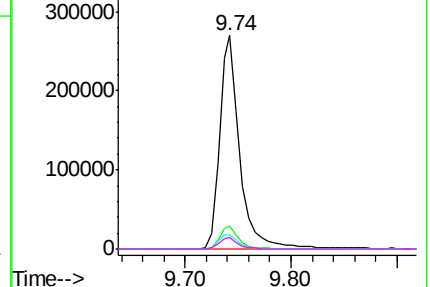







#23
Nitrobenzene-d5
Concen: 78.13 ng
RT: 8.62 min Scan# 1136
Delta R.T. -0.02 min
Lab File: BF094910.D
Acq: 5 May 2017 11:13

Instrument :
BNA_F
ClientSampleId :
IP-TP(0-5)

Tgt Ion: 82 Resp: 445422
Ion Ratio Lower Upper
82 100
128 49.2 34.0 51.0
54 47.0 42.2 63.2

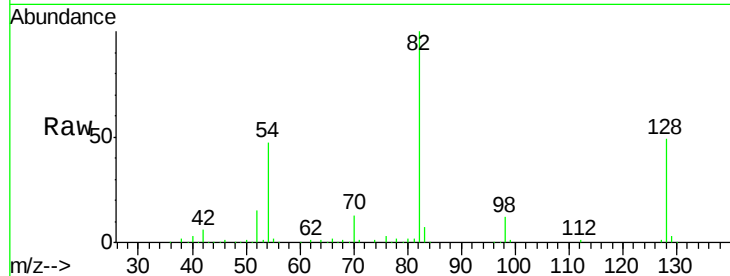


Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

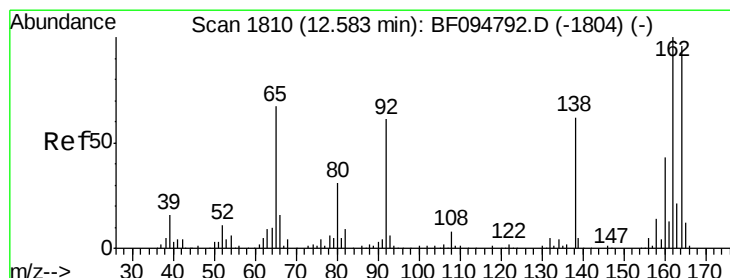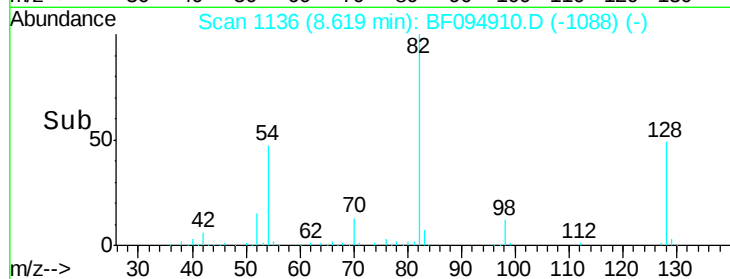
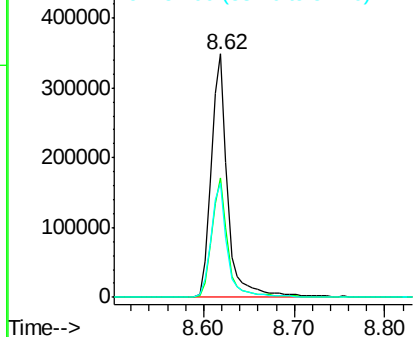


#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 12.57 min Scan# 1808
Delta R.T. -0.01 min
Lab File: BF094910.D
Acq: 5 May 2017 11:13

Tgt Ion: 164 Resp: 165185
Ion Ratio Lower Upper
164 100
162 103.1 82.6 123.8
160 45.2 36.2 54.2

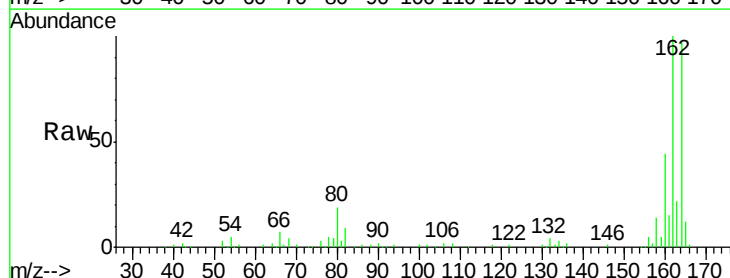

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

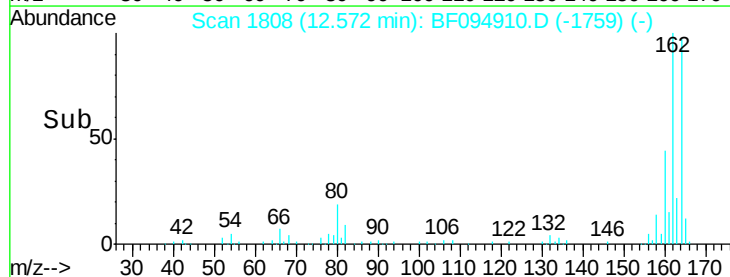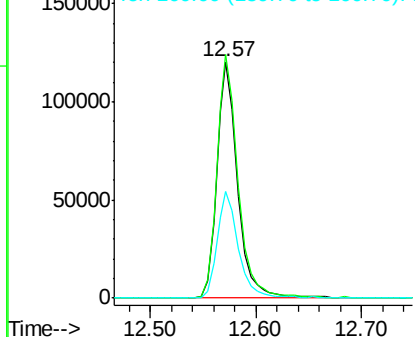







#41
 2,4,6-Tribromophenol
 Concen: 119.56 ng
 RT: 13.87 min Scan# 2028
 Delta R.T. -0.02 min
 Lab File: BF094910.D
 Acq: 5 May 2017 11:13

Instrument :
 BNA_F
 ClientSampleId :
 IP-TP(0-5)

Tgt Ion: 330 Resp: 161744
 Ion Ratio Lower Upper
 330 100
 332 96.1 76.6 115.0
 141 39.1 31.4 47.2

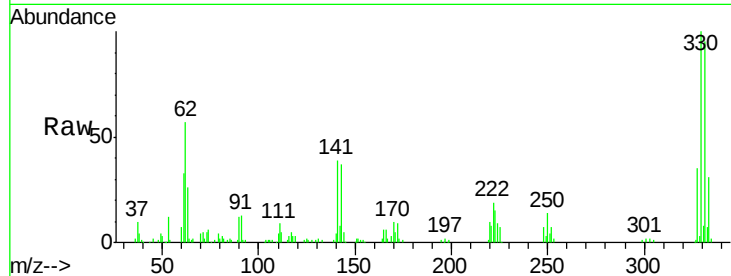


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

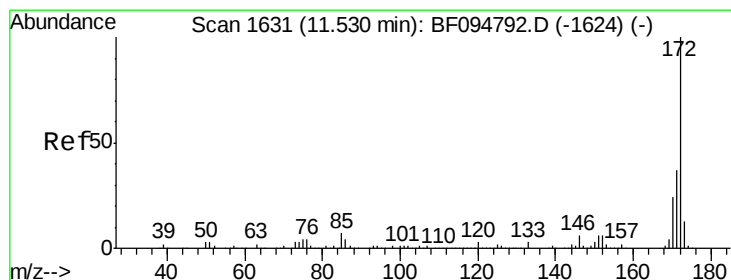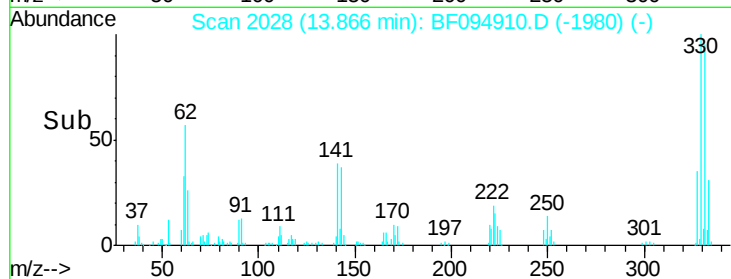
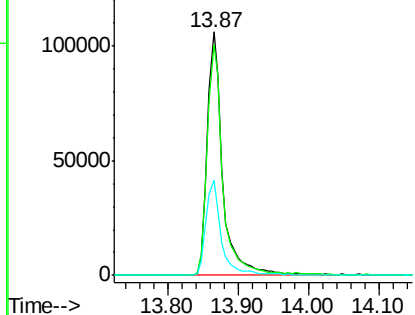



#44
 2-Fluorobiphenyl
 Concen: 79.62 ng
 RT: 11.51 min Scan# 1628
 Delta R.T. -0.02 min
 Lab File: BF094910.D
 Acq: 5 May 2017 11:13

Tgt Ion: 172 Resp: 913729
 Ion Ratio Lower Upper
 172 100
 171 36.0 29.6 44.4
 170 23.5 19.8 29.8

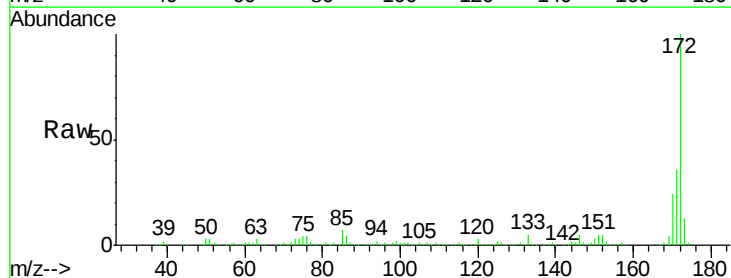

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

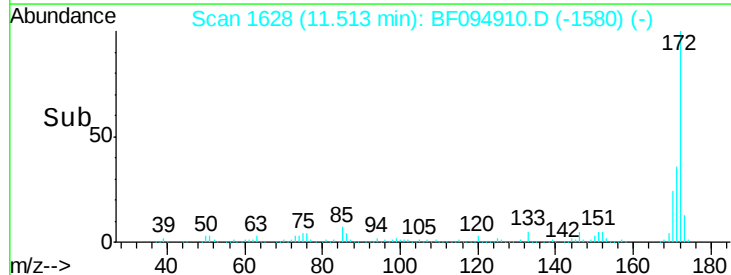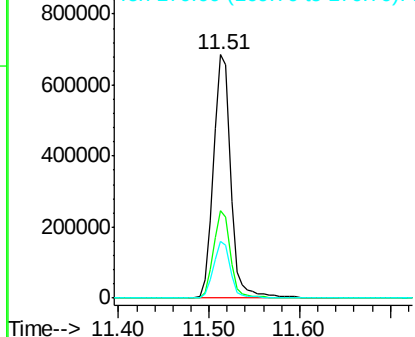


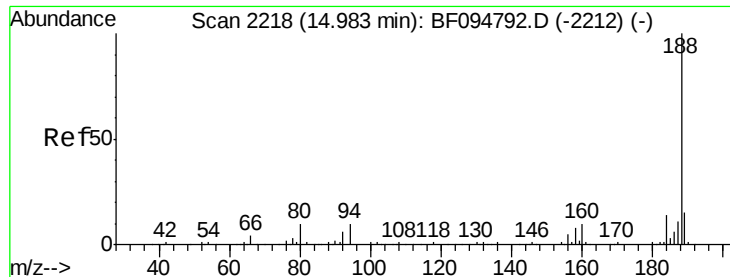




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 14.97 min Scan# 2216
Delta R.T. -0.01 min
Lab File: BF094910.D
Acq: 5 May 2017 11:13

Instrument :
BNA_F
ClientSampled :
IP-TP(0-5)

Tgt Ion	Ratio	Lower	Upper
188	100		
94	9.9	9.4	14.2
80	11.3	10.2	15.2

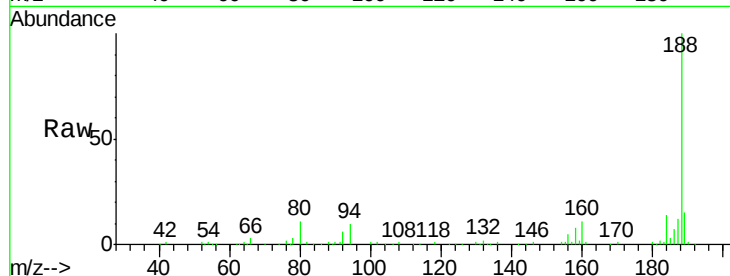


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

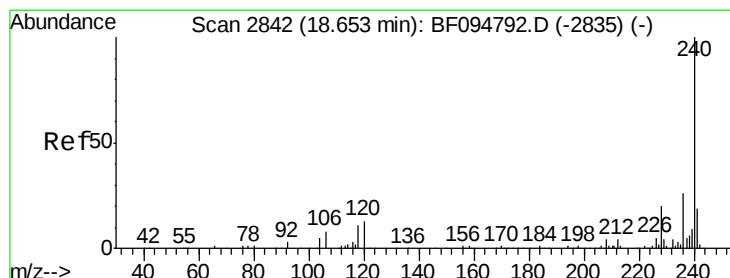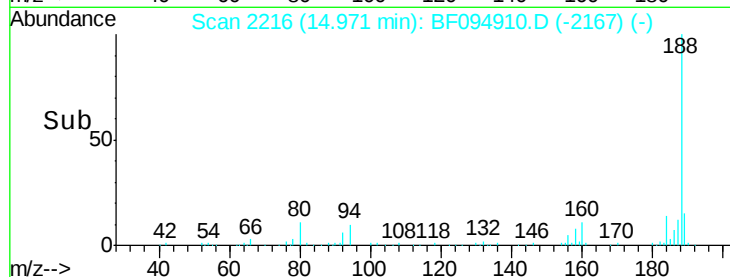
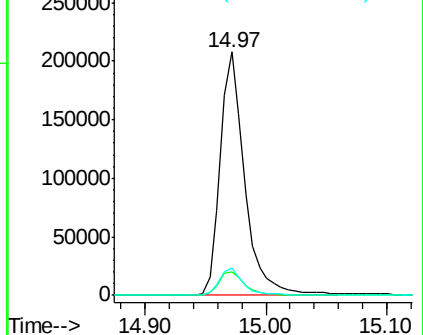


#75
Chrysene-d12
Concen: 20.00 ng
RT: 18.64 min Scan# 2839
Delta R.T. -0.02 min
Lab File: BF094910.D
Acq: 5 May 2017 11:13

Tgt Ion	Ratio	Lower	Upper
240	100		
120	13.4	5.8	8.8#
236	25.3	20.5	30.7

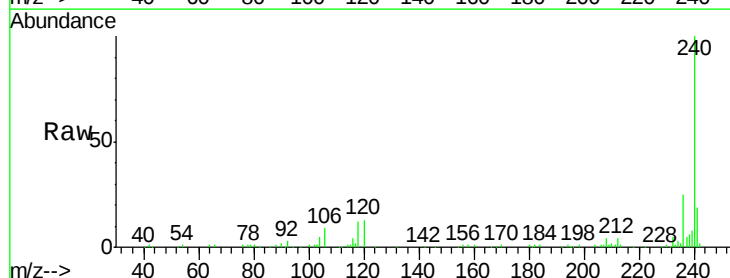

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



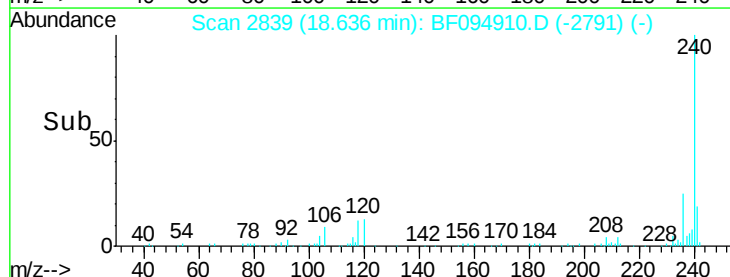
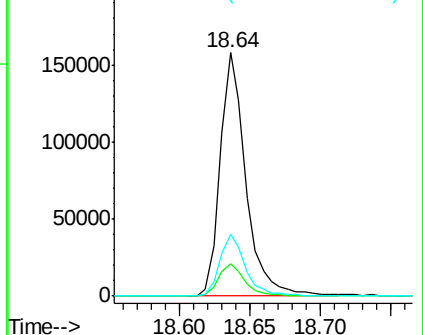




#78
 Terphenyl-d14
 Concen: 79.29 ng
 RT: 17.29 min Scan# 2611
 Delta R.T. -0.02 min
 Lab File: BF094910.D
 Acq: 5 May 2017 11:13

Instrument :
 BNA_F
 ClientSampleId :
 IP-TP(0-5)

Tgt Ion:244 Resp: 718711
 Ion Ratio Lower Upper
 244 100
 212 6.9 6.0 9.0
 122 13.7 10.3 15.5

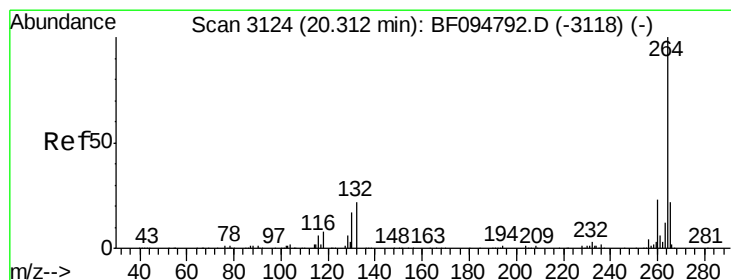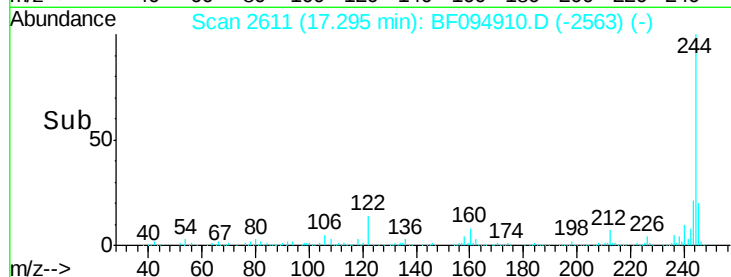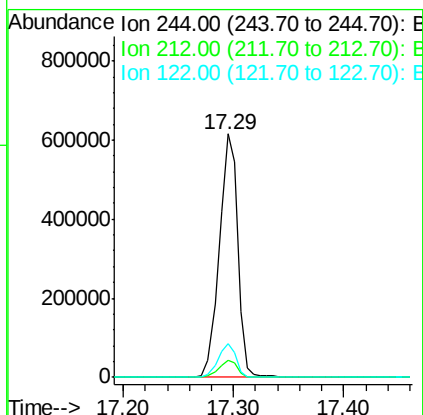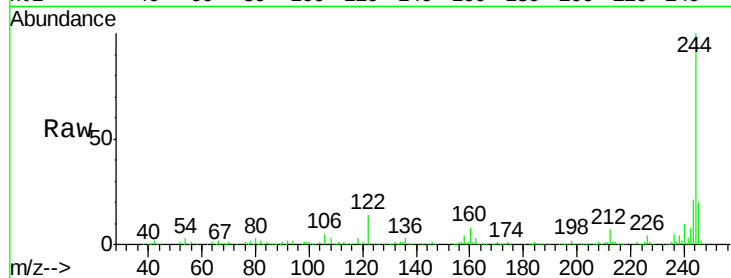

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 20.30 min Scan# 3122
 Delta R.T. -0.01 min
 Lab File: BF094910.D
 Acq: 5 May 2017 11:13

Tgt Ion:264 Resp: 174866
 Ion Ratio Lower Upper
 264 100
 260 24.1 19.5 29.3
 265 21.3 17.2 25.8

