

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050417\
 Data File : BF094916.D
 Acq On : 5 May 2017 14:26
 Operator : SJ/MA
 Sample : I2949-02
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-07-COMP

Quant Time: May 05 15:24:48 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 03 17:24:51 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	80921	20.00	ng	-0.01
21) Naphthalene-d8	9.74	136	333916	20.00	ng	-0.01
38) Acenaphthene-d10	12.57	164	159769	20.00	ng	-0.01
63) Phenanthrene-d10	14.97	188	299619	20.00	ng	-0.01
75) Chrysene-d12	18.64	240	217271	20.00	ng	-0.02
86) Perylene-d12	20.30	264	153513	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.67	112	676558	139.39	ng	-0.01
7) Phenol-d6	7.26	99	836799	143.69	ng	-0.02
23) Nitrobenzene-d5	8.62	82	483531	91.31	ng	-0.02
41) 2,4,6-Tribromophenol	13.87	330	185346	141.65	ng	-0.02
44) 2-Fluorobiphenyl	11.51	172	971543	87.53	ng	-0.02
78) Terphenyl-d14	17.29	244	794858	80.58	ng	-0.02
Target Compounds						
49) Dimethylphthalate	12.21	163	89507	6.82	ng	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050417\
Data File : BF094916.D
Acq On : 5 May 2017 14:26
Operator : SJ/MA
Sample : I2949-02
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-07-COMP

Quant Time: May 05 15:24:48 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

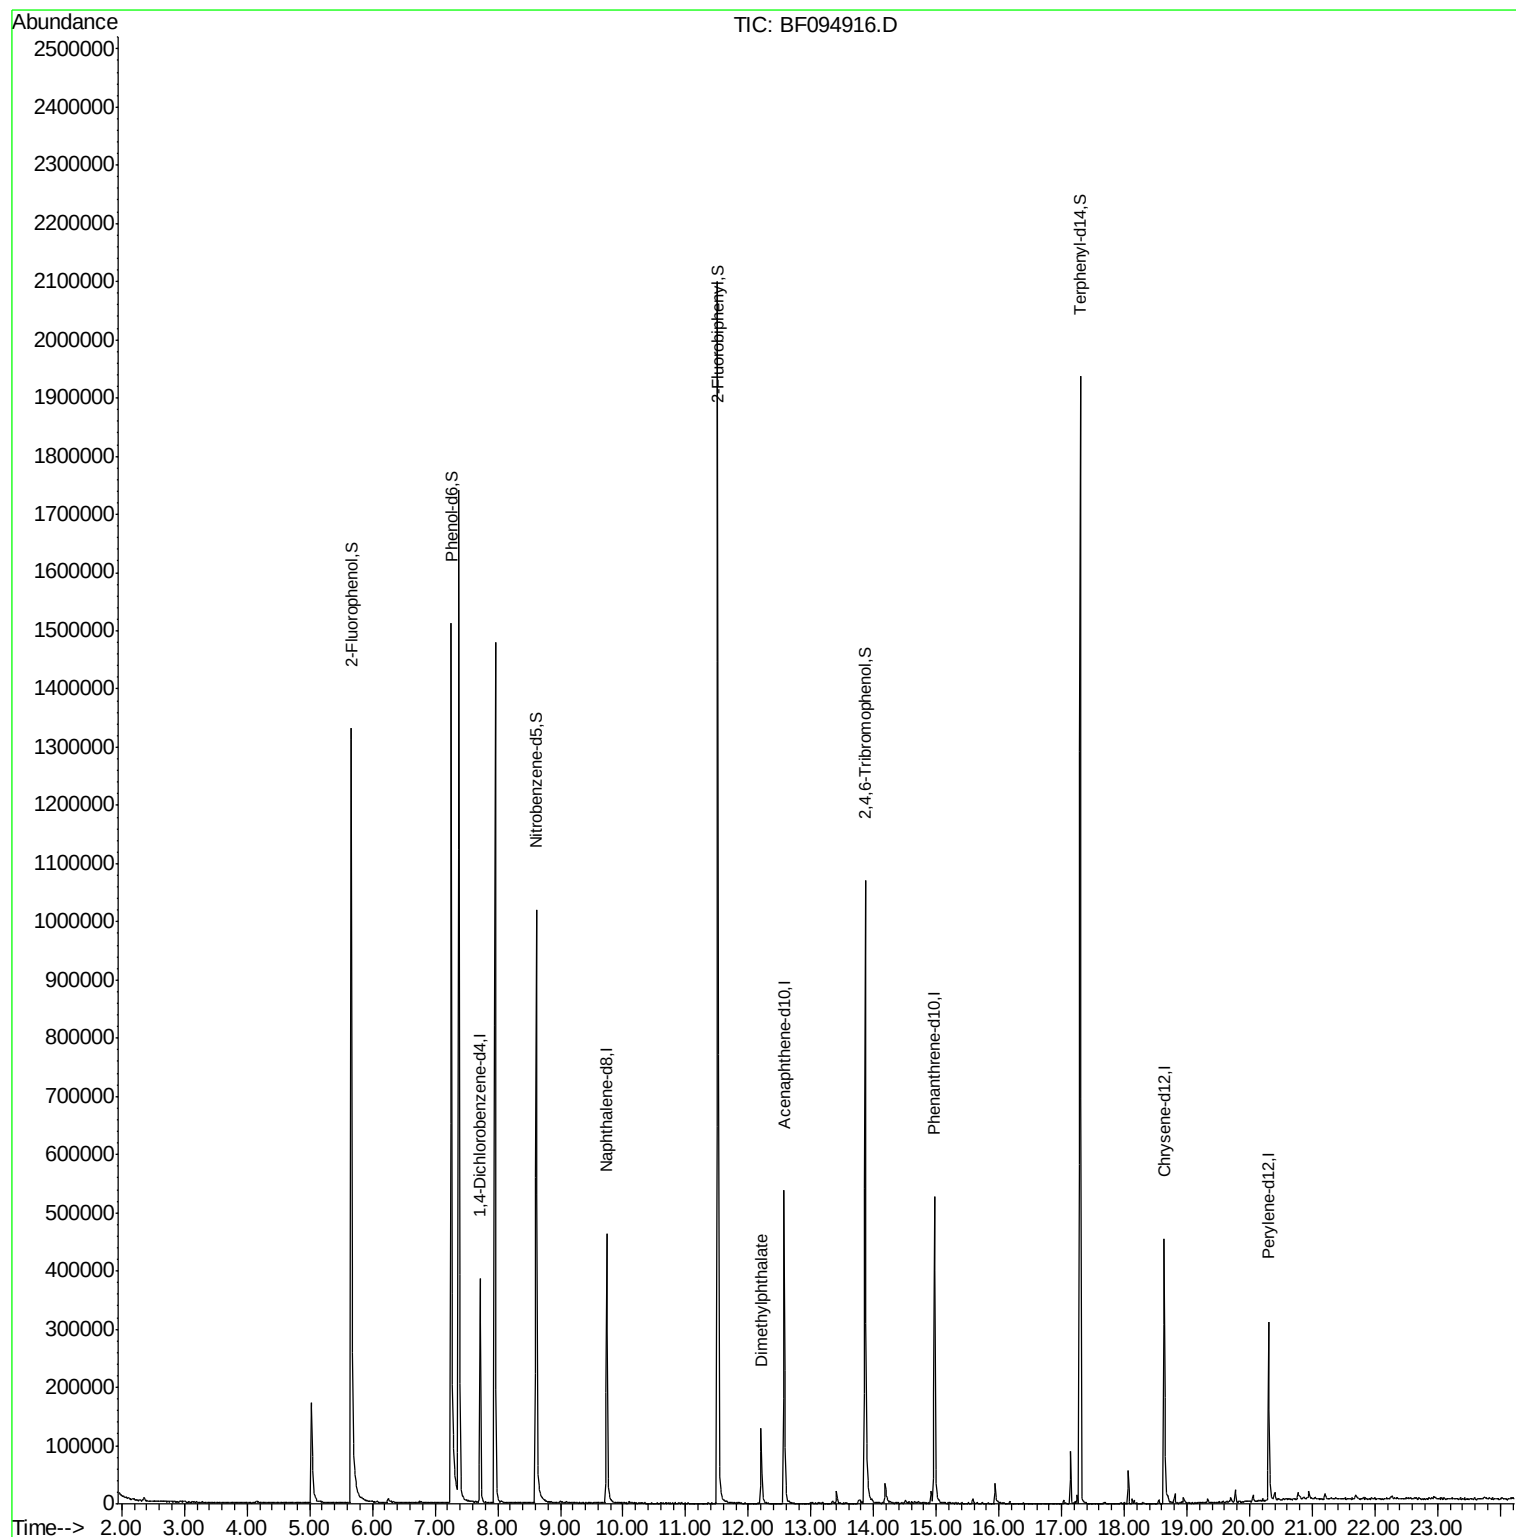

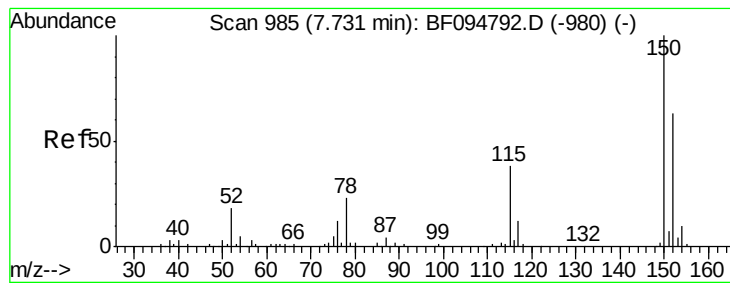


#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.72 min Scan# 983
 Delta R.T. -0.01 min
 Lab File: BF094916.D
 Acq: 5 May 2017 14:26

Instrument :
 BNA_F
 ClientSampleId :
 SB-07-COMP

Tgt Ion:152 Resp: 80921
 Ion Ratio Lower Upper
 152 100
 150 159.7 126.2 189.2
 115 61.8 52.2 78.2

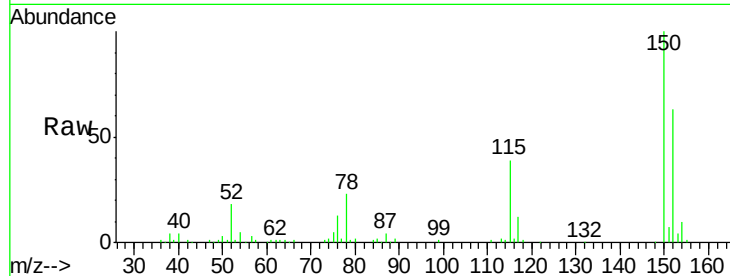


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

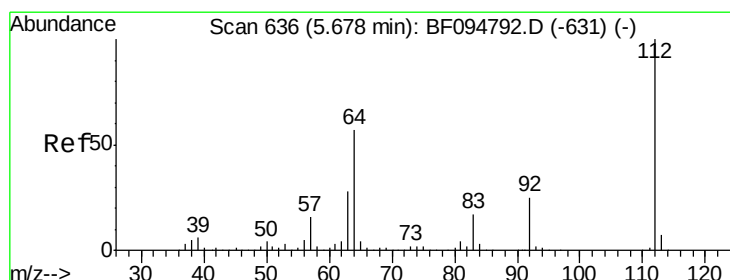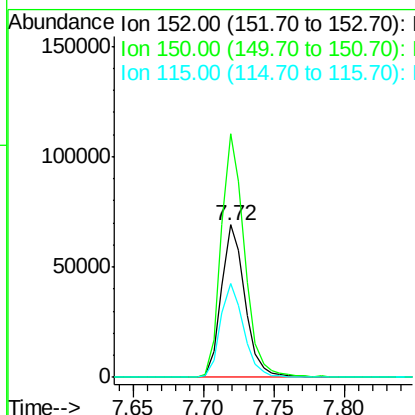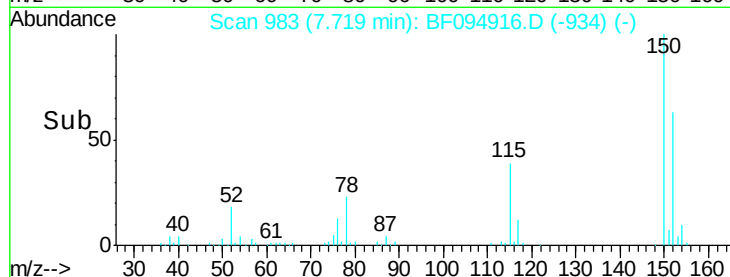



#5


2-Fluorophenol
 Concen: 139.39 ng
 RT: 5.67 min Scan# 634
 Delta R.T. -0.01 min
 Lab File: BF094916.D
 Acq: 5 May 2017 14:26

Tgt Ion:112 Resp: 676558
 Ion Ratio Lower Upper
 112 100
 64 52.7 46.0 69.0
 63 26.8 23.4 35.0

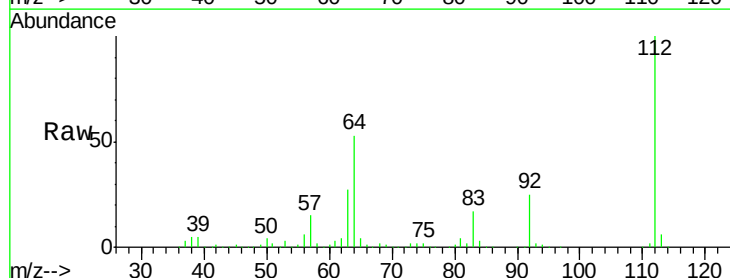

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

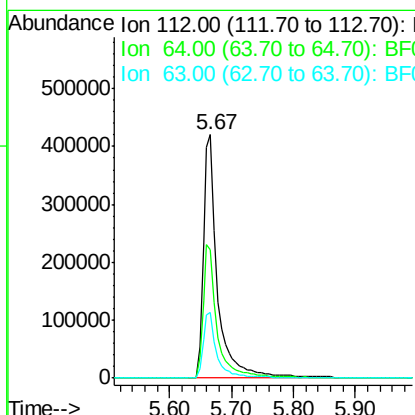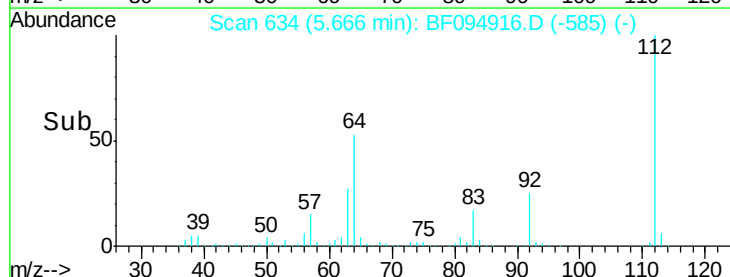

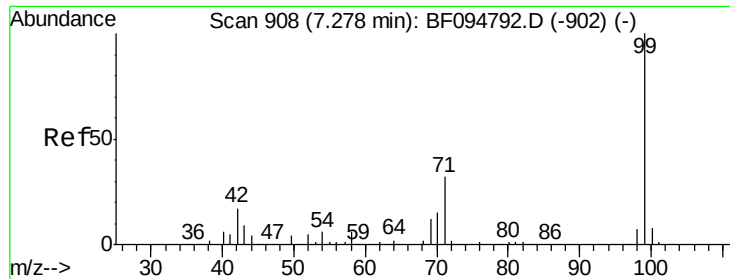

#7

Phenol-d6

Concen: 143.69 ng

RT: 7.26 min Scan# 905

Delta R.T. -0.02 min

Lab File: BF094916.D

Acq: 5 May 2017 14:26

Instrument :

BNA_F

ClientSampleId :

SB-07-COMP


Tgt Ion: 99 Resp: 836799

Ion Ratio Lower Upper

99 100

42 16.7 13.5 20.3




71 32.7 24.5 36.7

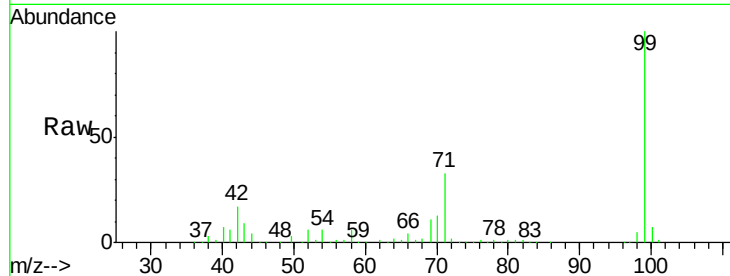

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

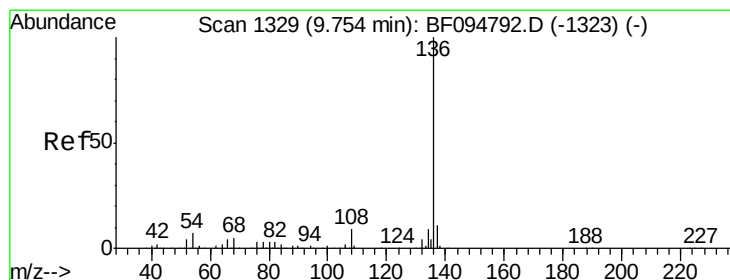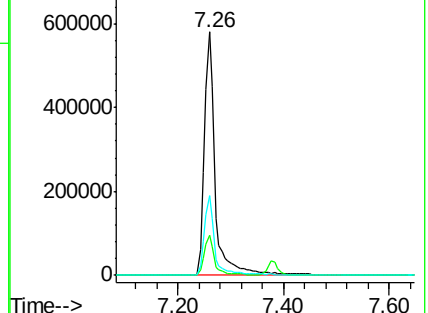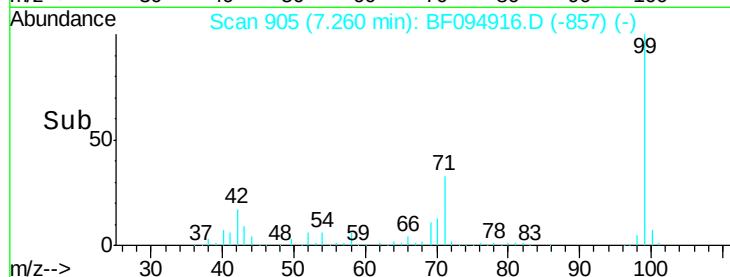

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.74 min Scan# 1327

Delta R.T. -0.01 min

Lab File: BF094916.D

Acq: 5 May 2017 14:26

Tgt Ion: 136 Resp: 333916


Ion Ratio Lower Upper

136 100

137 10.9 8.5 12.7

54 6.8 4.9 7.3

68 5.1 4.1 6.1


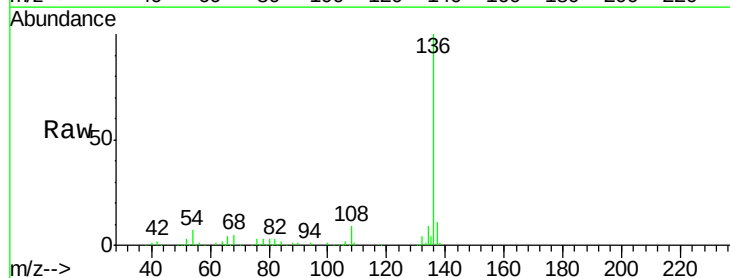



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

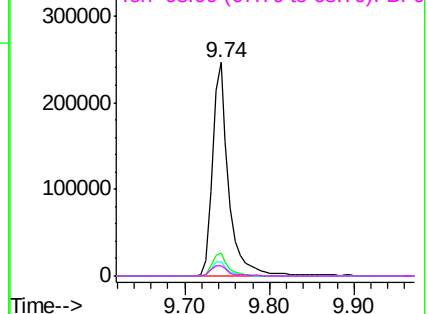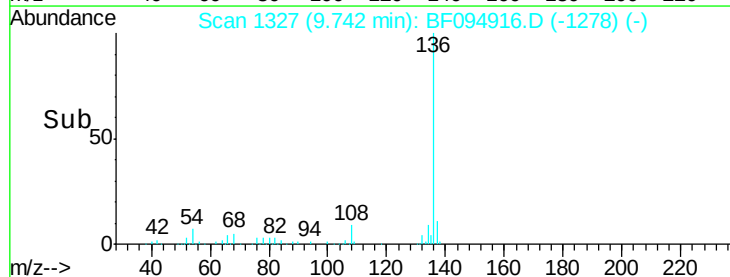


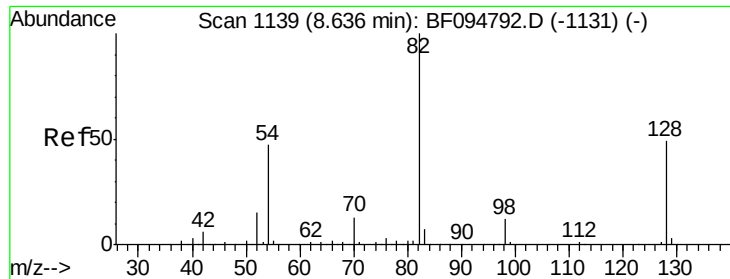




#23
 Nitrobenzene-d5
 Concen: 91.31 ng
 RT: 8.62 min Scan# 1136
 Delta R.T. -0.02 min
 Lab File: BF094916.D
 Acq: 5 May 2017 14:26

Instrument :
 BNA_F
 ClientSampleId :
 SB-07-COMP

Tgt Ion: 82 Resp: 483531
 Ion Ratio Lower Upper
 82 100
 128 47.8 34.0 51.0
 54 47.0 42.2 63.2

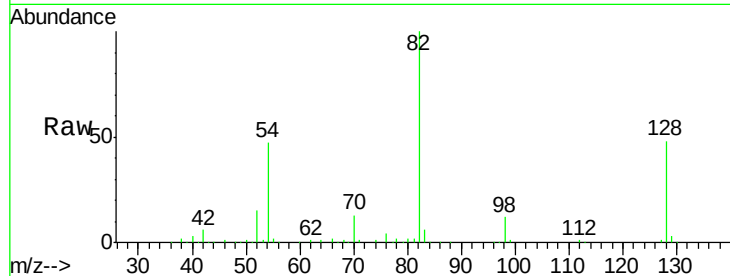


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

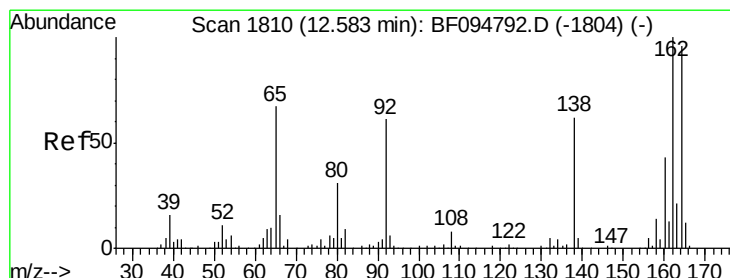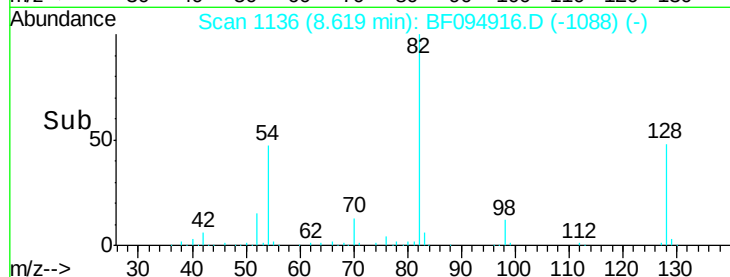
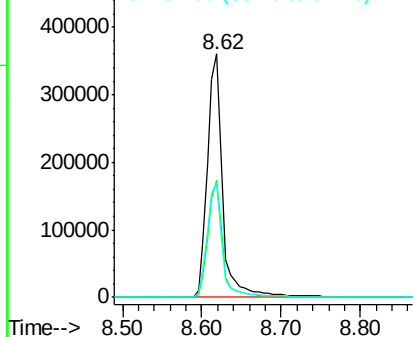



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 12.57 min Scan# 1808
 Delta R.T. -0.01 min
 Lab File: BF094916.D
 Acq: 5 May 2017 14:26

Tgt Ion: 164 Resp: 159769
 Ion Ratio Lower Upper
 164 100
 162 105.2 82.6 123.8
 160 46.1 36.2 54.2

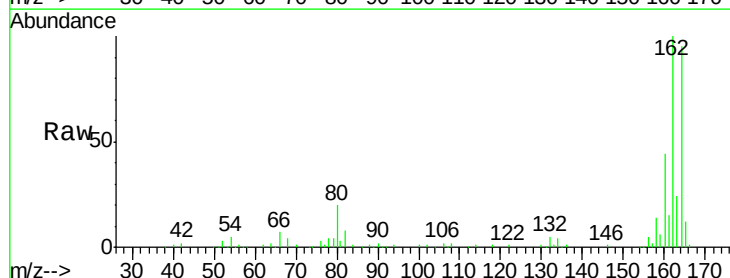

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E



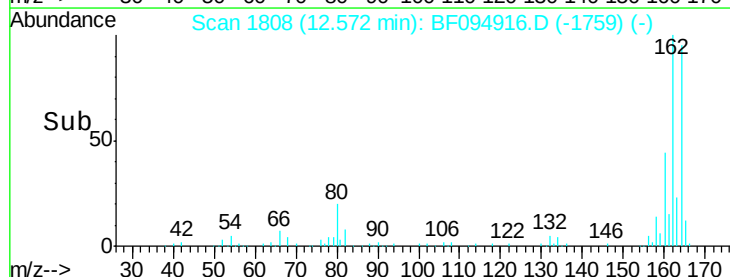
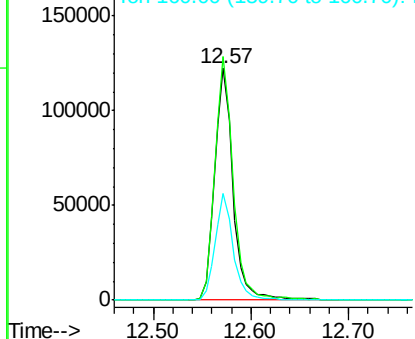


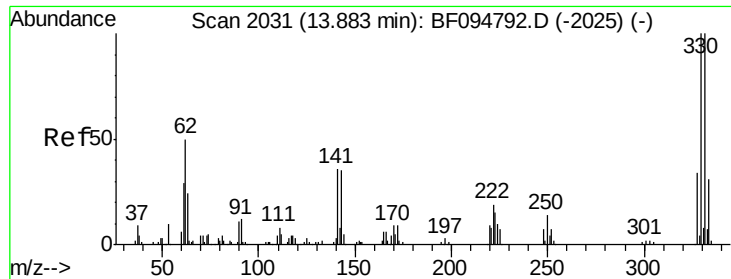

#41
 2,4,6-Tribromophenol
 Concen: 141.65 ng
 RT: 13.87 min Scan# 2028
 Delta R.T. -0.02 min
 Lab File: BF094916.D
 Acq: 5 May 2017 14:26




Instrument :
 BNA_F
 ClientSampleId :
 SB-07-COMP


Tgt Ion: 330 Resp: 185346
 Ion Ratio Lower Upper
 330 100
 332 95.9 76.6 115.0
 141 40.0 31.4 47.2

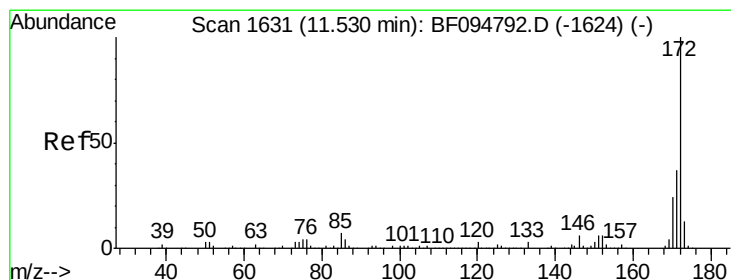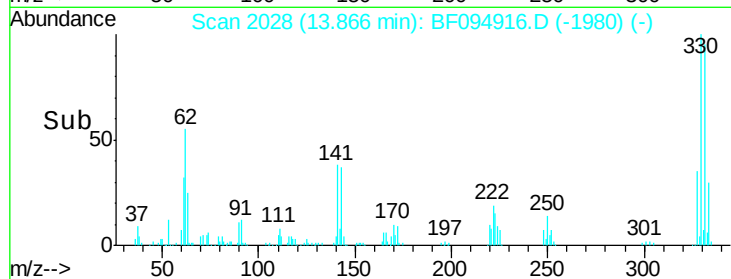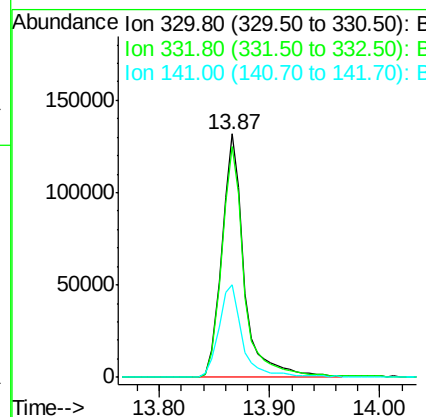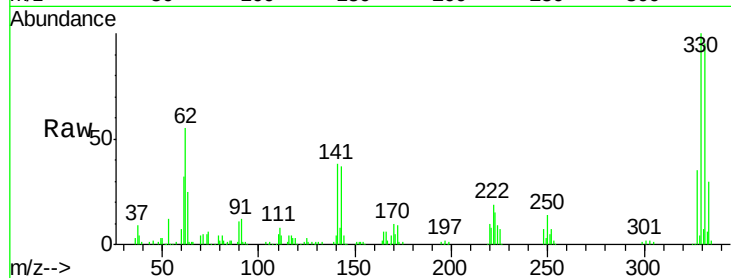

#44
 2-Fluorobiphenyl
 Concen: 87.53 ng
 RT: 11.51 min Scan# 1628
 Delta R.T. -0.02 min
 Lab File: BF094916.D
 Acq: 5 May 2017 14:26

Tgt Ion: 172 Resp: 971543
 Ion Ratio Lower Upper
 172 100
 171 35.7 29.6 44.4
 170 23.6 19.8 29.8

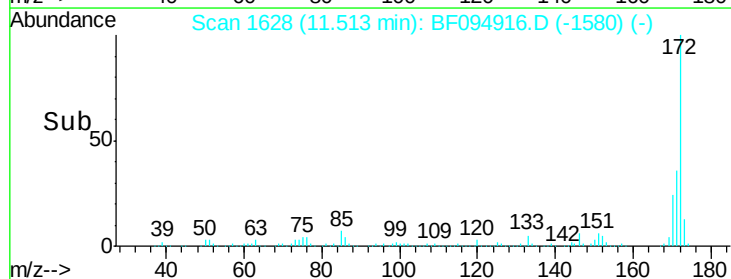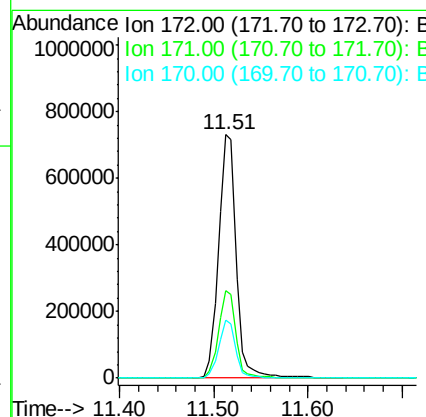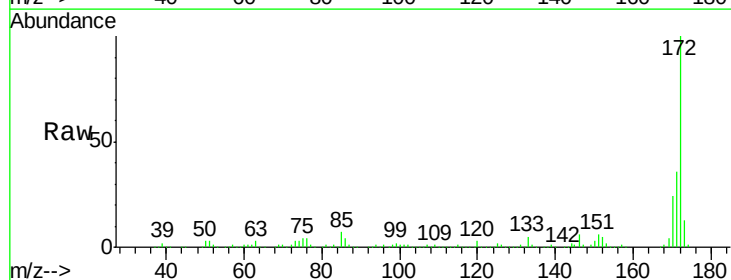

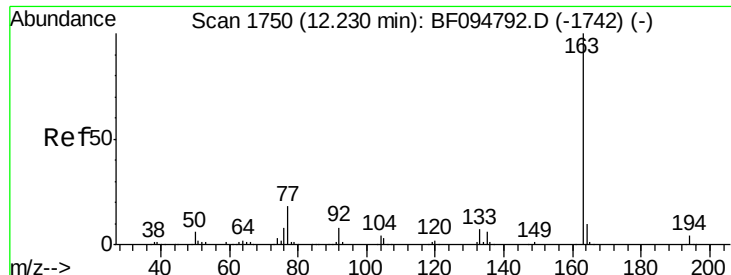

#49

Dimethylphthalate

Concen: 6.82 ng

RT: 12.21 min Scan# 1746

Delta R.T. -0.02 min

Lab File: BF094916.D

Acq: 5 May 2017 14:26

Instrument :

BNA_F

ClientSampleId :

SB-07-COMP


Tgt Ion:163 Resp: 89507

Ion Ratio Lower Upper

163 100

194 3.3 2.6 4.0




164 9.2 8.4 12.6

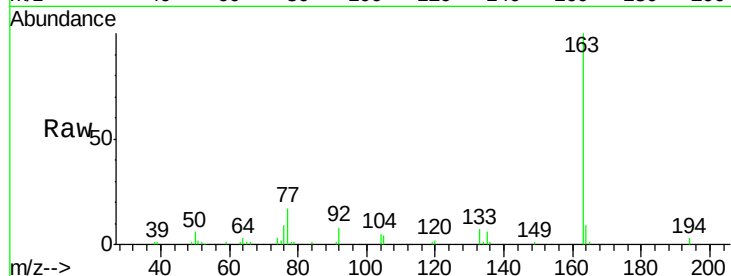

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

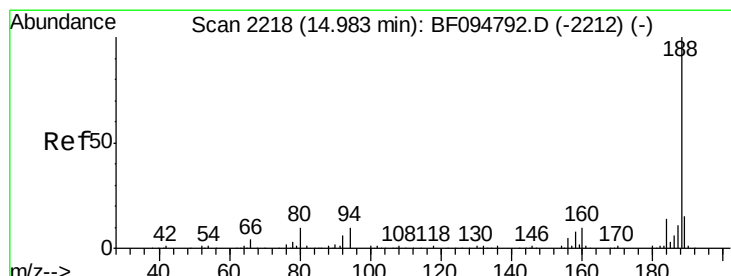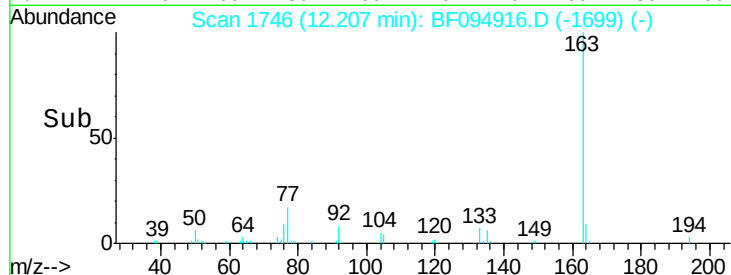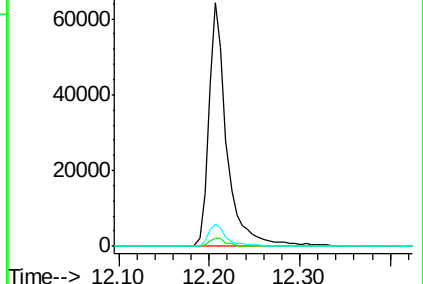

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 14.97 min Scan# 2216

Delta R.T. -0.01 min

Lab File: BF094916.D

Acq: 5 May 2017 14:26


Tgt Ion:188 Resp: 299619

Ion Ratio Lower Upper

188 100

94 9.9 9.4 14.2



80 10.4 10.2 15.2

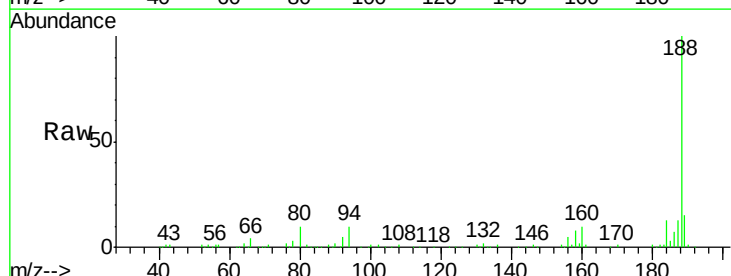


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0



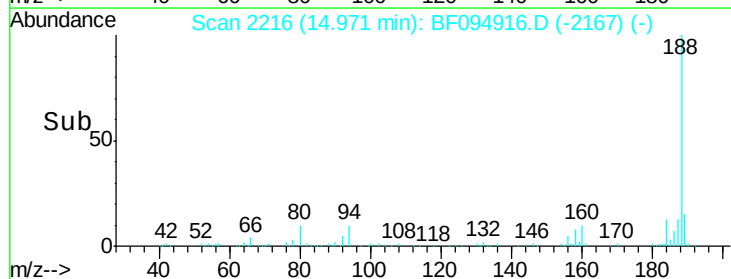
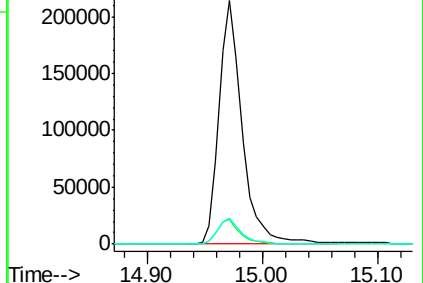


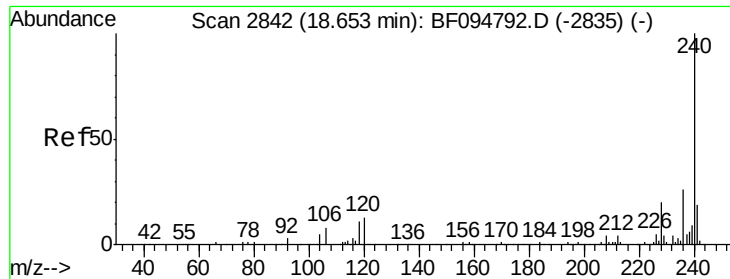

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 18.64 min Scan# 2839
 Delta R.T. -0.02 min
 Lab File: BF094916.D
 Acq: 5 May 2017 14:26




Instrument :
 BNA_F
 ClientSampleId :
 SB-07-COMP


Tgt Ion:240 Resp: 217271
 Ion Ratio Lower Upper
 240 100
 120 14.5 5.8 8.8#
 236 24.3 20.5 30.7

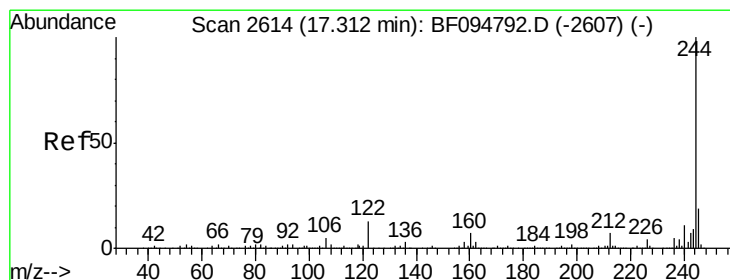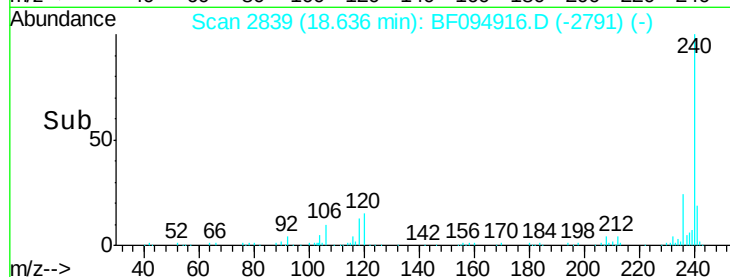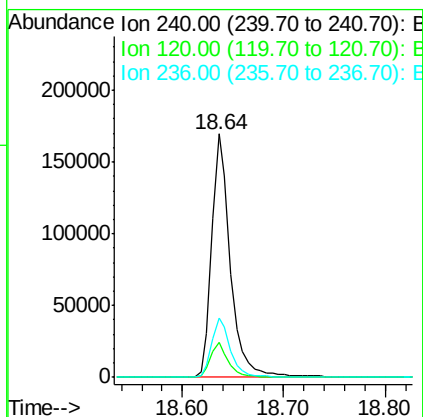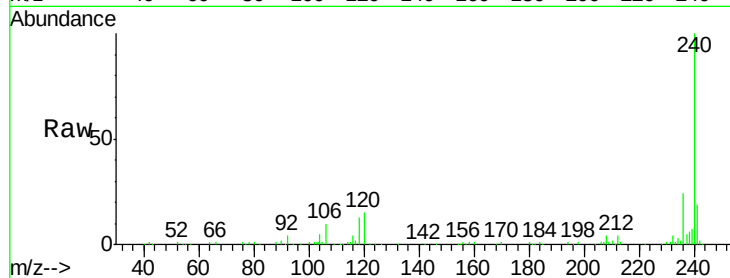

#78
 Terphenyl-d14
 Concen: 80.58 ng
 RT: 17.29 min Scan# 2611
 Delta R.T. -0.02 min
 Lab File: BF094916.D
 Acq: 5 May 2017 14:26

Tgt Ion:244 Resp: 794858
 Ion Ratio Lower Upper
 244 100
 212 6.9 6.0 9.0
 122 14.1 10.3 15.5

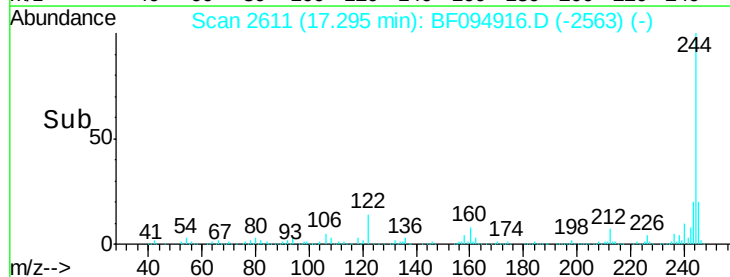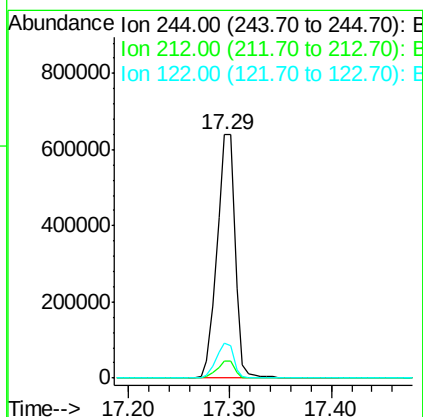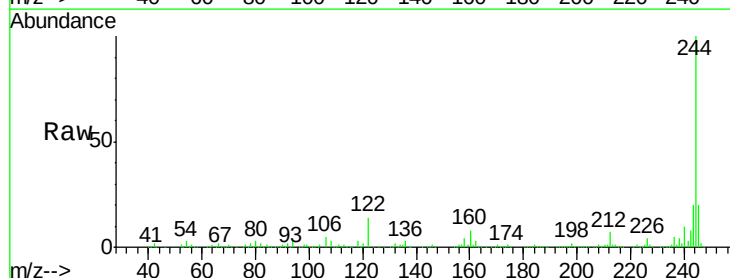


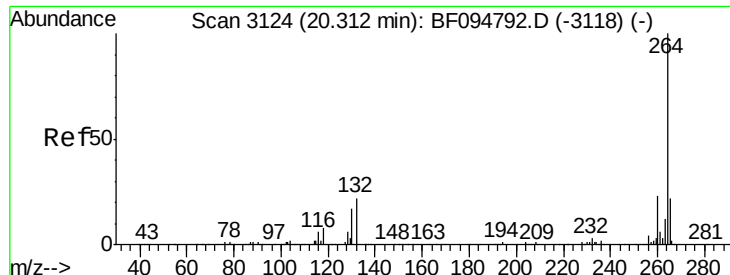

#86
Perylene-d12
Concen: 20.00 ng
RT: 20.30 min Scan# 3122
Delta R.T. -0.01 min
Lab File: BF094916.D
Acq: 5 May 2017 14:26

Instrument :
BNA_F
ClientSampleId :
SB-07-COMP

Tgt Ion: 264 Resp: 153513
Ion Ratio Lower Upper
264 100
260 22.9 19.5 29.3
265 21.4 17.2 25.8

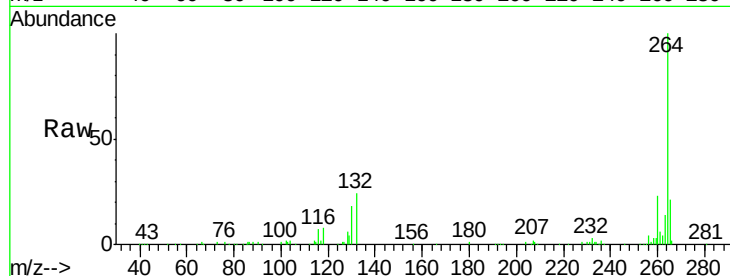

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

