


Data Path : Z:\HPCHEM1\BNA_F\Data\BF050417\
 Data File : BF094873.D
 Acq On : 4 May 2017 14:40
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 03 17:24:51 2017

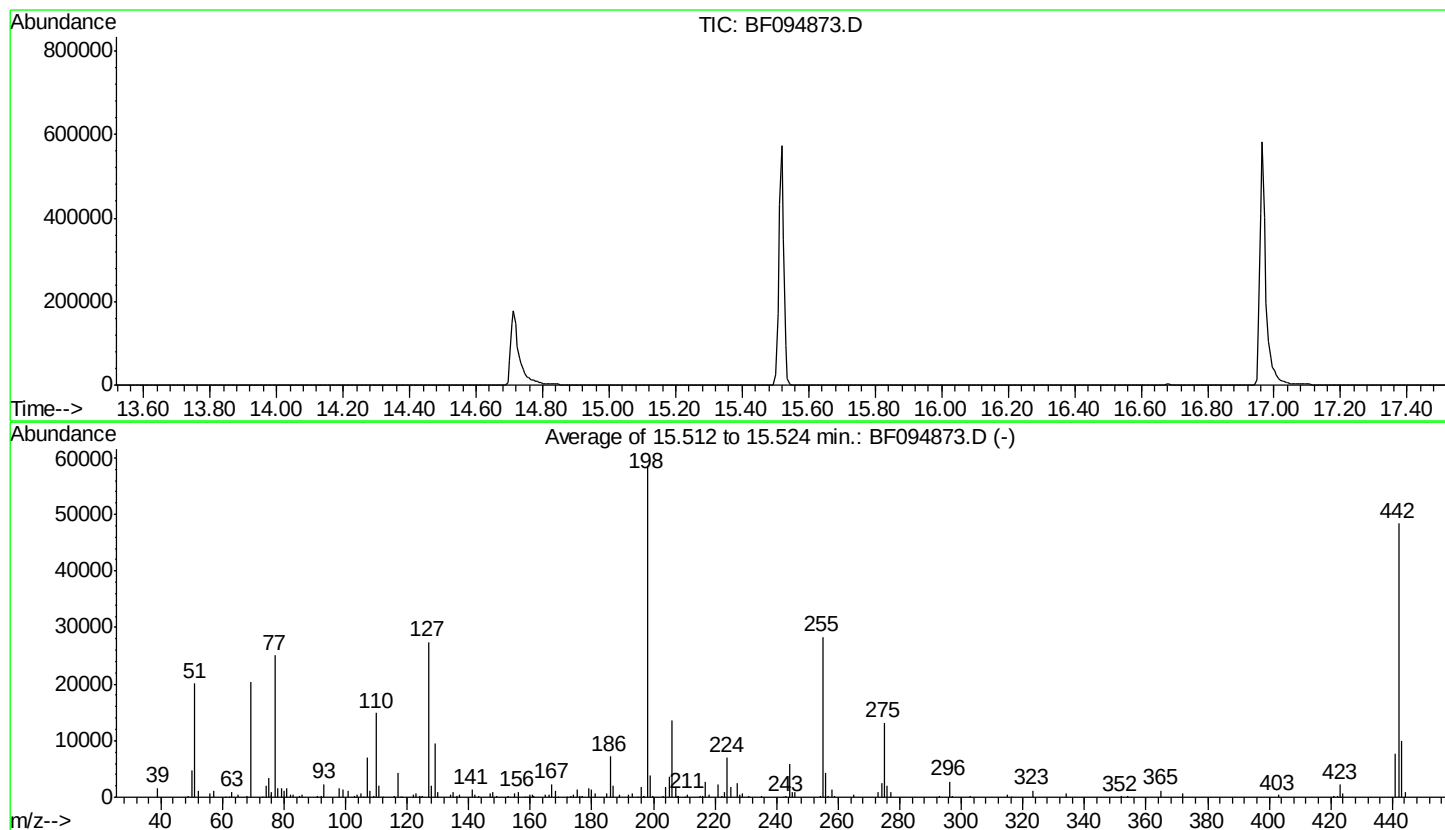

AutoFind: Scans 2308, 2309, 2310; Background Corrected with Scan 2303

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	20086	PASS
68	69	0.00	2	0.9	189	PASS
69	198	0.00	100	34.7	20365	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.9	27480	PASS
197	198	0.00	2	0.4	214	PASS
198	198	100	100	100.0	58613	PASS
199	198	5	9	6.4	3743	PASS
275	198	10	60	22.5	13191	PASS
365	198	1	100	2.0	1149	PASS
441	442	0.01	24	16.0	7725	PASS
442	198	50	100	82.5	48376	PASS
443	442	15	24	20.4	9870	PASS