

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050421\
 Data File : BF123816.D
 Acq On : 4 May 2021 19:20
 Operator : JU/CG
 Sample : M2252-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 STONE-2

Quant Time: May 05 05:13:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 04 12:58:27 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.798	152	212190	20.00	ng	-0.01
21) Naphthalene-d8	8.080	136	783446	20.00	ng	-0.02
39) Acenaphthene-d10	9.839	164	374472	20.00	ng	-0.01
64) Phenanthrene-d10	11.321	188	626743	20.00	ng	-0.02
76) Chrysene-d12	13.986	240	360216	20.00	ng	# 0.00
86) Perylene-d12	15.468	264	360193	20.00	ng	0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.416	112	1012527	75.60	ng	0.00
7) Phenol-d6	6.434	99	1336467	72.44	ng	-0.01
23) Nitrobenzene-d5	7.363	82	929953	53.58	ng	-0.01
42) 2,4,6-Tribromophenol	10.627	330	335770	72.03	ng	-0.02
45) 2-Fluorobiphenyl	9.163	172	1459670	56.77	ng	-0.01
79) Terphenyl-d14	12.921	244	1096096	58.59	ng	0.00
Target Compounds						
74) Di-n-butylphthalate	11.892	149	155654	4.20	ng	98
84) Bis(2-ethylhexyl)phtha...	13.974	149	354298	23.88	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050421\
Data File : BF123816.D
Acq On : 4 May 2021 19:20
Operator : JU/CG
Sample : M2252-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
STONE-2

Quant Time: May 05 05:13:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 04 12:58:27 2021
Response via : Initial Calibration




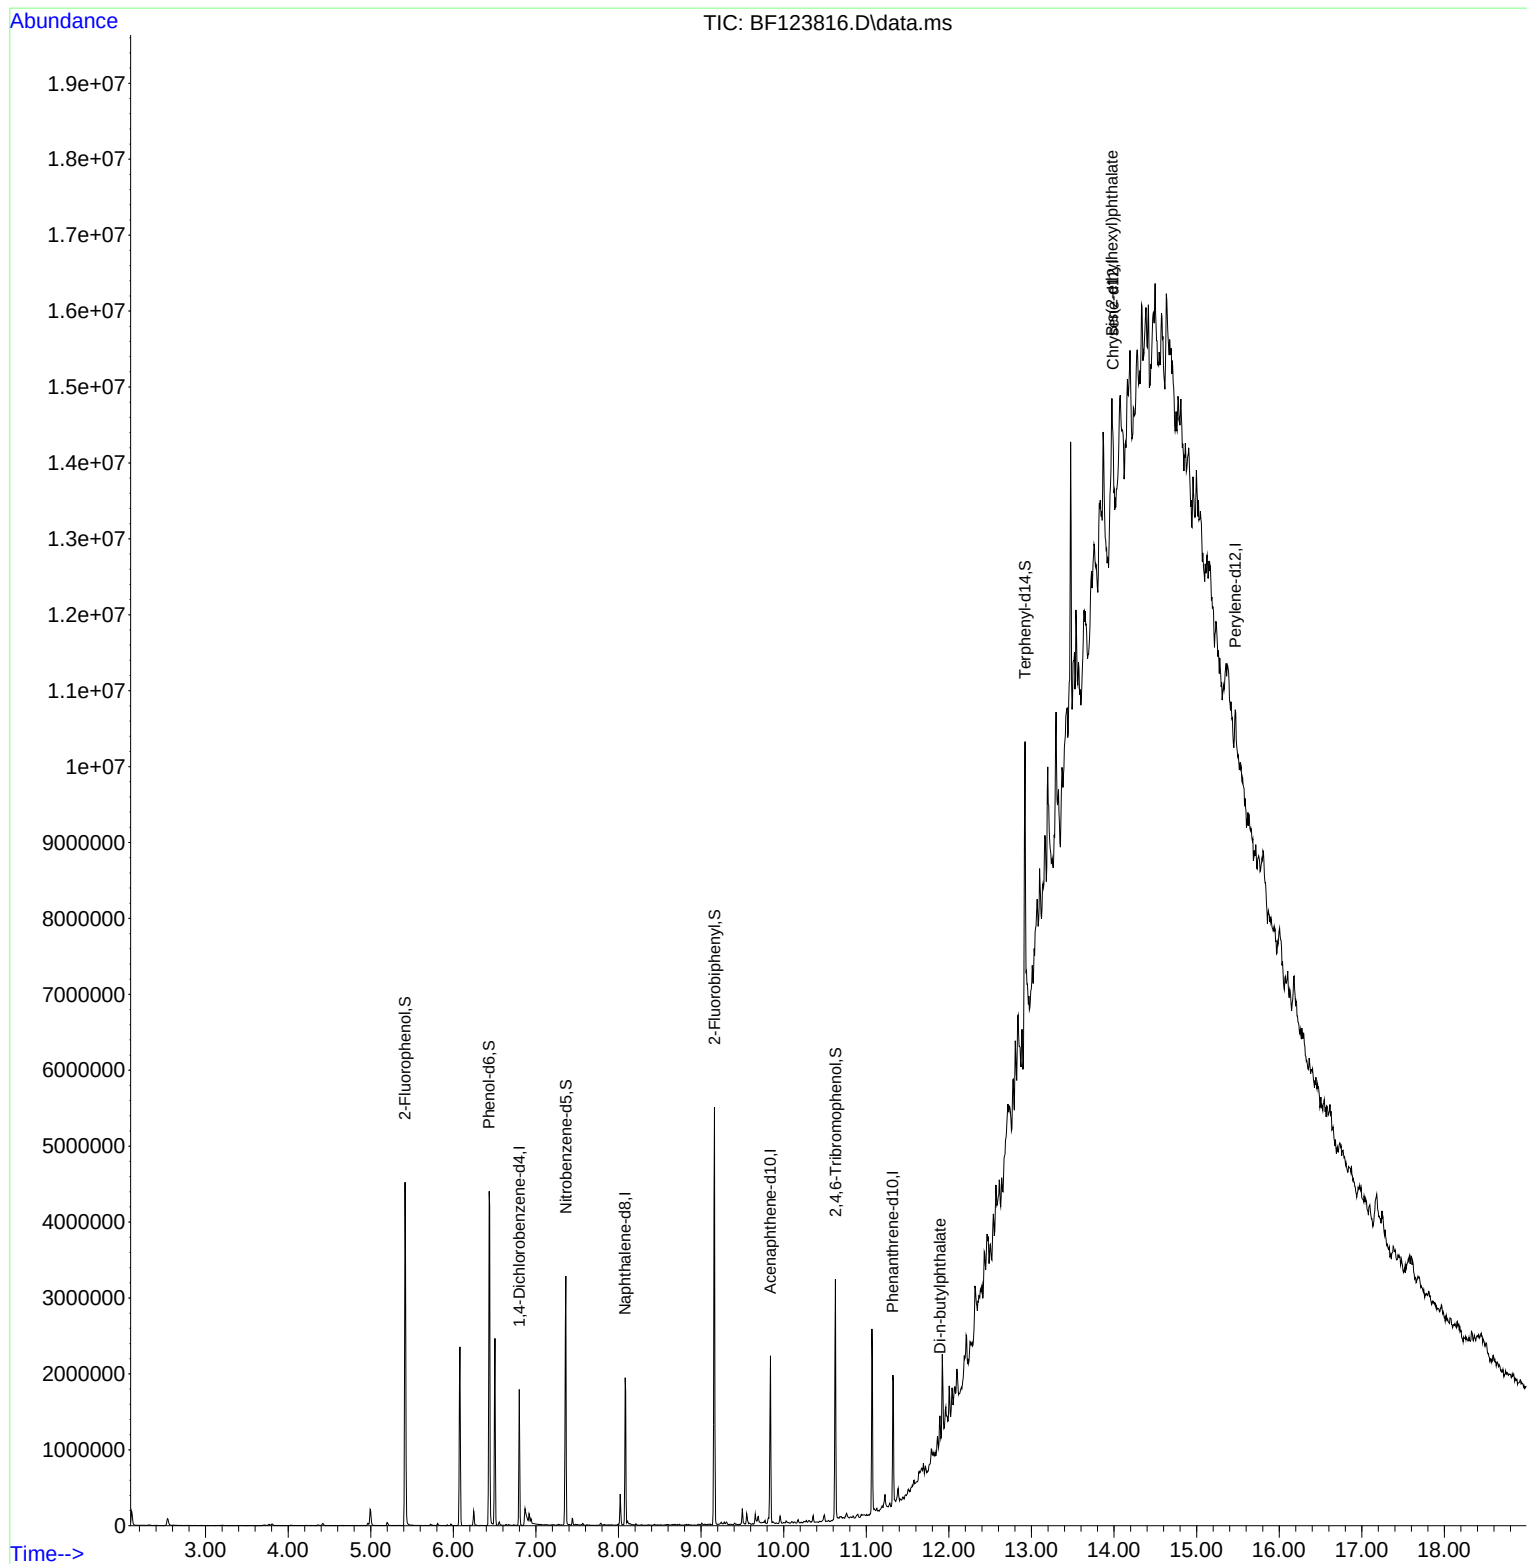


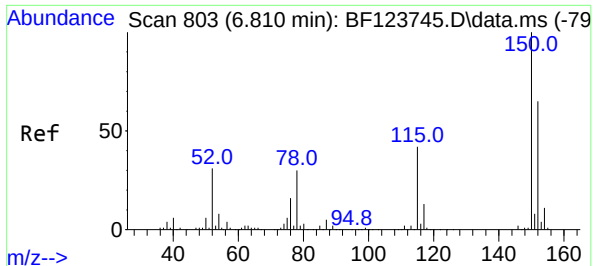

#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.798 min Scan# 801
Delta R.T. -0.012 min
Lab File: BF123816.D
Acq: 4 May 2021 19:20




Instrument :
BNA_F
ClientSampleId :
STONE-2


Tgt Ion:152 Resp: 212190
Ion Ratio Lower Upper
152 100
150 157.3 127.0 190.6
115 64.5 54.3 81.5

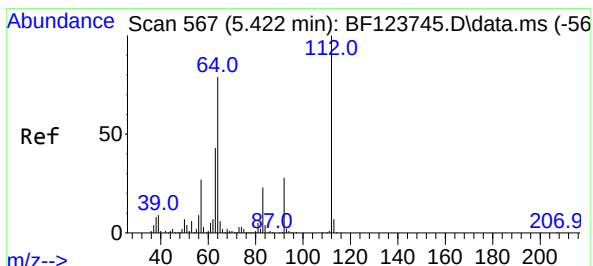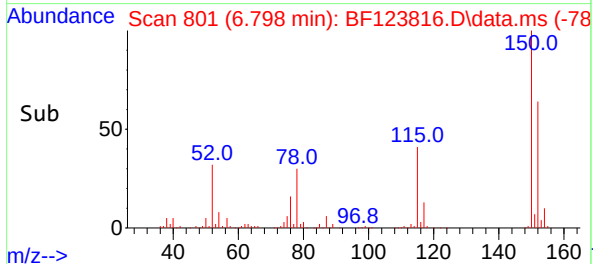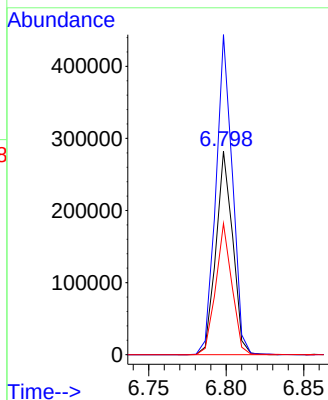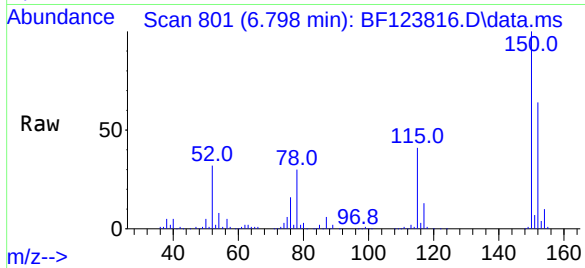

#5
2-Fluorophenol
Concen: 75.60 ng
RT: 5.416 min Scan# 566
Delta R.T. -0.006 min
Lab File: BF123816.D
Acq: 4 May 2021 19:20

Tgt Ion:112 Resp: 1012527
Ion Ratio Lower Upper
112 100
64 78.9 61.4 92.0
63 43.4 33.0 49.4


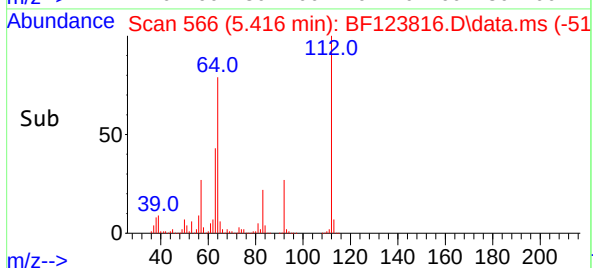
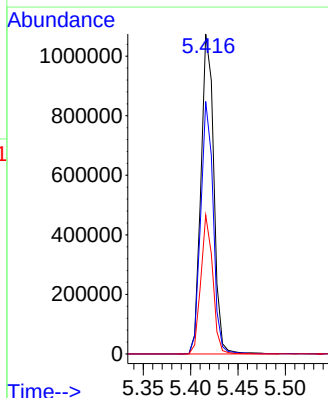
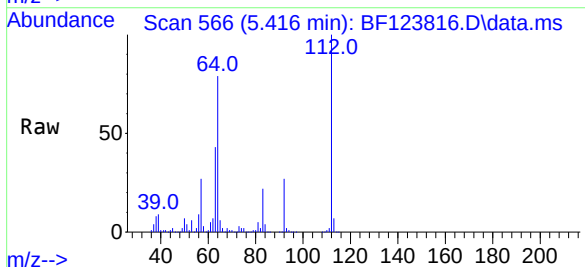




#7
Phenol-d6
Concen: 72.44 ng
RT: 6.434 min Scan# 739
Delta R.T. -0.012 min
Lab File: BF123816.D
Acq: 4 May 2021 19:20




Instrument :
BNA_F
ClientSampleId :
STONE-2


Tgt Ion: 99 Resp: 1336467
Ion Ratio Lower Upper
99 100
42 25.0 19.8 29.8
71 39.3 31.1 46.7

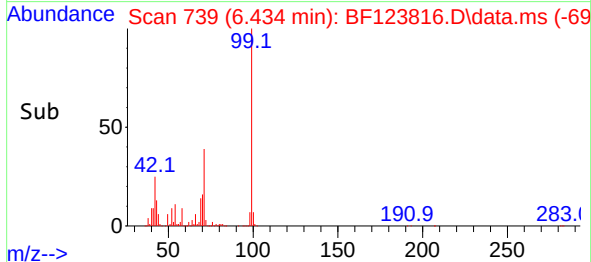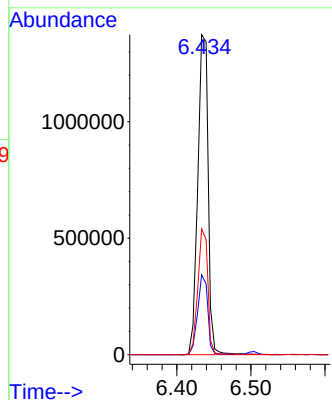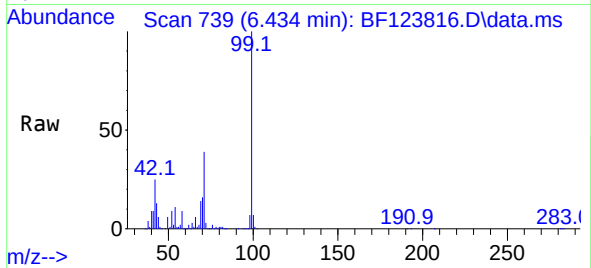

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.080 min Scan# 1019
Delta R.T. -0.018 min
Lab File: BF123816.D
Acq: 4 May 2021 19:20

Tgt Ion: 136 Resp: 783446
Ion Ratio Lower Upper
136 100
137 11.5 8.7 13.1
54 12.9 9.8 14.6
68 6.0 4.1 6.1


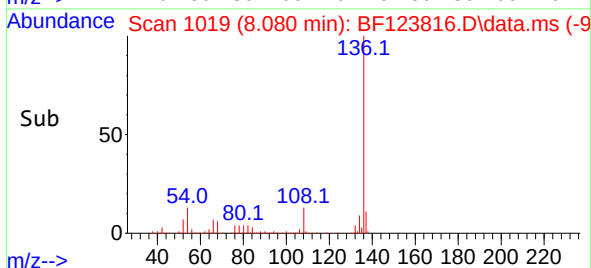
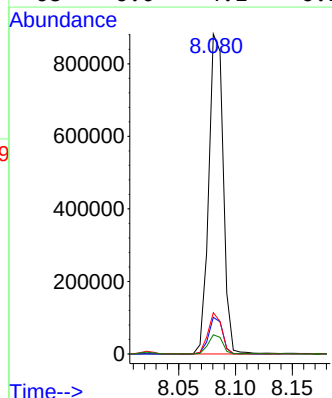
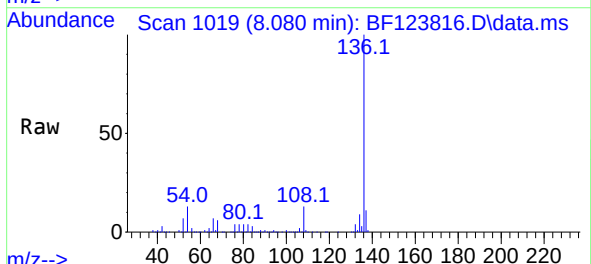




#23
Nitrobenzene-d5
Concen: 53.58 ng
RT: 7.363 min Scan# 897
Delta R.T. -0.012 min
Lab File: BF123816.D
Acq: 4 May 2021 19:20




Instrument :
BNA_F
ClientSampleId :
STONE-2


Tgt Ion: 82 Resp: 929953
Ion Ratio Lower Upper
82 100
128 39.7 29.4 44.2
54 64.6 54.1 81.1

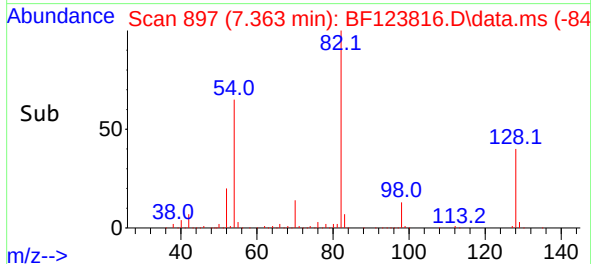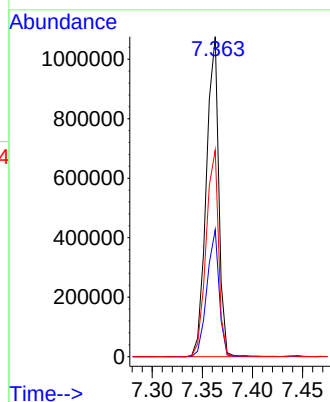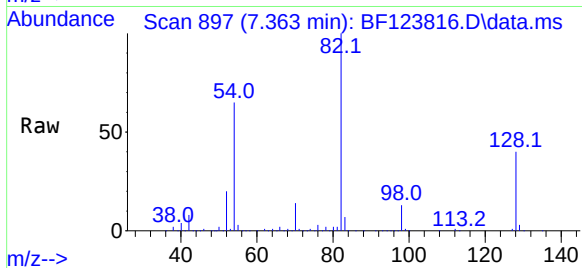

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.839 min Scan# 1318
Delta R.T. -0.012 min
Lab File: BF123816.D
Acq: 4 May 2021 19:20

Tgt Ion:164 Resp: 374472
Ion Ratio Lower Upper
164 100
162 99.8 80.7 121.1
160 43.9 37.3 55.9


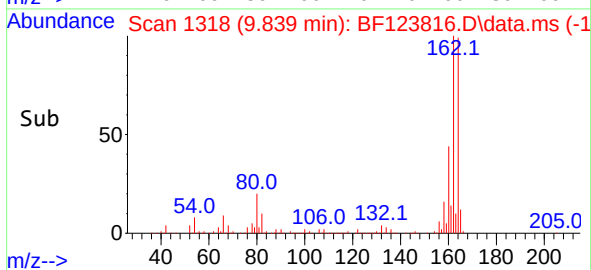
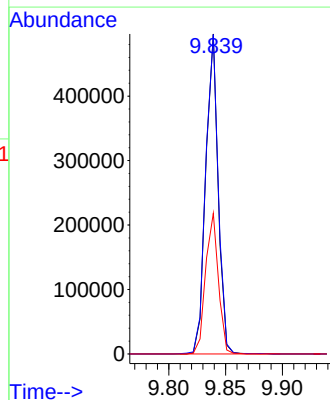
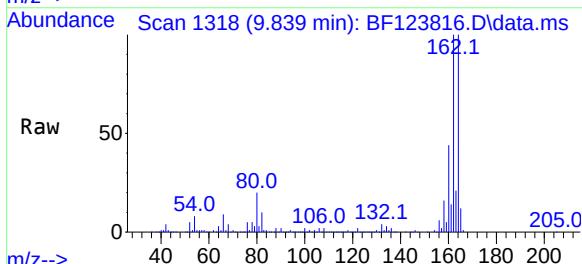


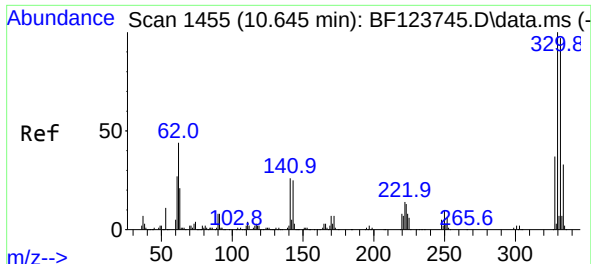

#42
2,4,6-Tribromophenol
Concen: 72.03 ng
RT: 10.627 min Scan# 1452
Delta R.T. -0.018 min
Lab File: BF123816.D
Acq: 4 May 2021 19:20




Instrument :
BNA_F
ClientSampleId :
STONE-2


Tgt Ion:330 Resp: 335770
Ion Ratio Lower Upper
330 100
332 95.4 77.1 115.7
141 32.5 27.9 41.9

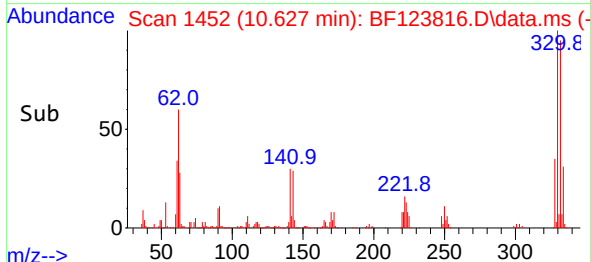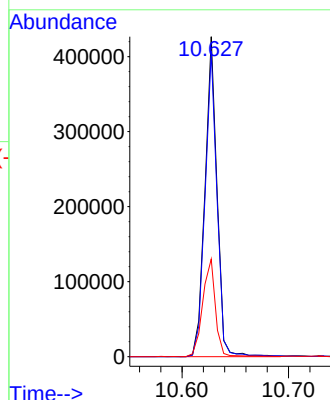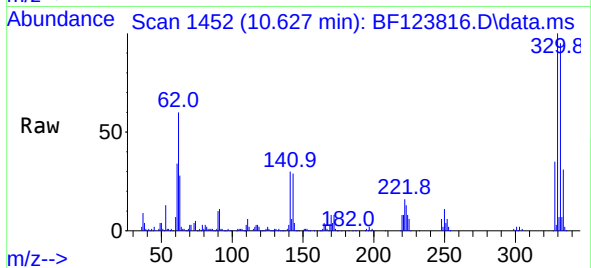

#45
2-Fluorobiphenyl
Concen: 56.77 ng
RT: 9.163 min Scan# 1203
Delta R.T. -0.012 min
Lab File: BF123816.D
Acq: 4 May 2021 19:20

Tgt Ion:172 Resp: 1459670
Ion Ratio Lower Upper
172 100
171 35.0 28.1 42.1
170 23.5 19.2 28.8

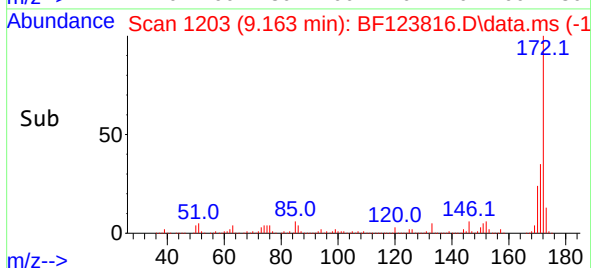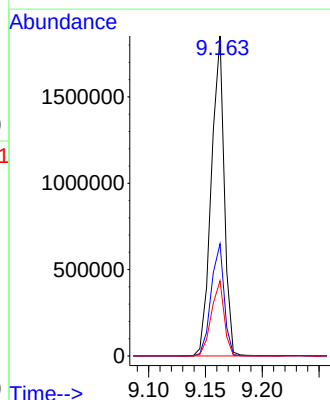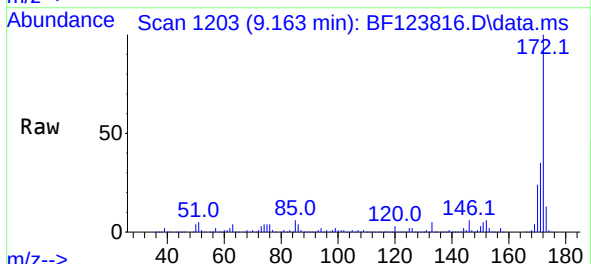







#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.321 min Scan# 1570
Delta R.T. -0.018 min
Lab File: BF123816.D
Acq: 4 May 2021 19:20

Instrument :
BNA_F
ClientSampleId :
STONE-2

Tgt Ion:188 Resp: 626743




Ion	Ratio	Lower	Upper
188	100		
94	10.2	6.9	10.3
80	11.0	8.2	12.2

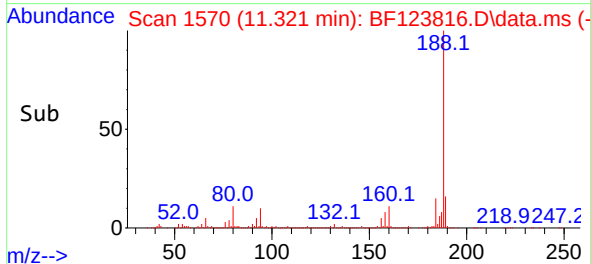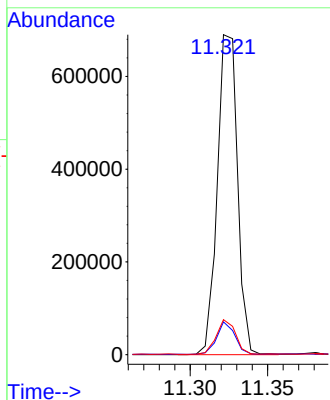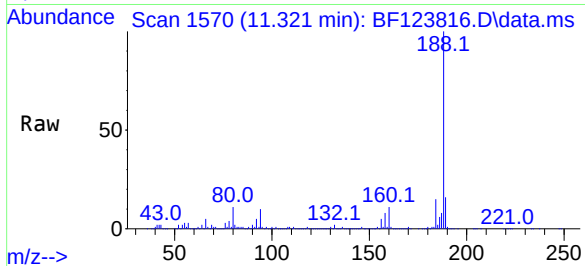


#74
Di-n-butylphthalate
Concen: 4.20 ng
RT: 11.892 min Scan# 1667
Delta R.T. -0.012 min
Lab File: BF123816.D
Acq: 4 May 2021 19:20

Tgt Ion:149 Resp: 155654

Ion	Ratio	Lower	Upper
149	100		
150	8.6	7.8	11.8
104	5.3	4.6	6.8


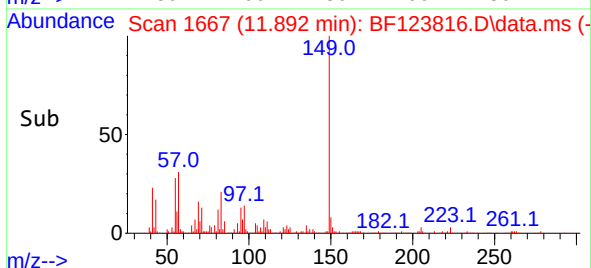
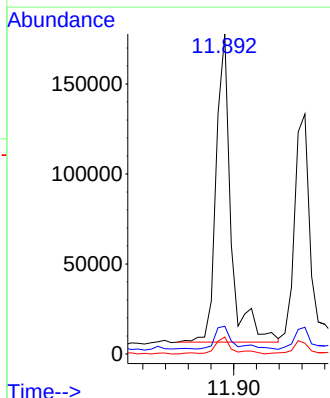
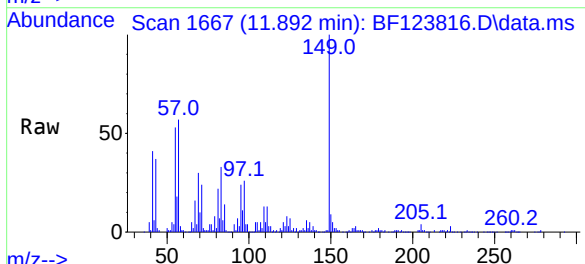




#76
Chrysene-d12
Concen: 20.00 ng
RT: 13.986 min Scan# 2023
Delta R.T. -0.000 min
Lab File: BF123816.D
Acq: 4 May 2021 19:20




Instrument :
BNA_F
ClientSampleId :
STONE-2


Tgt Ion:240 Resp: 360216
Ion Ratio Lower Upper
240 100
120 12.0 7.2 10.8#
236 24.7 19.0 28.4

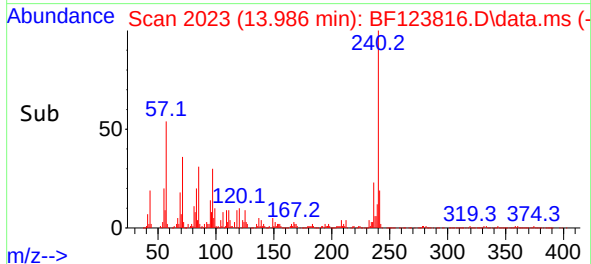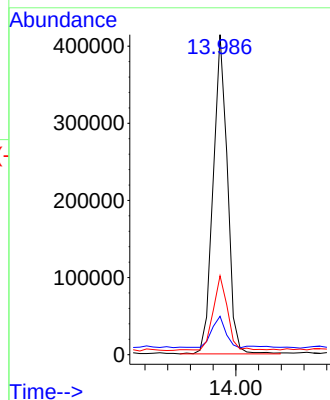

#79
Terphenyl-d14
Concen: 58.59 ng
RT: 12.921 min Scan# 1842
Delta R.T. -0.006 min
Lab File: BF123816.D
Acq: 4 May 2021 19:20

Tgt Ion:244 Resp: 1096096
Ion Ratio Lower Upper
244 100
212 6.6 5.7 8.5
122 9.9 9.7 14.5


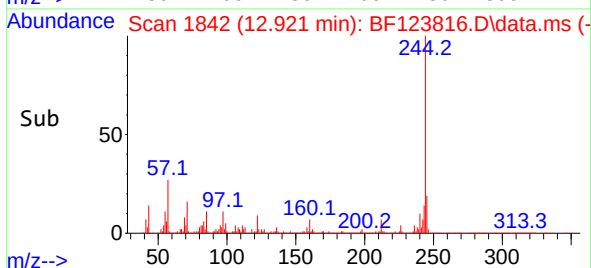
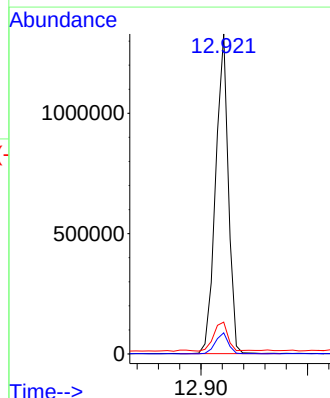
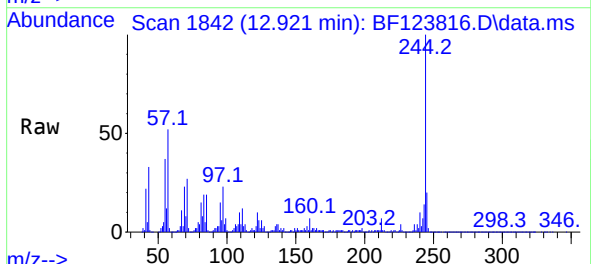




#84
Bis(2-ethylhexyl)phthalate
Concen: 23.88 ng
RT: 13.974 min Scan# 2021
Delta R.T. 0.012 min
Lab File: BF123816.D
Acq: 4 May 2021 19:20

Instrument :
BNA_F
ClientSampleId :
STONE-2

Tgt Ion:149 Resp: 354298
Ion Ratio Lower Upper
149 100
167 27.8 21.8 32.6
279 4.7 3.3 4.9

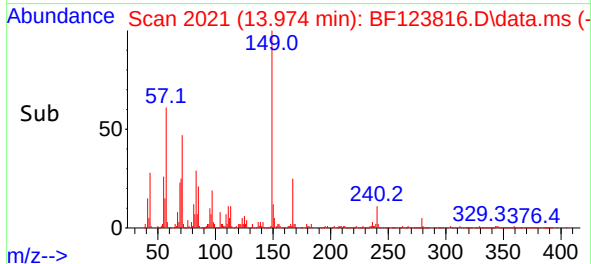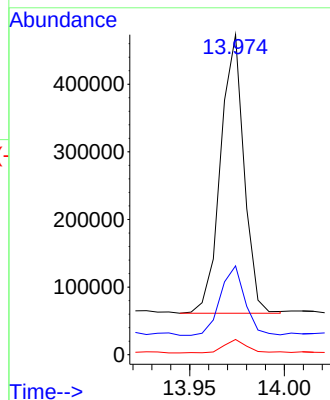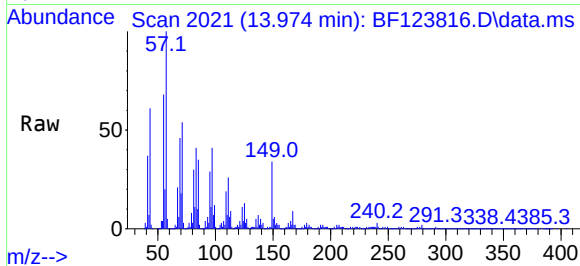

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.468 min Scan# 2275
Delta R.T. 0.029 min
Lab File: BF123816.D
Acq: 4 May 2021 19:20

Tgt Ion:264 Resp: 360193
Ion Ratio Lower Upper
264 100
260 23.9 18.7 28.1
265 21.3 17.8 26.8

