

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050421\
 Data File : BF123806.D
 Acq On : 4 May 2021 13:52
 Operator : JU/CG
 Sample : PB136158BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB136158BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123806.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.110	3	4	10	rVB	289612	253246	2.97%	0.436%
2	2.216	17	22	29	rVB	342813	428637	5.02%	0.738%
3	5.028	492	500	510	rBV	361688	504443	5.91%	0.869%
4	5.434	564	569	572	rBV	8520235	8123079	95.21%	13.989%
5	6.439	735	740	743	rBV	7065488	8275870	97.00%	14.252%
6	6.798	797	801	805	rBV	2014329	1569022	18.39%	2.702%
7	7.363	891	897	900	rBV	4884569	5471099	64.13%	9.422%
8	8.081	1014	1019	1023	rBV	2082309	2006029	23.51%	3.455%
9	9.163	1197	1203	1206	rBV	8760016	8136834	95.37%	14.012%
10	9.839	1313	1318	1321	rBV	2572552	2109303	24.72%	3.632%
11	10.633	1447	1453	1456	rBV	5521737	5513970	64.63%	9.495%
12	11.327	1566	1571	1574	rBV	2616098	2245992	26.33%	3.868%
13	12.921	1836	1842	1845	rBV	9007745	8531588	100.00%	14.692%
14	13.839	1994	1998	2003	rVB	121370	142090	1.67%	0.245%
15	13.968	2016	2020	2023	rBV	2361943	1961593	22.99%	3.378%
16	14.745	2146	2152	2156	rBV	86602	91984	1.08%	0.158%
17	15.080	2205	2209	2215	rVB	138021	163535	1.92%	0.282%
18	15.421	2262	2267	2271	rBV	1361186	1662757	19.49%	2.863%
19	15.457	2271	2273	2280	rVB	162746	184731	2.17%	0.318%
20	15.886	2340	2346	2352	rBV	155839	237820	2.79%	0.410%
21	16.386	2425	2431	2436	rBV2	116655	221458	2.60%	0.381%
22	16.968	2523	2530	2537	rVB2	78739	148103	1.74%	0.255%
23	17.651	2642	2646	2652	rVB2	41843	86354	1.01%	0.149%




Sum of corrected areas: 58069537

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050421\
Data File : BF123806.D
Acq On : 4 May 2021 13:52
Operator : JU/CG
Sample : PB136158BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136158BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

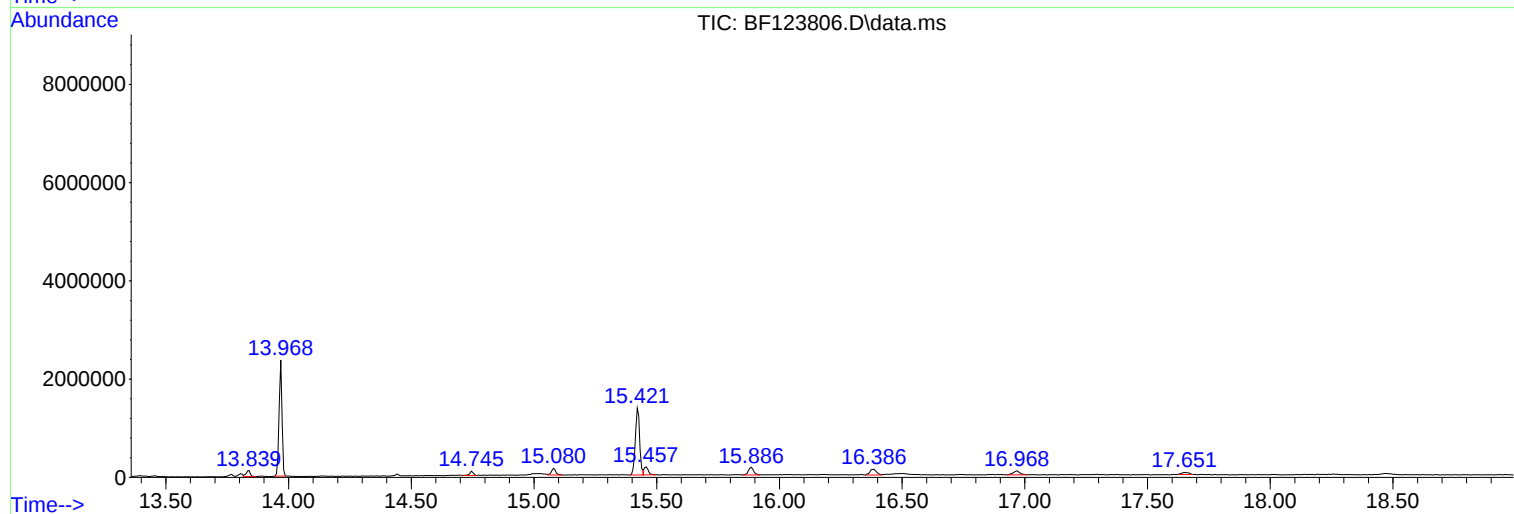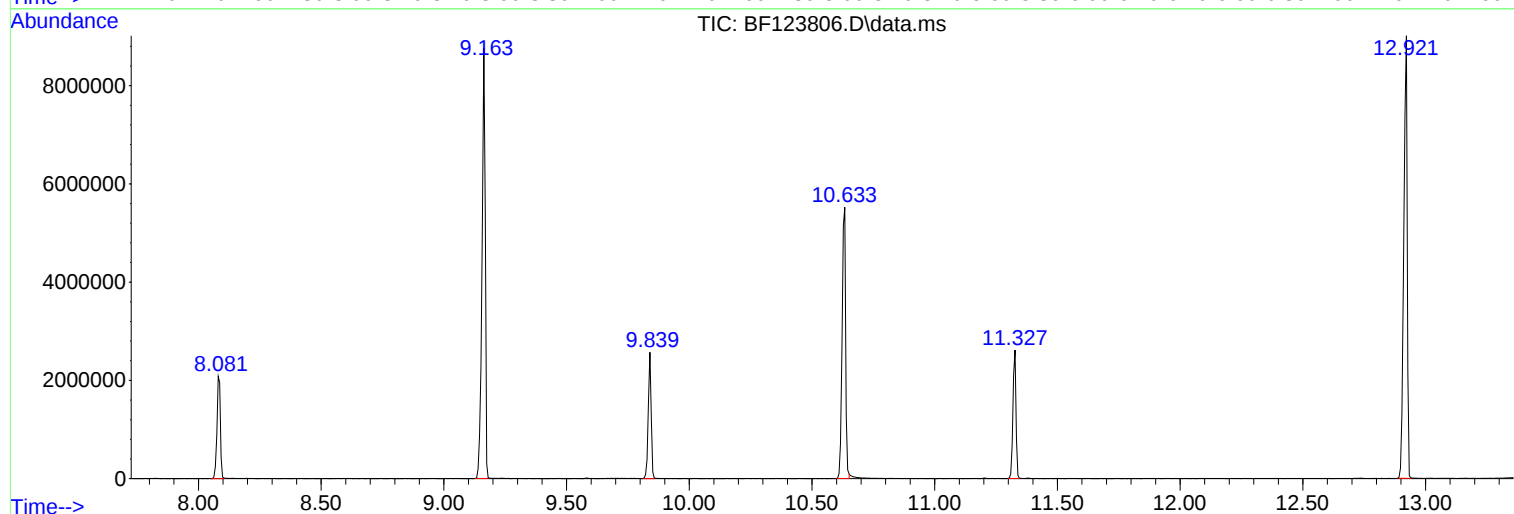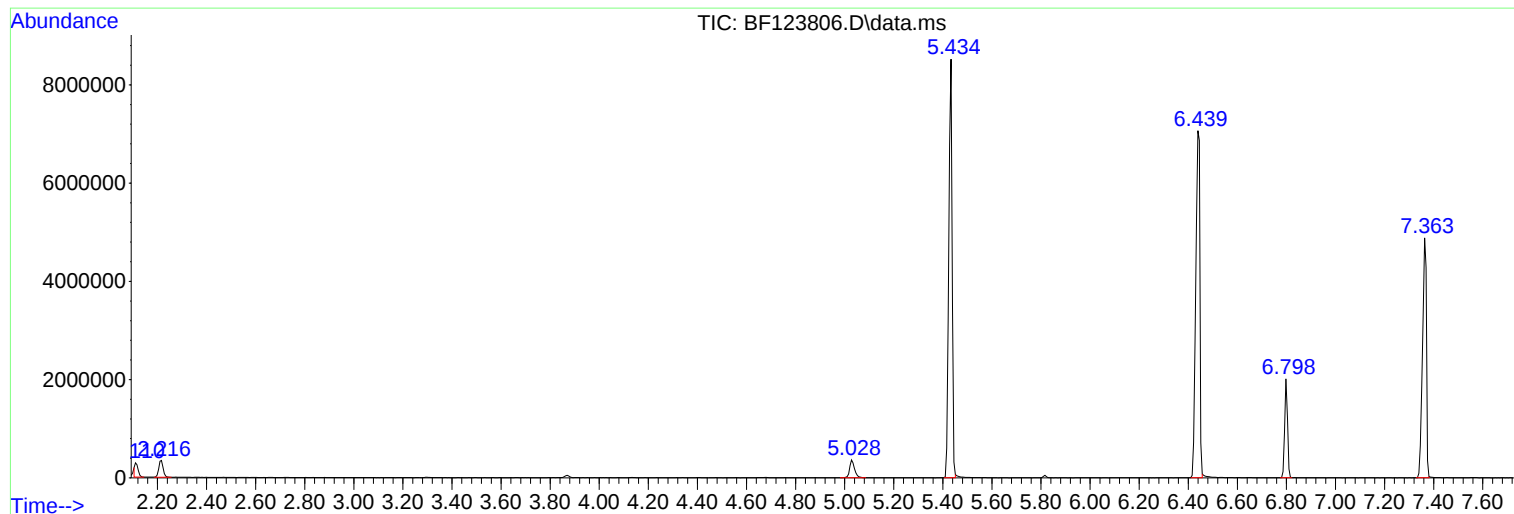

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050421\
Data File : BF123806.D
Acq On : 4 May 2021 13:52
Operator : JU/CG
Sample : PB136158BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136158BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050421\
Data File : BF123806.D
Acq On : 4 May 2021 13:52
Operator : JU/CG
Sample : PB136158BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136158BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------