


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050421\
 Data File : BF123802.D
 Acq On : 4 May 2021 11:42
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 04 12:58:27 2021

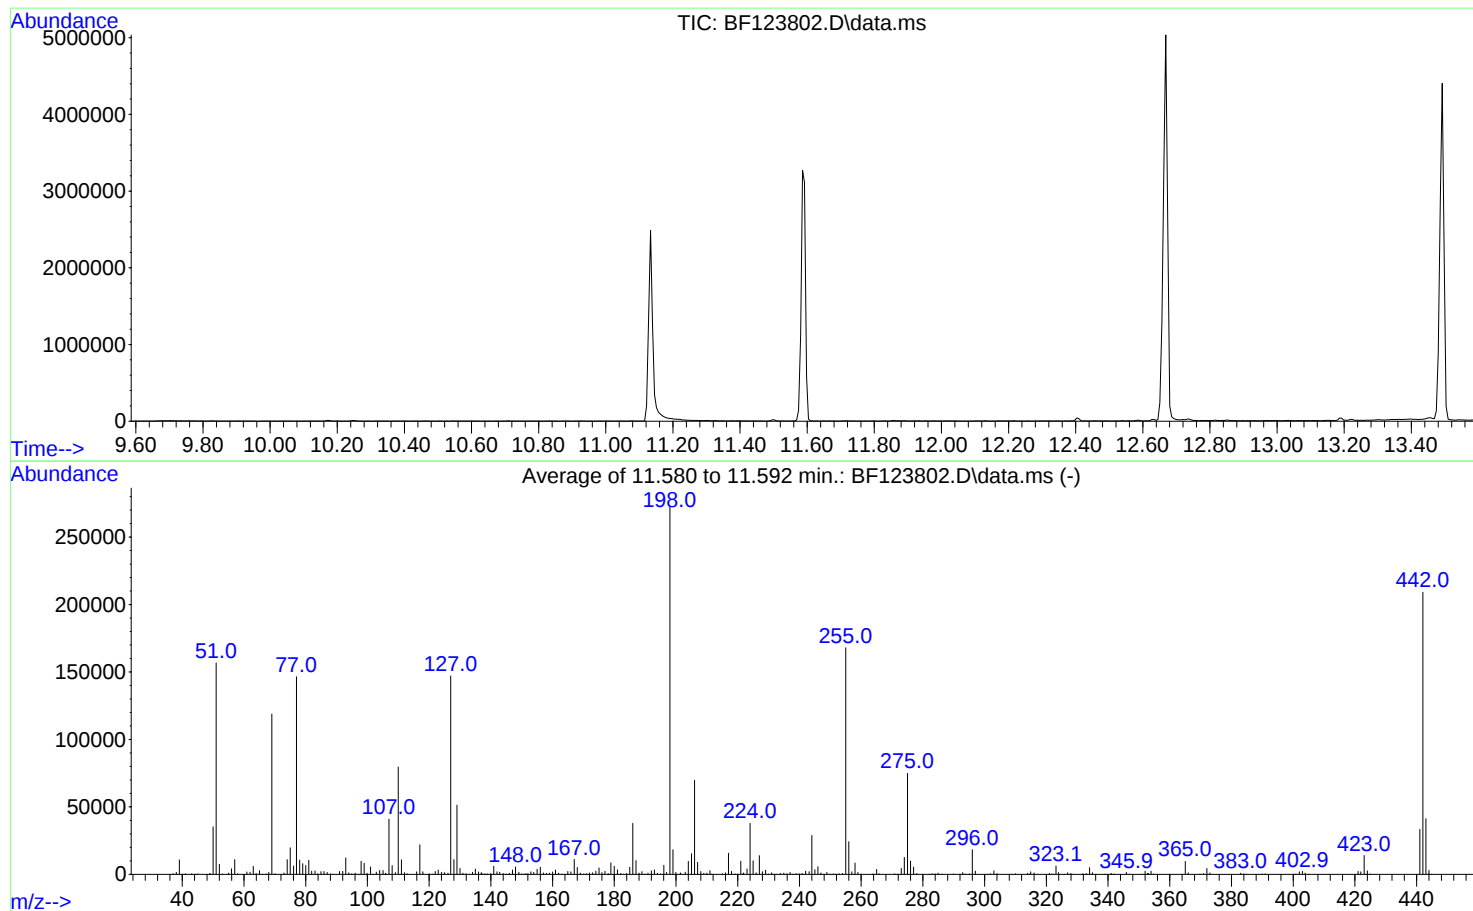




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.5	156672	PASS
68	69	0.00	2	1.2	1426	PASS
69	198	0.00	100	43.6	118787	PASS
70	69	0.00	2	0.4	517	PASS
127	198	10	80	53.9	147053	PASS
197	198	0.00	2	0.5	1479	PASS
198	198	100	100	100.0	272653	PASS
199	198	5	9	6.7	18216	PASS
275	198	10	60	27.4	74832	PASS
365	198	1	100	3.5	9677	PASS
441	198	0.01	100	12.2	33292	PASS
442	442	50	100	100.0	209040	PASS
443	442	15	24	19.7	41273	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050421\  
Data File : BF123802.D  
Acq On    : 4 May 2021 11:42  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 04 12:26:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 16:30:39 2021
Response via : Initial Calibration

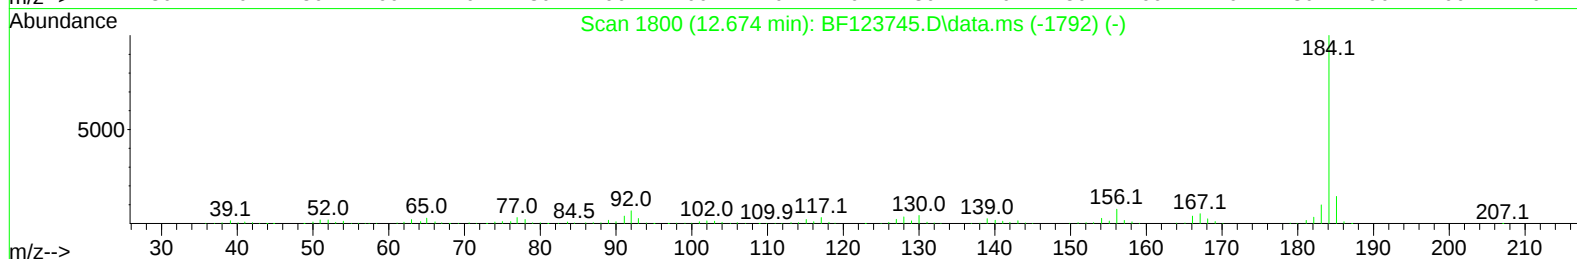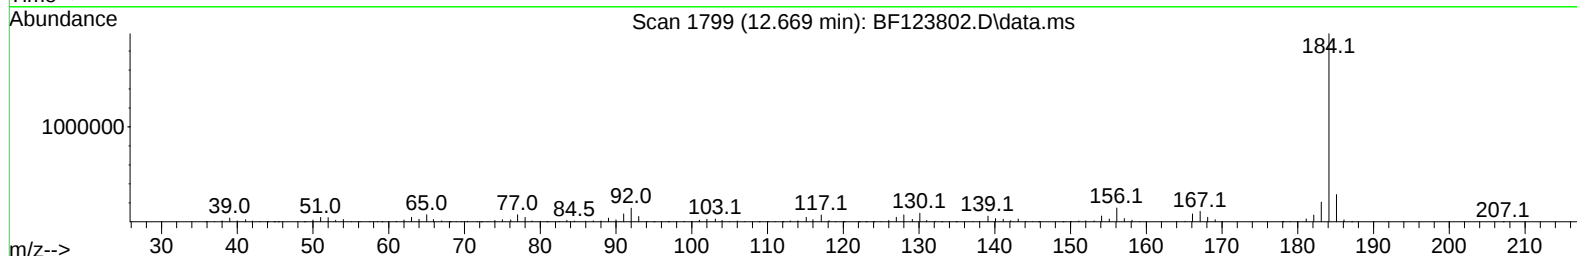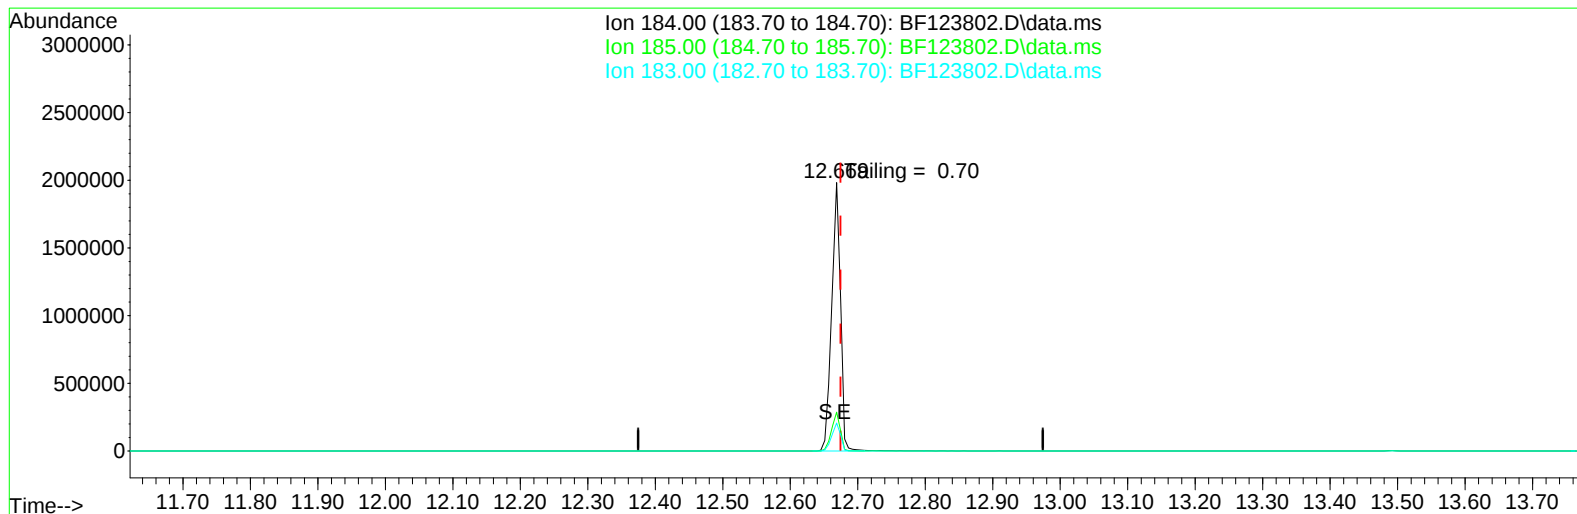

TIC: BF123802.D\data.ms

(77) Benzidine

12.669min (-0.006) 0.00 ng




response **1800395**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.49
183.00	9.80	10.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050421\
Data File : BF123802.D
Acq On : 4 May 2021 11:42
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 04 12:26:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 16:30:39 2021
Response via : Initial Calibration

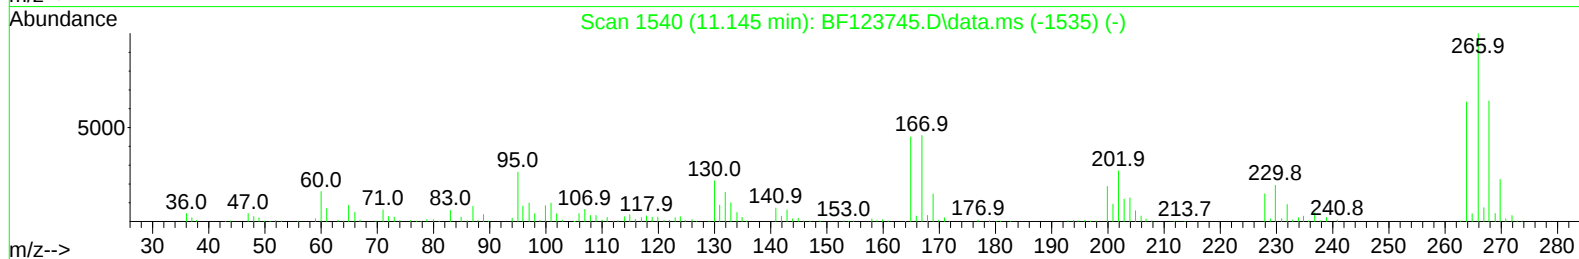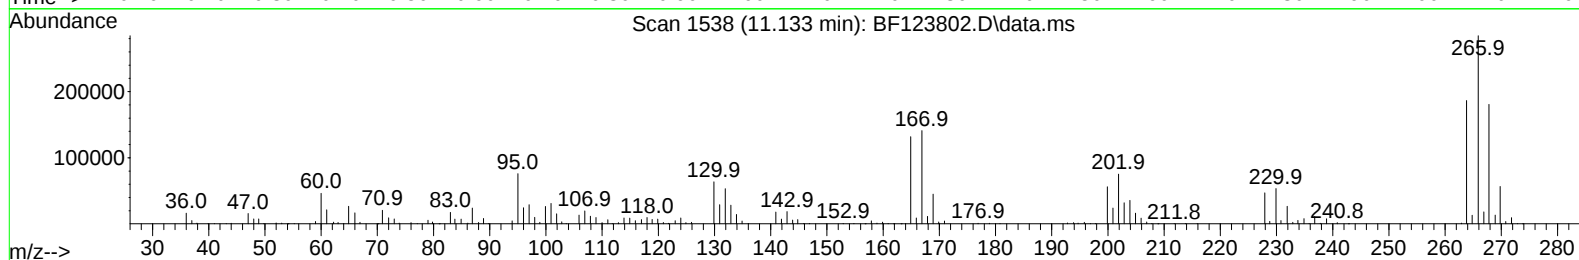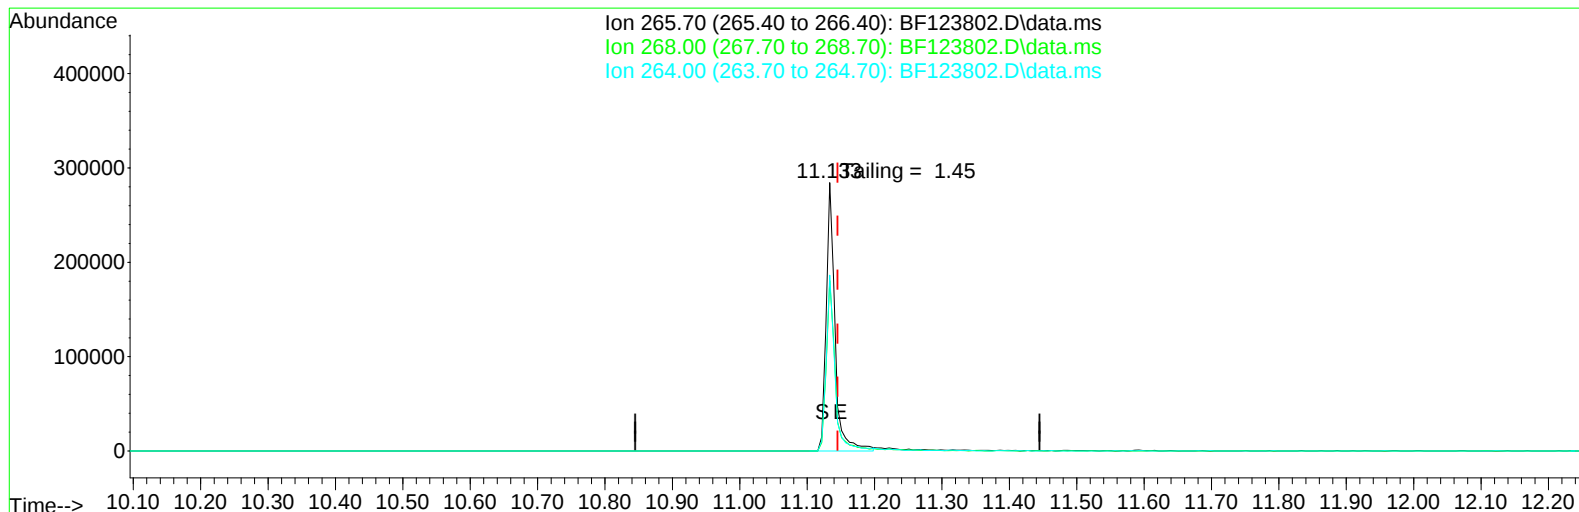

TIC: BF123802.D\data.ms

(70) Pentachlorophenol (C)

11.133min (-0.012) 42296.97 ng

response 265884

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.50
264.00	65.70	65.55
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/4/2021	BNA_F	<u>BF123802.D</u>
Compound Name	Response	Retention Time
DDT	712952	13.49
DDD	6068	13.19
DDE	1011	12.85
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7079	720031	0.98

Instrument :
BNA_F
ClientSampleId :
DFTPP