
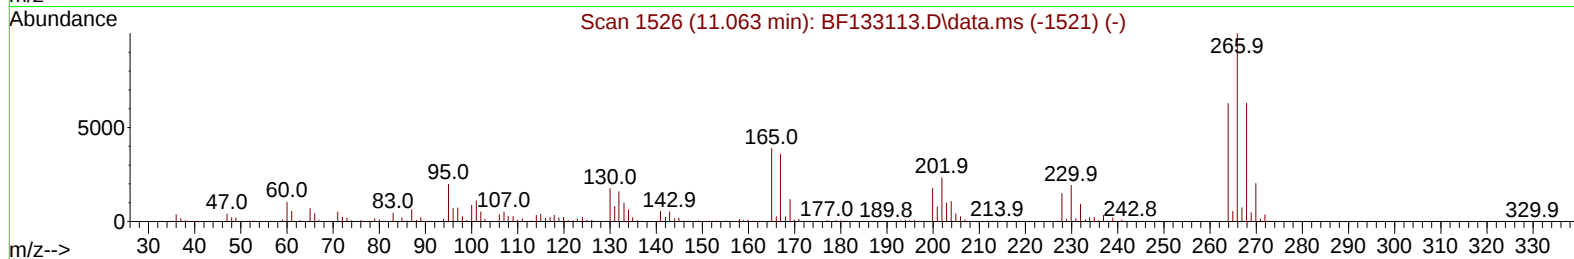
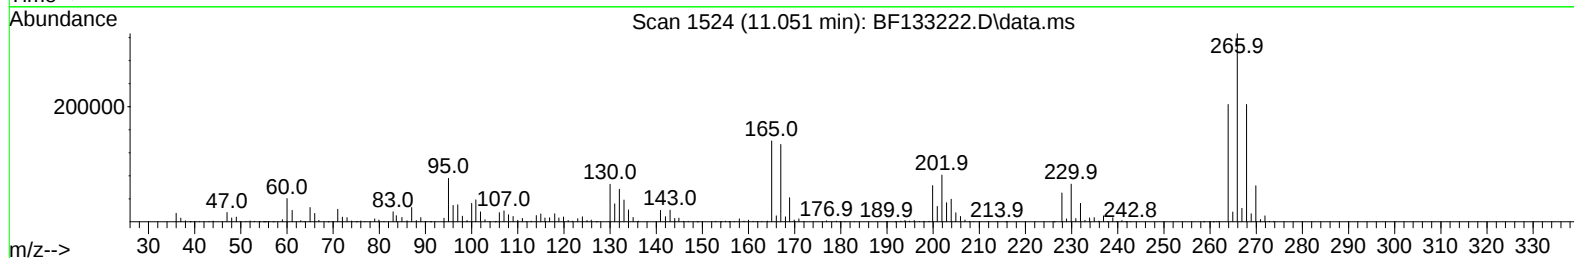


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF050423\  
Data File : BF133222.D  
Acq On : 04 May 2023 10:06  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 14:28:21 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu May 04 12:22:53 2023  
Response via : Initial Calibration

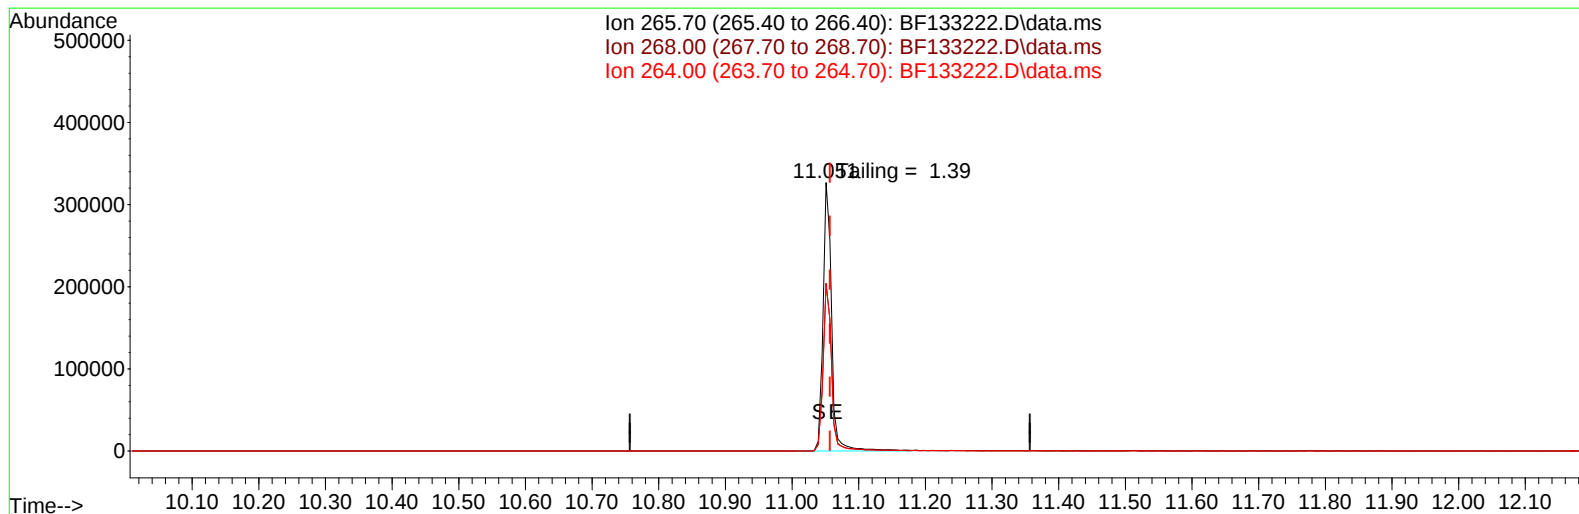

TIC: BF133222.D\data.ms

**(70) Pentachlorophenol (C)**




**11.051min (-0.006) 64197.69 ng**

**response 291658**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.00  | 62.42  |
| 264.00 | 63.30  | 62.38  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF050423\  
Data File : BF133222.D  
Acq On : 04 May 2023 10:06  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 14:28:21 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu May 04 12:22:53 2023  
Response via : Initial Calibration

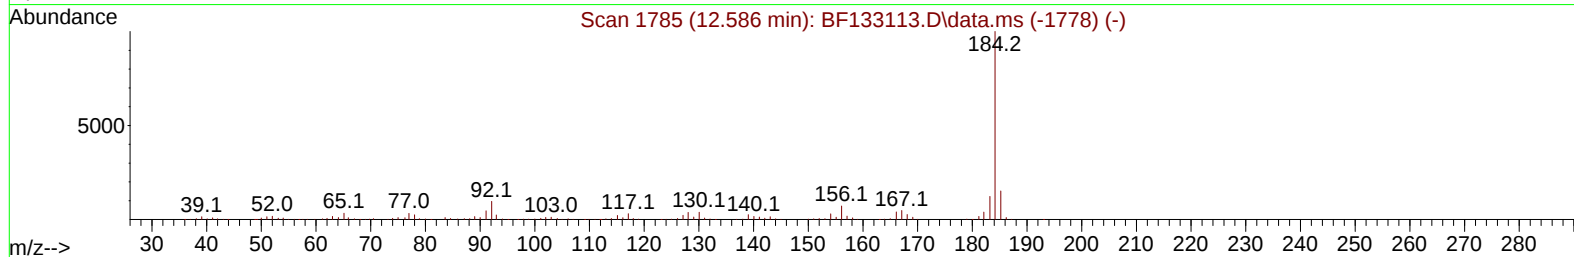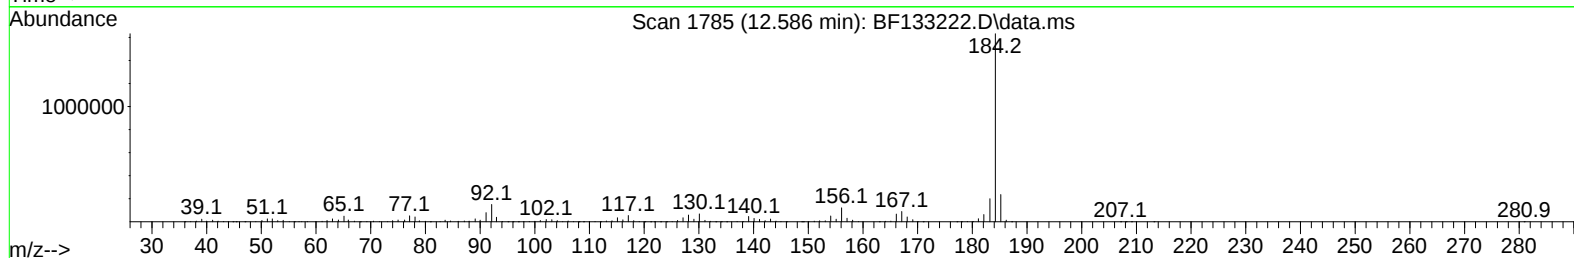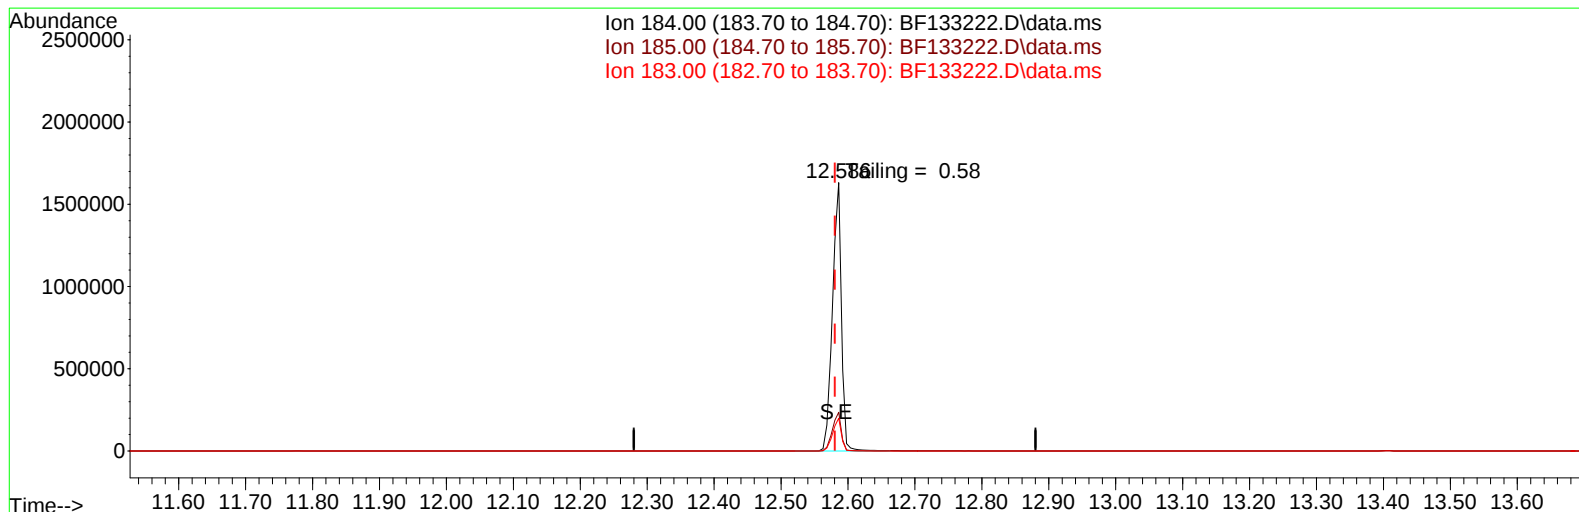

TIC: BF133222.D\data.ms

**(77) Benzidine**

12.586min (+ 0.006) 13454.26 ng

response 1522554

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 19.30  | 14.44# |
| 183.00 | 11.70  | 12.24  |
| 0.00   | 0.00   | 0.00   |