
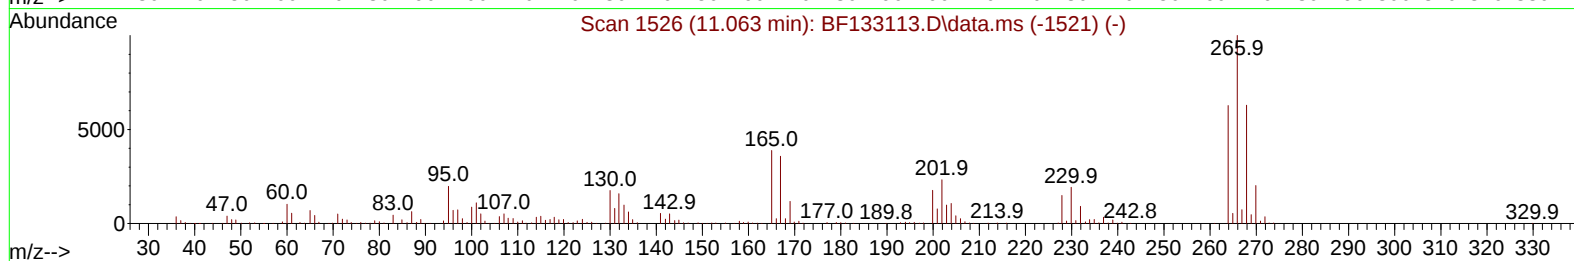
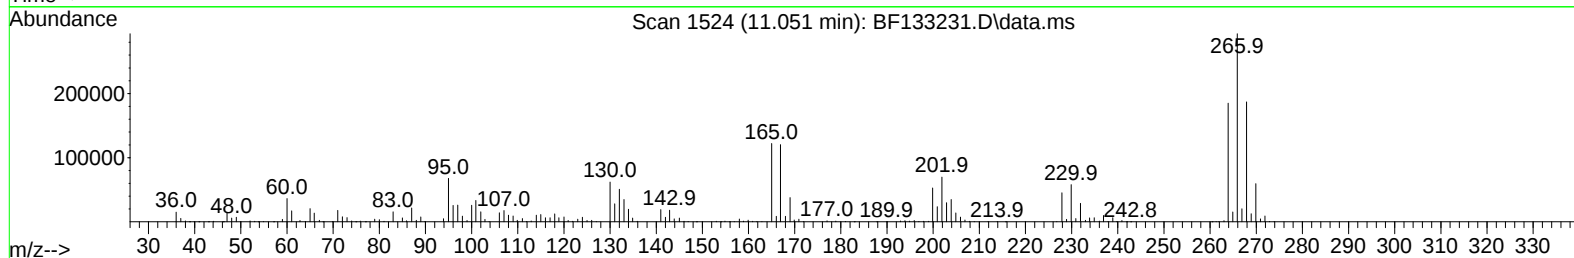


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050423\
Data File : BF133231.D
Acq On : 04 May 2023 15:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 16:01:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 04 12:22:53 2023
Response via : Initial Calibration

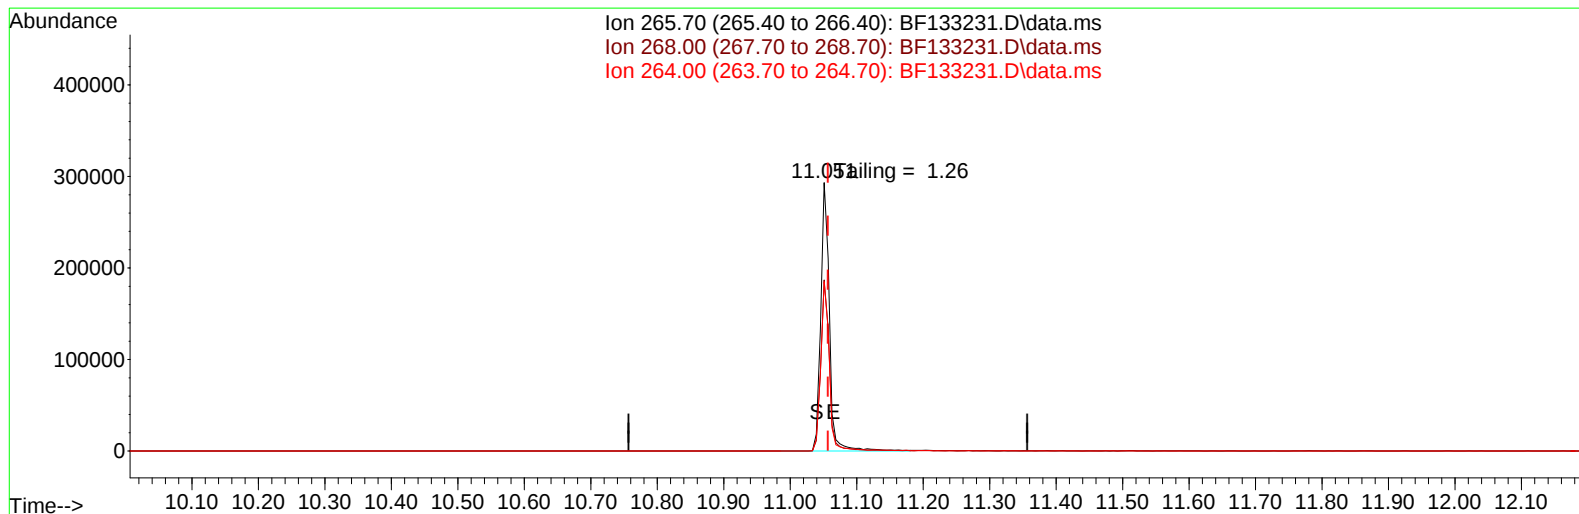

TIC: BF133231.D\data.ms

(70) Pentachlorophenol (C)




11.051min (-0.006) 137742.36 ng

response 264921

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.75
264.00	63.30	63.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050423\
Data File : BF133231.D
Acq On : 04 May 2023 15:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 16:01:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 04 12:22:53 2023
Response via : Initial Calibration

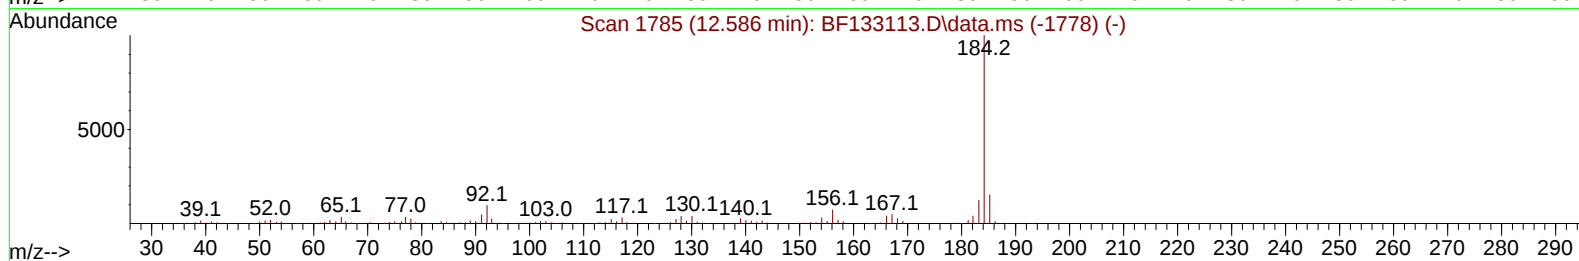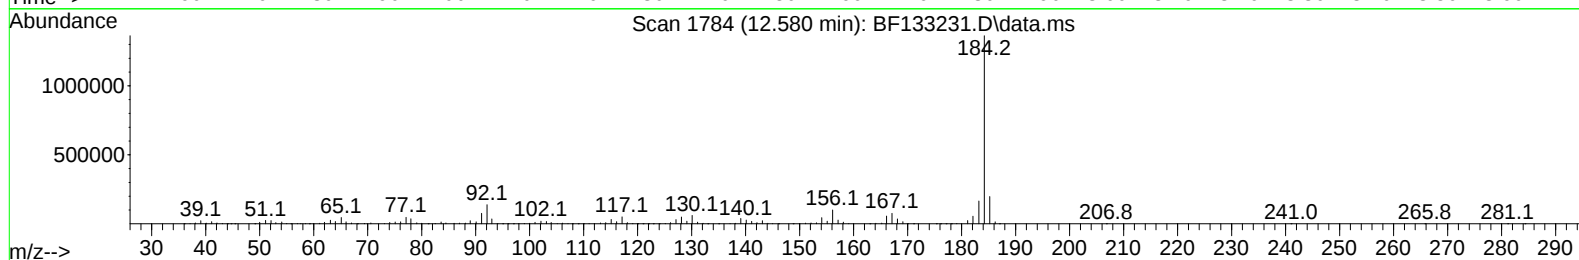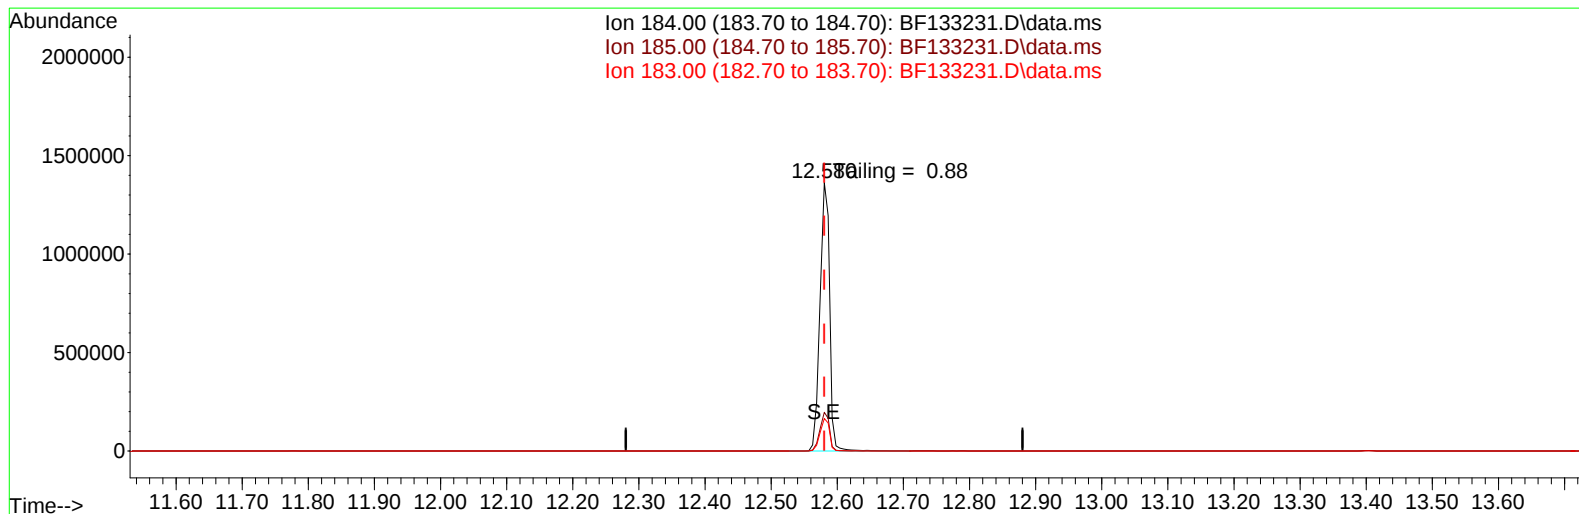

TIC: BF133231.D\data.ms

(77) Benzidine**12.580min (+ 0.000) 158822.58 ng****response 1385859**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.44#
183.00	11.70	12.12
0.00	0.00	0.00