


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050423\
Data File : BF133222.D
Acq On : 04 May 2023 10:06
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 05 10:49:34 2023

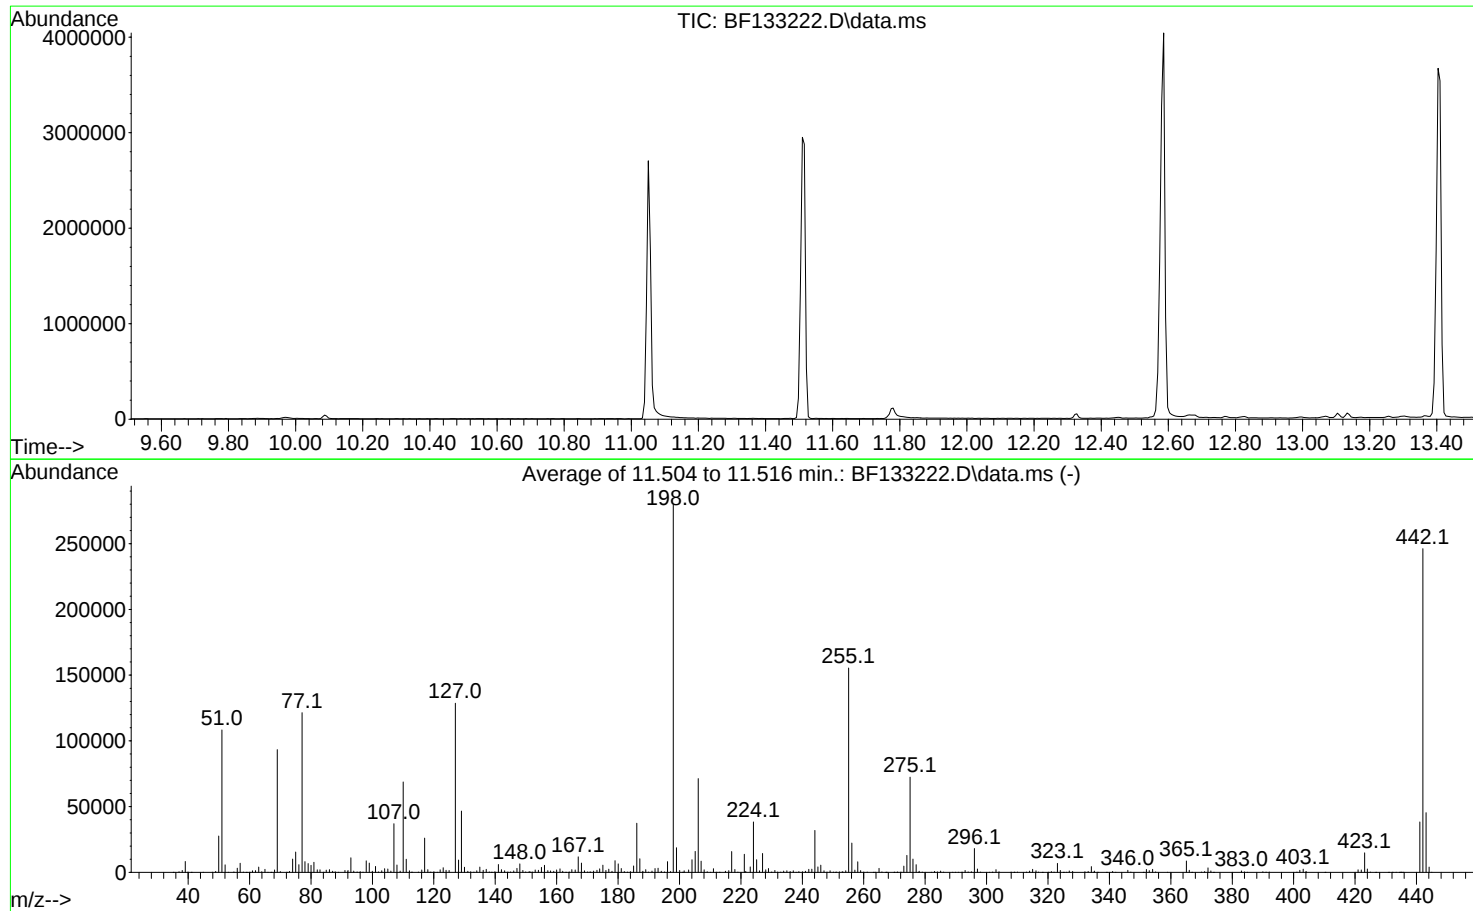

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	108257	PASS
68	69	0.00	2	1.9	1817	PASS
69	198	0.00	100	33.4	93405	PASS
70	69	0.00	2	0.6	575	PASS
127	198	10	80	46.0	128635	PASS
197	198	0.00	2	0.2	569	PASS
198	198	100	100	100.0	279787	PASS
199	198	5	9	6.7	18701	PASS
275	198	10	60	25.9	72469	PASS
365	198	1	100	3.1	8606	PASS
441	198	0.01	100	13.7	38317	PASS
442	442	50	100	100.0	246187	PASS
443	442	15	24	18.4	45402	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/4/2023	BNA_F	<u>BF133222.D</u>
Compound Name	Response	Retention Time
DDT	696617	13.41
DDD	14894	13.104
DDE	2413	12.768
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17307	713924	2.42

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050423\
Data File : BF133222.D
Acq On : 04 May 2023 10:06
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 04 14:28:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 04 12:22:53 2023
Response via : Initial Calibration

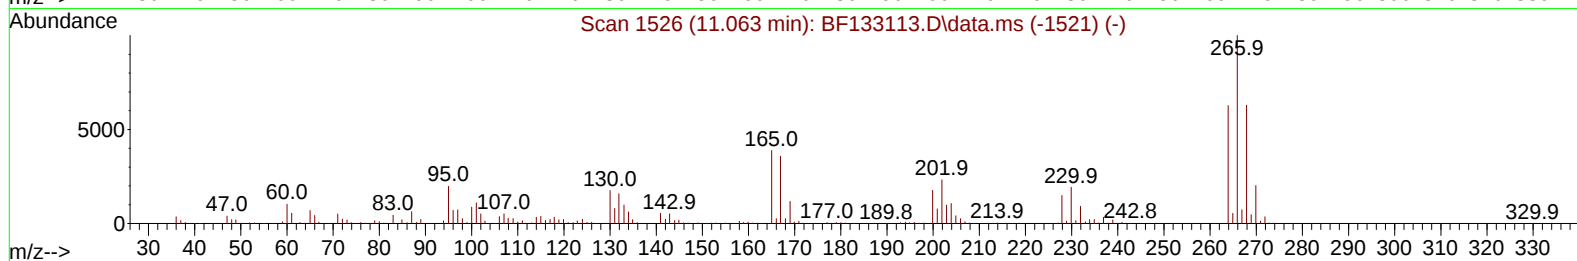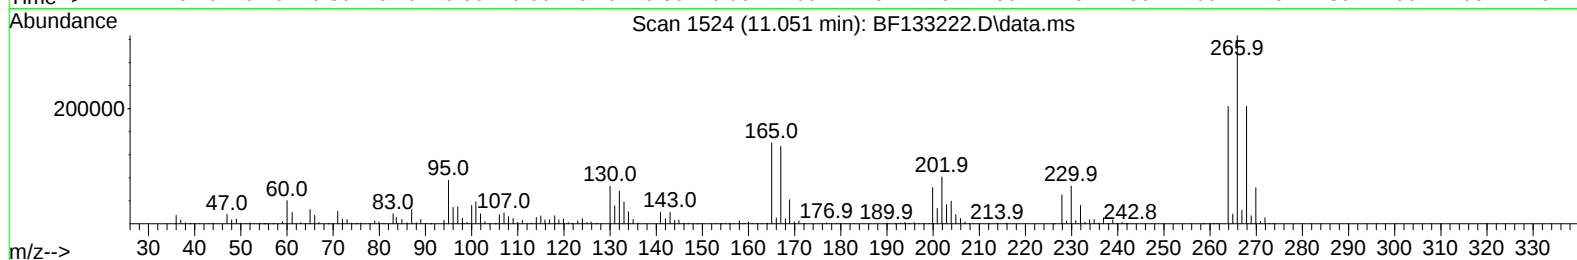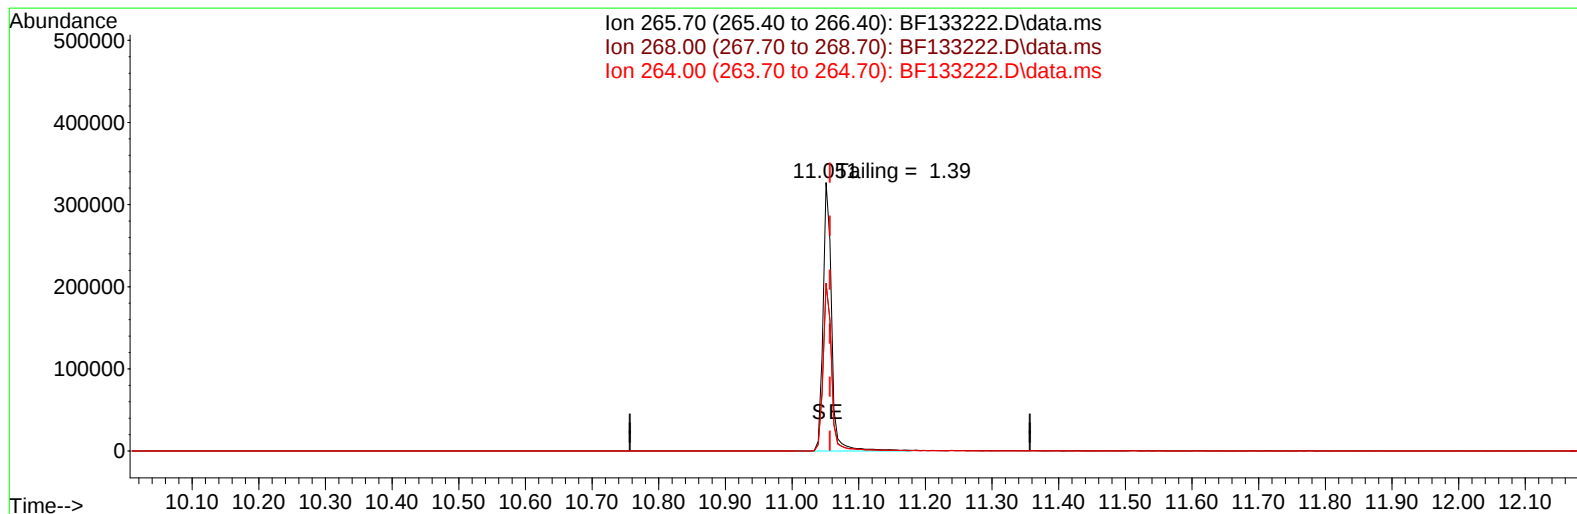

TIC: BF133222.D\data.ms

(70) Pentachlorophenol (C)

11.051min (-0.006) 64197.69 ng




response 291658

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	62.42
264.00	63.30	62.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050423\
Data File : BF133222.D
Acq On : 04 May 2023 10:06
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 04 14:28:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 04 12:22:53 2023
Response via : Initial Calibration

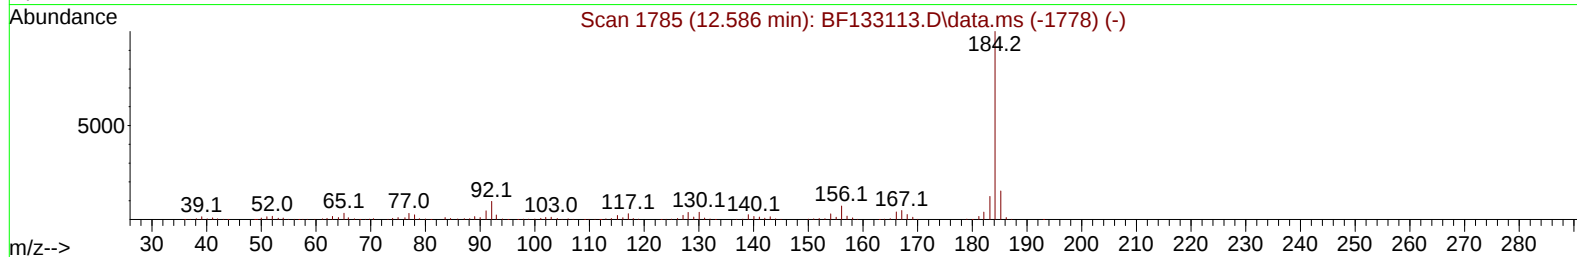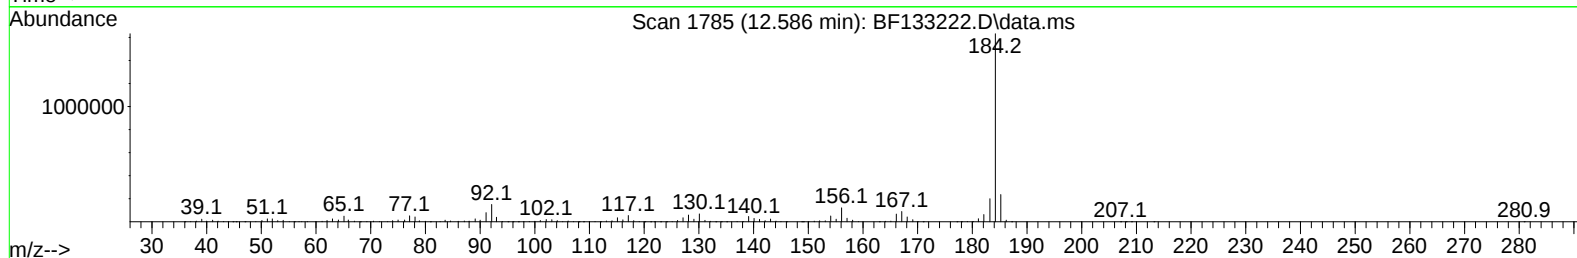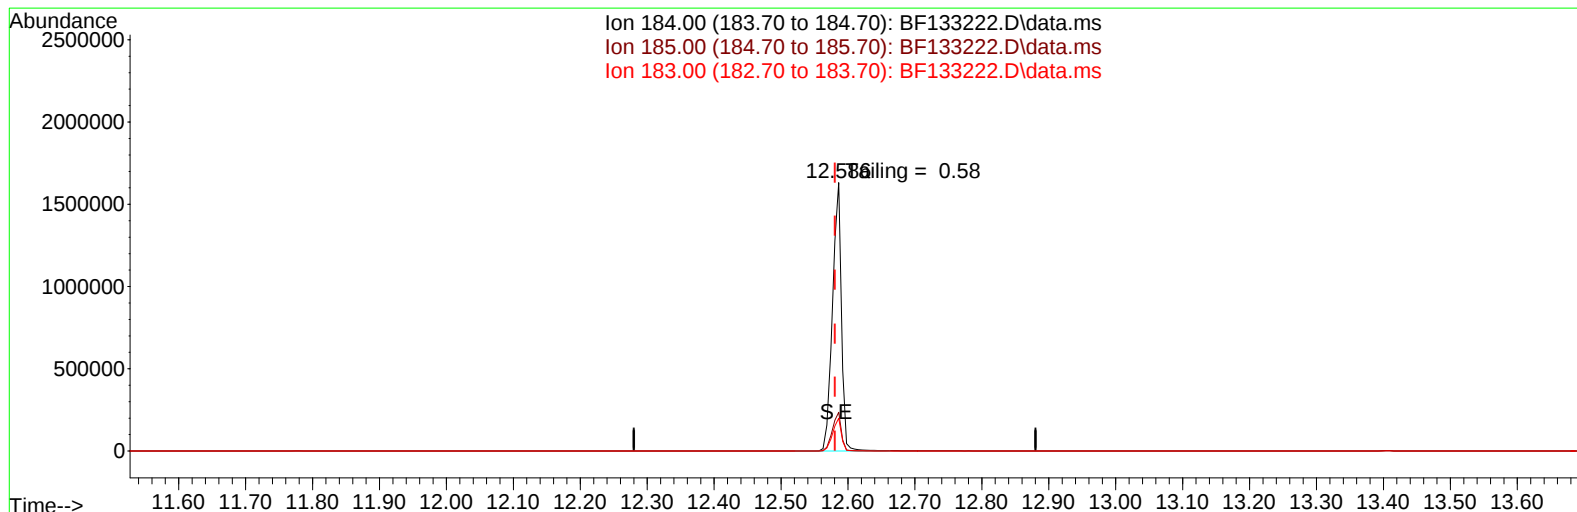

TIC: BF133222.D\data.ms

(77) Benzidine

12.586min (+ 0.006) 13454.26 ng

response 1522554

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.44#
183.00	11.70	12.24
0.00	0.00	0.00