
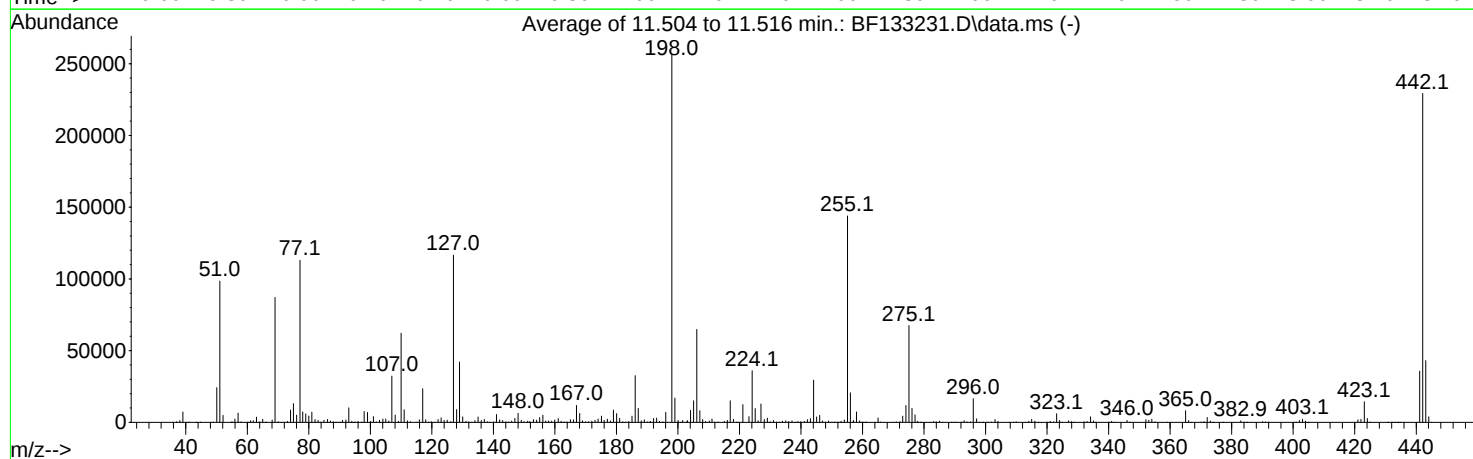


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF050423\  
 Data File : BF133231.D  
 Acq On : 04 May 2023 15:25  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042123.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri May 05 10:49:34 2023

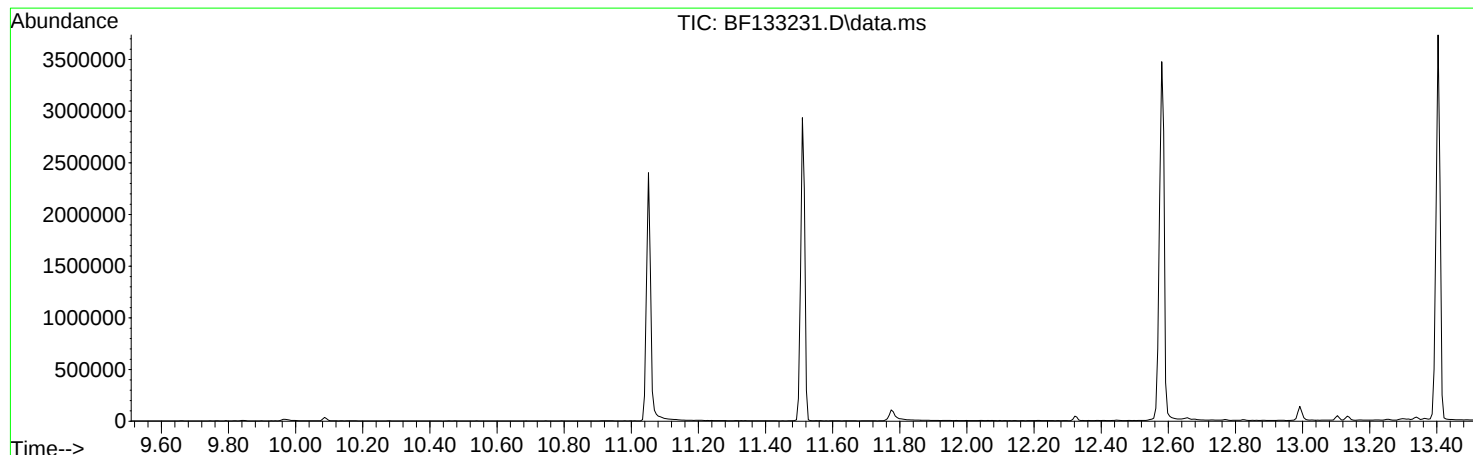

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1596

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 38.4         | 98517      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.9          | 1658       | PASS                |
| 69             | 198             | 0.00            | 100             | 34.0         | 87144      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 477        | PASS                |
| 127            | 198             | 10              | 80              | 45.5         | 116605     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 256448     | PASS                |
| 199            | 198             | 5               | 9               | 6.6          | 16970      | PASS                |
| 275            | 198             | 10              | 60              | 26.3         | 67443      | PASS                |
| 365            | 198             | 1               | 100             | 3.2          | 8148       | PASS                |
| 441            | 198             | 0.01            | 100             | 13.9         | 35713      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 229331     | PASS                |
| 443            | 442             | 15              | 24              | 18.8         | 43031      | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 5/4/2023      | BNA_F            | <u>BF133231.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 619764           | 13.404             |
| DDD           | 12692            | 13.104             |
| DDE           | 989              | 12.769             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 13681         | 633445           | 2.16               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF050423\  
Data File : BF133231.D  
Acq On : 04 May 2023 15:25  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: May 04 16:01:14 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu May 04 12:22:53 2023  
Response via : Initial Calibration

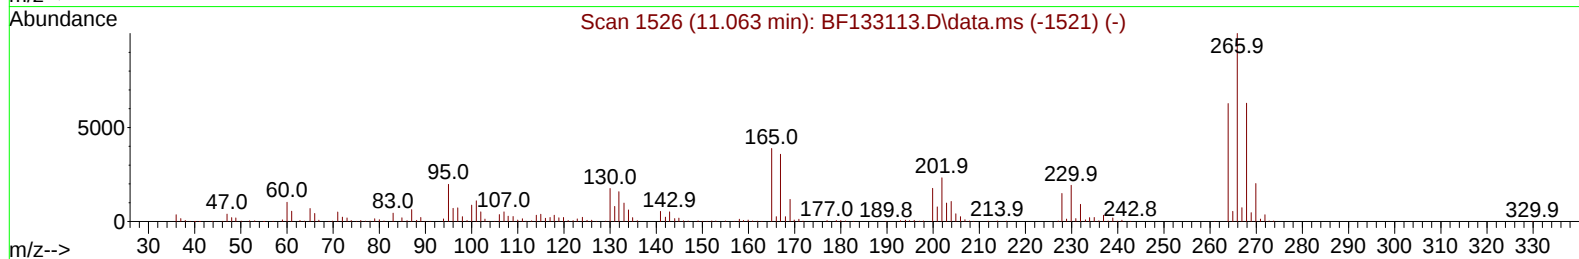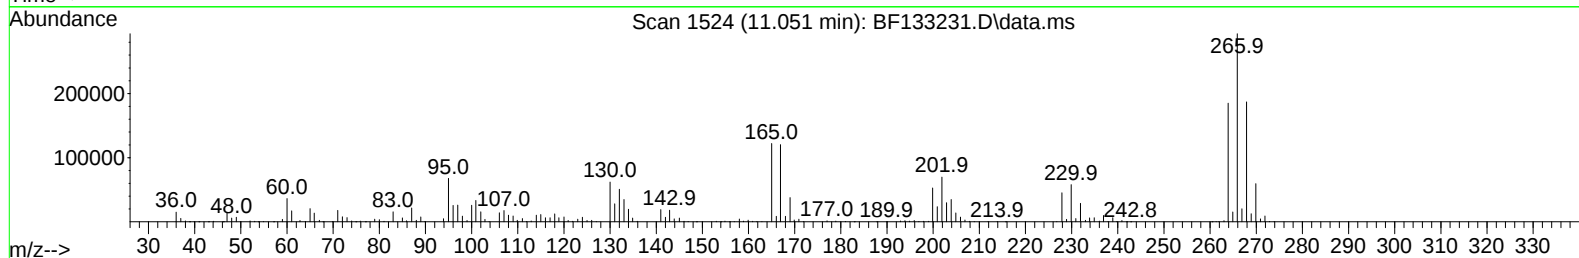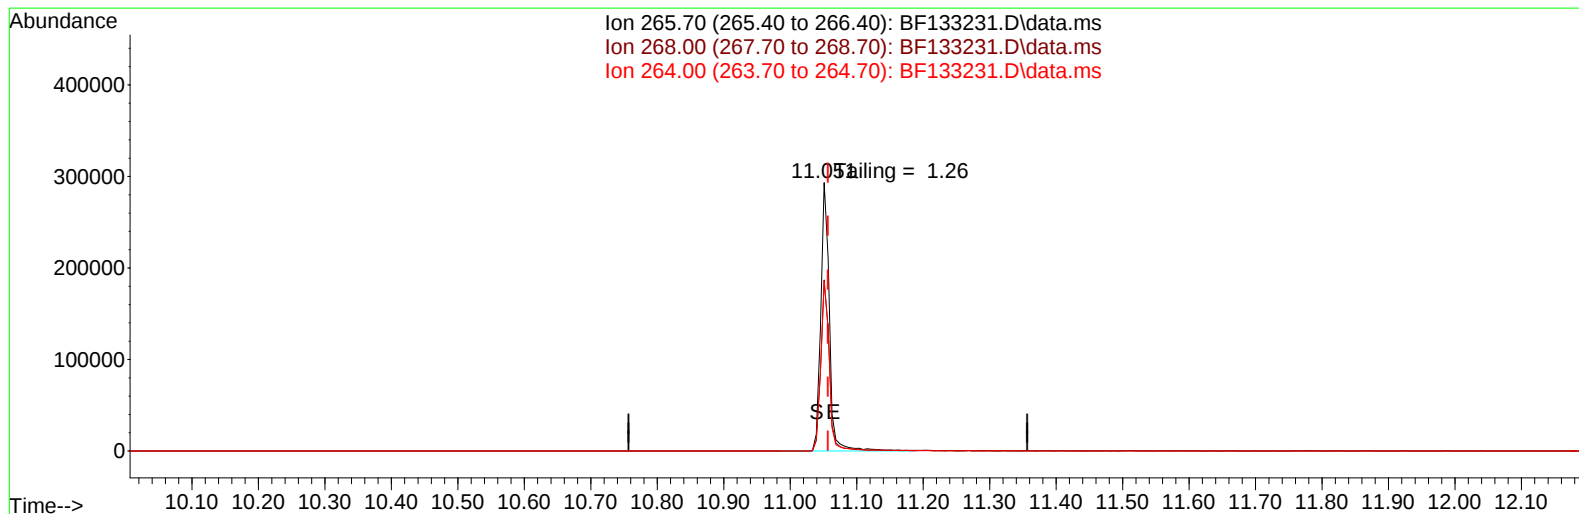

TIC: BF133231.D\data.ms

**(70) Pentachlorophenol (C)**

11.051min (-0.006) 137742.36 ng




response 264921

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.00  | 63.75  |
| 264.00 | 63.30  | 63.09  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF050423\  
Data File : BF133231.D  
Acq On : 04 May 2023 15:25  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: May 04 16:01:14 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu May 04 12:22:53 2023  
Response via : Initial Calibration

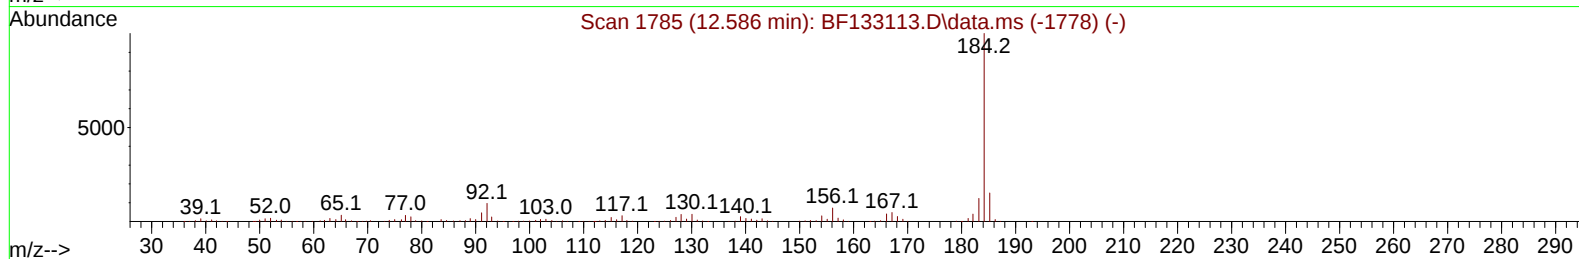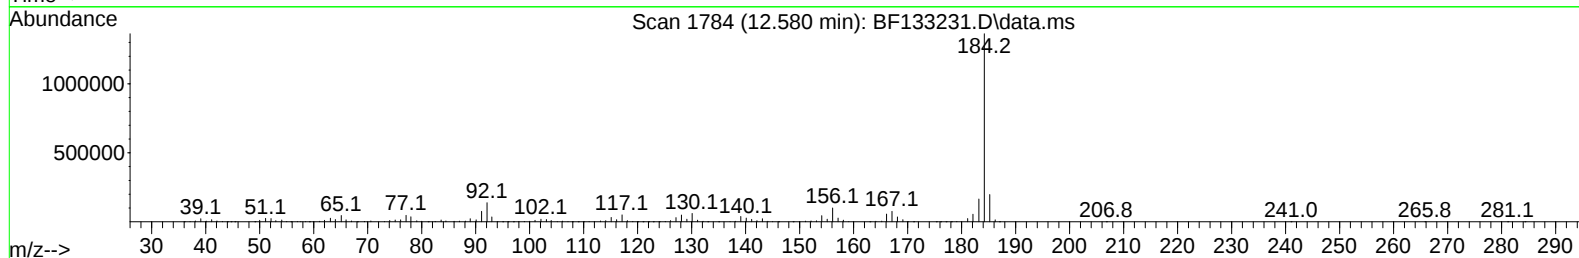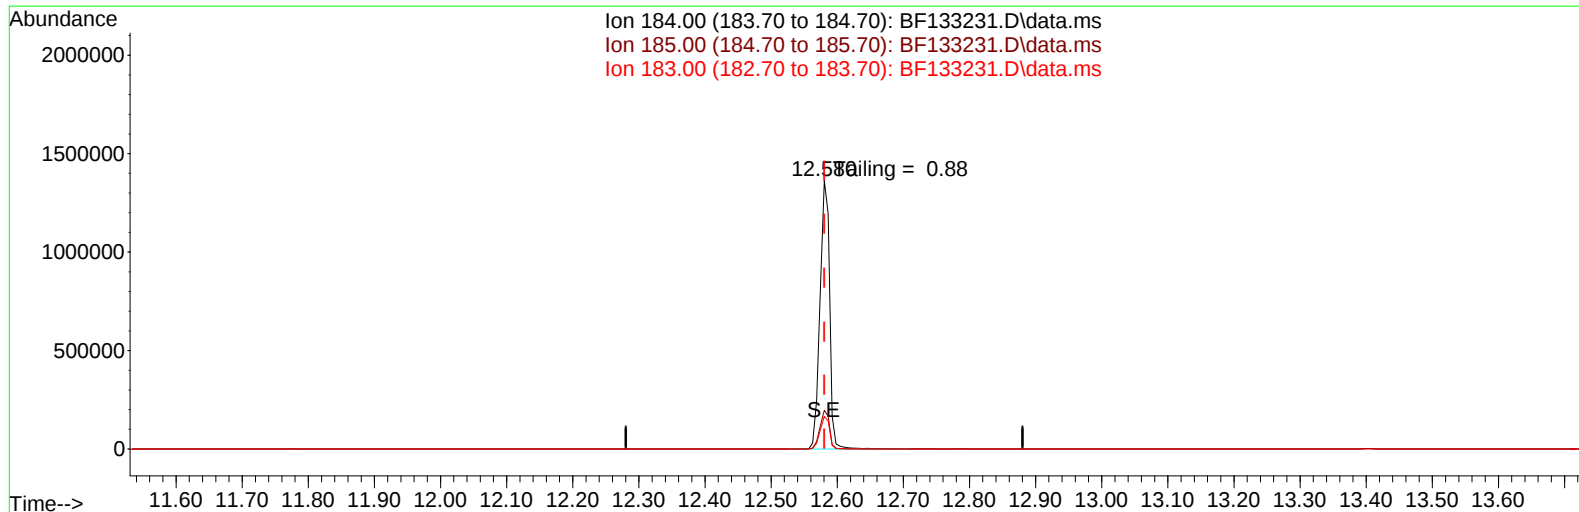

TIC: BF133231.D\data.ms

(77) Benzidine

12.580min (+ 0.000) 158822.58 ng

response 1385859

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 19.30  | 14.44# |
| 183.00 | 11.70  | 12.12  |
| 0.00   | 0.00   | 0.00   |