
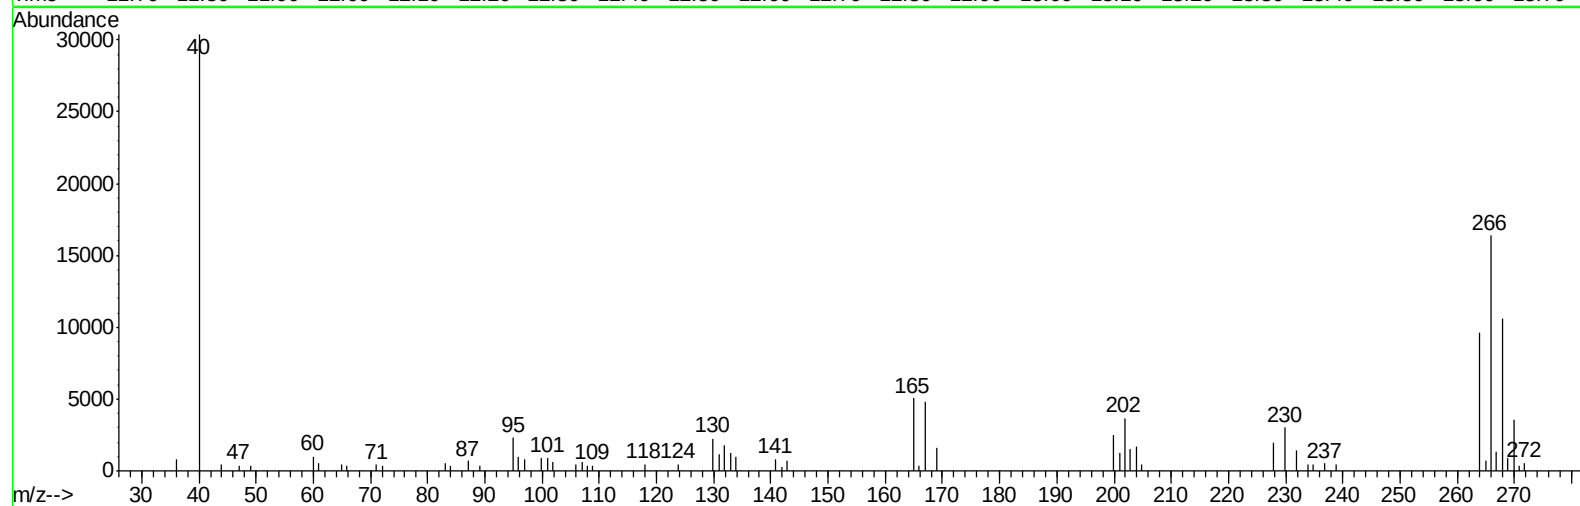


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF050515\  
Data File : BF078930.D  
Acq On : 5 May 2015 8:58  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 06:59:19 2015  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF043015.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed May 06 00:45:00 2015  
Response via : Initial Calibration

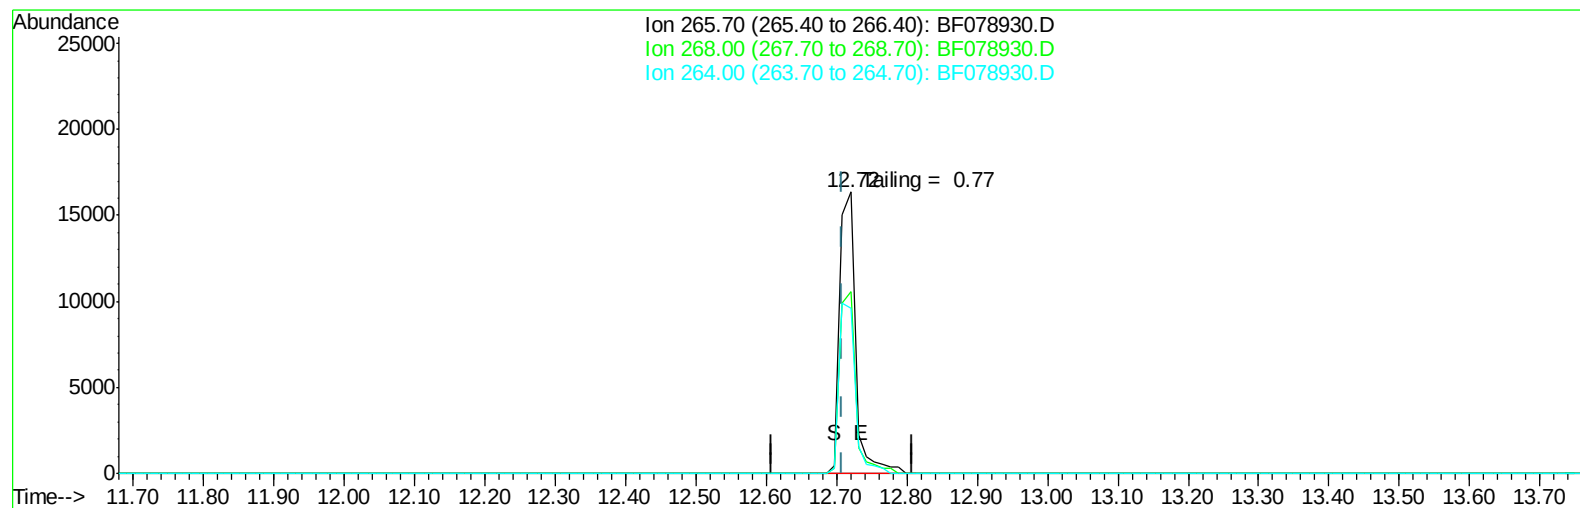

TIC: BF078930.D

(69) Pentachlorophenol (C)



12.720min (+0.011) 0.00ng

response 24964

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 68.80 | 64.53 |
| 264.00 | 60.20 | 58.72 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF050515\  
Data File : BF078930.D  
Acq On : 5 May 2015 8:58  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 06:59:19 2015  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF043015.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed May 06 00:45:00 2015  
Response via : Initial Calibration

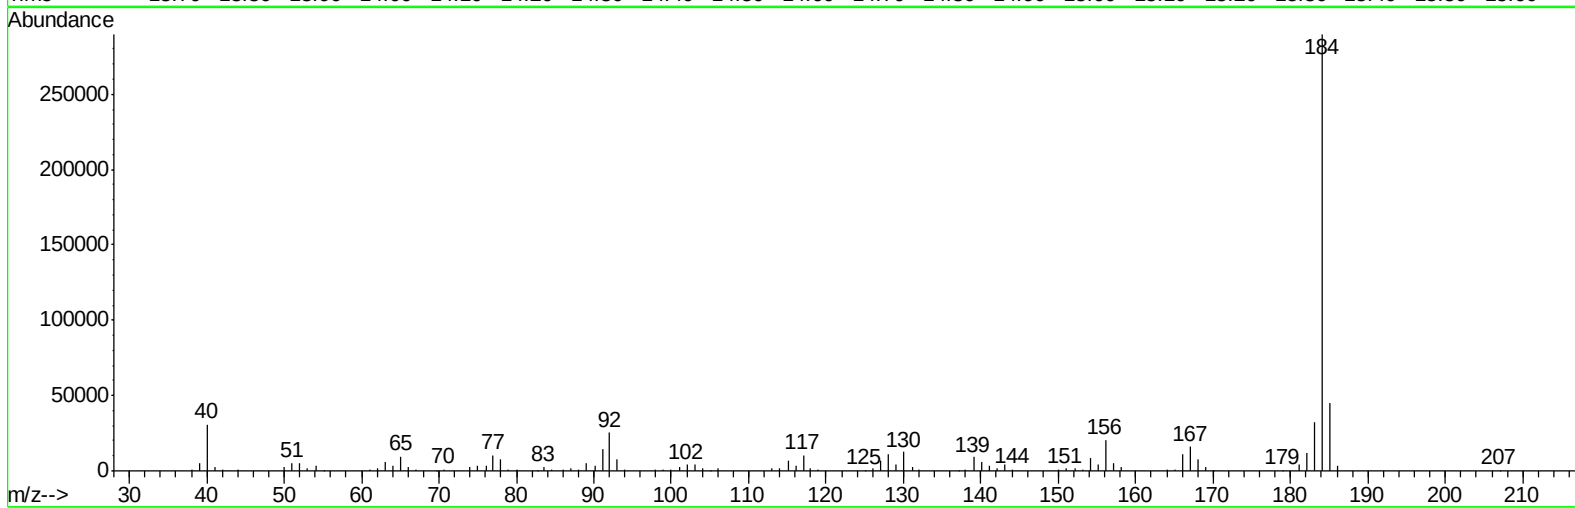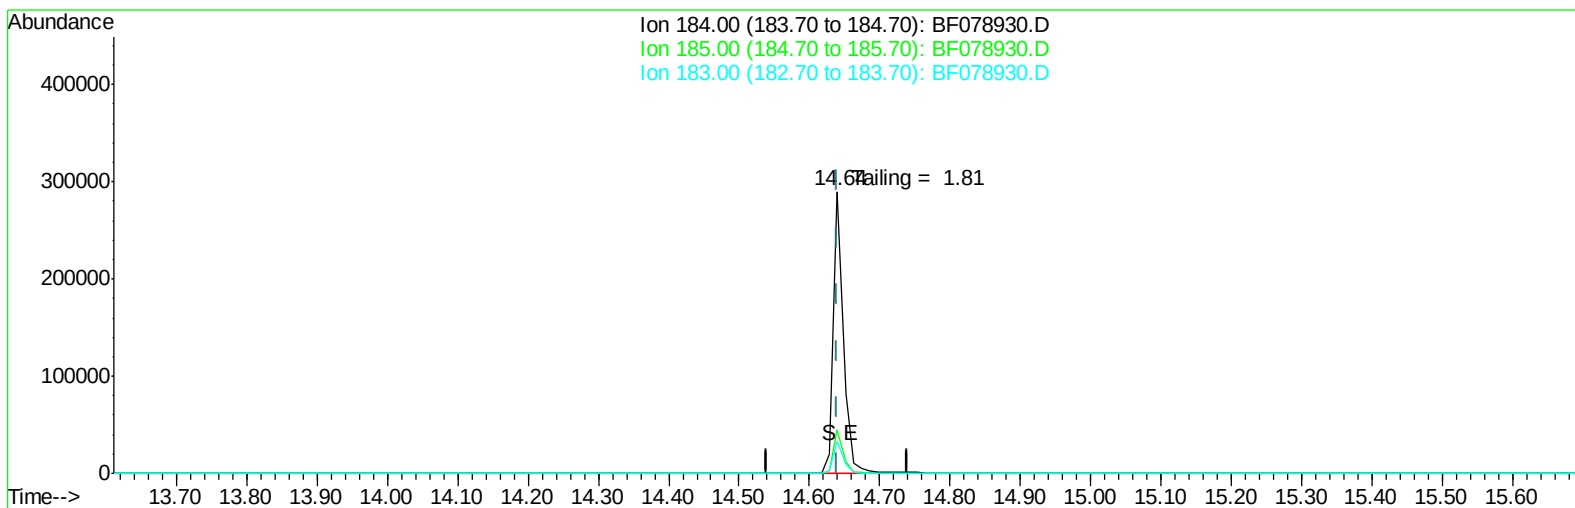

TIC: BF078930.D

(76) Benzidine

14.640min (0.000) 0.00ng

response 281854

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.40 | 15.50 |
| 183.00 | 10.50 | 11.24 |
| 0.00   | 0.00  | 0.00  |