
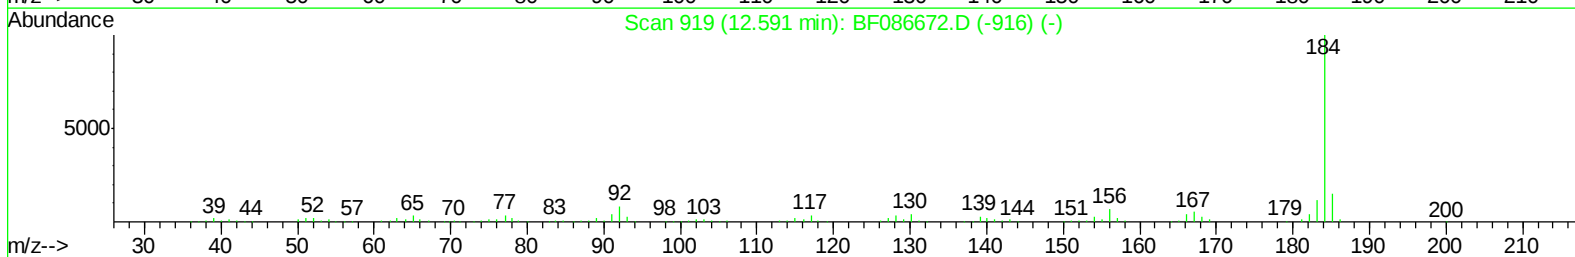
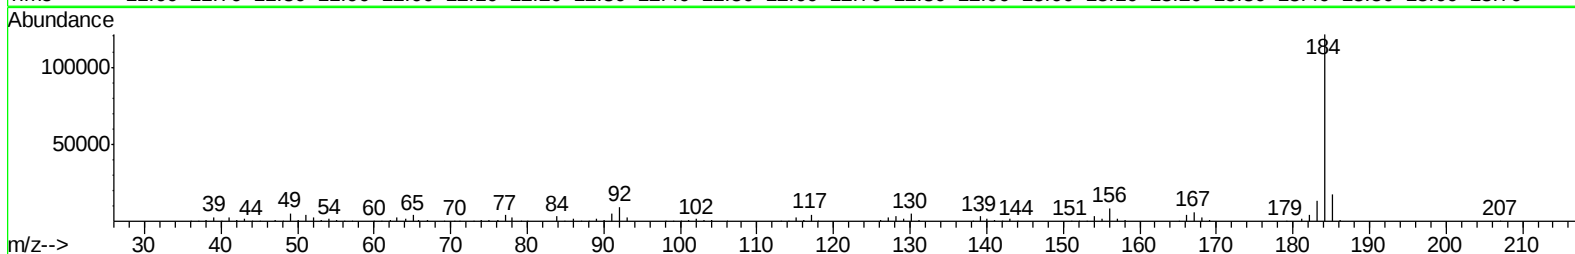


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050516\
Data File : BF086706.D
Acq On : 5 May 2016 13:37
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 03:49:35 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 04 15:12:53 2016
Response via : Initial Calibration

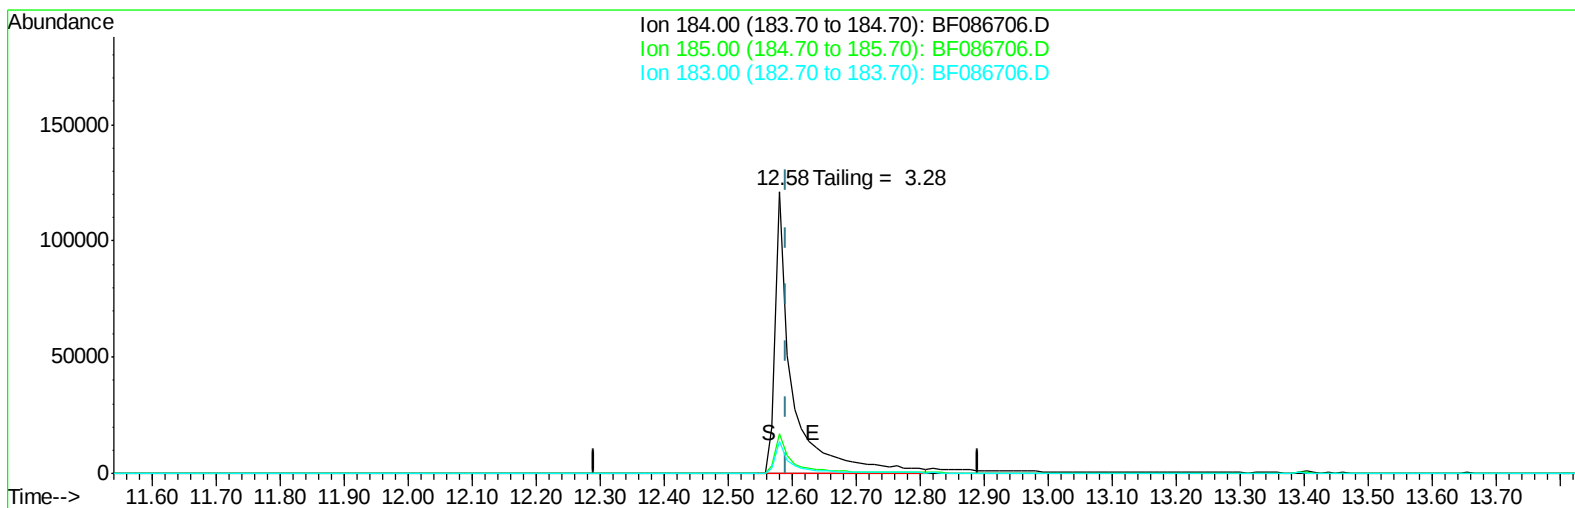

TIC: BF086706.D

(76) Benzidine




12.579min (-0.011) 0.00ng

response 226512

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	14.29
183.00	12.20	11.24
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050516\
Data File : BF086706.D
Acq On : 5 May 2016 13:37
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 03:49:35 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 04 15:12:53 2016
Response via : Initial Calibration

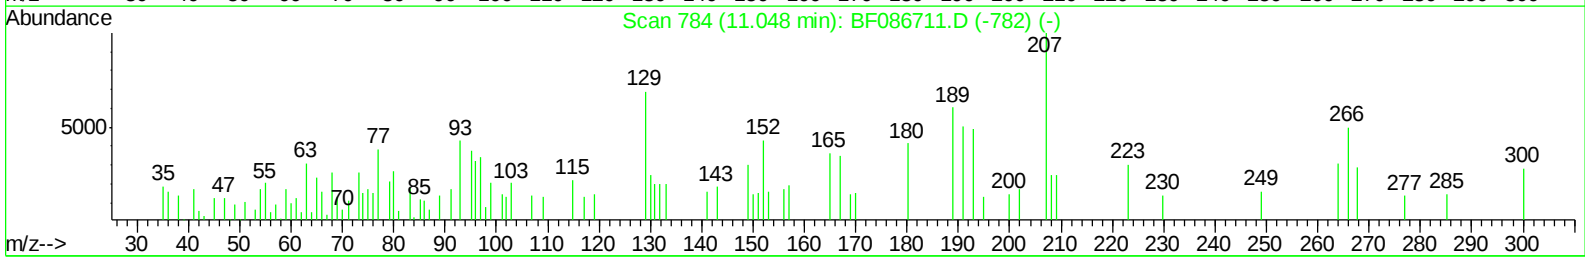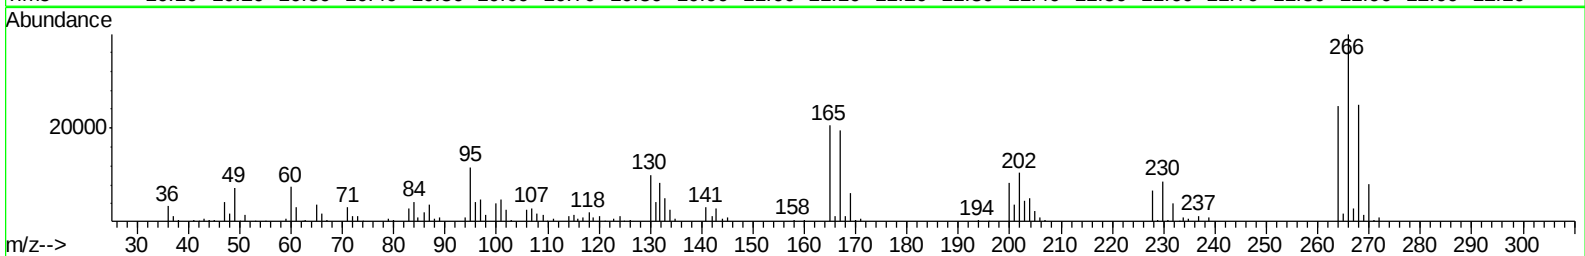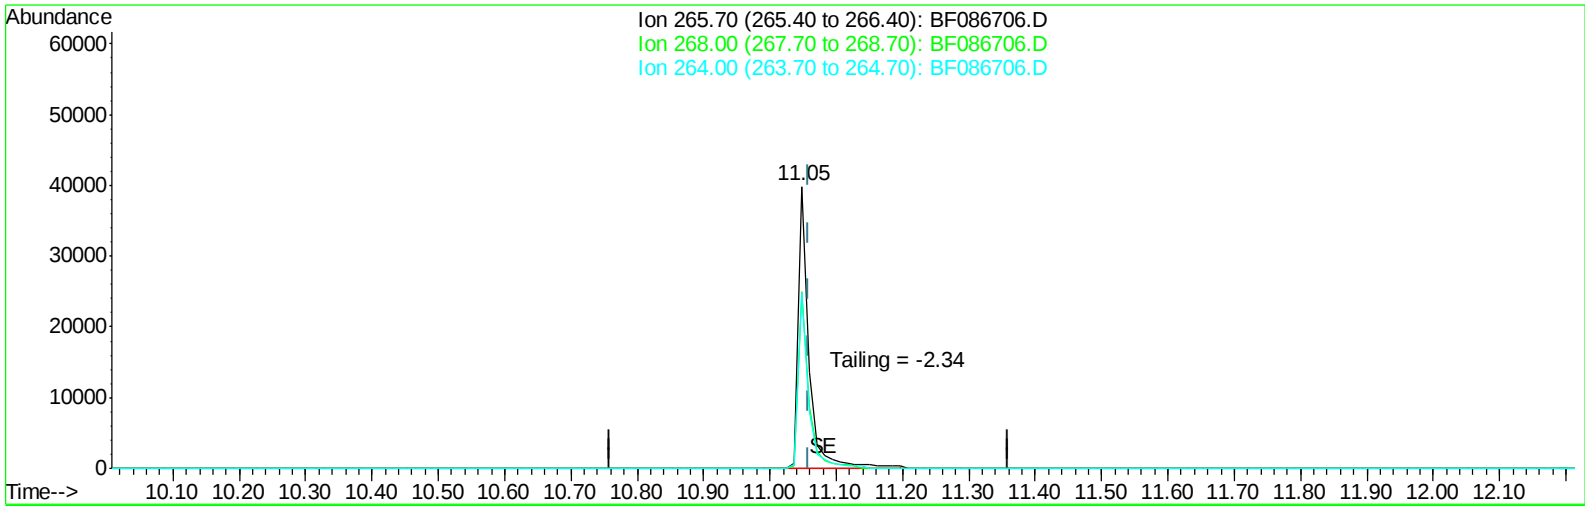

TIC: BF086706.D

(69) Pentachlorophenol (C)

11.048min (-0.011) 0.00ng m

response 44427

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	62.86
264.00	66.10	62.16
0.00	0.00	0.00