


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050516\
 Data File : BF086706.D
 Acq On : 5 May 2016 13:37
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 06 01:22:17 2016

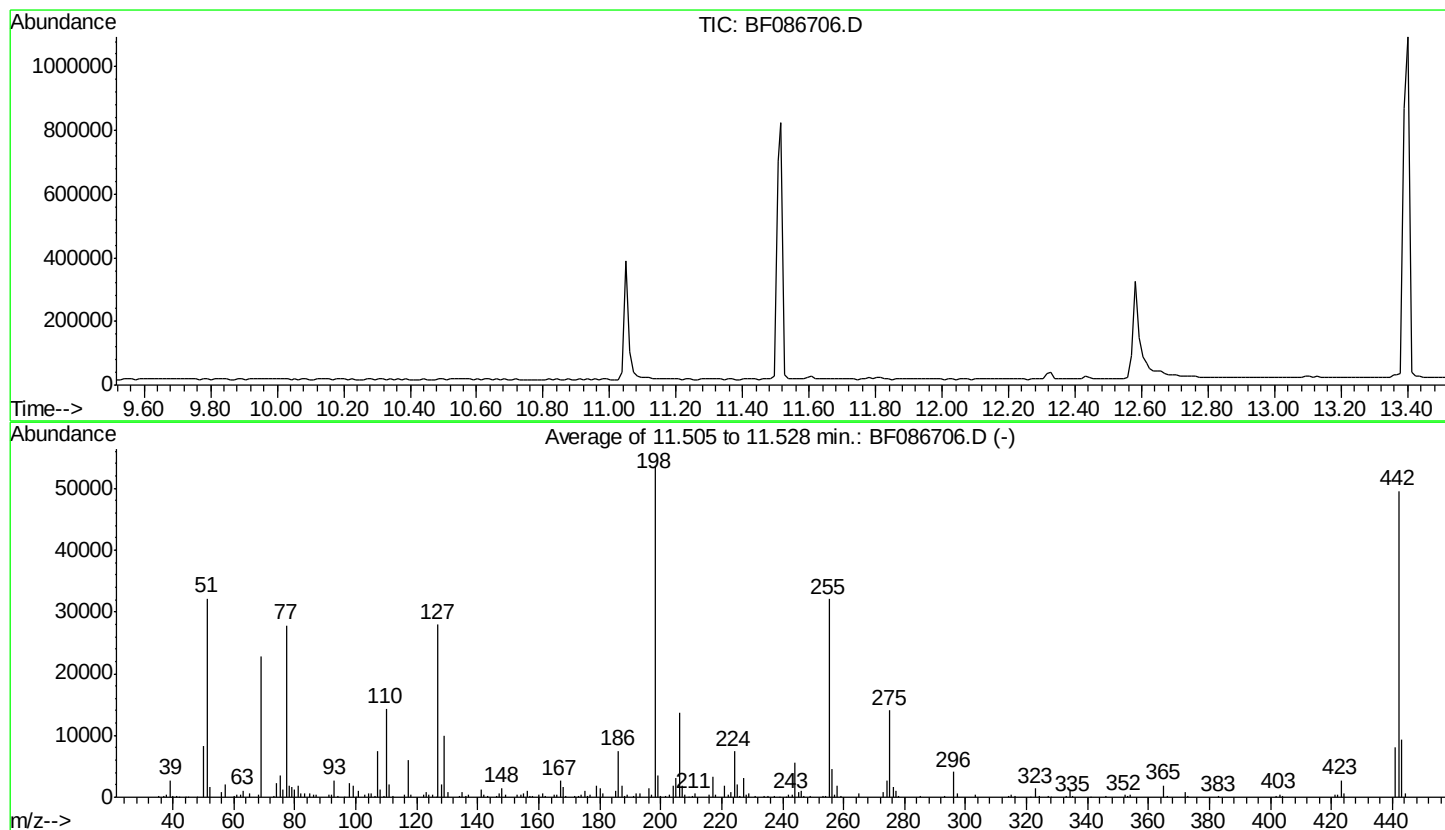

AutoFind: Scans 824, 825, 826; Background Corrected with Scan 820

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.9	32129	PASS
68	69	0.00	2	1.7	393	PASS
69	198	0.00	100	42.3	22722	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.0	27930	PASS
197	198	0.00	2	0.8	438	PASS
198	198	100	100	100.0	53672	PASS
199	198	5	9	6.8	3633	PASS
275	198	10	60	26.1	14012	PASS
365	198	1	100	3.7	1971	PASS
441	442	0.01	24	16.2	8037	PASS
442	198	50	100	92.3	49526	PASS
443	442	15	24	18.8	9313	PASS