
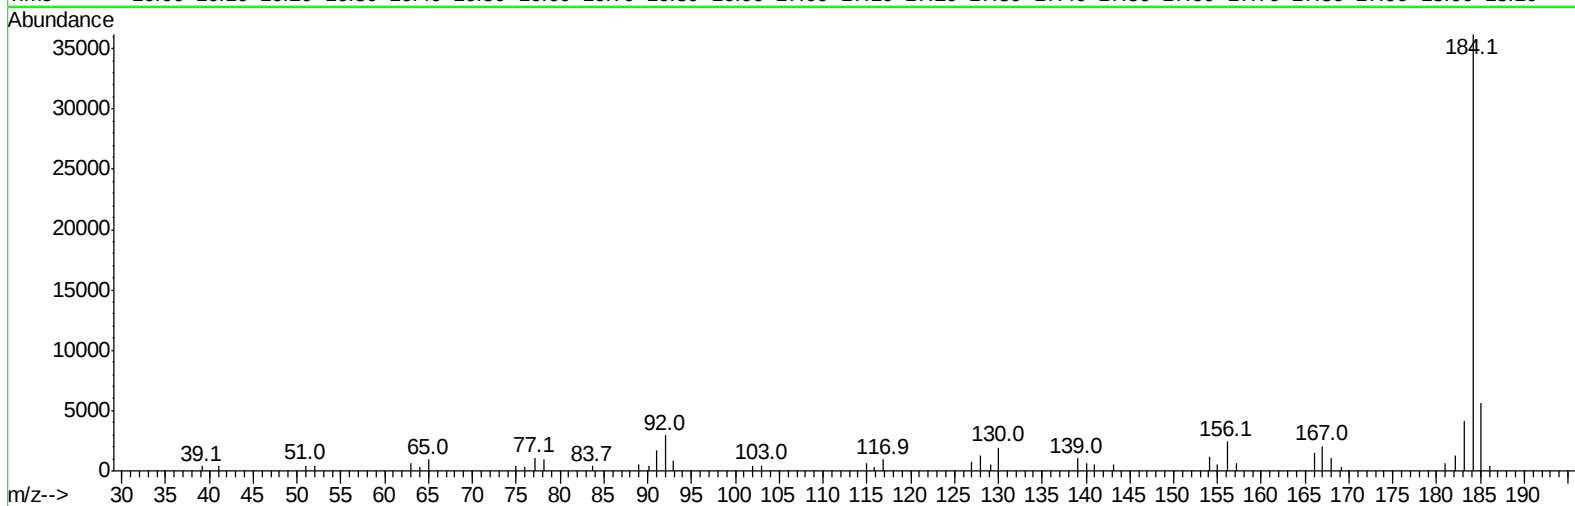


Data Path : Z:\HPCHEM1\BNA F\Data\BF050517\
Data File : BF094942.D
Acq On : 6 May 2017 4:47
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 02:45:05 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

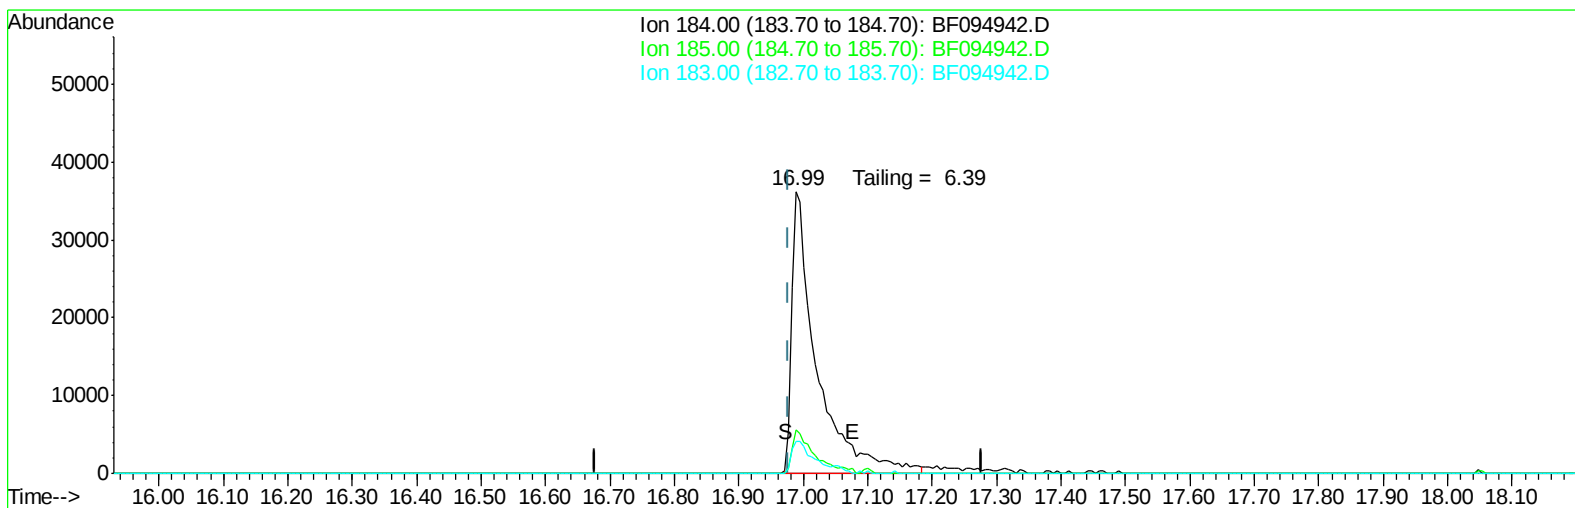

TIC: BF094942.D

(76) Benzidine



16.989min (+0.012) 0.00ng

response 97573

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	15.68
183.00	12.20	11.39
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF050517\
Data File : BF094942.D
Acq On : 6 May 2017 4:47
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 02:45:05 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

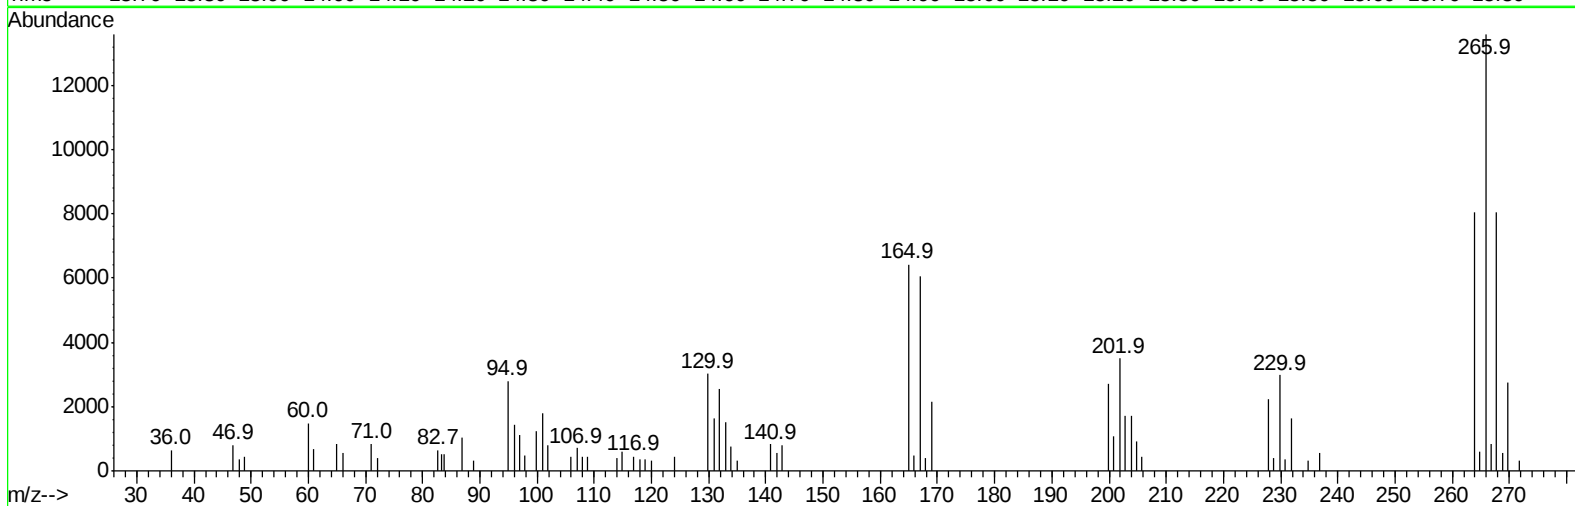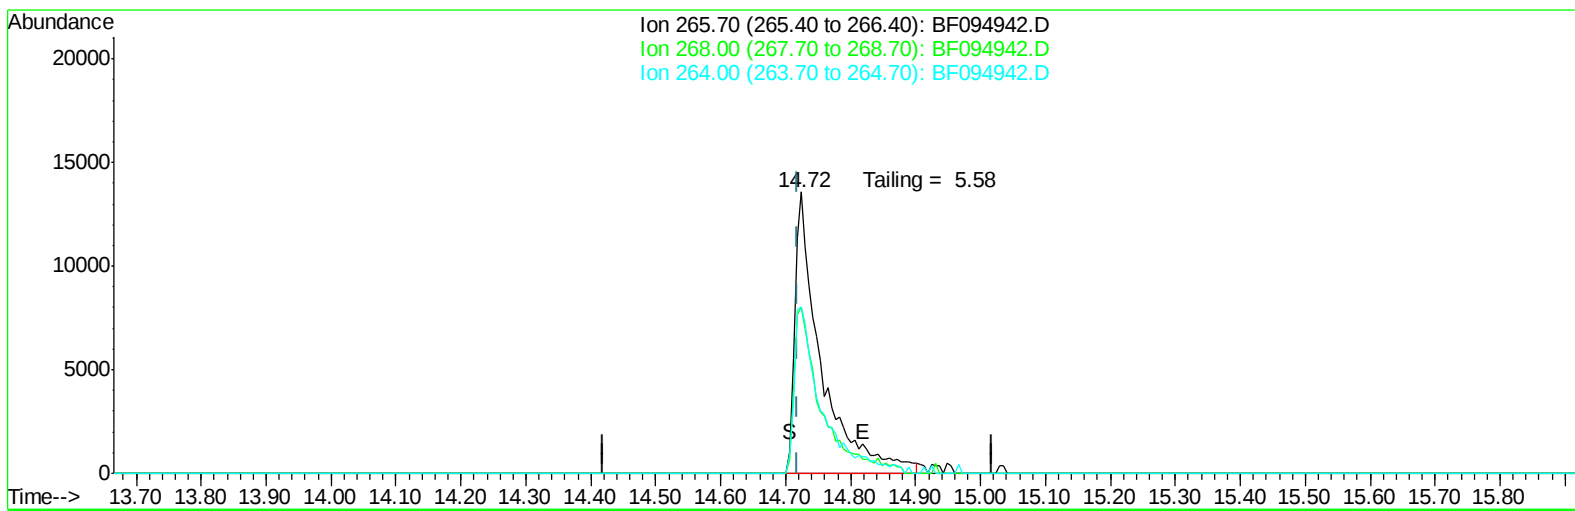

TIC: BF094942.D

(69) Pentachlorophenol (C)

14.724min (+0.006) 0.00ng

response 38108

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.12
264.00	64.60	59.32
0.00	0.00	0.00