

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050517\
 Data File : BF094927.D
 Acq On : 5 May 2017 20:42
 Operator : SJ/MA
 Sample : PB98725BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB98725BL

Quant Time: May 05 23:56:02 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 03 17:24:51 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	94264	20.00	ng	0.00
21) Naphthalene-d8	9.74	136	359855	20.00	ng	-0.01
38) Acenaphthene-d10	12.57	164	173017	20.00	ng	-0.01
63) Phenanthrene-d10	14.97	188	331348	20.00	ng	-0.01
75) Chrysene-d12	18.64	240	260129	20.00	ng	-0.01
86) Perylene-d12	20.31	264	164090	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.67	112	725001	128.23	ng	0.00
7) Phenol-d6	7.27	99	852176	125.62	ng	-0.01
23) Nitrobenzene-d5	8.62	82	513089	89.91	ng	-0.02
41) 2,4,6-Tribromophenol	13.87	330	204210	144.12	ng	-0.02
44) 2-Fluorobiphenyl	11.52	172	1042638	86.74	ng	-0.01
78) Terphenyl-d14	17.30	244	958963	81.20	ng	-0.01


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050517\
Data File : BF094927.D
Acq On : 5 May 2017 20:42
Operator : SJ/MA
Sample : PB98725BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB98725BL

Quant Time: May 05 23:56:02 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

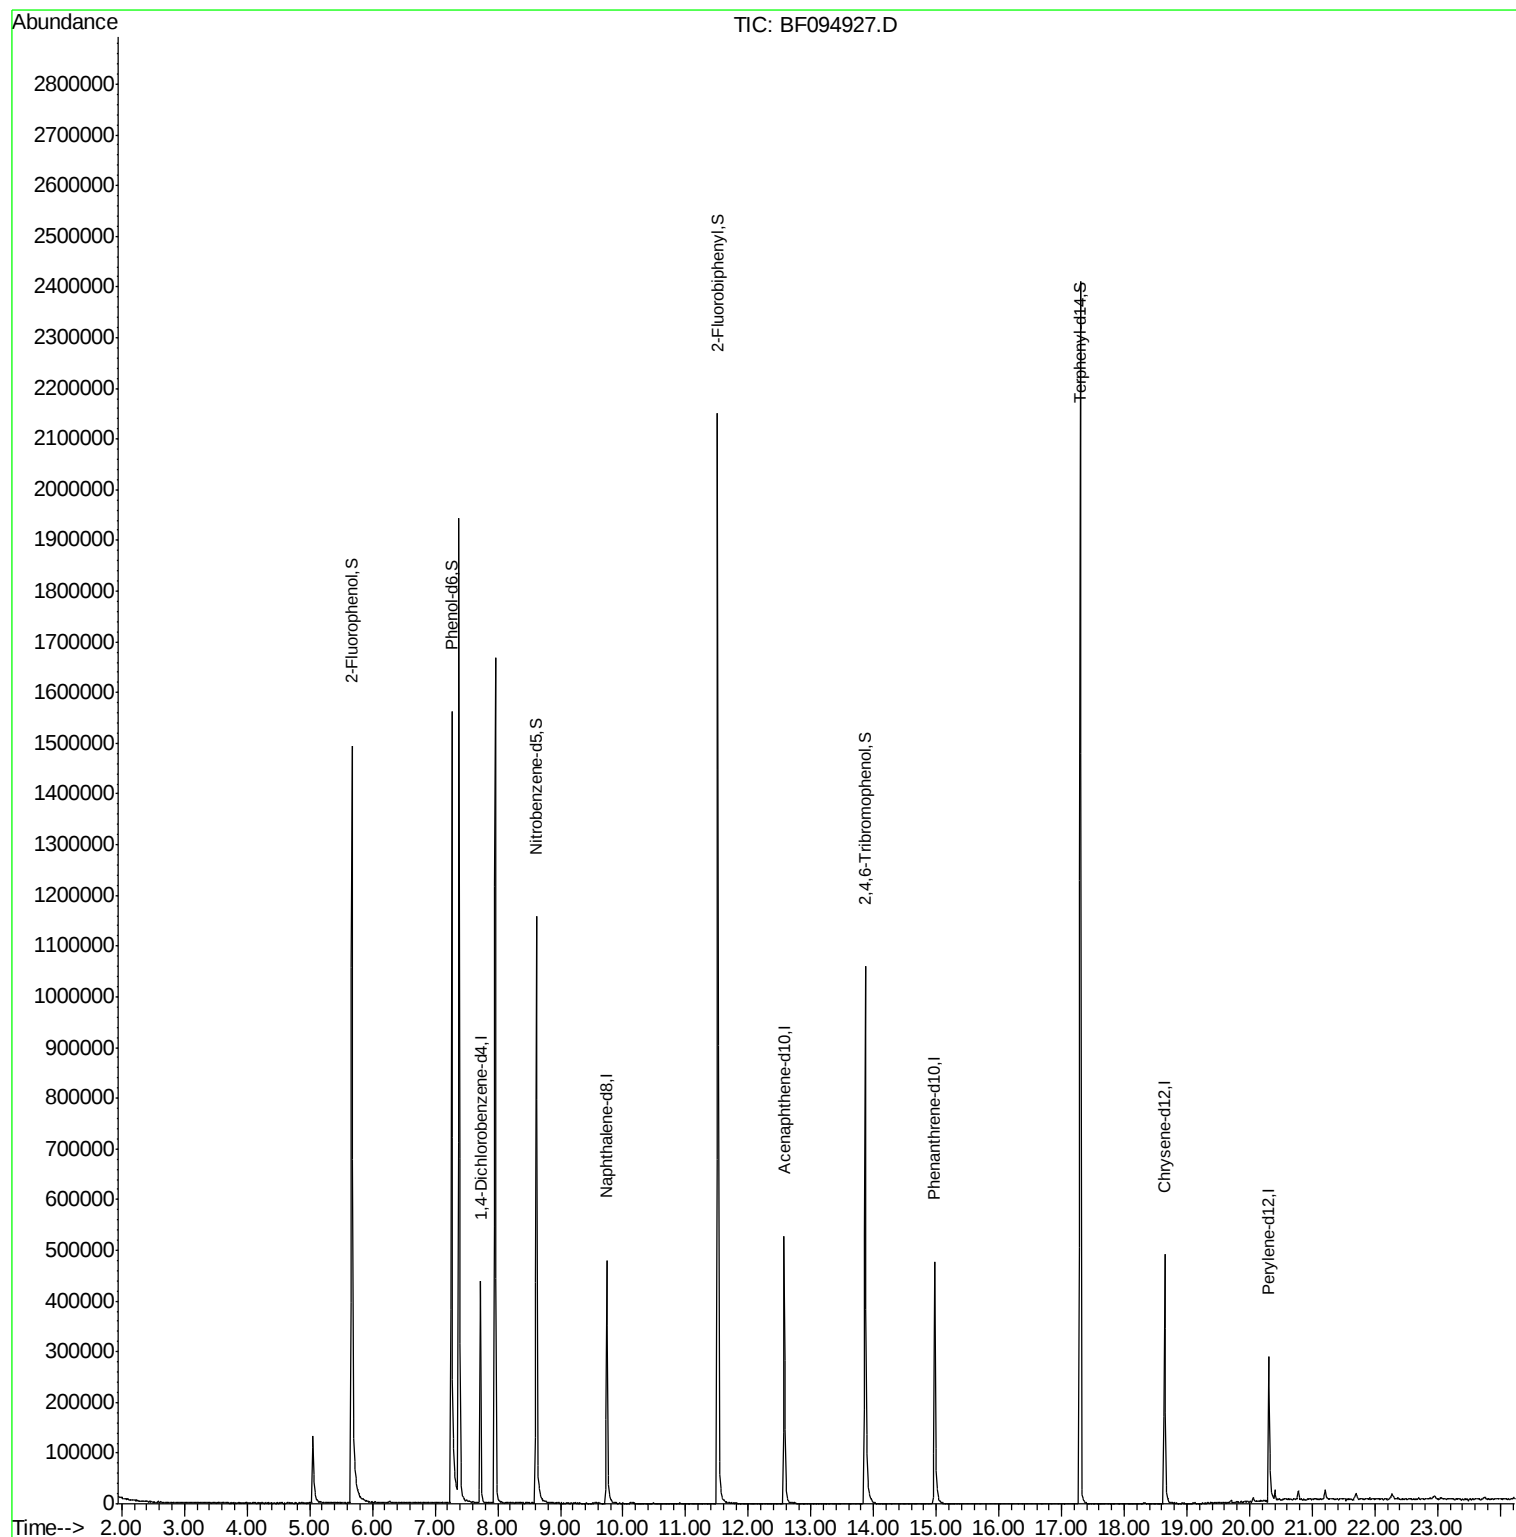




#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.72 min Scan# 984
 Delta R.T. -0.01 min
 Lab File: BF094927.D
 Acq: 5 May 2017 20:42

Instrument :
 BNA_F
 ClientSampleId :
 PB98725BL

Tgt Ion:152 Resp: 94264
 Ion Ratio Lower Upper
 152 100
 150 155.1 126.2 189.2
 115 59.0 52.2 78.2

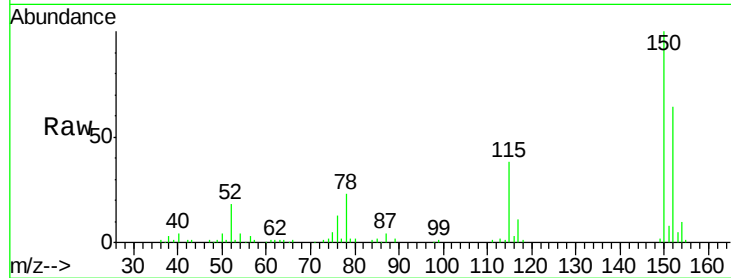


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

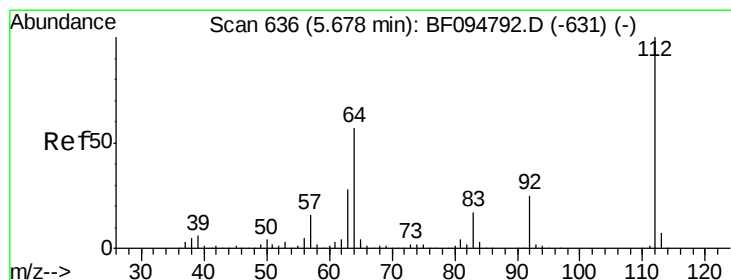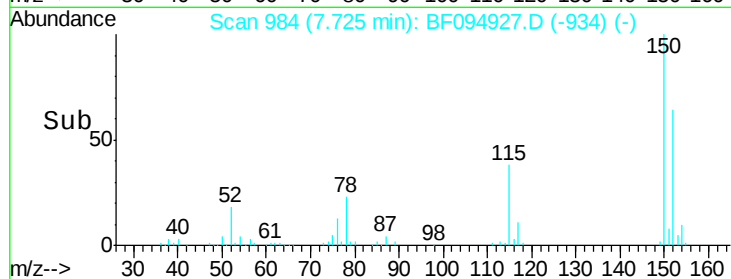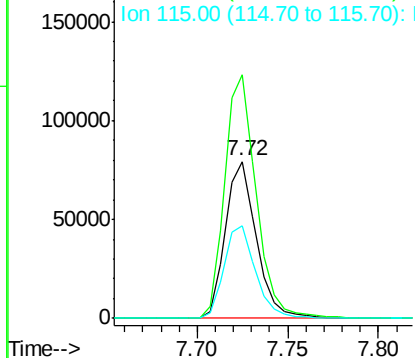



#5


2-Fluorophenol
 Concen: 128.23 ng
 RT: 5.67 min Scan# 635
 Delta R.T. -0.01 min
 Lab File: BF094927.D
 Acq: 5 May 2017 20:42

Tgt Ion:112 Resp: 725001
 Ion Ratio Lower Upper
 112 100
 64 56.3 46.0 69.0
 63 27.3 23.4 35.0

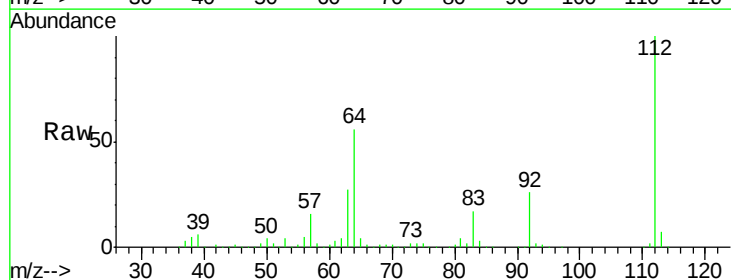

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

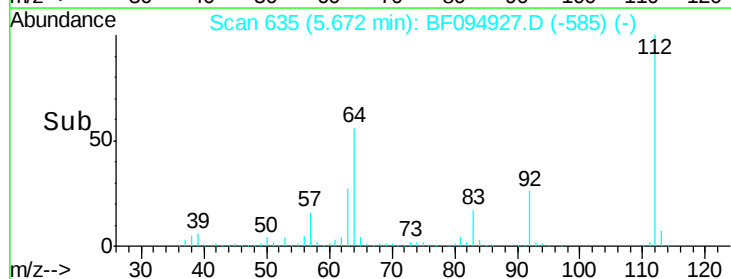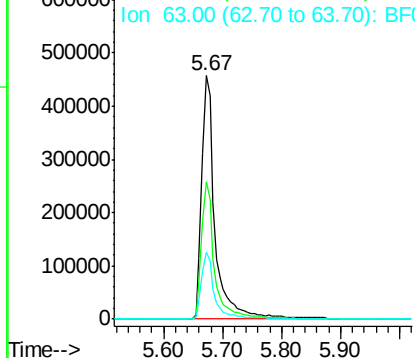

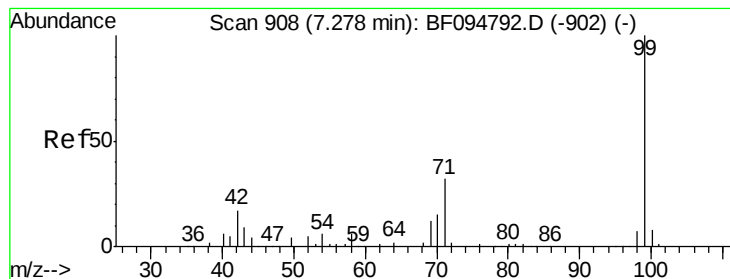

#7

Phenol-d6

Concen: 125.62 ng

RT: 7.27 min Scan# 906

Delta R.T. -0.01 min

Lab File: BF094927.D

Acq: 5 May 2017 20:42

Instrument :

BNA_F

ClientSampleId :

PB98725BL


Tgt Ion: 99 Resp: 852176

Ion Ratio Lower Upper

99 100

42 16.4 13.5 20.3




71 33.2 24.5 36.7

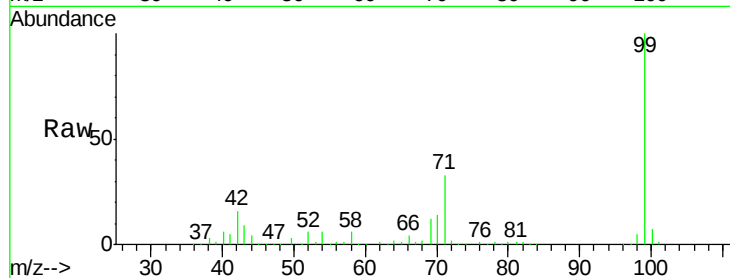

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

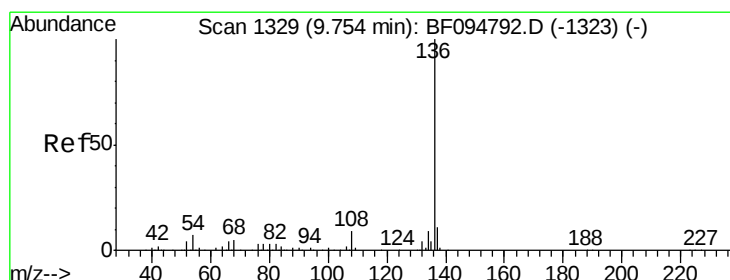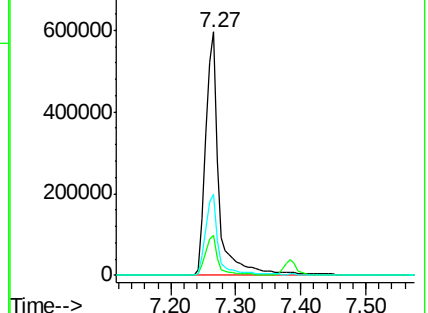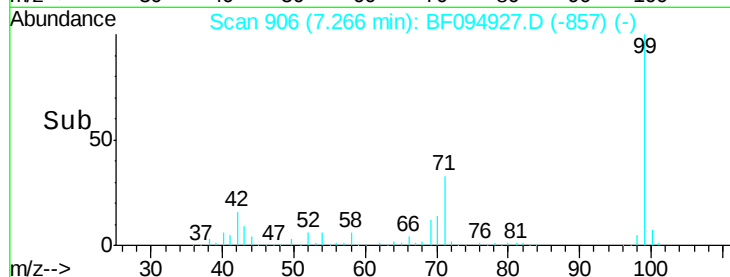

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.74 min Scan# 1327

Delta R.T. -0.01 min

Lab File: BF094927.D

Acq: 5 May 2017 20:42

Tgt Ion: 136 Resp: 359855


Ion Ratio Lower Upper

136 100

137 11.4 8.5 12.7

54 6.9 4.9 7.3

68 5.6 4.1 6.1


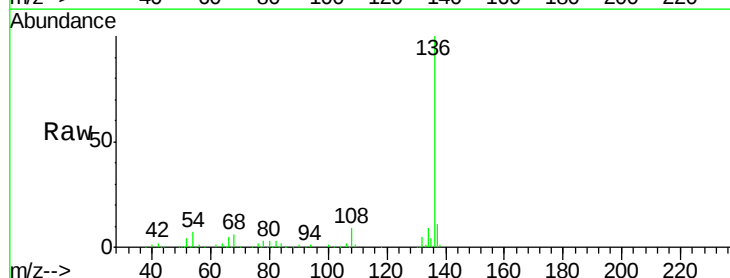



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

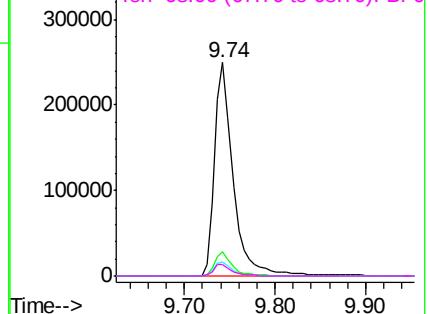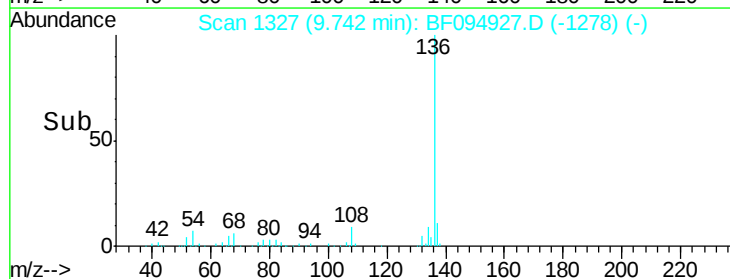


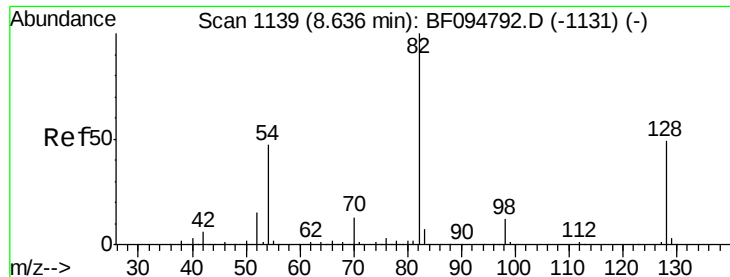




#23
 Nitrobenzene-d5
 Concen: 89.91 ng
 RT: 8.62 min Scan# 1136
 Delta R.T. -0.02 min
 Lab File: BF094927.D
 Acq: 5 May 2017 20:42

Instrument :
 BNA_F
 ClientSampleId :
 PB98725BL

Tgt Ion: 82 Resp: 513089
 Ion Ratio Lower Upper
 82 100
 128 46.7 34.0 51.0
 54 48.2 42.2 63.2

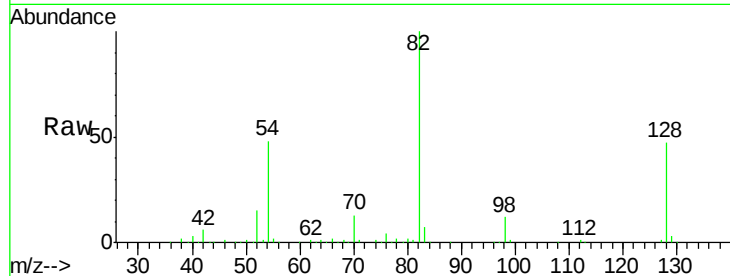


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

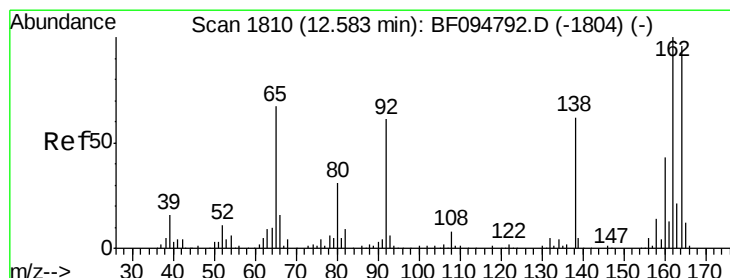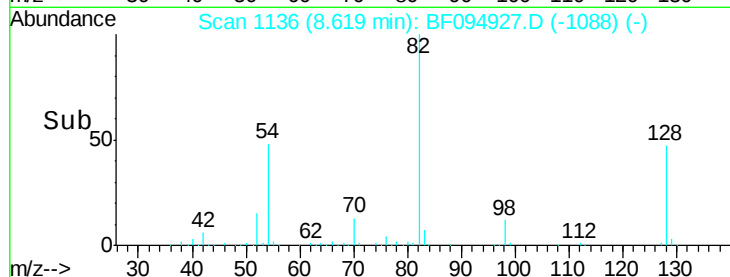
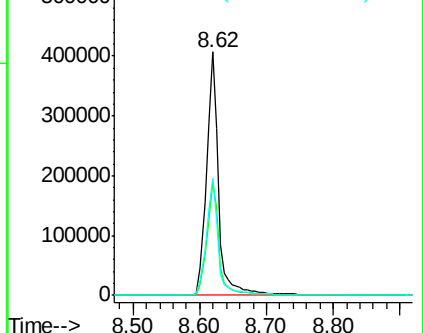


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 12.57 min Scan# 1808
 Delta R.T. -0.01 min
 Lab File: BF094927.D
 Acq: 5 May 2017 20:42

Tgt Ion: 164 Resp: 173017
 Ion Ratio Lower Upper
 164 100
 162 103.2 82.6 123.8
 160 43.8 36.2 54.2

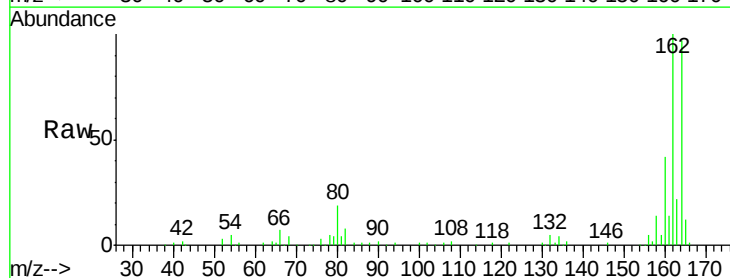

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E



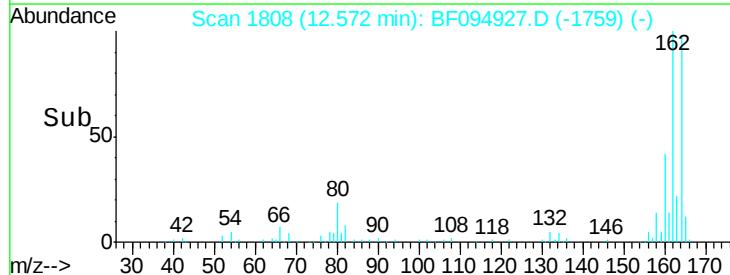
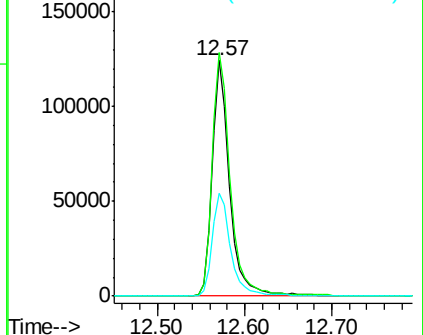




#41
 2,4,6-Tribromophenol
 Concen: 144.12 ng
 RT: 13.87 min Scan# 2028
 Delta R.T. -0.02 min
 Lab File: BF094927.D
 Acq: 5 May 2017 20:42




Instrument :
 BNA_F
 ClientSampleId :
 PB98725BL


Tgt Ion:330 Resp: 204210
 Ion Ratio Lower Upper
 330 100
 332 96.4 76.6 115.0
 141 39.5 31.4 47.2

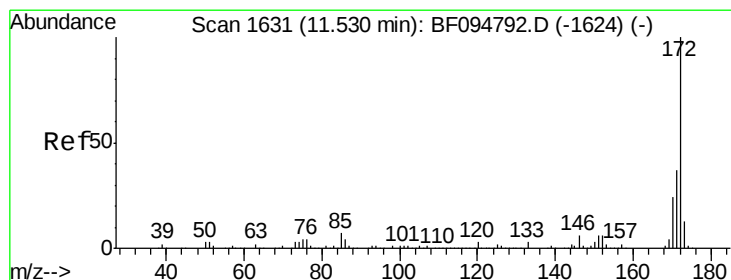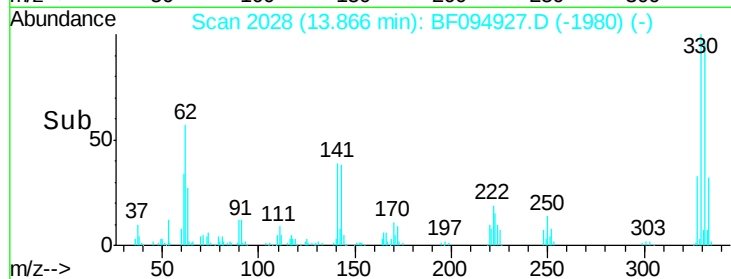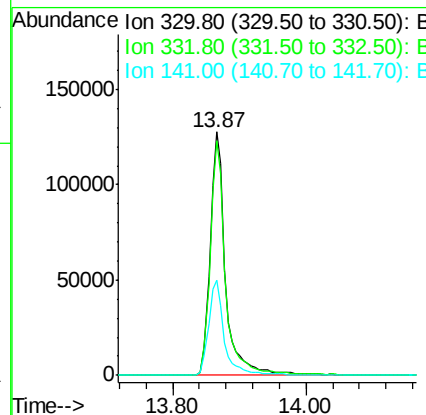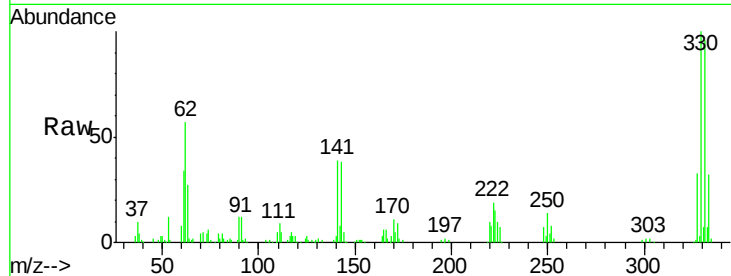

#44
 2-Fluorobiphenyl
 Concen: 86.74 ng
 RT: 11.52 min Scan# 1629
 Delta R.T. -0.01 min
 Lab File: BF094927.D
 Acq: 5 May 2017 20:42

Tgt Ion:172 Resp: 1042638
 Ion Ratio Lower Upper
 172 100
 171 35.9 29.6 44.4
 170 23.6 19.8 29.8

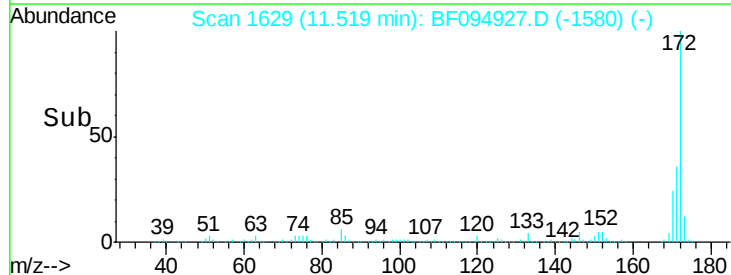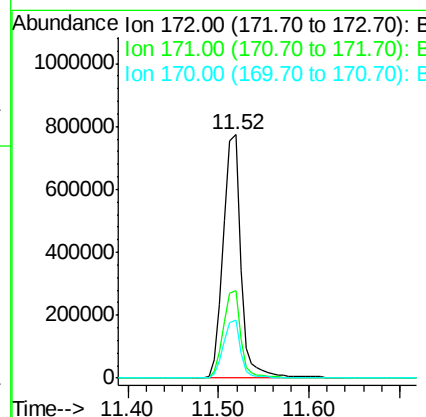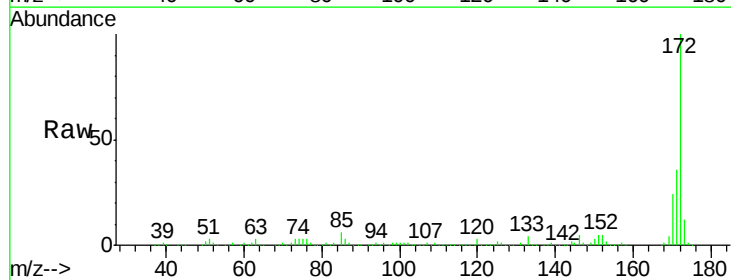


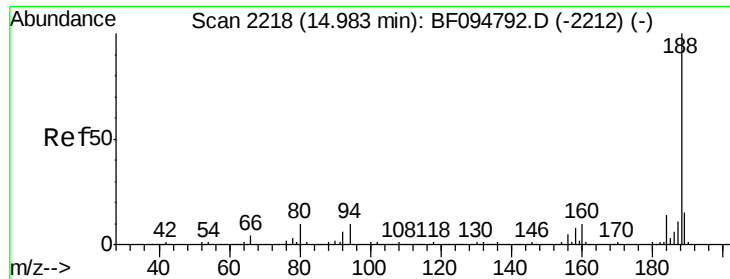




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 14.97 min Scan# 2216
Delta R.T. -0.01 min
Lab File: BF094927.D
Acq: 5 May 2017 20:42

Instrument :
BNA_F
ClientSampled :
PB98725BL

Tgt Ion:188 Resp: 331348
Ion Ratio Lower Upper
188 100
94 10.4 9.4 14.2
80 11.5 10.2 15.2

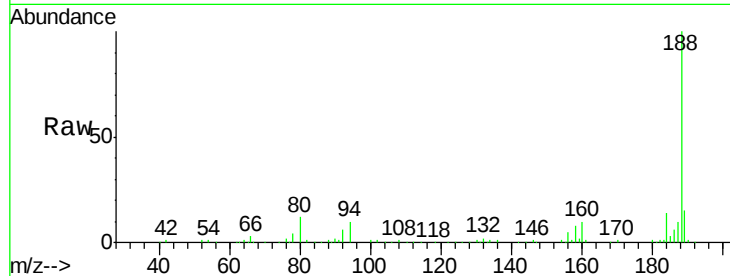


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

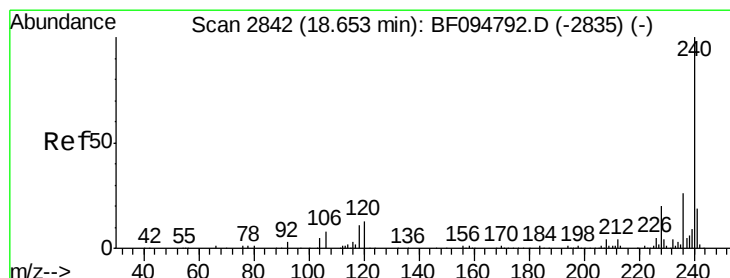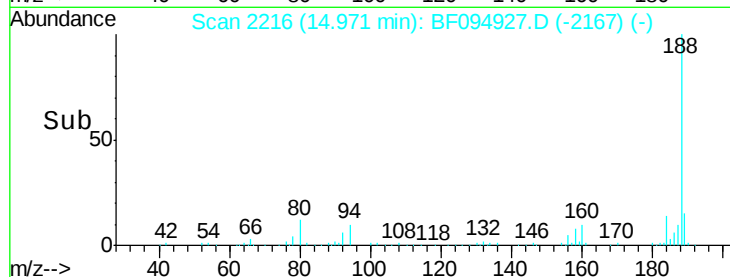
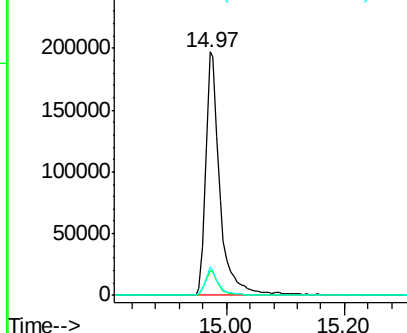


#75
Chrysene-d12
Concen: 20.00 ng
RT: 18.64 min Scan# 2840
Delta R.T. -0.01 min
Lab File: BF094927.D
Acq: 5 May 2017 20:42

Tgt Ion:240 Resp: 260129
Ion Ratio Lower Upper
240 100
120 13.3 5.8 8.8#
236 24.8 20.5 30.7

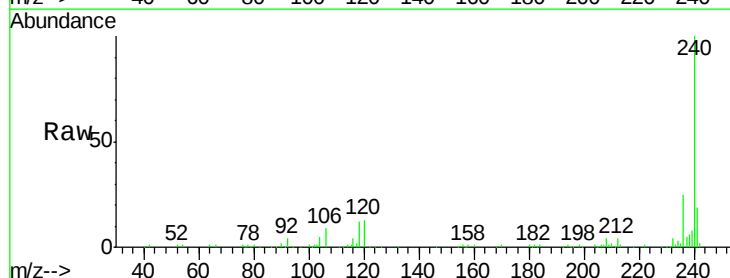

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

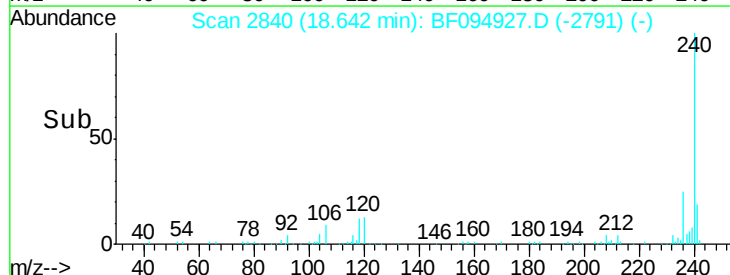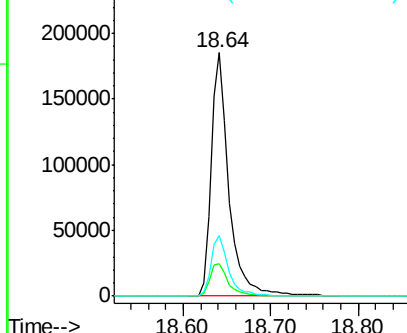



#78

Terphenyl-d14

Concen: 81.20 ng

RT: 17.30 min Scan# 2612

Delta R.T. -0.01 min

Lab File: BF094927.D

Acq: 5 May 2017 20:42

Instrument :

BNA_F

ClientSampleId :

PB98725BL


Tgt Ion:244 Resp: 958963

Ion Ratio Lower Upper

244 100

212 7.4 6.0 9.0




122 13.8 10.3 15.5

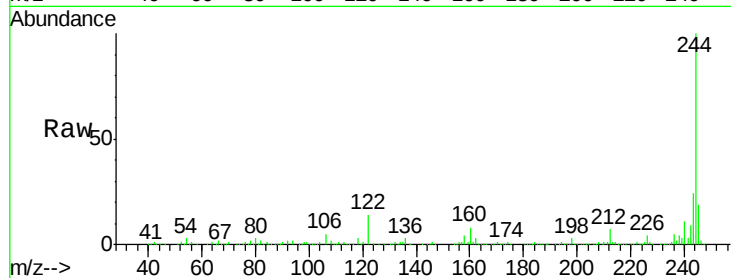

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

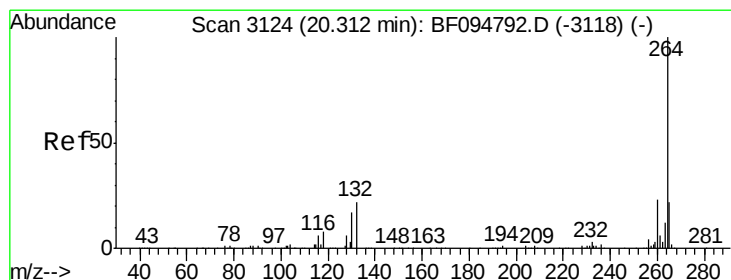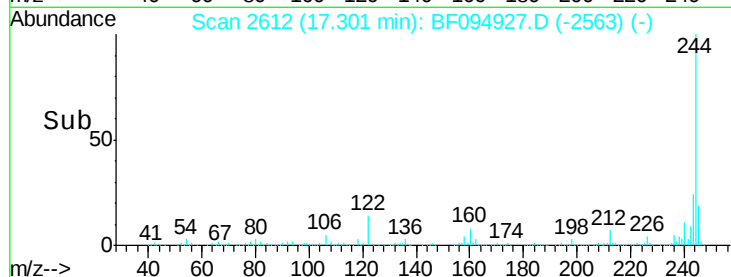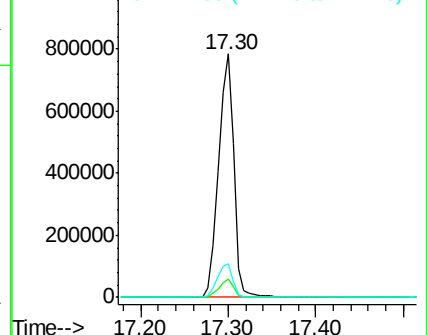

#86

Perylene-d12

Concen: 20.00 ng

RT: 20.31 min Scan# 3123

Delta R.T. -0.01 min

Lab File: BF094927.D

Acq: 5 May 2017 20:42


Tgt Ion:264 Resp: 164090

Ion Ratio Lower Upper

264 100

260 22.8 19.5 29.3

265 21.1 17.2 25.8

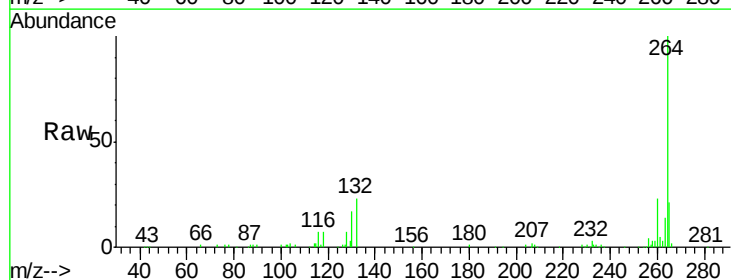

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

