


Data Path : Z:\HPCHEM1\BNA_F\Data\BF050517\
 Data File : BF094919.D
 Acq On : 5 May 2017 16:15
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 03 17:24:51 2017

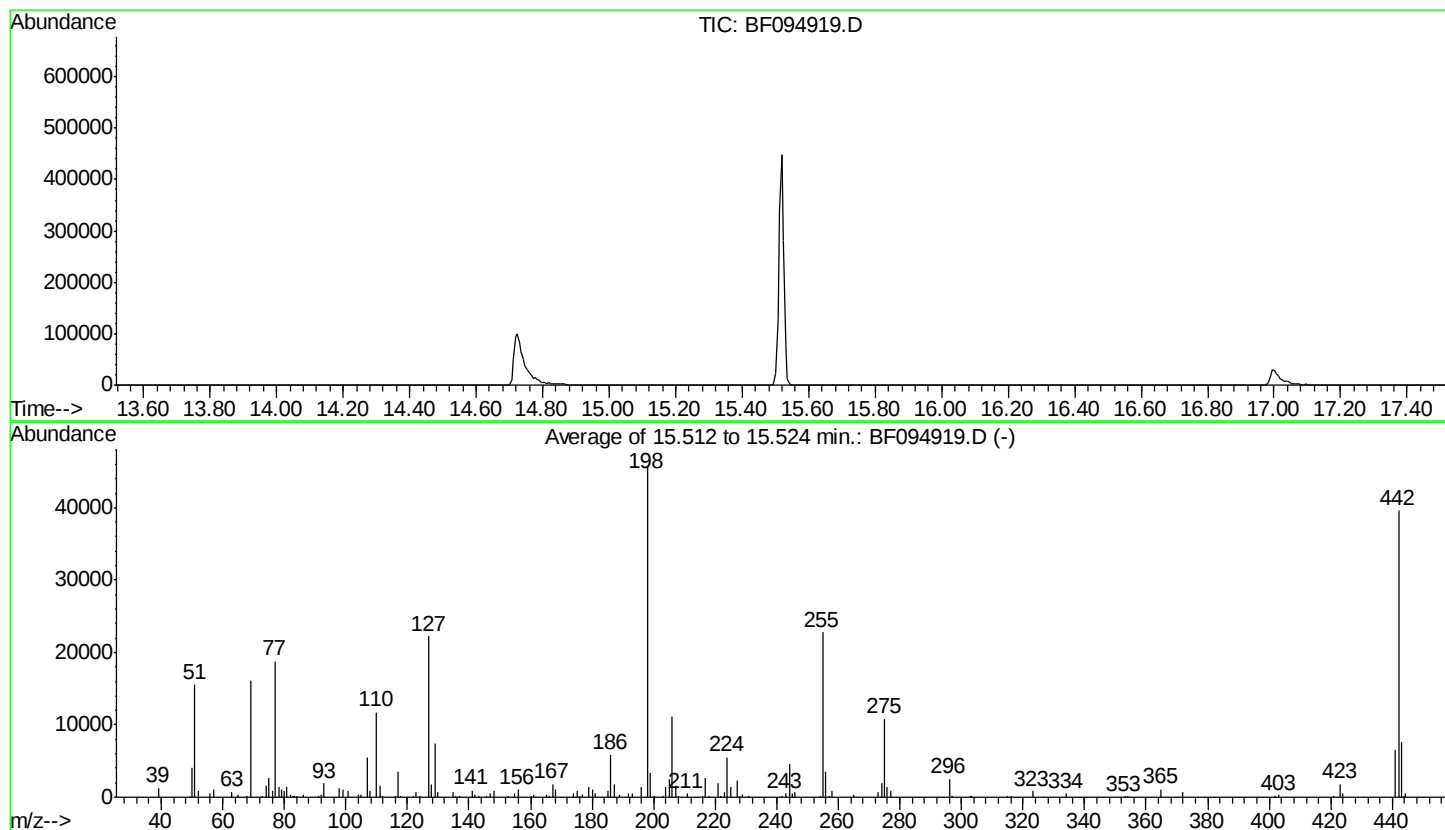

AutoFind: Scans 2308, 2309, 2310; Background Corrected with Scan 2302

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	15502	PASS
68	69	0.00	2	0.9	150	PASS
69	198	0.00	100	35.1	16092	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.5	22221	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45810	PASS
199	198	5	9	7.5	3442	PASS
275	198	10	60	23.6	10831	PASS
365	198	1	100	2.5	1127	PASS
441	442	0.01	24	16.5	6511	PASS
442	198	50	100	86.4	39557	PASS
443	442	15	24	19.2	7580	PASS