
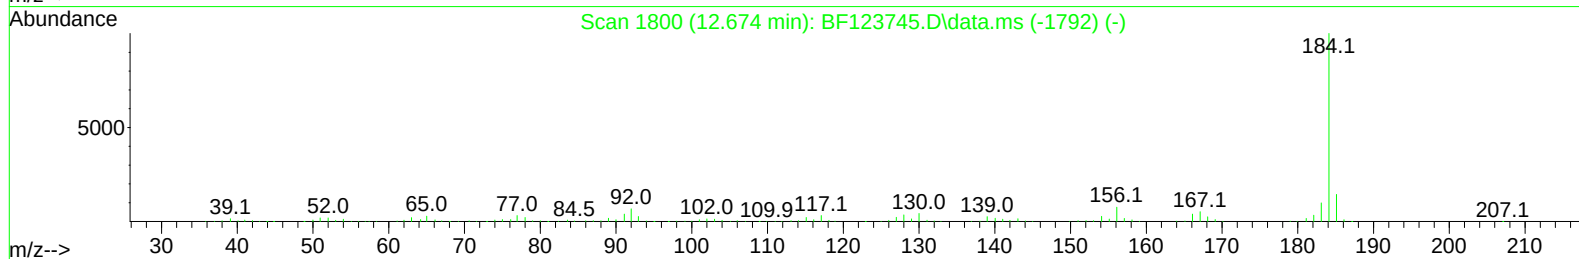
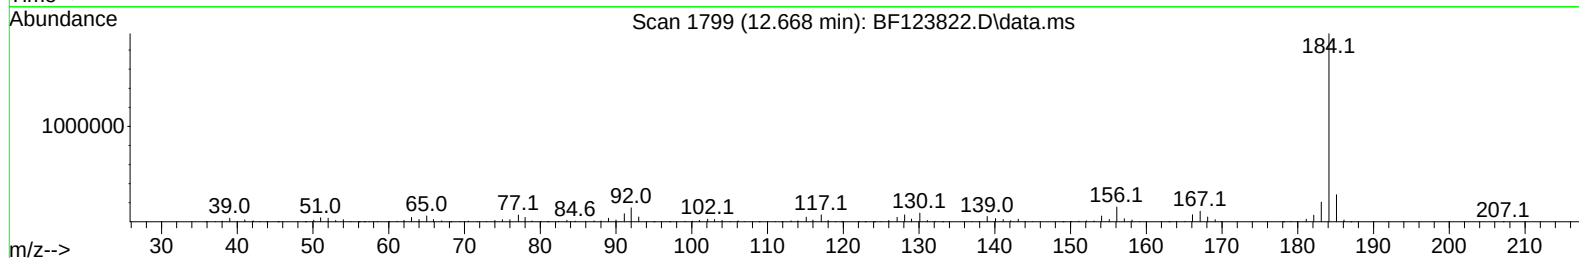


Quant Time: May 05 12:55:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 04 12:58:27 2021
Response via : Initial Calibration

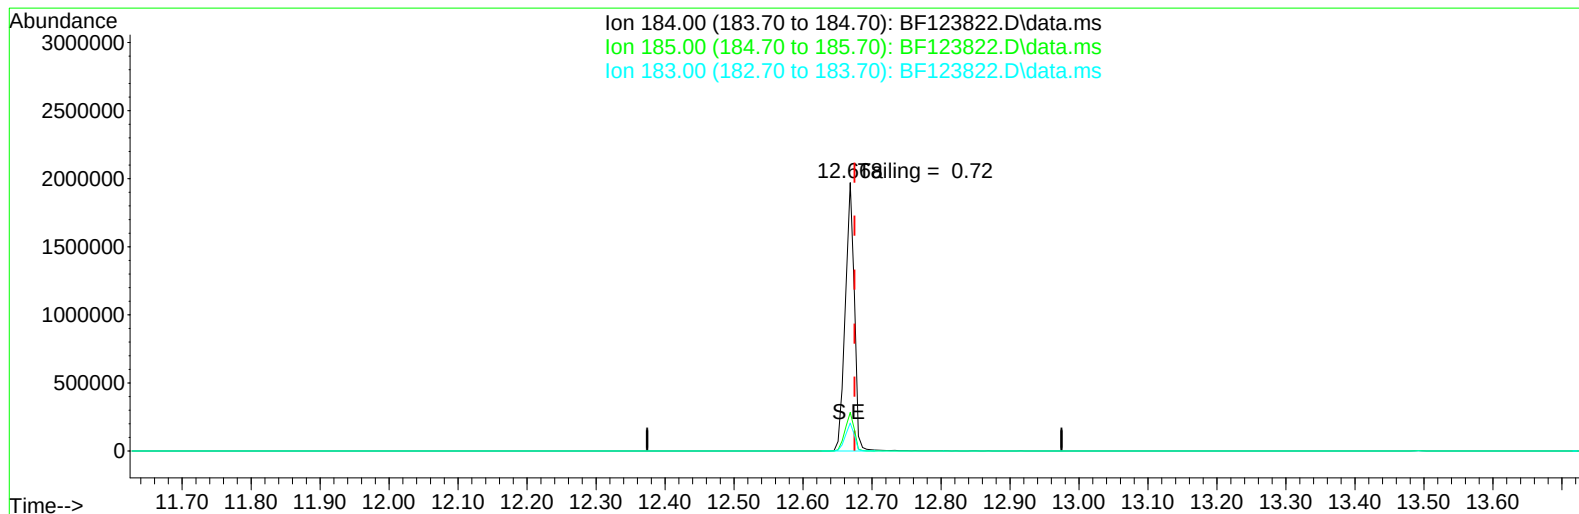

TIC: BF123822.D\data.ms

(77) Benzidine




12.668min (-0.006) 0.00 ng m

response **1788109**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.40
183.00	9.80	10.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050521\
 Data File : BF123822.D
 Acq On : 5 May 2021 12:05
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 05 12:55:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 04 12:58:27 2021
 Response via : Initial Calibration

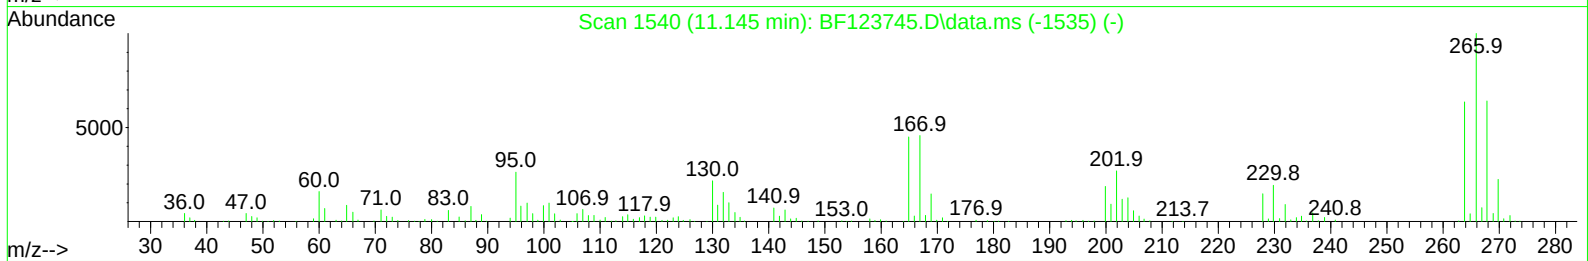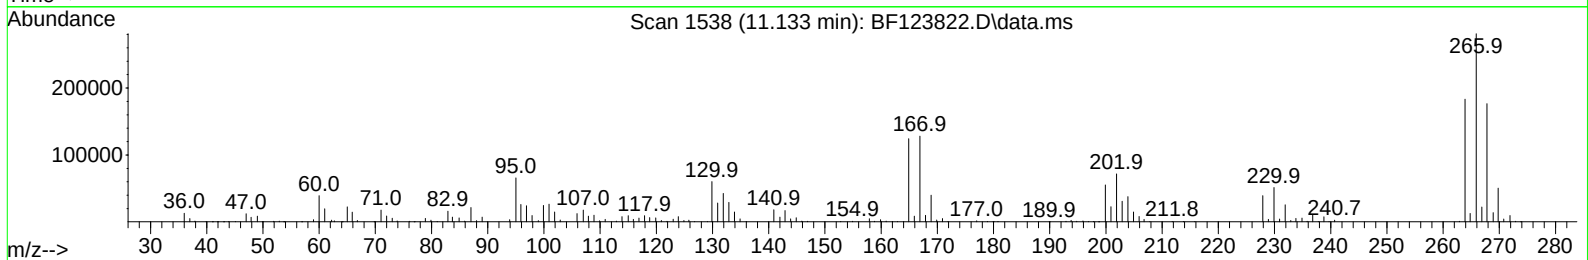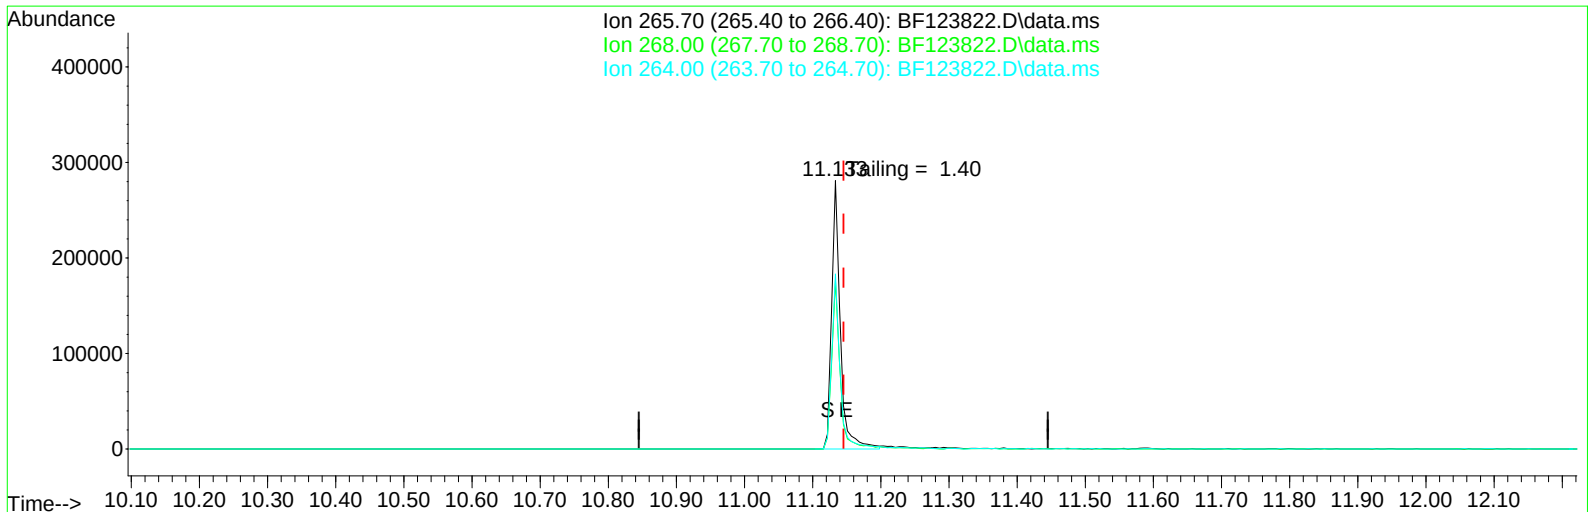

TIC: BF123822.D\data.ms

(70) Pentachlorophenol (C)

11.133min (-0.012) 31545.12 ng

response 253411

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.86
264.00	65.70	65.20
0.00	0.00	0.00