

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050521\
 Data File : BF123839.D
 Acq On : 5 May 2021 21:18
 Operator : JU/CG
 Sample : M2279-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EME-19

Manual Integrations
 APPROVED

mohammad
 5/6/2021 4:51:13 PM

Quant Time: May 06 00:51:48 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 05 13:09:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.792	152	234724	20.00	ng	0.00
21) Naphthalene-d8	8.075	136	891403	20.00	ng	# 0.00
39) Acenaphthene-d10	9.833	164	418810	20.00	ng	0.00
64) Phenanthrene-d10	11.321	188	674981	20.00	ng	0.00
76) Chrysene-d12	13.968	240	466298	20.00	ng	0.00
86) Perylene-d12	15.421	264	351899	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.410	112	1239958	83.69	ng	0.00
7) Phenol-d6	6.433	99	1612330	79.00	ng	0.00
23) Nitrobenzene-d5	7.357	82	1102751	55.85	ng	0.00
42) 2,4,6-Tribromophenol	10.627	330	375287	71.98	ng	0.00
45) 2-Fluorobiphenyl	9.157	172	1668980	58.03	ng	0.00
79) Terphenyl-d14	12.915	244	1297521	53.58	ng	0.00
Target Compounds						
						Qvalue
50) Dimethylphthalate	9.551	163	104082	3.53	ng	99
71) Phenanthrene	11.345	178	358793	10.13	ng	99
72) Anthracene	11.398	178	115551	3.28	ng	99
75) Fluoranthene	12.539	202	509664	13.20	ng	98
78) Pyrene	12.762	202	522024	14.42	ng	98
81) Benzo(a)anthracene	13.957	228	235427	8.33	ng	98
83) Chrysene	13.992	228	198781	6.99	ng	96
87) Indeno(1,2,3-cd)pyrene	16.862	276	74296	3.63	ng	99
88) Benzo(b)fluoranthene	15.004	252	210651m	8.88	ng	
89) Benzo(k)fluoranthene	15.027	252	57008m	2.52	ng	
90) Benzo(a)pyrene	15.362	252	152329	7.51	ng	97
92) Benzo(g,h,i)perylene	17.297	276	68250	3.94	ng	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050521\
Data File : BF123839.D
Acq On : 5 May 2021 21:18
Operator : JU/CG
Sample : M2279-08
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
EME-19

Manual Integrations
APPROVED

mohammad
5/6/2021 4:51:13 PM

Quant Time: May 06 00:51:48 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 05 13:09:28 2021
Response via : Initial Calibration

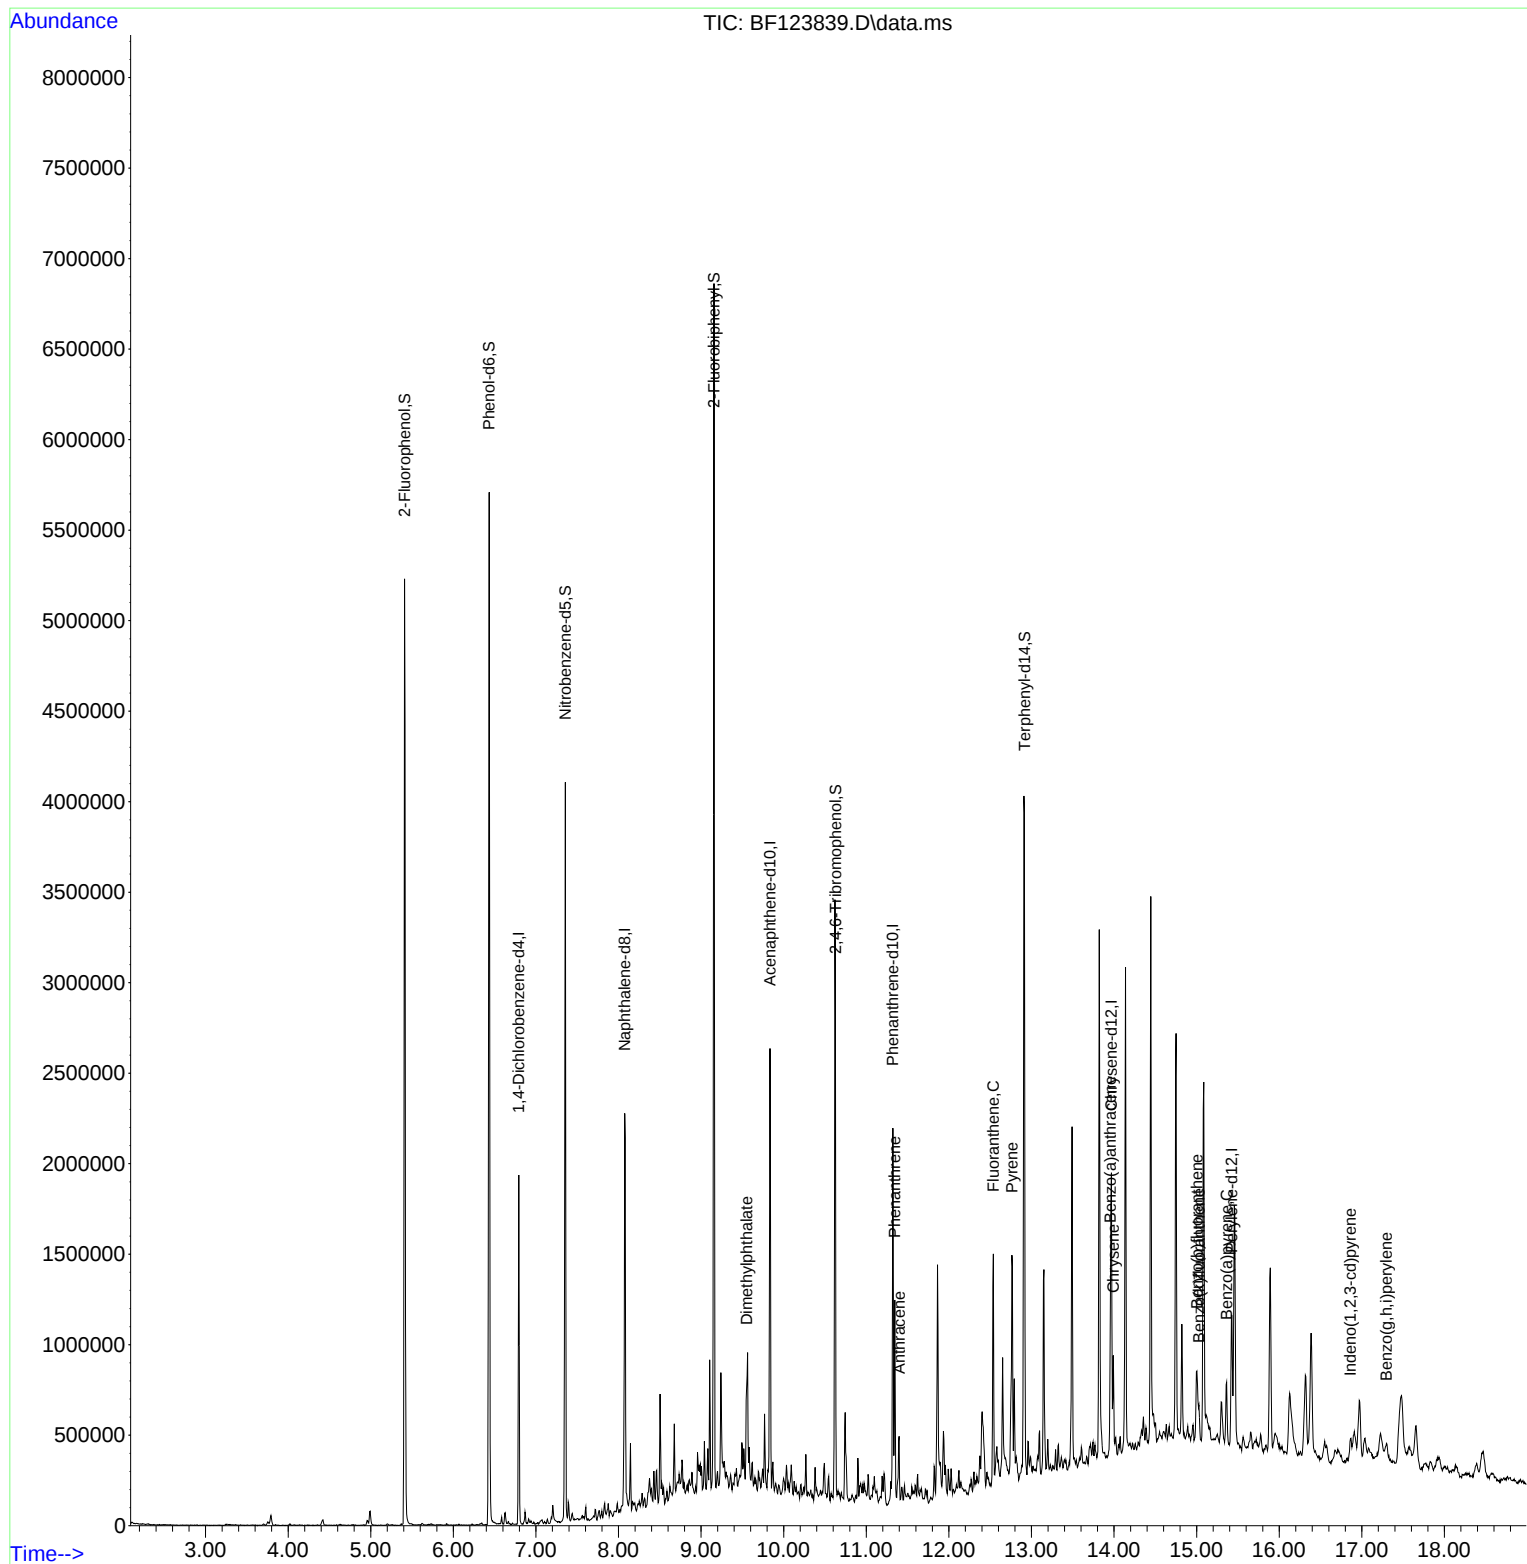

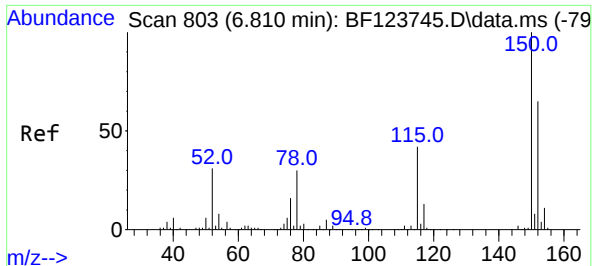





#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.792 min Scan# 800
Delta R.T. -0.006 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18

Tgt Ion:152 Resp: 234724
Ion Ratio Lower Upper
152 100
150 155.1 127.0 190.6
115 61.2 54.3 81.5

Instrument :
BNA_F
ClientSampled :
EME-19




Manual Integrations
APPROVED


mohammad
5/6/2021 4:51:13 PM

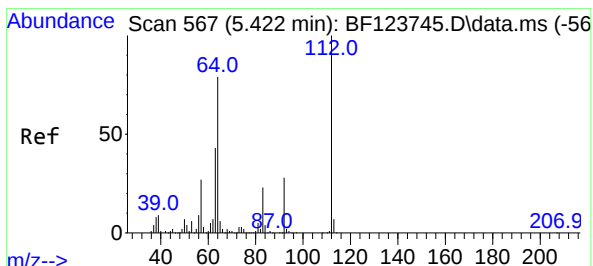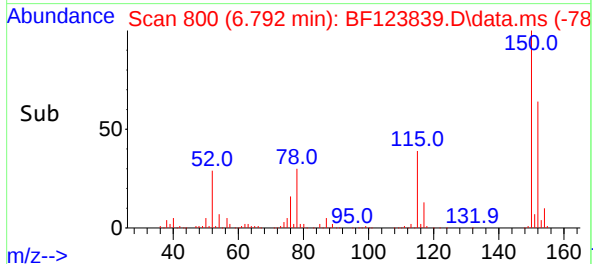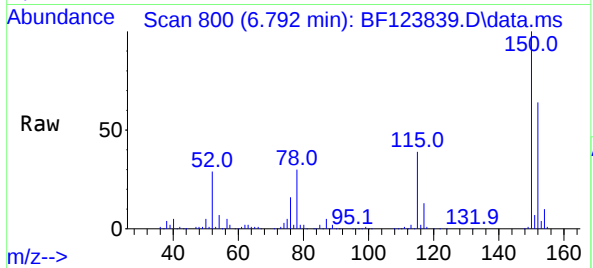

#5
2-Fluorophenol
Concen: 83.69 ng
RT: 5.410 min Scan# 565
Delta R.T. -0.000 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18

Tgt Ion:112 Resp: 1239958
Ion Ratio Lower Upper
112 100
64 78.0 61.4 92.0
63 41.2 33.0 49.4

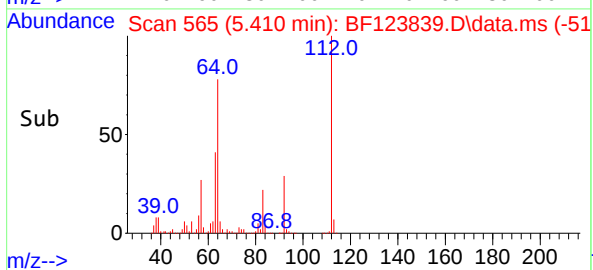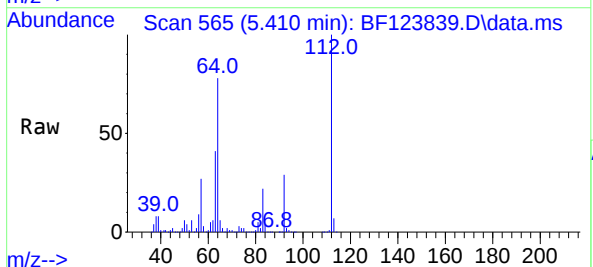



#7
Phenol-d6
Concen: 79.00 ng
RT: 6.433 min Scan# 739
Delta R.T. -0.006 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18





Tgt Ion: 99 Resp: 1612330

Ion	Ratio	Lower	Upper
99	100		
42	23.4	19.8	29.8
71	39.2	31.1	46.7

Instrument :
BNA_F
ClientSampleId :
EME-19

Manual Integrations
APPROVED




mohammad
5/6/2021 4:51:13 PM




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.075 min Scan# 1018
Delta R.T. -0.006 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18

Tgt Ion: 136 Resp: 891403

Ion	Ratio	Lower	Upper
136	100		
137	11.3	8.7	13.1
54	12.8	9.8	14.6
68	6.2	4.1	6.1

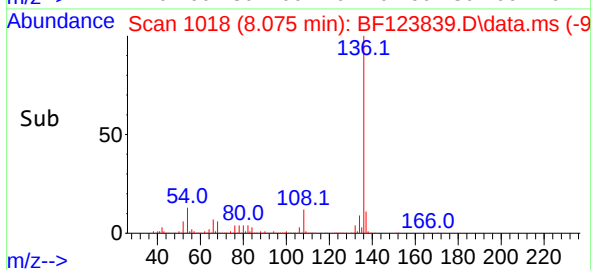

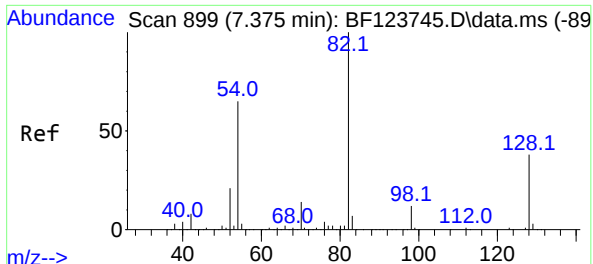

#23
Nitrobenzene-d5
Concen: 55.85 ng
RT: 7.357 min Scan# 896
Delta R.T. -0.006 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18





Tgt Ion: 82 Resp: 1102751

Ion	Ratio	Lower	Upper
82	100		
128	38.9	29.4	44.2
54	63.8	54.1	81.1

Instrument :
BNA_F
ClientSampleId :
EME-19

Manual Integrations
APPROVED




mohammad
5/6/2021 4:51:13 PM

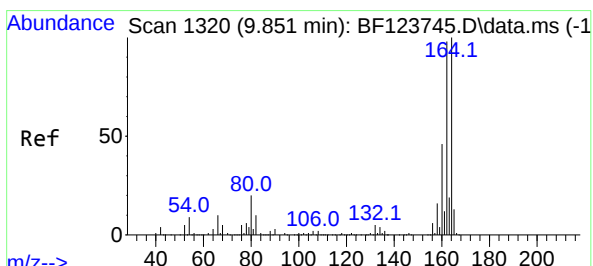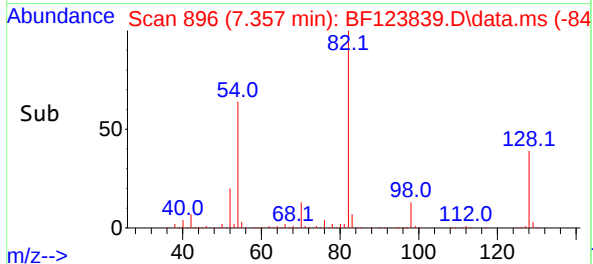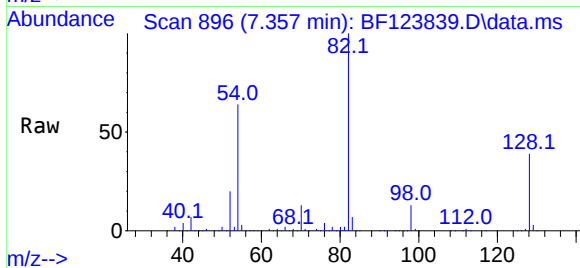


#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.833 min Scan# 1317
Delta R.T. -0.006 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18


Tgt Ion:164 Resp: 418810

Ion	Ratio	Lower	Upper
164	100		
162	98.9	80.7	121.1
160	44.5	37.3	55.9

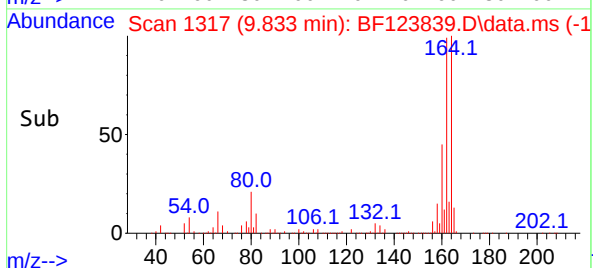

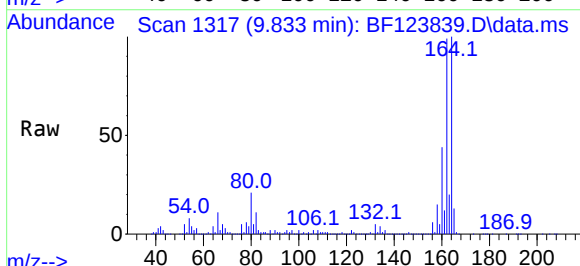





#42
2,4,6-Tribromophenol
Concen: 71.98 ng
RT: 10.627 min Scan# 1452
Delta R.T. -0.006 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18





Tgt Ion: 330 Resp: 375287
Ion Ratio Lower Upper
330 100
332 95.8 77.1 115.7
141 32.4 27.9 41.9

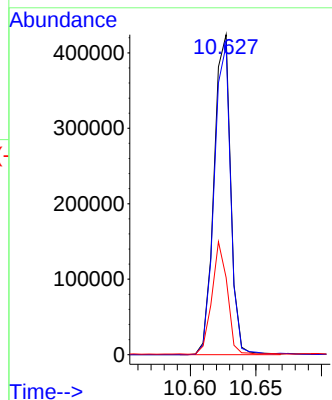

#45
2-Fluorobiphenyl
Concen: 58.03 ng
RT: 9.157 min Scan# 1202
Delta R.T. -0.006 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18

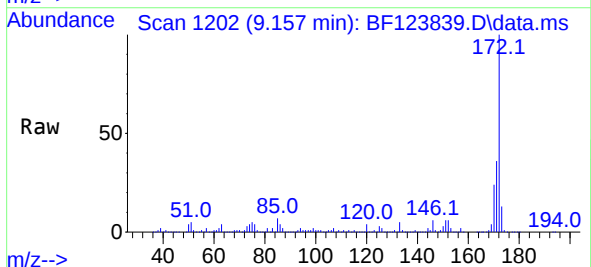


Tgt Ion: 172 Resp: 1668980
Ion Ratio Lower Upper
172 100
171 35.7 28.1 42.1
170 24.0 19.2 28.8

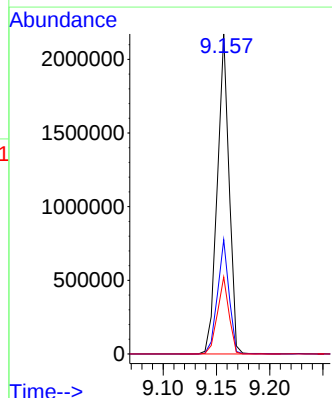

Instrument :
BNA_F
ClientSampleId :
EME-19

Manual Integrations
APPROVED

mohammad
5/6/2021 4:51:13 PM







#50
Dimethylphthalate
Concen: 3.53 ng
RT: 9.551 min Scan# 1269
Delta R.T. -0.012 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18

Tgt Ion:163 Resp: 104082
Ion Ratio Lower Upper
163 100
194 4.1 3.1 4.7
164 10.0 8.2 12.2

Instrument :
BNA_F
ClientSampleId :
EME-19




Manual Integrations
APPROVED


mohammad
5/6/2021 4:51:13 PM

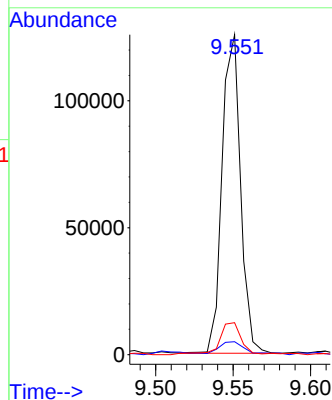

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.321 min Scan# 1570
Delta R.T. -0.006 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18


Tgt Ion:188 Resp: 674981
Ion Ratio Lower Upper
188 100
94 9.4 6.9 10.3
80 10.0 8.2 12.2

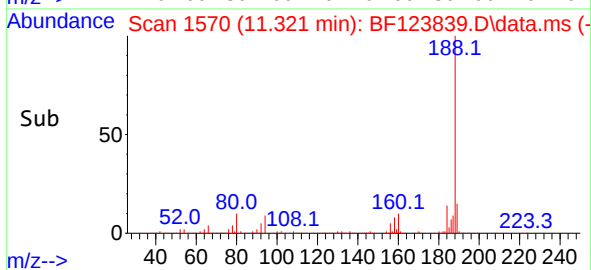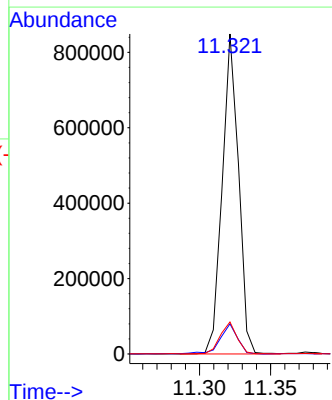



#71
Phenanthrene
Concen: 10.13 ng
RT: 11.345 min Scan# 1574
Delta R.T. -0.006 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18




Instrument :
BNA_F
ClientSampled :
EME-19




Tgt Ion:178 Resp: 358793
Ion Ratio Lower Upper
178 100
176 18.4 15.6 23.4
179 15.6 12.5 18.7

Manual Integrations
APPROVED



mohammad
5/6/2021 4:51:13 PM

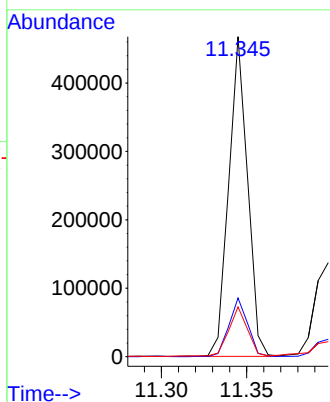


#72
Anthracene
Concen: 3.28 ng
RT: 11.398 min Scan# 1583
Delta R.T. -0.006 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18



Tgt Ion:178 Resp: 115551
Ion Ratio Lower Upper
178 100
176 18.5 15.4 23.0
179 16.0 12.6 18.8









#75
Fluoranthene
Concen: 13.20 ng
RT: 12.539 min Scan# 1777
Delta R.T. -0.006 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18

Tgt Ion:	202	Resp:	509664
Ion Ratio	Lower	Upper	
202	100		
101	9.8	0.0	30.9
203	17.9	0.0	37.5

Instrument :
BNA_F
ClientSampled :
EME-19




Manual Integrations
APPROVED


mohammad
5/6/2021 4:51:13 PM

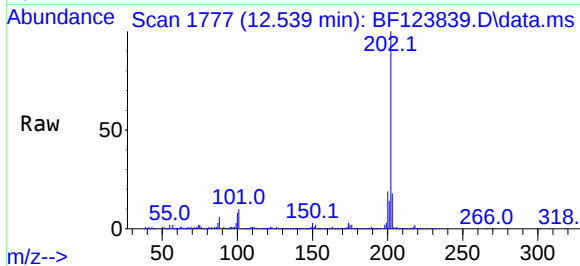

#76
Chrysene-d12
Concen: 20.00 ng
RT: 13.968 min Scan# 2020
Delta R.T. -0.006 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18

Tgt Ion:	240	Resp:	466298
Ion Ratio	Lower	Upper	
240	100		
120	9.5	7.2	10.8
236	23.1	19.0	28.4

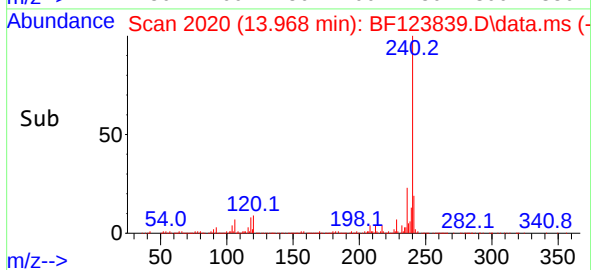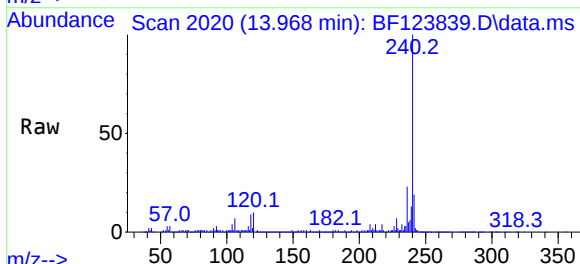







#78
Pyrene
Concen: 14.42 ng
RT: 12.762 min Scan# 1815
Delta R.T. -0.012 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18

Tgt Ion:	202	Resp:	522024
Ion Ratio	Lower	Upper	
202	100		
200	18.8	16.1	24.1
203	18.2	14.8	22.2

Instrument :
BNA_F
ClientSampled :
EME-19




Manual Integrations
APPROVED


mohammad
5/6/2021 4:51:13 PM




#79
Terphenyl-d14
Concen: 53.58 ng
RT: 12.915 min Scan# 1841
Delta R.T. -0.000 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18

Tgt Ion:	244	Resp:	1297521
Ion Ratio	Lower	Upper	
244	100		
212	7.0	5.7	8.5
122	9.0	9.7	14.5#

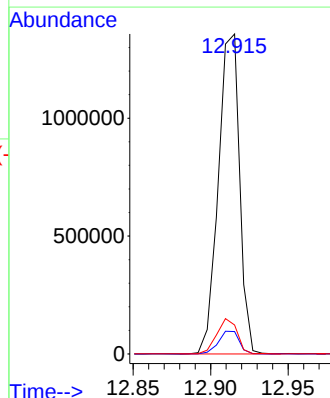



#81
Benzo(a)anthracene
Concen: 8.33 ng
RT: 13.957 min Scan# 2018
Delta R.T. -0.006 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18






Tgt Ion:228 Resp: 235427
Ion Ratio Lower Upper
228 100
226 28.5 22.4 33.6
229 21.5 16.0 24.0


Instrument :
BNA_F
ClientSampled :
EME-19

Manual Integrations
APPROVED



mohammad
5/6/2021 4:51:13 PM

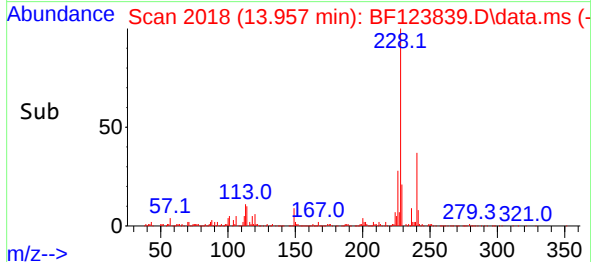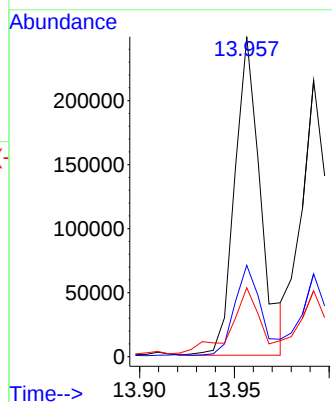


#83
Chrysene
Concen: 6.99 ng
RT: 13.992 min Scan# 2024
Delta R.T. -0.012 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18




Tgt Ion:228 Resp: 198781
Ion Ratio Lower Upper
228 100
226 30.0 24.3 36.5
229 23.8 16.2 24.2

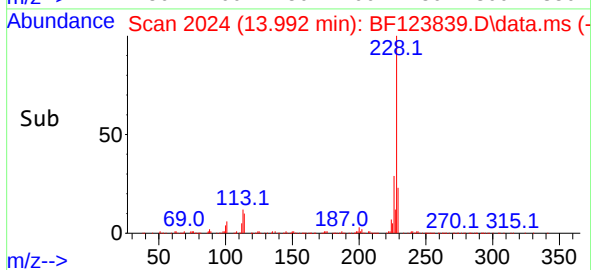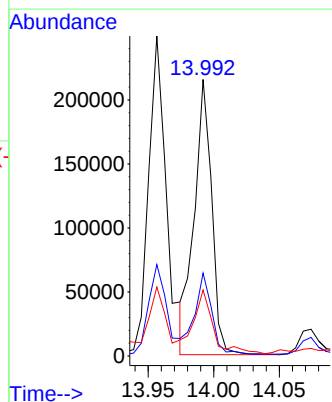



#86
Perylene-d12
Concen: 20.00 ng
RT: 15.421 min Scan# 2267
Delta R.T. -0.006 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18




Instrument :
BNA_F
ClientSampled :
EME-19

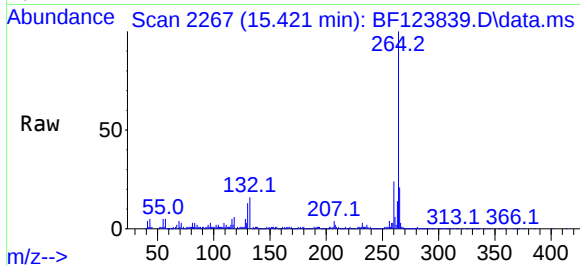


Tgt Ion:264 Resp: 351899
Ion Ratio Lower Upper
264 100
260 23.8 18.7 28.1
265 21.4 17.8 26.8

Manual Integrations
APPROVED



mohammad
5/6/2021 4:51:13 PM




#87
Indeno(1,2,3-cd)pyrene
Concen: 3.63 ng
RT: 16.862 min Scan# 2512
Delta R.T. -0.018 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18

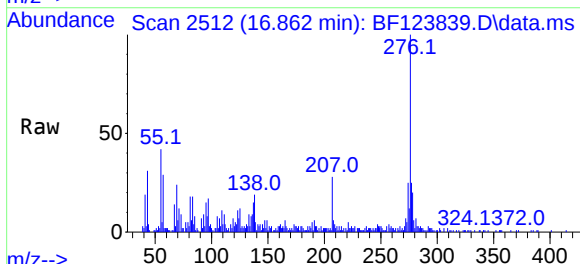


Tgt Ion:276 Resp: 74296
Ion Ratio Lower Upper
276 100
138 20.7 16.2 24.2
277 25.2 20.1 30.1









#88
Benzo(b)fluoranthene
Concen: 8.88 ng m
RT: 15.004 min Scan# 2196
Delta R.T. -0.006 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18





Tgt Ion:252 Resp: 210651
Ion Ratio Lower Upper
252 100
253 23.5 18.1 27.1
125 13.1 6.2 9.4#

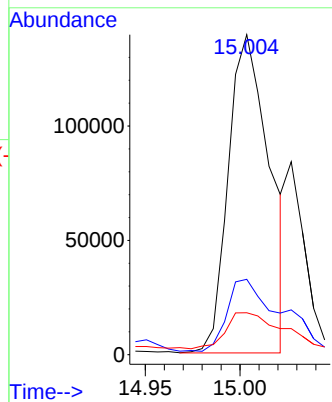

#89
Benzo(k)fluoranthene
Concen: 2.52 ng m
RT: 15.027 min Scan# 2200
Delta R.T. -0.012 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18

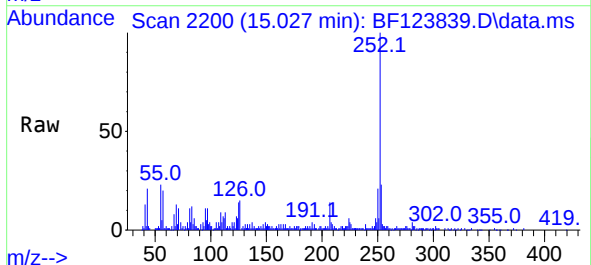


Tgt Ion:252 Resp: 57008
Ion Ratio Lower Upper
252 100
253 23.2 17.9 26.9
125 13.5 7.0 10.6#

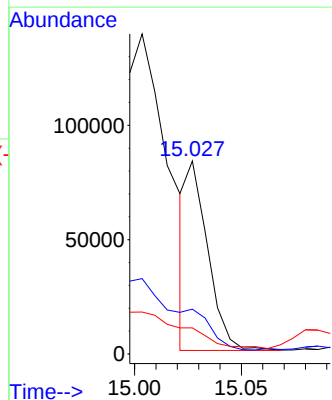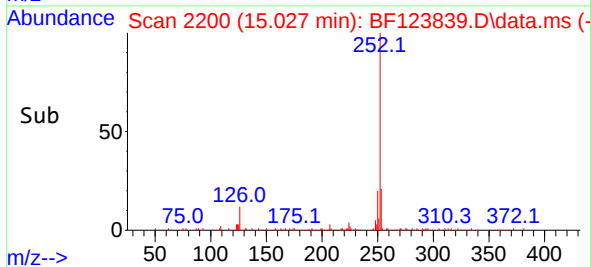

Instrument :
BNA_F
ClientSampled :
EME-19

Manual Integrations
APPROVED

mohammad
5/6/2021 4:51:13 PM







#90
Benzo(a)pyrene
Concen: 7.51 ng
RT: 15.362 min Scan# 2257
Delta R.T. -0.006 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18

Tgt Ion:	252	Resp:	152329
Ion Ratio	Lower	Upper	
252	100		
253	21.5	18.4	27.6
125	11.1	8.0	12.0

Instrument :
BNA_F
ClientSampled :
EME-19

Manual Integrations
APPROVED

mohammad
5/6/2021 4:51:13 PM

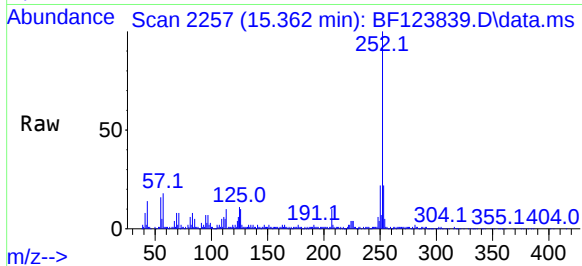

#92
Benzo(g,h,i)perylene
Concen: 3.94 ng
RT: 17.297 min Scan# 2586
Delta R.T. -0.018 min
Lab File: BF123839.D
Acq: 5 May 2021 21:18

Tgt Ion:	276	Resp:	68250
Ion Ratio	Lower	Upper	
276	100		
277	26.9	18.2	27.2
138	17.9	13.8	20.6

