
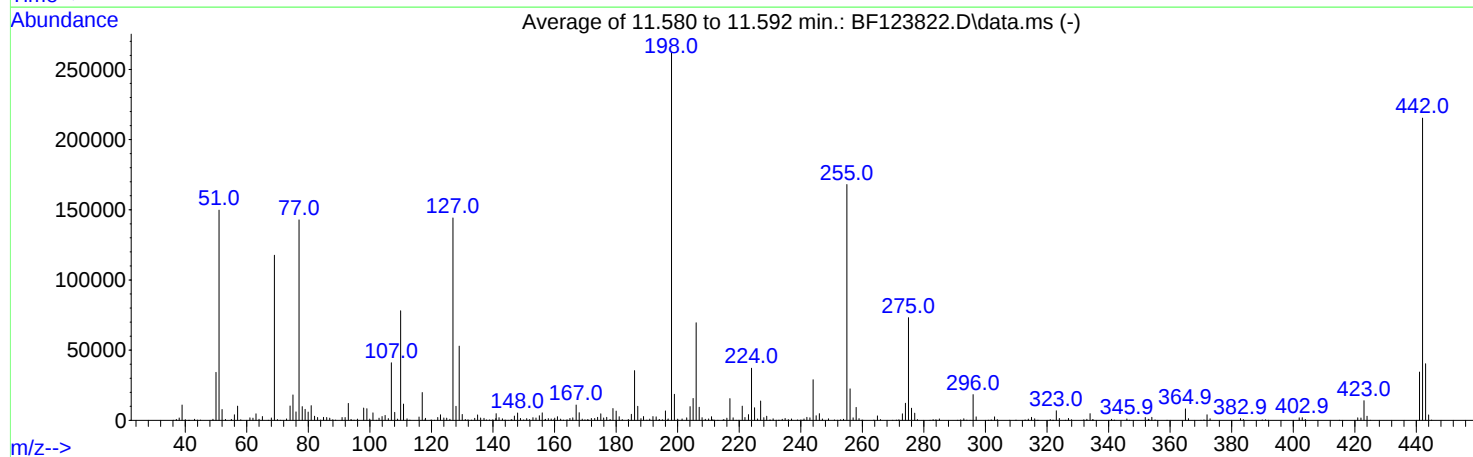


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050521\
 Data File : BF123822.D
 Acq On : 5 May 2021 12:05
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 05 13:09:28 2021

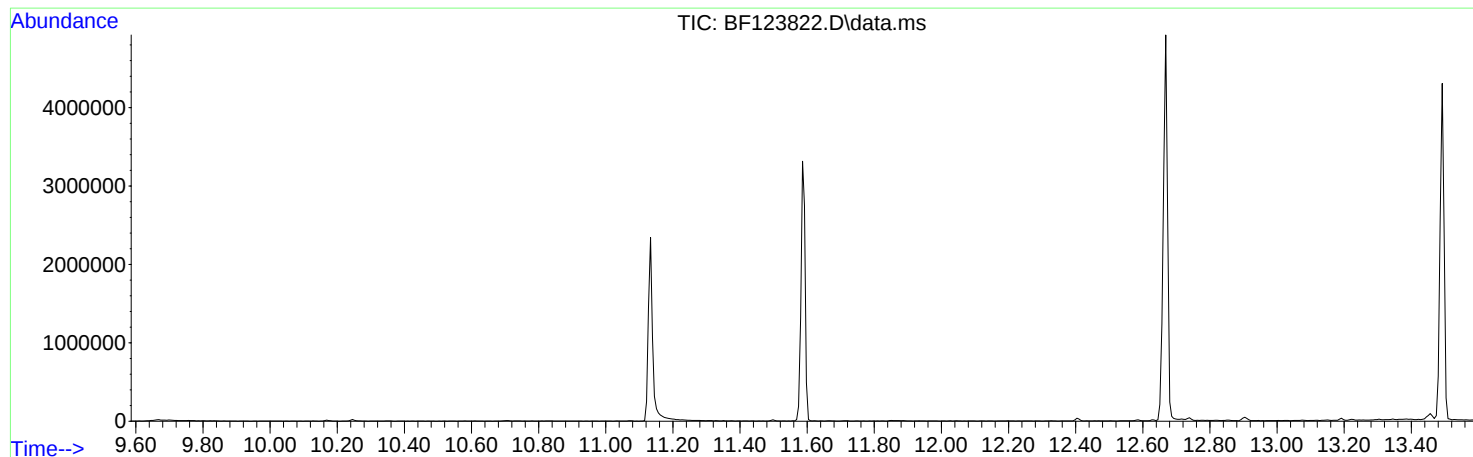




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.1	149763	PASS
68	69	0.00	2	1.5	1764	PASS
69	198	0.00	100	44.9	117635	PASS
70	69	0.00	2	0.5	624	PASS
127	198	10	80	55.0	144216	PASS
197	198	0.00	2	0.4	1027	PASS
198	198	100	100	100.0	262059	PASS
199	198	5	9	7.1	18581	PASS
275	198	10	60	27.9	73189	PASS
365	198	1	100	3.2	8270	PASS
441	198	0.01	100	13.1	34459	PASS
442	442	50	100	100.0	215355	PASS
443	442	15	24	18.7	40312	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050521\
 Data File : BF123822.D
 Acq On : 5 May 2021 12:05
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 05 12:55:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 04 12:58:27 2021
 Response via : Initial Calibration

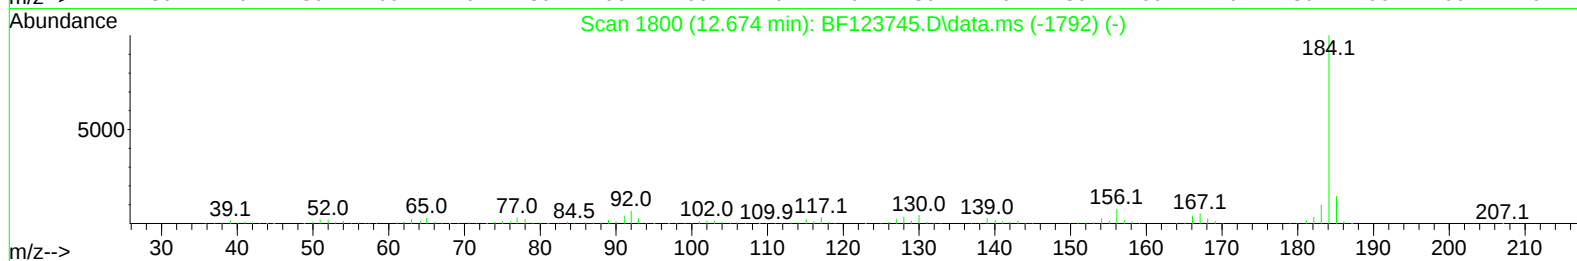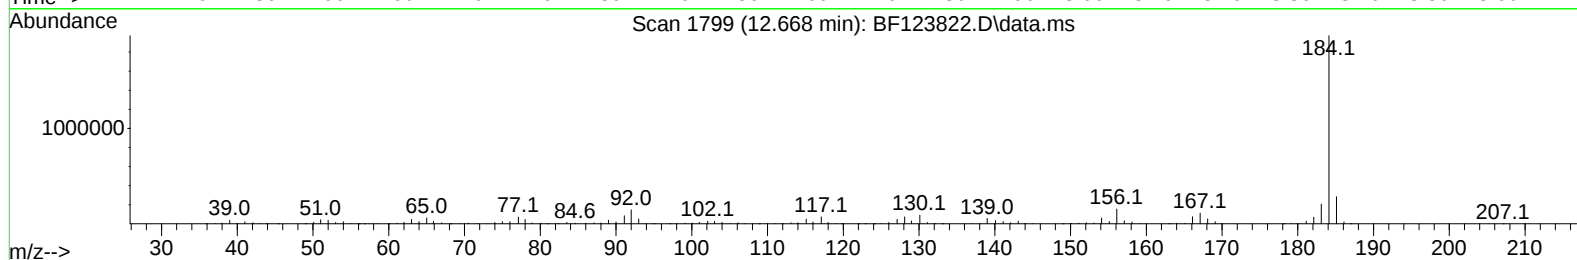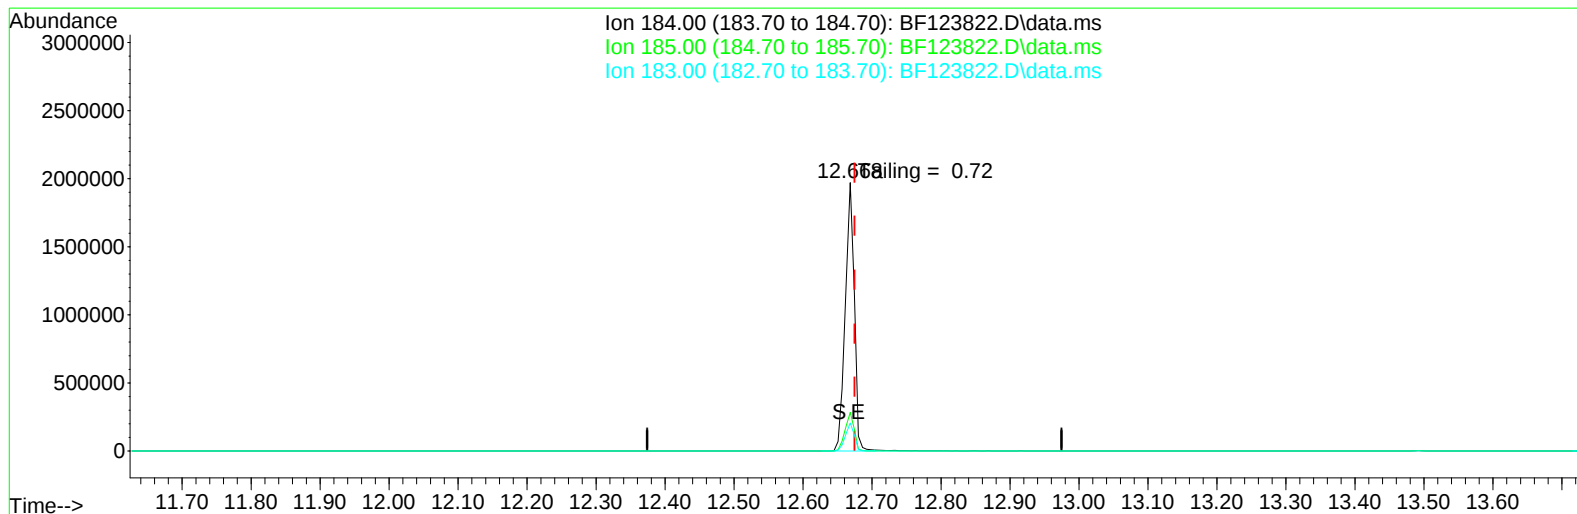

TIC: BF123822.D\data.ms

(77) Benzidine

12.668min (-0.006) 0.00 ng m




response 1788109

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.40
183.00	9.80	10.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050521\
 Data File : BF123822.D
 Acq On : 5 May 2021 12:05
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 05 12:55:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 04 12:58:27 2021
 Response via : Initial Calibration

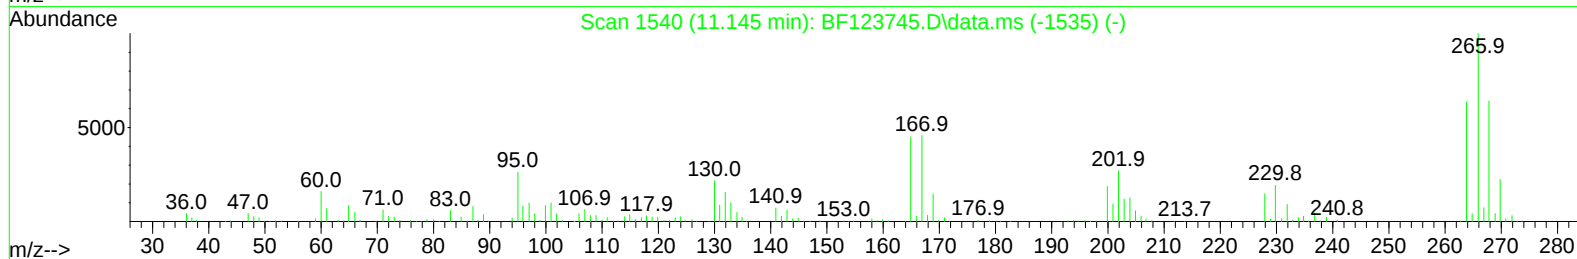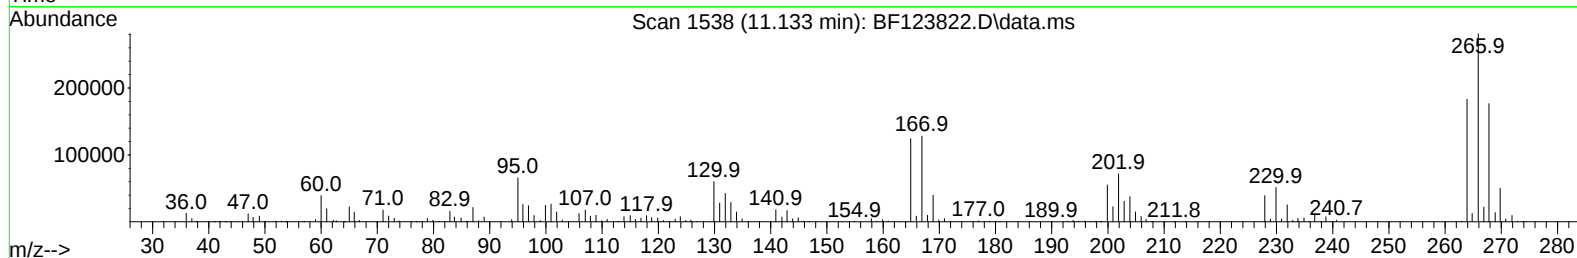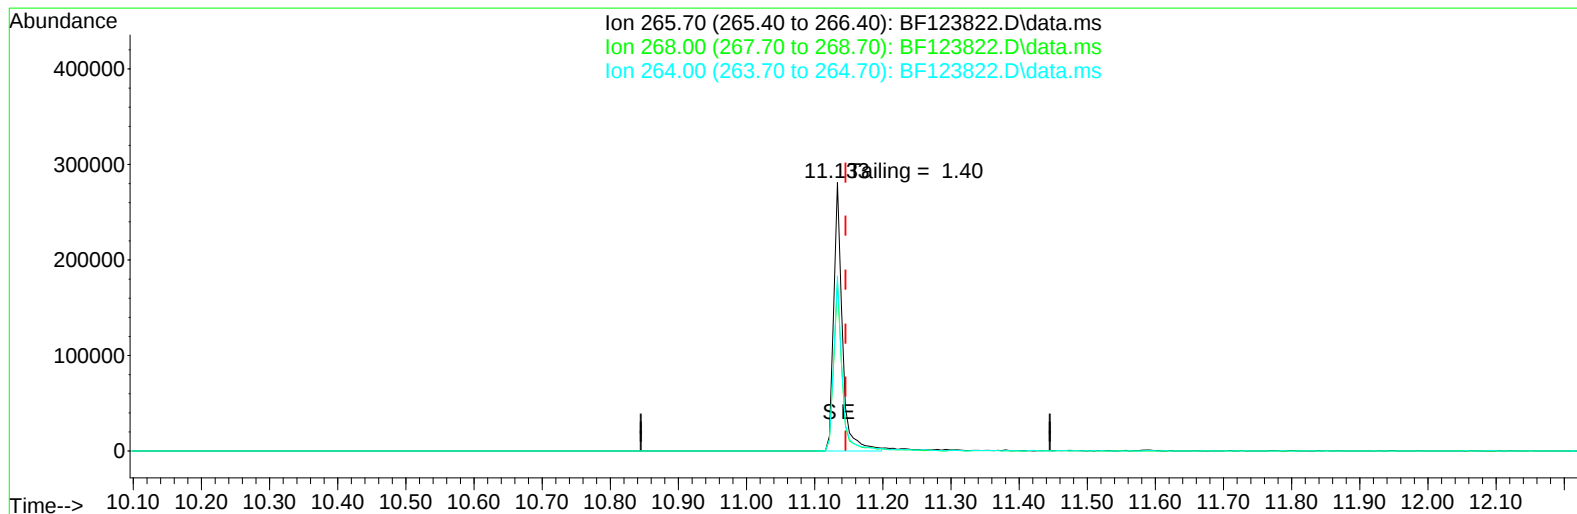

TIC: BF123822.D\data.ms

(70) Pentachlorophenol (C)

11.133min (-0.012) 31545.12 ng

response 253411

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.86
264.00	65.70	65.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
05/05/2021	BNA_F	<u>BF123822.D</u>
Compound Name	Response	Retention Time
DDT	682662	13.49
DDD	4238	13.19
DDE	1402	12.85
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5640	688302	0.82