

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050522\
 Data File : BF128106.D
 Acq On : 05 May 2022 20:50
 Operator : CG\JU
 Sample : N2703-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-28

Quant Time: May 06 05:02:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 05 17:56:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.904	152	87345	20.000	ng	0.00
21) Naphthalene-d8	8.187	136	344812	20.000	ng	-0.01
39) Acenaphthene-d10	9.945	164	197225	20.000	ng	0.00
64) Phenanthrene-d10	11.434	188	345342	20.000	ng	-0.01
76) Chrysene-d12	14.080	240	197996	20.000	ng	-0.01
86) Perylene-d12	15.580	264	195723	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.528	112	565852	103.186	ng	0.00
7) Phenol-d6	6.534	99	735630	103.383	ng	-0.01
23) Nitrobenzene-d5	7.469	82	529029	72.147	ng	-0.01
42) 2,4,6-Tribromophenol	10.739	330	214136	107.855	ng	0.00
45) 2-Fluorobiphenyl	9.263	172	906424	77.751	ng	0.00
79) Terphenyl-d14	13.022	244	843790	77.927	ng	-0.01


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050522\
Data File : BF128106.D
Acq On : 05 May 2022 20:50
Operator : CG\JU
Sample : N2703-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-28

Quant Time: May 06 05:02:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 17:56:23 2022
Response via : Initial Calibration



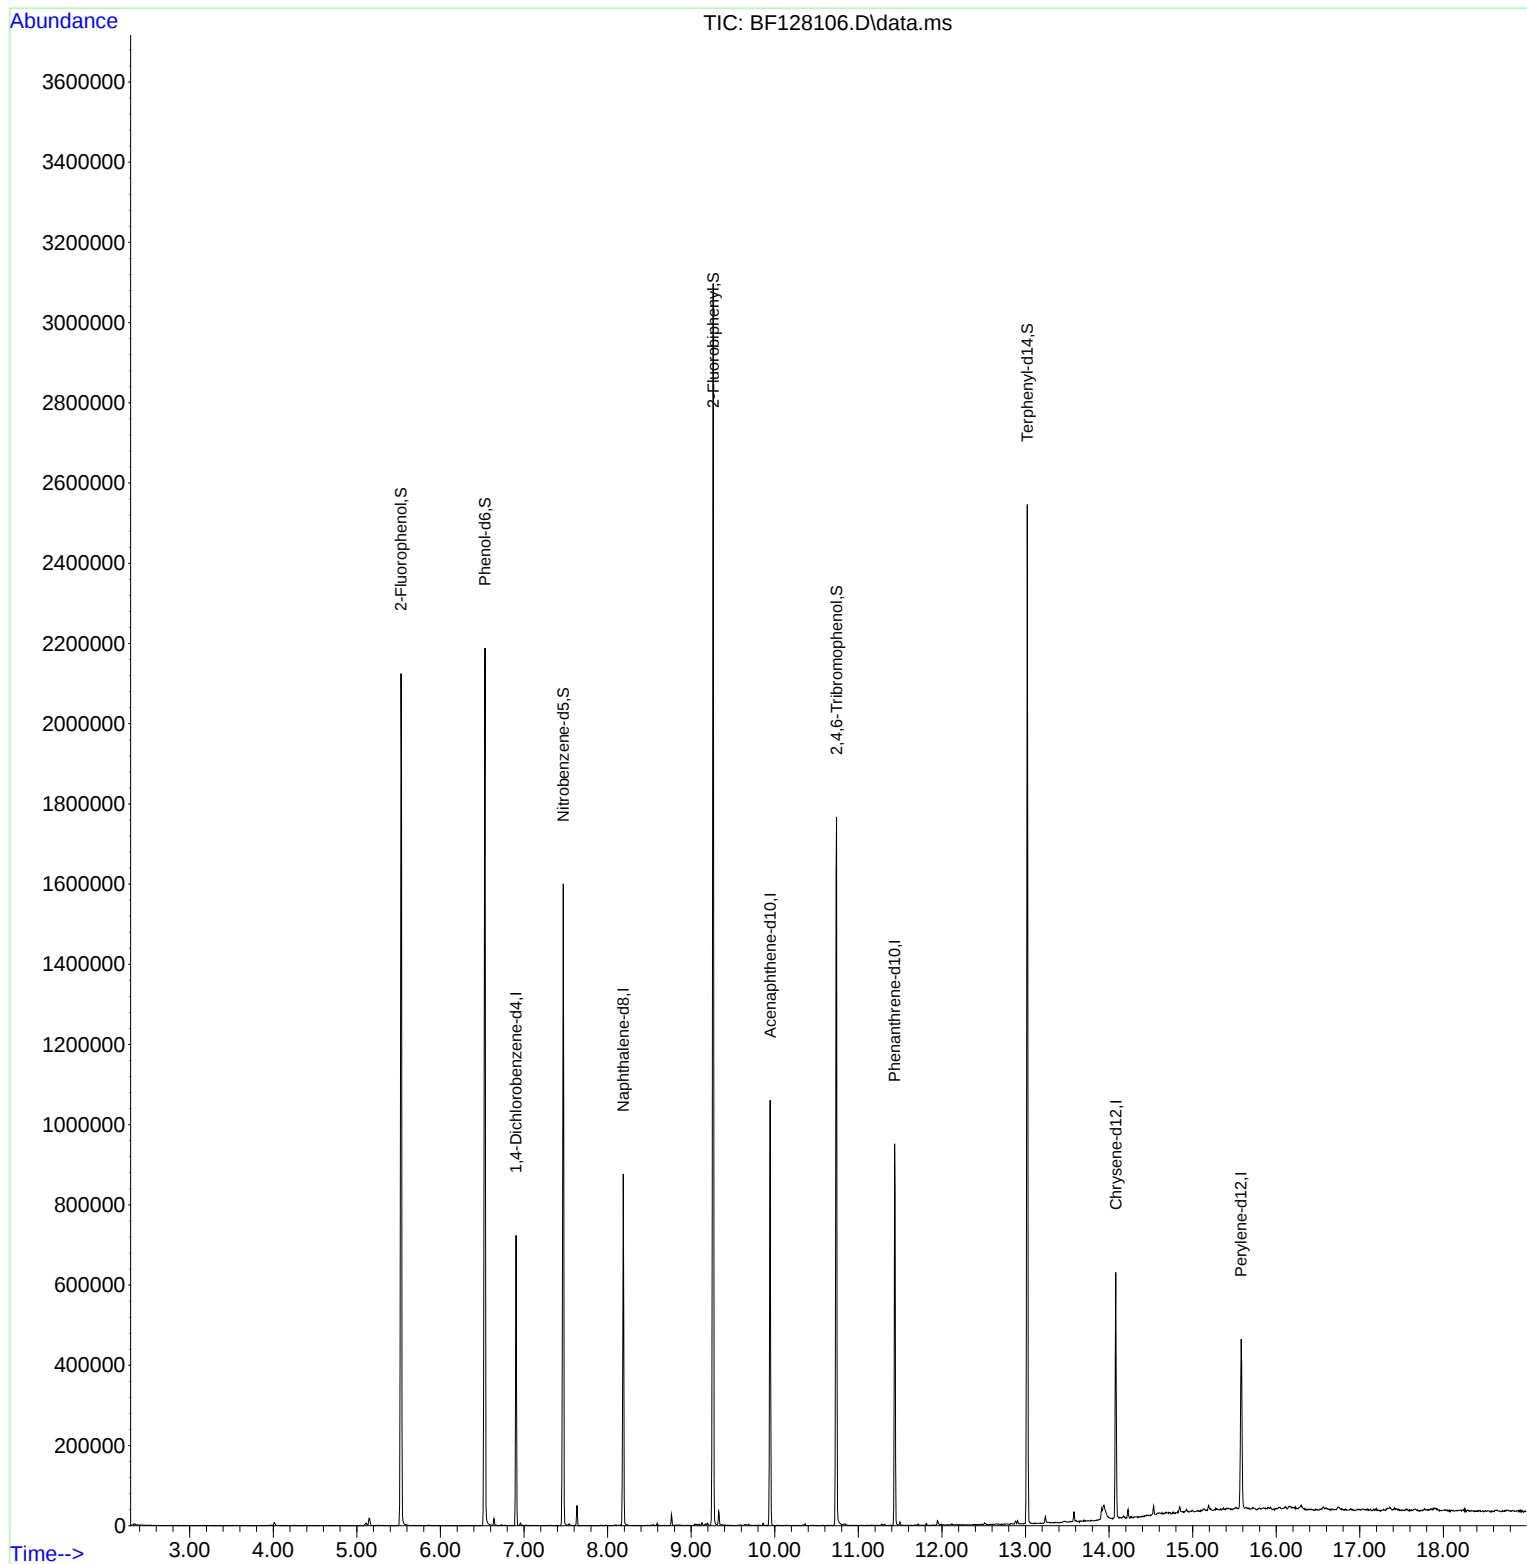




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.904 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF128106.D
Acq: 05 May 2022 20:50




Instrument :
BNA_F
ClientSampleId :
TP-28

Tgt Ion:152 Resp: 87345
Ion Ratio Lower Upper
152 100
150 160.0 125.3 187.9
115 66.1 48.8 73.2

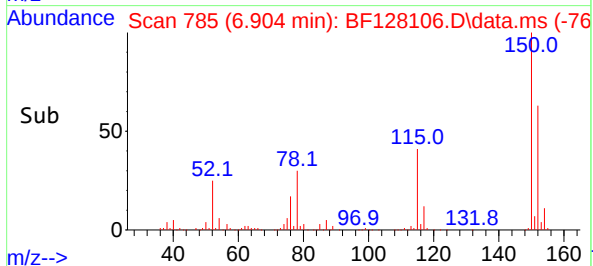
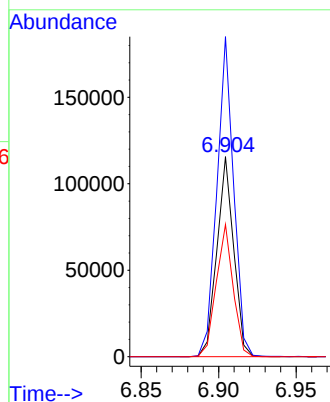
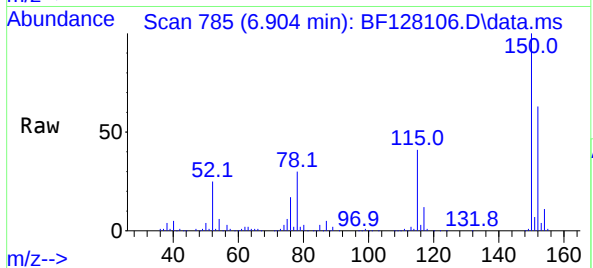


#5
2-Fluorophenol
Concen: 103.186 ng
RT: 5.528 min Scan# 551
Delta R.T. -0.006 min
Lab File: BF128106.D
Acq: 05 May 2022 20:50

Tgt Ion:112 Resp: 565852
Ion Ratio Lower Upper
112 100
64 66.8 49.5 74.3
63 36.2 26.3 39.5

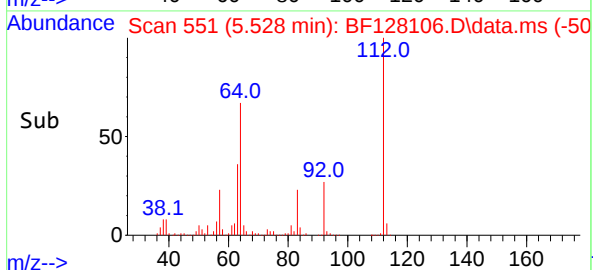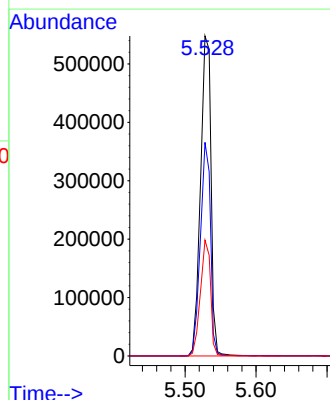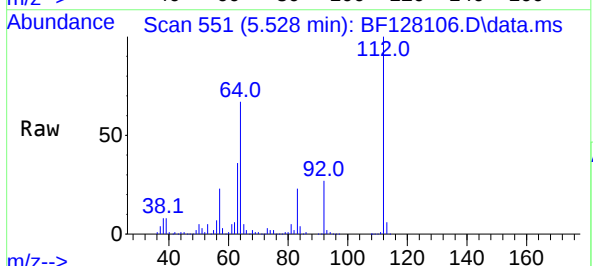

Abundance Scan 728 (6.569 min): BF127861.D\data.ms (-72

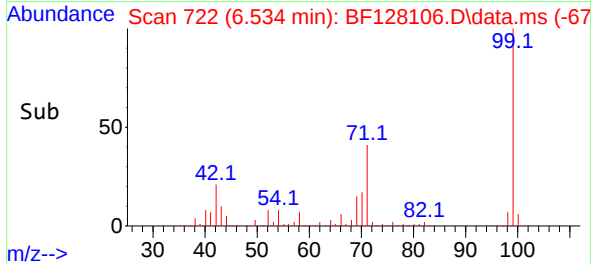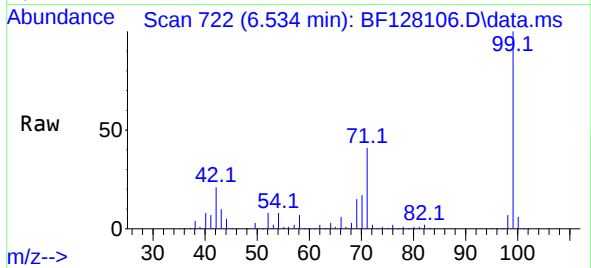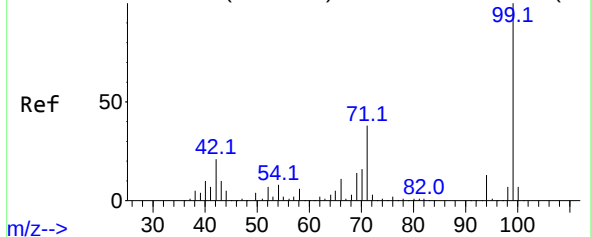

#7

Phenol-d6

Concen: 103.383 ng

RT: 6.534 min Scan# 71

Delta R.T. -0.012 min

Lab File: BF128106.D

Acq: 05 May 2022 20:50

Instrument :

BNA_F

ClientSampleId :

TP-28


Tgt Ion: 99 Resp: 735630

Ion Ratio Lower Upper




99 100

42 21.4 16.6 24.8

71 40.6 30.0 45.0

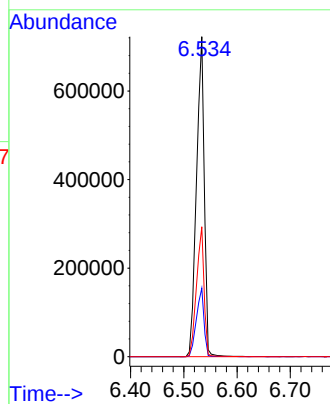

Abundance Scan 1010 (8.228 min): BF127861.D\data.ms (-1

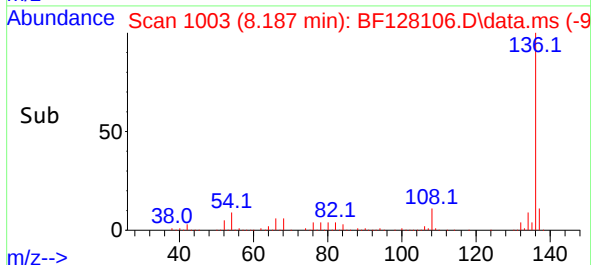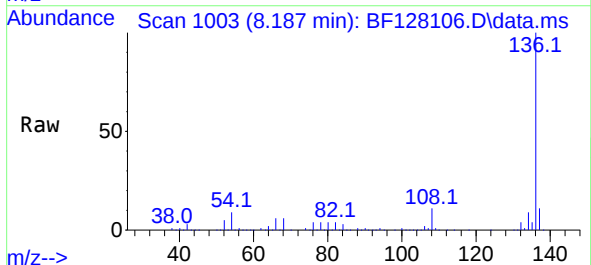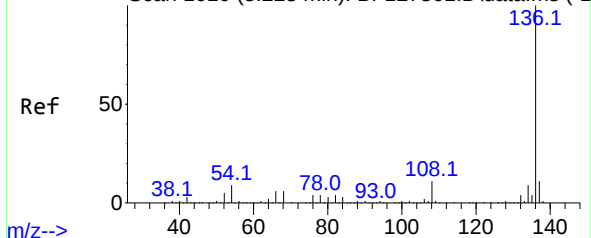

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.187 min Scan# 1003

Delta R.T. -0.012 min

Lab File: BF128106.D

Acq: 05 May 2022 20:50

Tgt Ion: 136 Resp: 344812


Ion Ratio Lower Upper

136 100

137 10.8 8.6 13.0

54 8.7 6.8 10.2

68 5.9 5.1 7.7




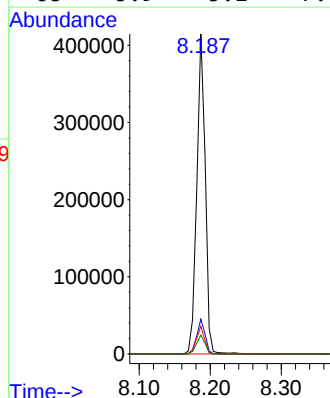




#23
Nitrobenzene-d5
Concen: 72.147 ng
RT: 7.469 min Scan# 81
Delta R.T. -0.012 min
Lab File: BF128106.D
Acq: 05 May 2022 20:50




Instrument :
BNA_F
ClientSampleId :
TP-28


Tgt Ion: 82 Resp: 529029
Ion Ratio Lower Upper
82 100
128 36.7 30.0 45.0
54 52.0 41.3 61.9

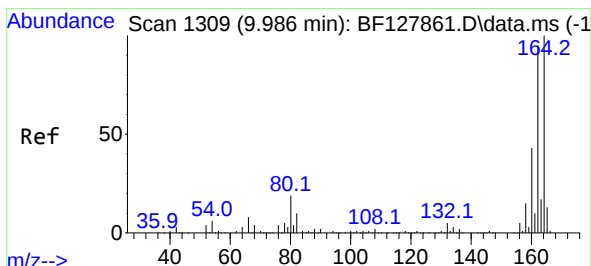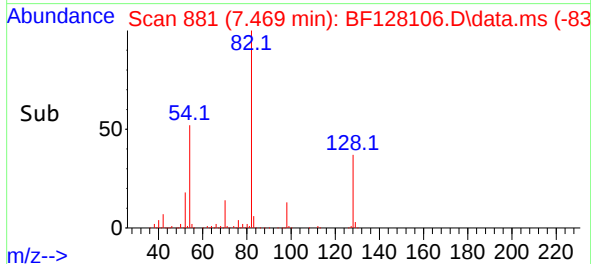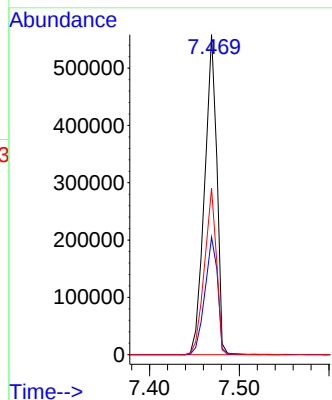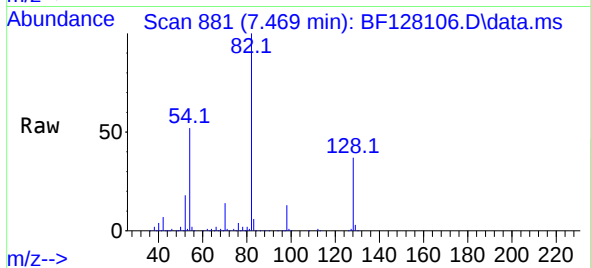

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.945 min Scan# 1302
Delta R.T. -0.006 min
Lab File: BF128106.D
Acq: 05 May 2022 20:50

Tgt Ion: 164 Resp: 197225
Ion Ratio Lower Upper
164 100
162 95.9 76.0 114.0
160 43.6 34.8 52.2


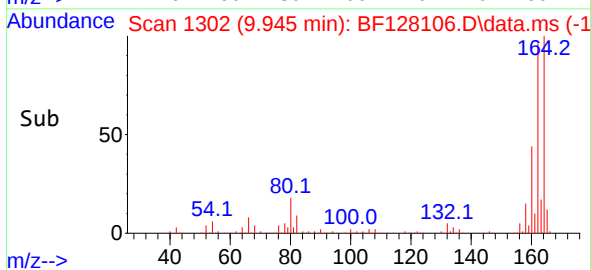
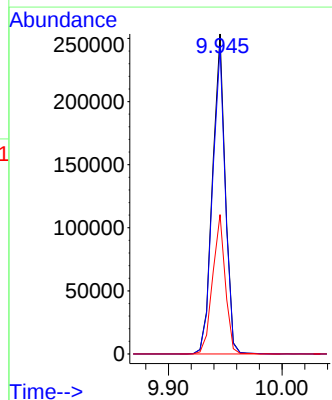
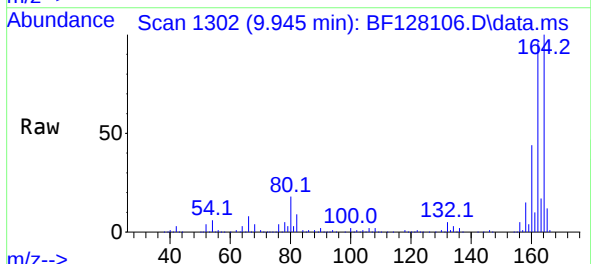


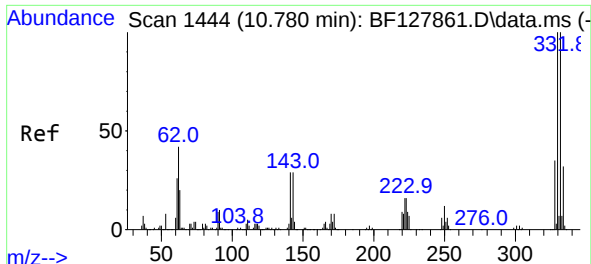

#42
2,4,6-Tribromophenol
Concen: 107.855 ng
RT: 10.739 min Scan# 1444
Delta R.T. -0.006 min
Lab File: BF128106.D
Acq: 05 May 2022 20:50




Instrument :
BNA_F
ClientSampleId :
TP-28

Tgt Ion:330 Resp: 214136
Ion Ratio Lower Upper
330 100
332 95.8 79.0 118.4
141 33.7 28.9 43.3

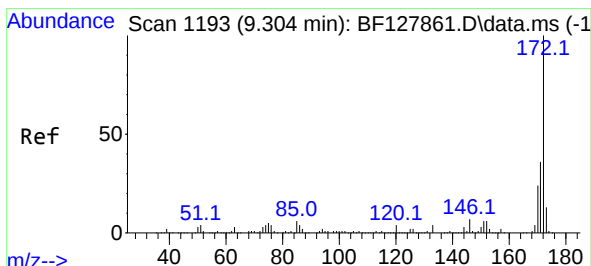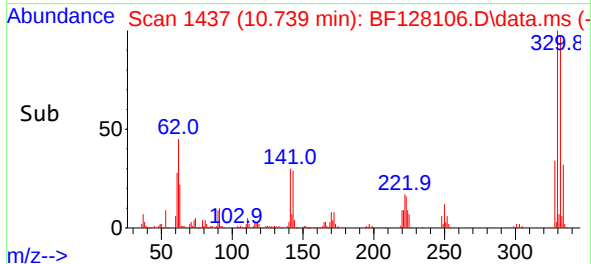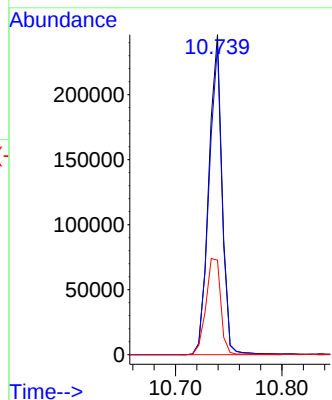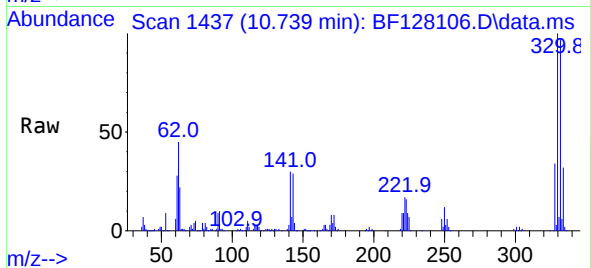

#45
2-Fluorobiphenyl
Concen: 77.751 ng
RT: 9.263 min Scan# 1186
Delta R.T. -0.006 min
Lab File: BF128106.D
Acq: 05 May 2022 20:50

Tgt Ion:172 Resp: 906424
Ion Ratio Lower Upper
172 100
171 34.7 28.6 42.8
170 23.6 19.1 28.7


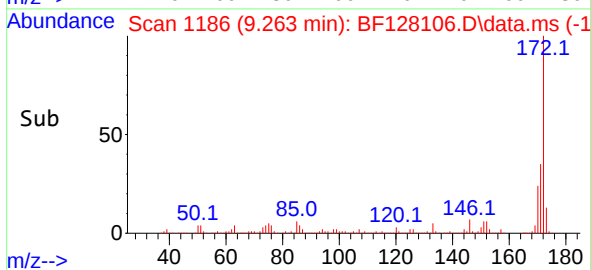
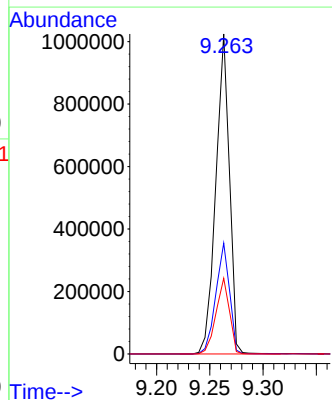
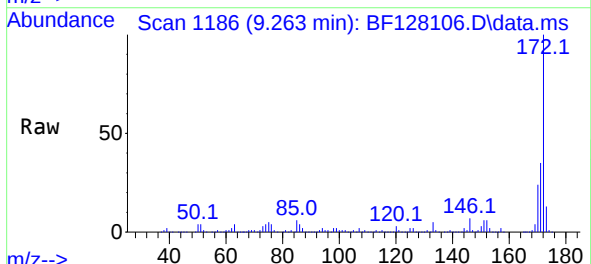




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.434 min Scan# 11
Delta R.T. -0.012 min
Lab File: BF128106.D
Acq: 05 May 2022 20:50




Instrument :
BNA_F
ClientSampleId :
TP-28


Tgt Ion:188 Resp: 345342
Ion Ratio Lower Upper
188 100
94 9.0 8.0 12.0
80 10.6 8.9 13.3

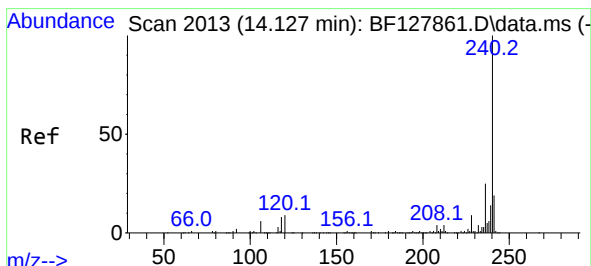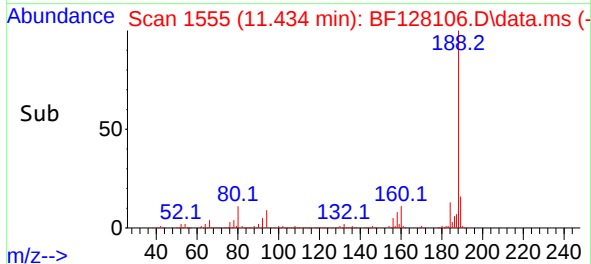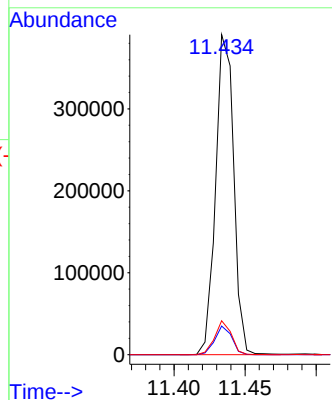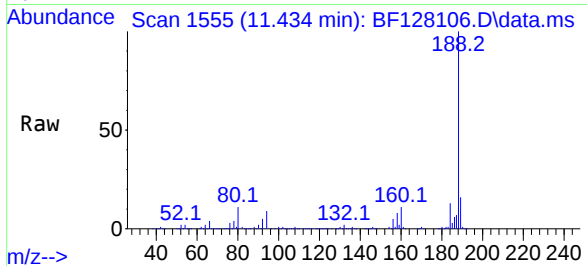

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.080 min Scan# 2005
Delta R.T. -0.012 min
Lab File: BF128106.D
Acq: 05 May 2022 20:50

Tgt Ion:240 Resp: 197996
Ion Ratio Lower Upper
240 100
120 9.0 7.0 10.6
236 26.0 20.3 30.5


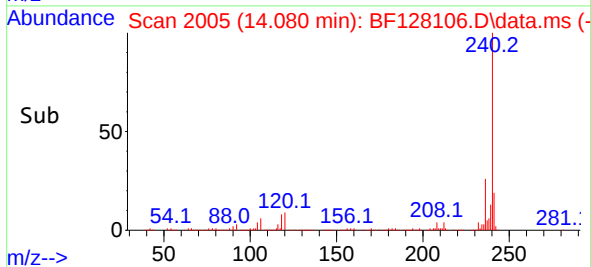
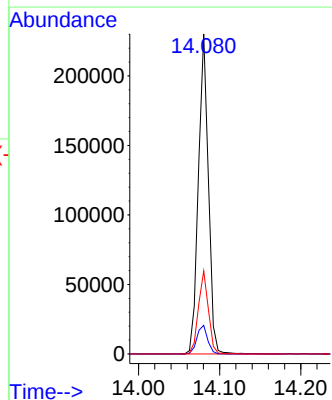
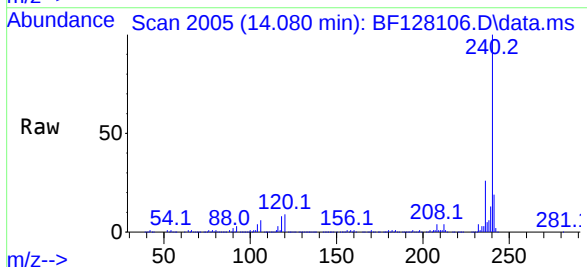


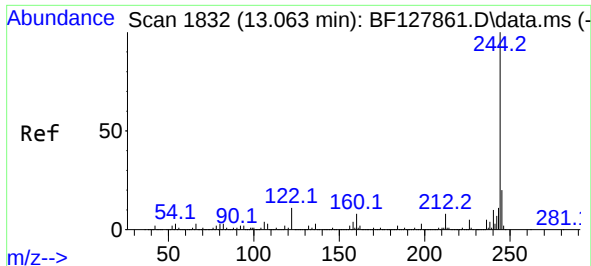

#79
 Terphenyl-d14
 Concen: 77.927 ng
 RT: 13.022 min Scan# 1825
 Delta R.T. -0.012 min
 Lab File: BF128106.D
 Acq: 05 May 2022 20:50

Instrument :
 BNA_F
 ClientSampleId :
 TP-28

Tgt Ion:244 Resp: 843790
 Ion Ratio Lower Upper
 244 100
 212 7.5 6.2 9.4
 122 10.2 8.6 12.8

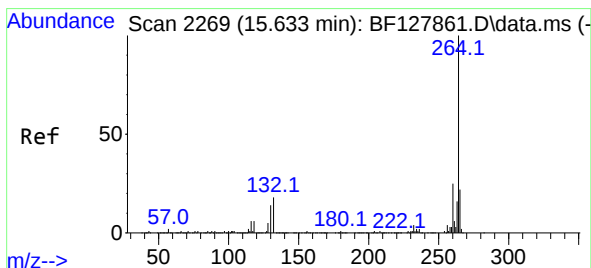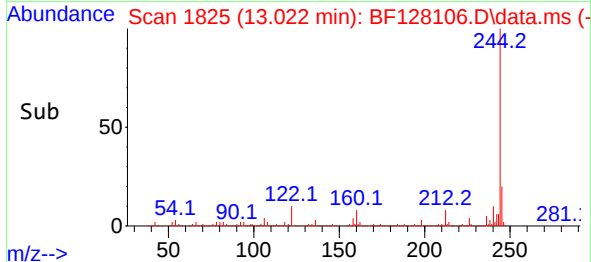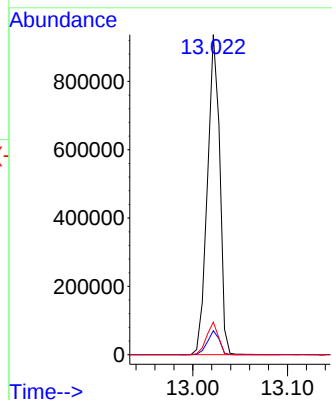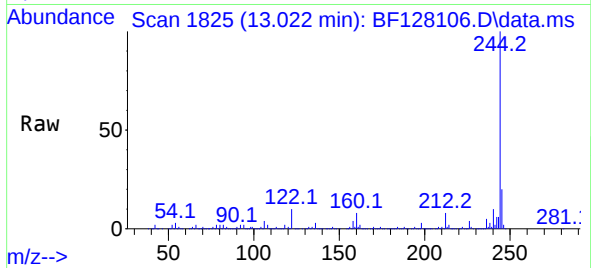

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.580 min Scan# 2260
 Delta R.T. -0.012 min
 Lab File: BF128106.D
 Acq: 05 May 2022 20:50

Tgt Ion:264 Resp: 195723
 Ion Ratio Lower Upper
 264 100
 260 23.2 20.1 30.1
 265 20.9 17.5 26.3

