

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050522\
 Data File : BF128092.D
 Acq On : 05 May 2022 14:04
 Operator : CG\JU
 Sample : PB144601BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144601BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128092.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.540	548	553	556	rBV	2906266	2909060	74.60%	12.651%
2	6.540	717	723	726	rBV	2651781	2996076	76.83%	13.030%
3	6.904	781	785	789	rBV	768529	617486	15.83%	2.685%
4	7.469	876	881	884	rBV	1797945	2065887	52.98%	8.984%
5	8.187	998	1003	1007	rBV	874582	810307	20.78%	3.524%
6	9.263	1180	1186	1189	rBV	3411752	3601791	92.36%	15.664%
7	9.945	1296	1302	1306	rBV	1068159	944478	24.22%	4.107%
8	10.739	1431	1437	1441	rBV	2344902	2294856	58.85%	9.980%
9	11.439	1552	1556	1559	rBV	1199283	983690	25.23%	4.278%
10	13.027	1821	1826	1829	rBV	3794717	3899601	100.00%	16.959%
11	14.086	2002	2006	2009	rBV	942255	845321	21.68%	3.676%
12	15.586	2255	2261	2266	rBV	588809	726540	18.63%	3.160%
13	17.462	2569	2580	2595	rVB3	64959	299248	7.67%	1.301%




Sum of corrected areas: 22994341

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050522\
Data File : BF128092.D
Acq On : 05 May 2022 14:04
Operator : CG\JU
Sample : PB144601BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144601BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

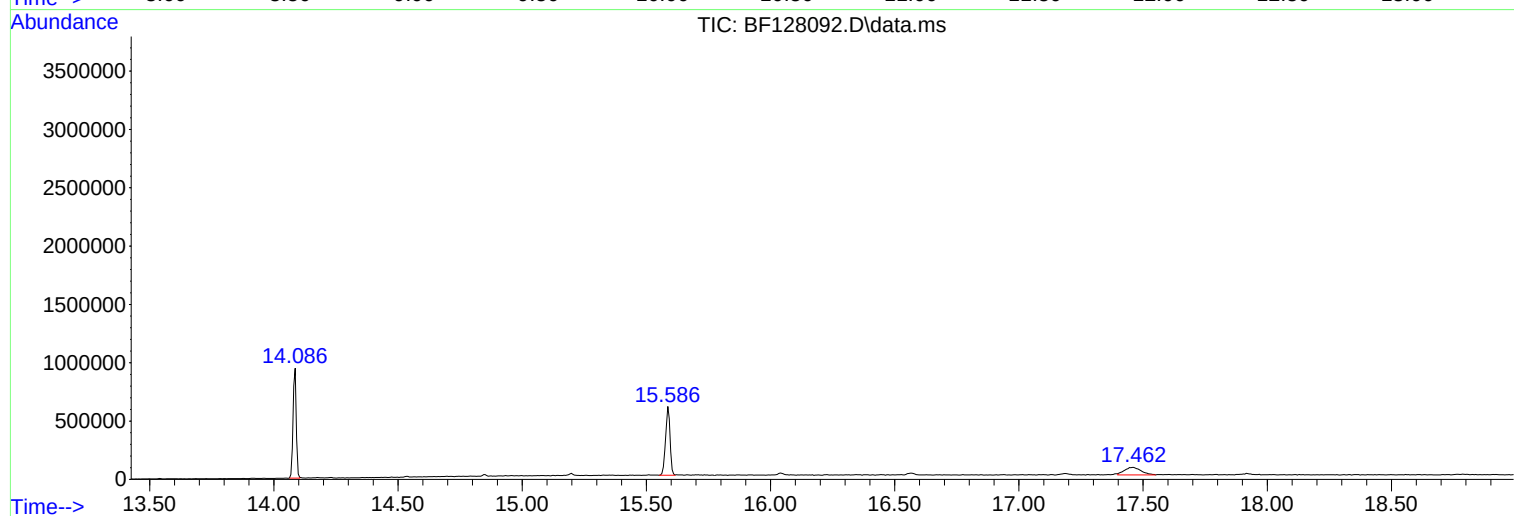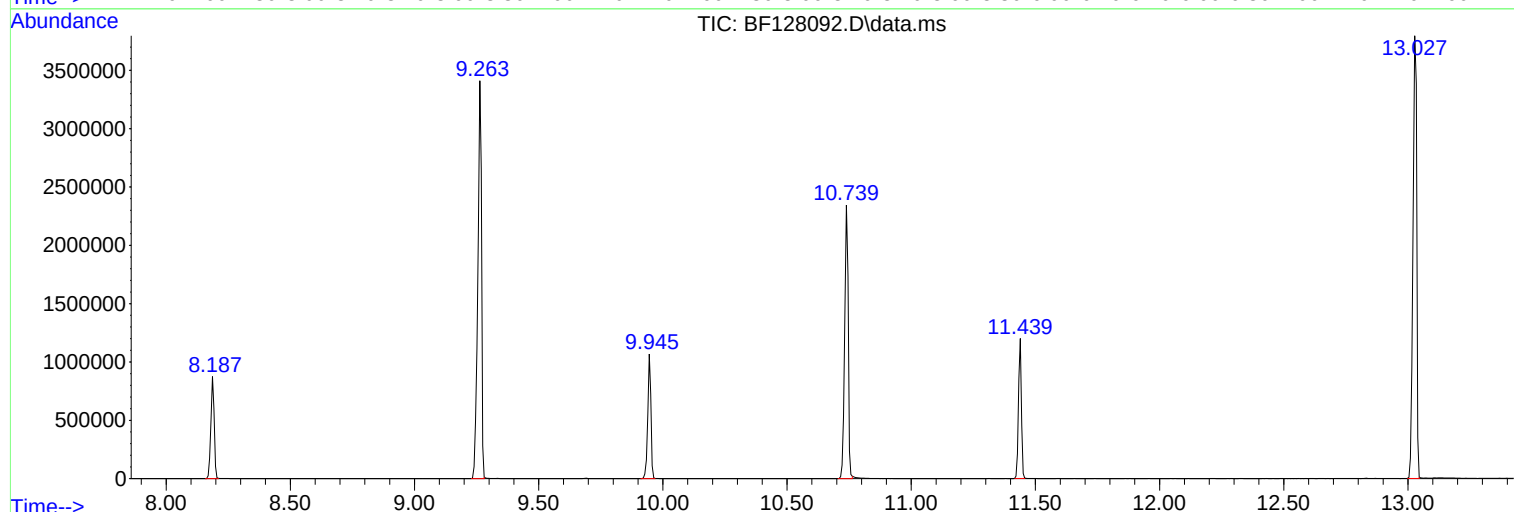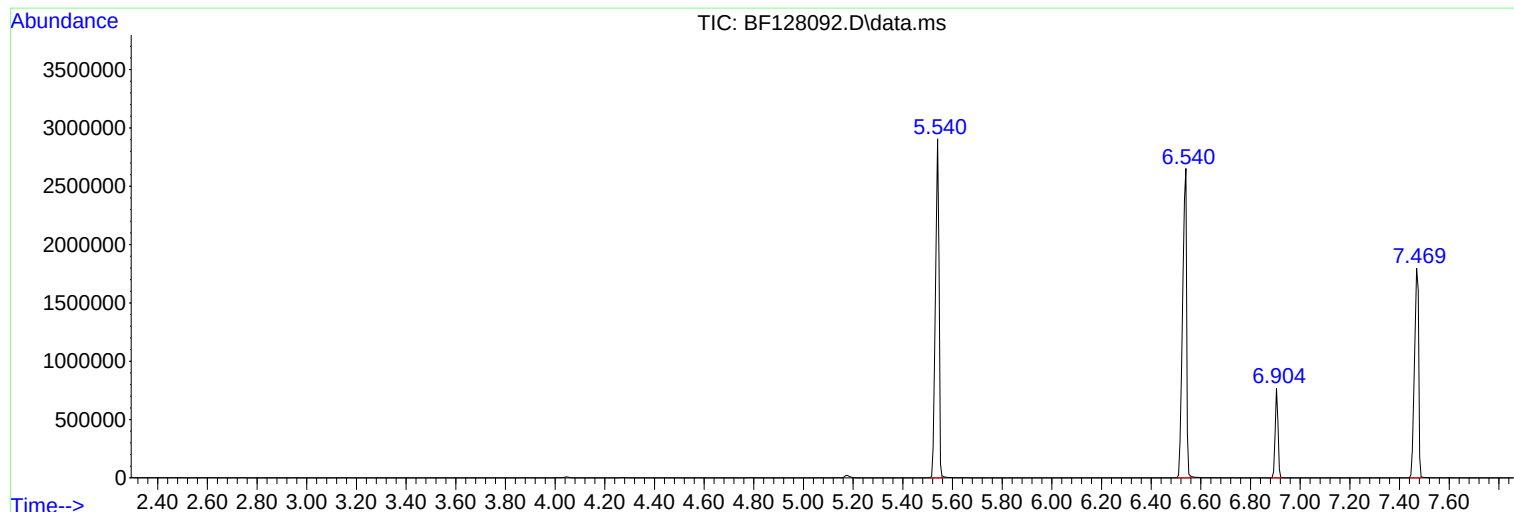

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050522\
Data File : BF128092.D
Acq On : 05 May 2022 14:04
Operator : CG\JU
Sample : PB144601BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB144601BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (1,1'-Biphenyl)-4,4'-diamin... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
17.462	8.24 ng	299248	Perylene-d12	15.586	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	(1,1'-Biphenyl)-4,4'-diamine, N...	360	C26H20N2	006311-48-4	94
2	1,10-Phenanthroline, 2,9-dimethy...	360	C26H20N2	004733-39-5	52
3	N,N'-di-2-Naphthyl-p-phenylenedi...	360	C26H20N2	000093-46-9	49
4	Benzaldehyde, 4-hydroxy-3,5-dime...	360	C18H20N2O6	014414-32-5	47
5	1H-isindole-1,3(2H)-dione, 2-[5...	360	C21H16N2O4	1000398-48-8	43

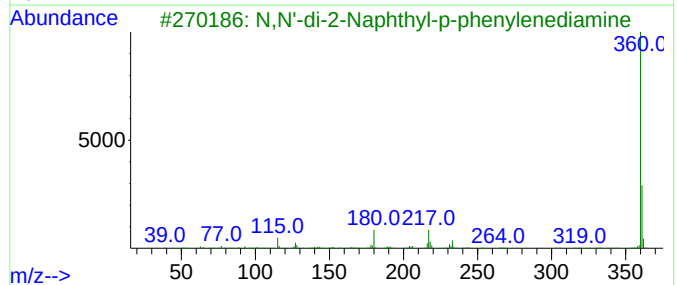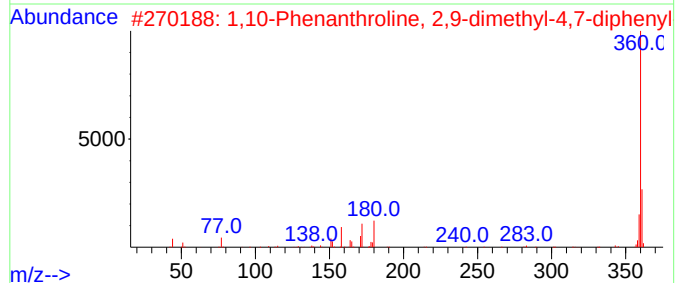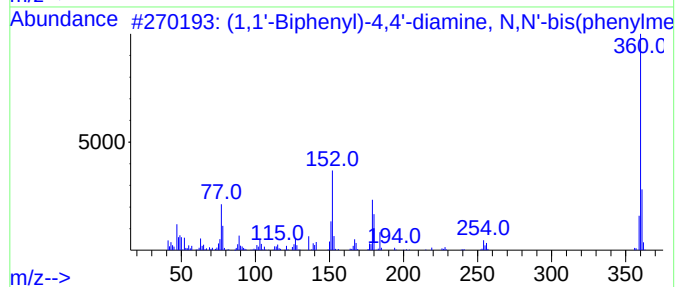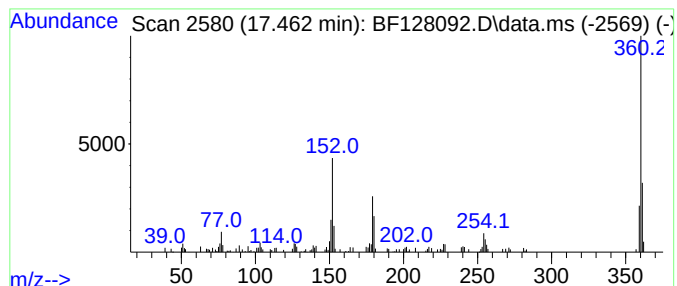

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050522\
Data File : BF128092.D
Acq On : 05 May 2022 14:04
Operator : CG\JU
Sample : PB144601BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144601BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(1,1'-Biphenyl)...	17.462	8.2	ng	299248	6	15.586	726540	20.0