

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF050522\  
 Data File : BF128094.D  
 Acq On : 05 May 2022 15:04  
 Operator : CG\JU  
 Sample : N2672-03  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 03

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128094.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.534       | 547           | 552         | 555          | rBV      | 2331986        | 2194799       | 73.63%          | 7.879%        |
| 2         | 6.534       | 717           | 722         | 725          | rBV      | 2208768        | 2314710       | 77.66%          | 8.310%        |
| 3         | 6.904       | 781           | 785         | 789          | rBV      | 809304         | 641822        | 21.53%          | 2.304%        |
| 4         | 7.469       | 876           | 881         | 884          | rBV      | 1591961        | 1582231       | 53.08%          | 5.680%        |
| 5         | 8.186       | 999           | 1003        | 1007         | rBV      | 979680         | 844154        | 28.32%          | 3.030%        |
| 6         | 9.263       | 1180          | 1186        | 1189         | rBV      | 3133240        | 2855577       | 95.80%          | 10.251%       |
| 7         | 9.945       | 1296          | 1302        | 1305         | rBV      | 1247429        | 1026083       | 34.42%          | 3.684%        |
| 8         | 9.975       | 1305          | 1307        | 1311         | rVB      | 38955          | 33754         | 1.13%           | 0.121%        |
| 9         | 10.145      | 1330          | 1336        | 1339         | rBV3     | 25574          | 36157         | 1.21%           | 0.130%        |
| 10        | 10.492      | 1392          | 1395        | 1401         | rVB      | 43940          | 38786         | 1.30%           | 0.139%        |
| 11        | 10.739      | 1432          | 1437        | 1440         | rBV      | 2257298        | 1992830       | 66.86%          | 7.154%        |
| 12        | 10.839      | 1451          | 1454        | 1464         | rVB6     | 24787          | 45248         | 1.52%           | 0.162%        |
| 13        | 11.039      | 1481          | 1488        | 1491         | rBV3     | 29663          | 46730         | 1.57%           | 0.168%        |
| 14        | 11.292      | 1525          | 1531        | 1534         | rBV3     | 36981          | 58122         | 1.95%           | 0.209%        |
| 15        | 11.333      | 1536          | 1538        | 1543         | rVB      | 38542          | 32884         | 1.10%           | 0.118%        |
| 16        | 11.439      | 1552          | 1556        | 1558         | rBV      | 1370494        | 1123671       | 37.70%          | 4.034%        |
| 17        | 11.463      | 1558          | 1560        | 1563         | rVB      | 662305         | 488222        | 16.38%          | 1.753%        |
| 18        | 11.510      | 1563          | 1568        | 1571         | rBV      | 124791         | 118761        | 3.98%           | 0.426%        |
| 19        | 11.669      | 1592          | 1595        | 1601         | rBV2     | 37874          | 55471         | 1.86%           | 0.199%        |
| 20        | 11.816      | 1617          | 1620        | 1623         | rVB      | 50752          | 40407         | 1.36%           | 0.145%        |
| 21        | 11.939      | 1635          | 1641        | 1644         | rBV2     | 224018         | 331934        | 11.14%          | 1.192%        |
| 22        | 11.969      | 1644          | 1646        | 1649         | rVV      | 239613         | 195595        | 6.56%           | 0.702%        |
| 23        | 12.016      | 1651          | 1654        | 1656         | rVV      | 69531          | 62982         | 2.11%           | 0.226%        |
| 24        | 12.051      | 1656          | 1660        | 1662         | rVV2     | 260296         | 280627        | 9.41%           | 1.007%        |
| 25        | 12.074      | 1662          | 1664        | 1667         | rVB      | 145438         | 113517        | 3.81%           | 0.408%        |
| 26        | 12.233      | 1688          | 1691        | 1694         | rBV      | 133080         | 111939        | 3.76%           | 0.402%        |
| 27        | 12.263      | 1694          | 1696        | 1702         | rVB      | 50819          | 50914         | 1.71%           | 0.183%        |
| 28        | 12.380      | 1714          | 1716        | 1719         | rVB      | 49585          | 41109         | 1.38%           | 0.148%        |
| 29        | 12.492      | 1731          | 1735        | 1737         | rBV      | 137181         | 167173        | 5.61%           | 0.600%        |
| 30        | 12.527      | 1737          | 1741        | 1743         | rVV4     | 185721         | 227770        | 7.64%           | 0.818%        |
| 31        | 12.574      | 1746          | 1749        | 1753         | rBV3     | 68842          | 93051         | 3.12%           | 0.334%        |
| 32        | 12.610      | 1753          | 1755        | 1759         | rVB2     | 55348          | 44338         | 1.49%           | 0.159%        |
| 33        | 12.657      | 1759          | 1763        | 1768         | rBV      | 1041037        | 944166        | 31.68%          | 3.390%        |
| 34        | 12.886      | 1795          | 1802        | 1807         | rBV      | 1251441        | 1276284       | 42.82%          | 4.582%        |
| 35        | 12.933      | 1807          | 1810        | 1814         | rVB2     | 67418          | 76369         | 2.56%           | 0.274%        |
| 36        | 13.027      | 1818          | 1826        | 1829         | rBV      | 3179364        | 2980719       | 100.00%         | 10.701%       |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF050522\  
 Data File : BF128094.D  
 Acq On : 05 May 2022 15:04  
 Operator : CG\JU  
 Sample : N2672-03  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 03

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042222.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

|    |        |      |      |      |      |        |         |        |        |
|----|--------|------|------|------|------|--------|---------|--------|--------|
| 37 | 13.098 | 1834 | 1838 | 1846 | rVV3 | 94229  | 147200  | 4.94%  | 0.528% |
| 38 | 13.186 | 1850 | 1853 | 1854 | rVV3 | 82934  | 82851   | 2.78%  | 0.297% |
| 39 | 13.210 | 1854 | 1857 | 1860 | rVB  | 208576 | 210488  | 7.06%  | 0.756% |
| 40 | 13.280 | 1865 | 1869 | 1871 | rVV  | 154069 | 137388  | 4.61%  | 0.493% |
| 41 | 13.316 | 1871 | 1875 | 1877 | rVV2 | 155137 | 144946  | 4.86%  | 0.520% |
| 42 | 13.339 | 1877 | 1879 | 1882 | rVB  | 69728  | 57577   | 1.93%  | 0.207% |
| 43 | 13.410 | 1888 | 1891 | 1893 | rBV  | 112779 | 92059   | 3.09%  | 0.330% |
| 44 | 13.439 | 1893 | 1896 | 1899 | rVV  | 114590 | 98823   | 3.32%  | 0.355% |
| 45 | 13.639 | 1927 | 1930 | 1932 | rVV2 | 33759  | 37210   | 1.25%  | 0.134% |
| 46 | 13.698 | 1936 | 1940 | 1942 | rBV2 | 30257  | 48080   | 1.61%  | 0.173% |
| 47 | 13.721 | 1942 | 1944 | 1948 | rVB  | 53885  | 58615   | 1.97%  | 0.210% |
| 48 | 13.833 | 1957 | 1963 | 1965 | rBV3 | 78725  | 97658   | 3.28%  | 0.351% |
| 49 | 13.863 | 1965 | 1968 | 1970 | rVV  | 92261  | 86315   | 2.90%  | 0.310% |
| 50 | 13.886 | 1970 | 1972 | 1975 | rVV2 | 55121  | 69667   | 2.34%  | 0.250% |
| 51 | 13.933 | 1976 | 1980 | 1988 | rVB3 | 111052 | 227631  | 7.64%  | 0.817% |
| 52 | 14.086 | 2001 | 2006 | 2008 | rBV2 | 911745 | 1141827 | 38.31% | 4.099% |
| 53 | 14.110 | 2008 | 2010 | 2017 | rVB  | 408740 | 356860  | 11.97% | 1.281% |
| 54 | 14.192 | 2021 | 2024 | 2026 | rBV  | 60868  | 50197   | 1.68%  | 0.180% |
| 55 | 14.233 | 2028 | 2031 | 2037 | rBV5 | 24903  | 49929   | 1.68%  | 0.179% |
| 56 | 14.468 | 2067 | 2071 | 2074 | rVV  | 90102  | 85531   | 2.87%  | 0.307% |
| 57 | 14.504 | 2074 | 2077 | 2080 | rVB  | 52354  | 45815   | 1.54%  | 0.164% |
| 58 | 14.592 | 2090 | 2092 | 2094 | rBV  | 39876  | 38564   | 1.29%  | 0.138% |
| 59 | 14.615 | 2094 | 2096 | 2100 | rVB  | 71501  | 66541   | 2.23%  | 0.239% |
| 60 | 14.768 | 2119 | 2122 | 2127 | rBV4 | 24194  | 38275   | 1.28%  | 0.137% |
| 61 | 14.927 | 2146 | 2149 | 2153 | rVB  | 63379  | 56436   | 1.89%  | 0.203% |
| 62 | 15.139 | 2181 | 2185 | 2189 | rBV  | 204434 | 332771  | 11.16% | 1.195% |
| 63 | 15.251 | 2201 | 2204 | 2208 | rBV  | 39230  | 41928   | 1.41%  | 0.151% |
| 64 | 15.457 | 2234 | 2239 | 2245 | rVB  | 135644 | 186989  | 6.27%  | 0.671% |
| 65 | 15.521 | 2245 | 2250 | 2254 | rVB  | 210782 | 264271  | 8.87%  | 0.949% |
| 66 | 15.586 | 2255 | 2261 | 2265 | rBV  | 487367 | 610649  | 20.49% | 2.192% |
| 67 | 16.162 | 2356 | 2359 | 2364 | rBV3 | 22795  | 38381   | 1.29%  | 0.138% |
| 68 | 17.104 | 2514 | 2519 | 2527 | rVB2 | 78762  | 158000  | 5.30%  | 0.567% |
| 69 | 17.568 | 2593 | 2598 | 2606 | rVB2 | 66232  | 127233  | 4.27%  | 0.457% |




Sum of corrected areas: 27855611

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF050522\  
Data File : BF128094.D  
Acq On : 05 May 2022 15:04  
Operator : CG\JU  
Sample : N2672-03  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
03

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042222.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

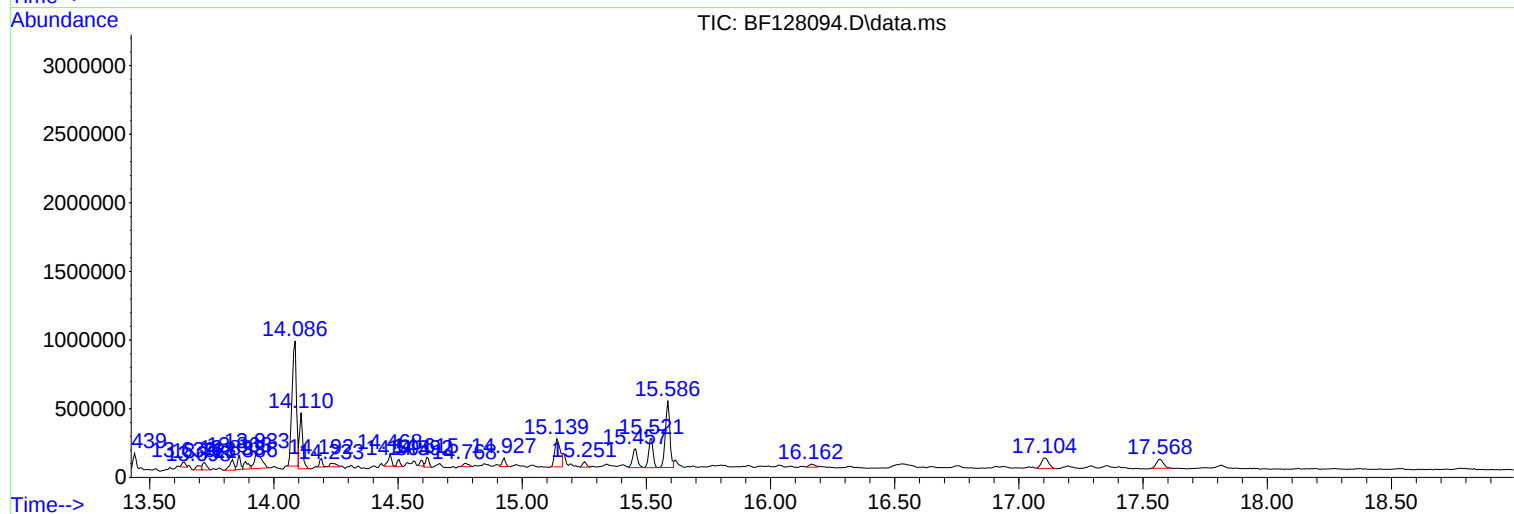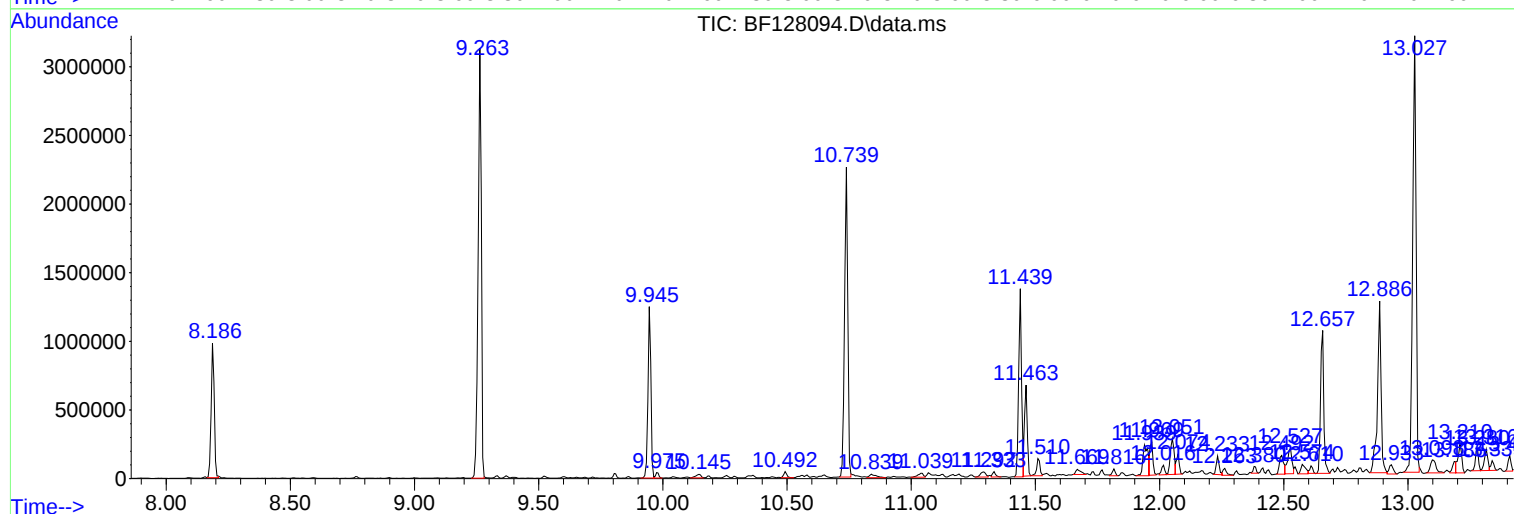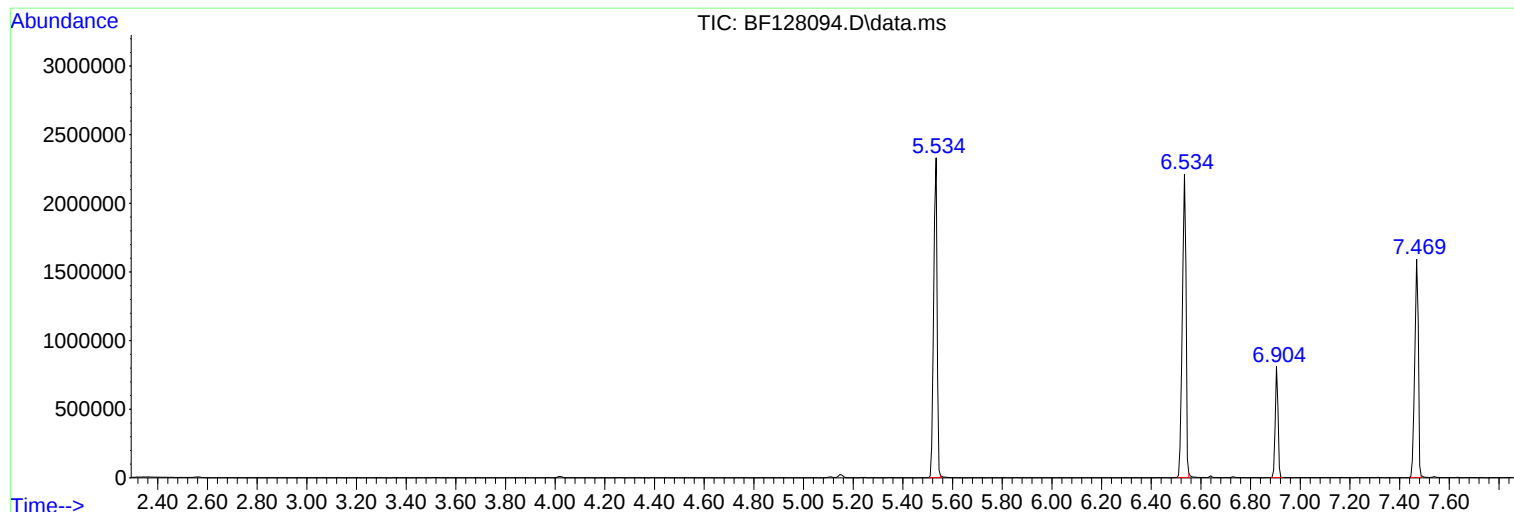

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF050522\  
Data File : BF128094.D  
Acq On : 05 May 2022 15:04  
Operator : CG\JU  
Sample : N2672-03  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
03

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042222.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF050522\  
Data File : BF128094.D  
Acq On : 05 May 2022 15:04  
Operator : CG\JU  
Sample : N2672-03  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
03

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042222.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|