

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050522\
 Data File : BF128097.D
 Acq On : 05 May 2022 16:30
 Operator : CG\JU
 Sample : N2672-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 10

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128097.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.534	547	552	555	rBV	2548319	2382515	76.16%	12.354%
2	6.534	717	722	725	rBV	2240434	2492015	79.66%	12.922%
3	6.904	781	785	789	rBV	702299	544408	17.40%	2.823%
4	7.469	876	881	884	rBV	1664853	1719597	54.97%	8.917%
5	8.186	999	1003	1007	rBV	825558	731044	23.37%	3.791%
6	9.263	1181	1186	1189	rBV	3269657	3016202	96.41%	15.640%
7	9.945	1297	1302	1306	rBV	1069004	874671	27.96%	4.536%
8	10.739	1432	1437	1440	rBV	2432867	2161366	69.09%	11.208%
9	11.439	1552	1556	1559	rBV	1163263	955821	30.55%	4.956%
10	13.027	1821	1826	1829	rBV	3492613	3128446	100.00%	16.222%
11	13.939	1974	1981	1992	rBV5	38567	110573	3.53%	0.573%
12	14.080	2001	2005	2009	rBV	712732	662581	21.18%	3.436%
13	15.580	2255	2260	2266	rBV	381847	505607	16.16%	2.622%




Sum of corrected areas: 19284846

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050522\
Data File : BF128097.D
Acq On : 05 May 2022 16:30
Operator : CG\JU
Sample : N2672-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

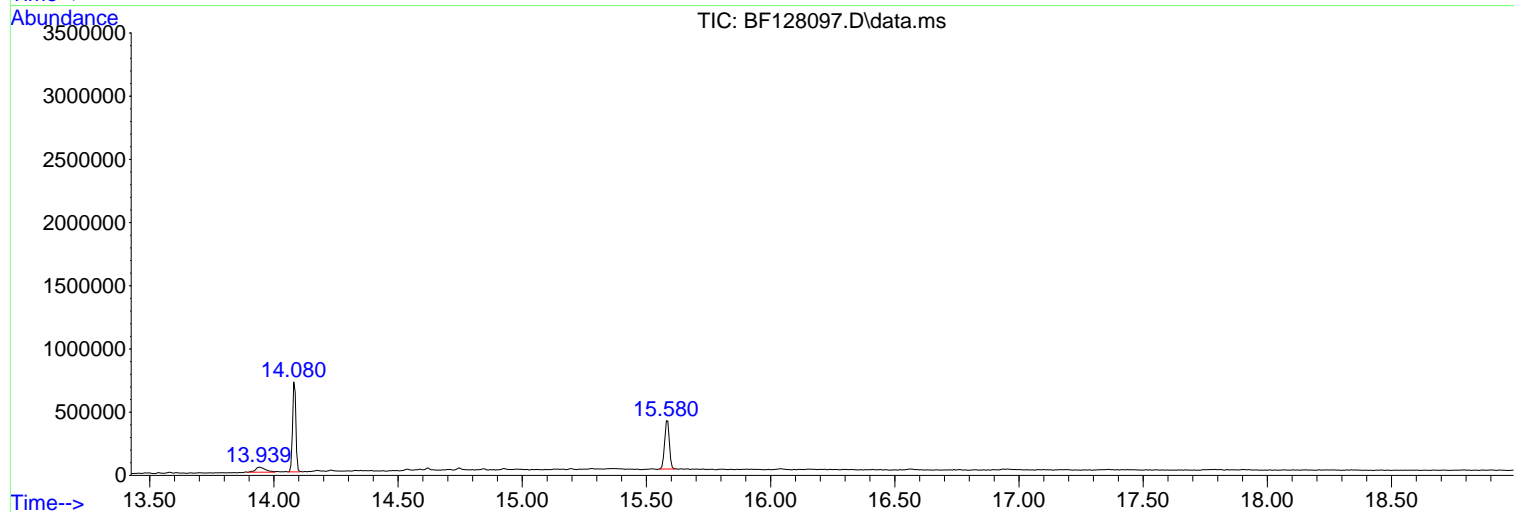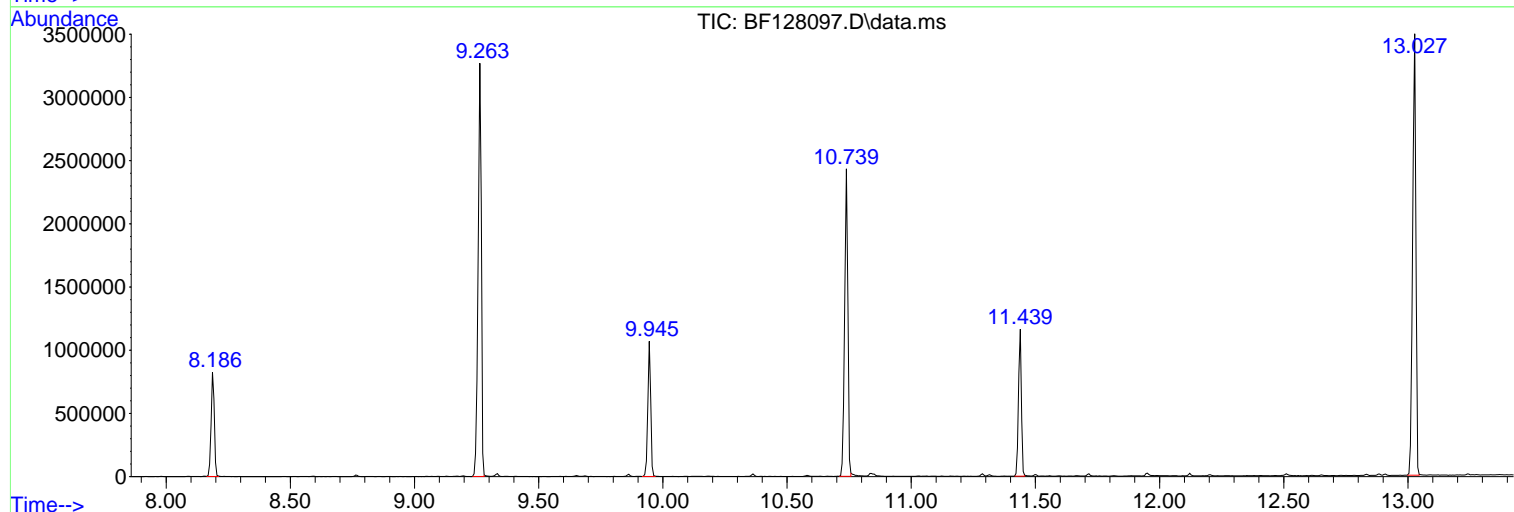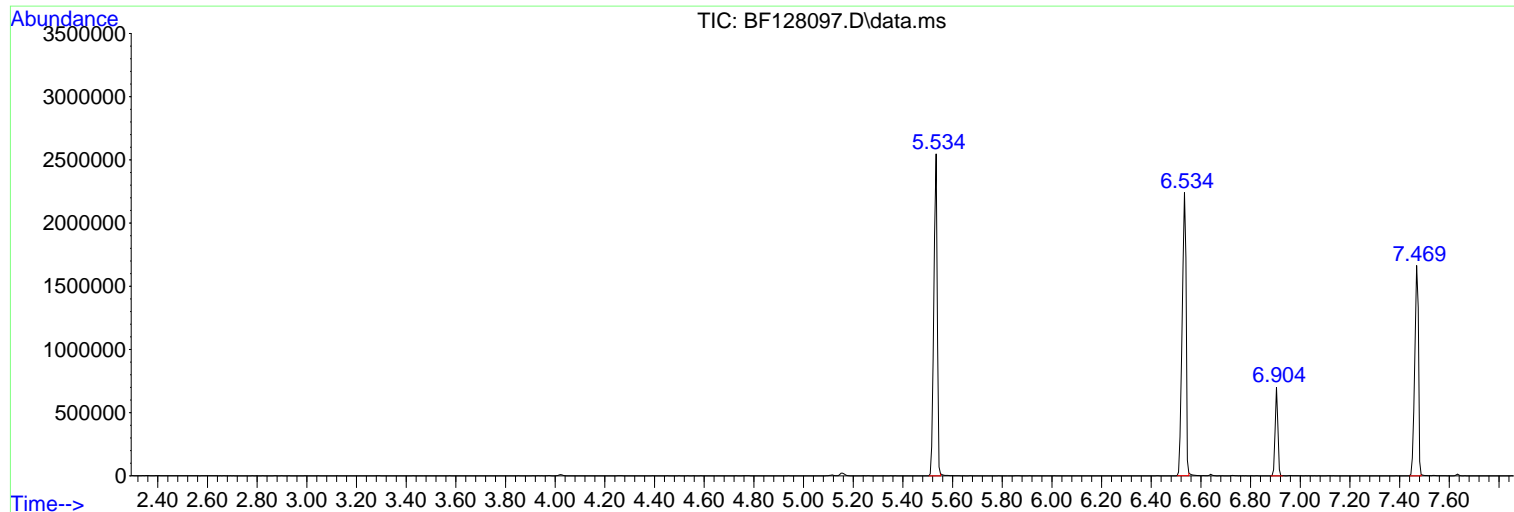

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050522\
Data File : BF128097.D
Acq On : 05 May 2022 16:30
Operator : CG\JU
Sample : N2672-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050522\
Data File : BF128097.D
Acq On : 05 May 2022 16:30
Operator : CG\JU
Sample : N2672-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------
