

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050522\
 Data File : BF128106.D
 Acq On : 05 May 2022 20:50
 Operator : CG\JU
 Sample : N2703-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-28

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128106.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.528	547	551	555	rBV	2123471	2116047	78.11%	12.744%
2	6.534	717	722	725	rBV	2187873	2184756	80.65%	13.158%
3	6.904	781	785	788	rBV	723891	550569	20.32%	3.316%
4	7.469	876	881	884	rBV	1600707	1508036	55.67%	9.082%
5	7.634	905	909	912	rVB	50511	40161	1.48%	0.242%
6	8.187	999	1003	1006	rBV	876858	720016	26.58%	4.336%
7	9.263	1181	1186	1189	rBV	3096668	2708964	100.00%	16.315%
8	9.328	1194	1197	1200	rVB	34377	30298	1.12%	0.182%
9	9.945	1298	1302	1305	rBV	1059773	832000	30.71%	5.011%
10	10.739	1432	1437	1440	rBV	1766347	1676391	61.88%	10.096%
11	11.434	1552	1555	1559	rBV	951082	827398	30.54%	4.983%
12	13.022	1821	1825	1828	rBV	2539993	2252162	83.14%	13.564%
13	13.939	1977	1981	1994	rVB5	33341	82911	3.06%	0.499%
14	14.080	2001	2005	2009	rBV	613700	532897	19.67%	3.209%
15	15.580	2255	2260	2267	rBV	422682	541551	19.99%	3.262%




Sum of corrected areas: 16604157

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050522\
Data File : BF128106.D
Acq On : 05 May 2022 20:50
Operator : CG\JU
Sample : N2703-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-28

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

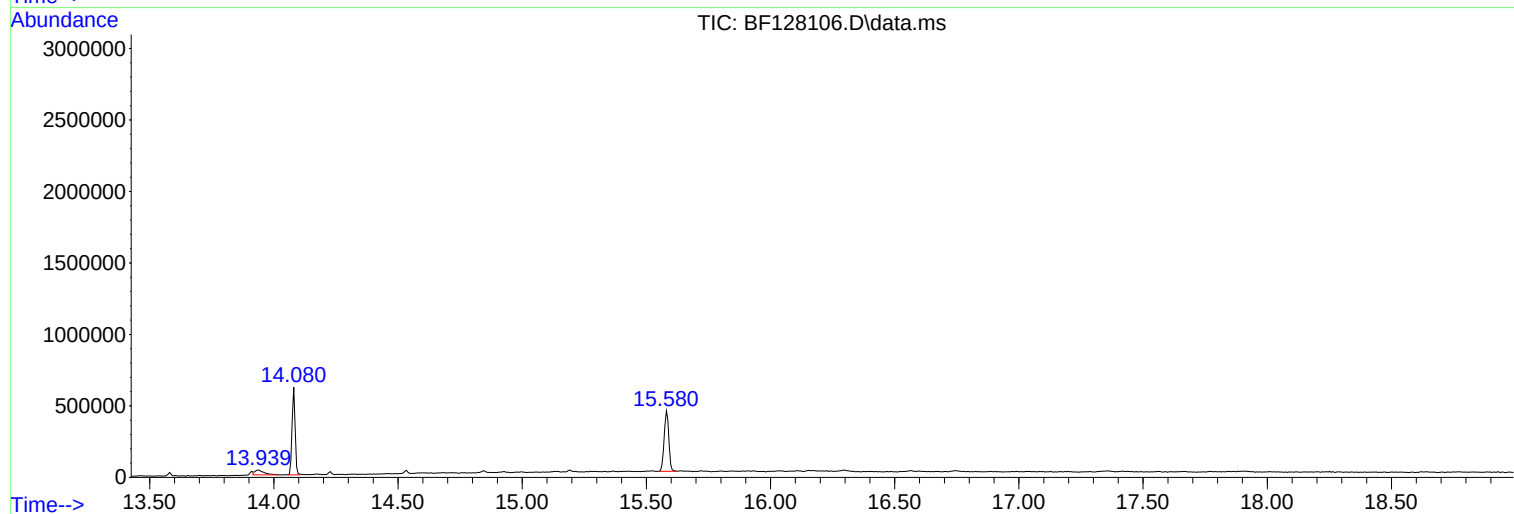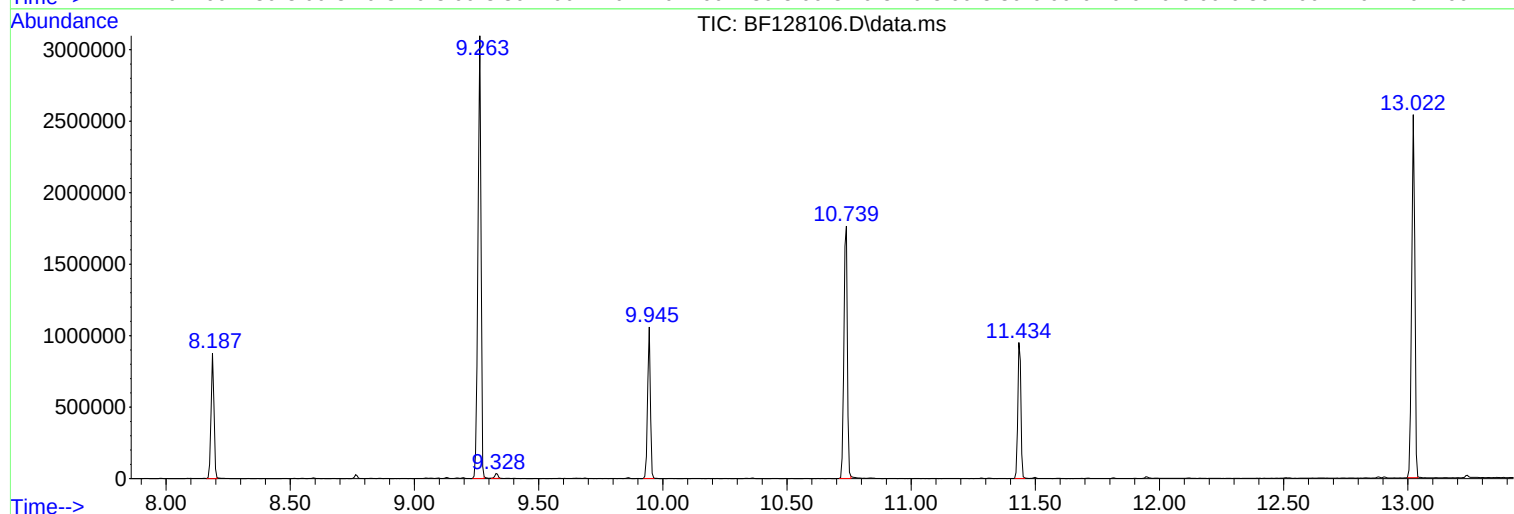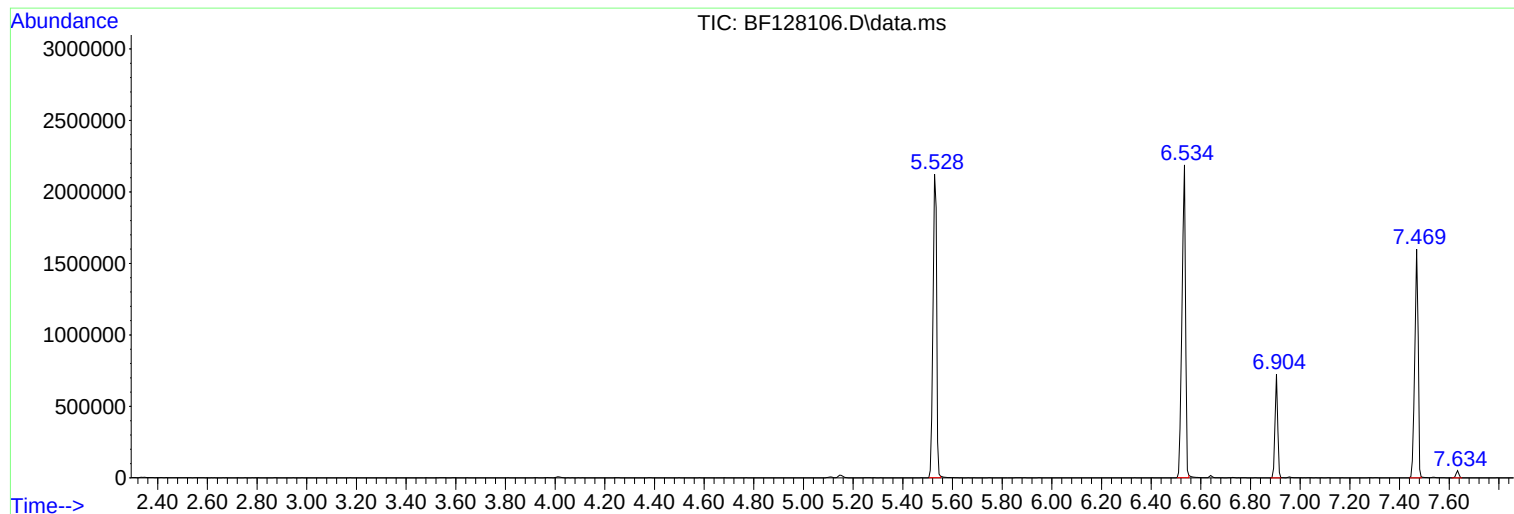

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050522\
Data File : BF128106.D
Acq On : 05 May 2022 20:50
Operator : CG\JU
Sample : N2703-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-28










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Hexadecanol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.939	3.11 ng	82911	Chrysene-d12	14.080

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Hexadecanol	242	C16H34O	036653-82-4	53
2			12-Bromo-1-dodecanol	264	C12H25BrO	003344-77-2	53
3			n-Heptadecanol-1	256	C17H36O	001454-85-9	53
4			Cyclohexane, 1,2-dimethyl-3-pent...	224	C16H32	062376-17-4	47
5			Bicyclo[3.1.1]heptan-3-one, 2,6,...	152	C10H16O	015358-88-0	38

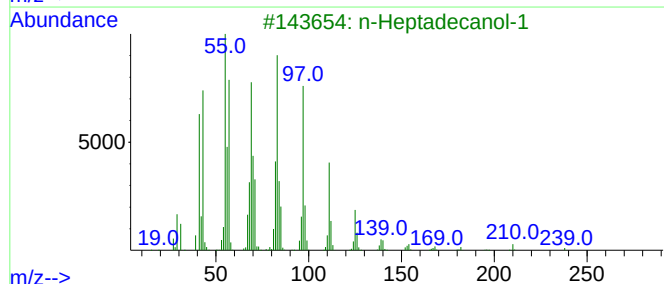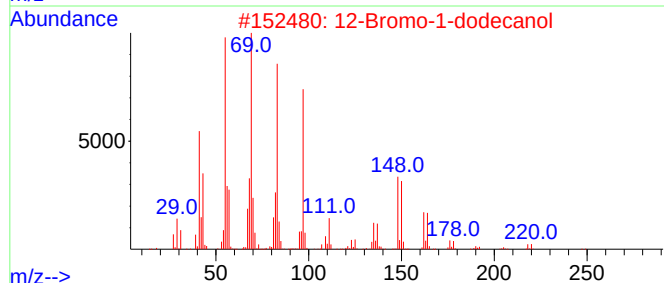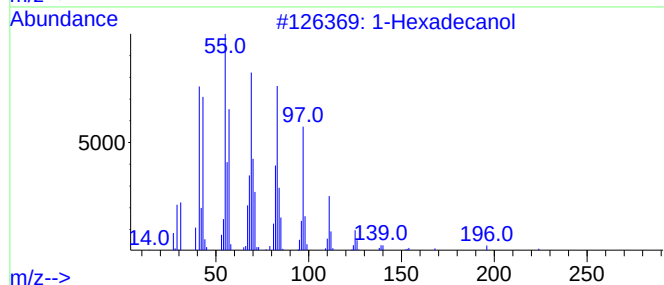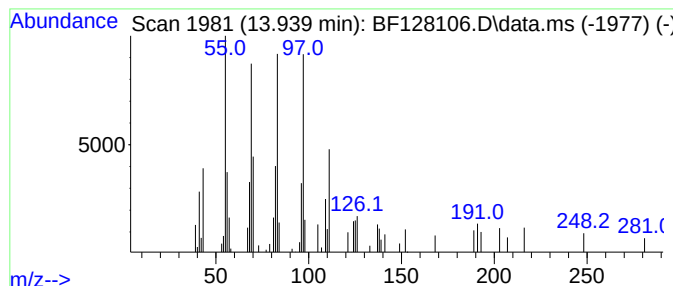

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050522\
Data File : BF128106.D
Acq On : 05 May 2022 20:50
Operator : CG\JU
Sample : N2703-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-28

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Hexadecanol	13.939	3.1	ng	82911	5	14.080	532897	20.0