


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050522\
 Data File : BF128085.D
 Acq On : 05 May 2022 10:04
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 05 17:56:23 2022

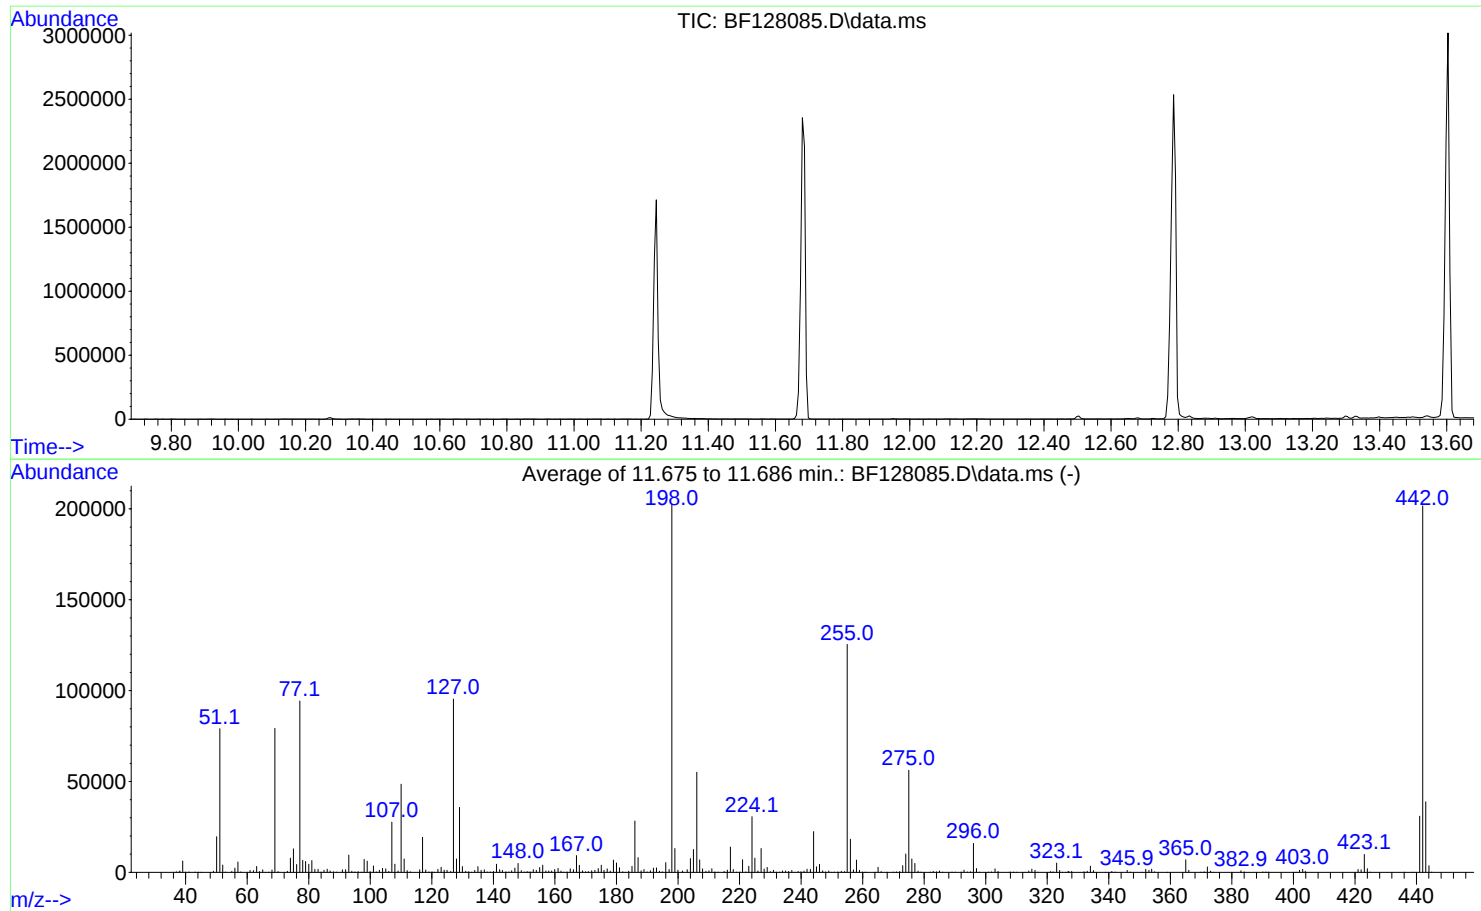




AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	79069	PASS
68	69	0.00	2	1.7	1348	PASS
69	198	0.00	100	39.1	79227	PASS
70	69	0.00	2	0.6	445	PASS
127	198	10	80	47.1	95397	PASS
197	198	0.00	2	0.8	1614	PASS
198	198	100	100	100.0	202408	PASS
199	198	5	9	6.5	13102	PASS
275	198	10	60	27.7	56139	PASS
365	198	1	100	3.4	6977	PASS
441	198	0.01	100	15.3	30919	PASS
442	442	50	100	100.0	201693	PASS
443	442	15	24	19.3	38876	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050522\
Data File : BF128085.D
Acq On : 05 May 2022 10:04
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 05 18:16:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 17:56:23 2022
Response via : Initial Calibration

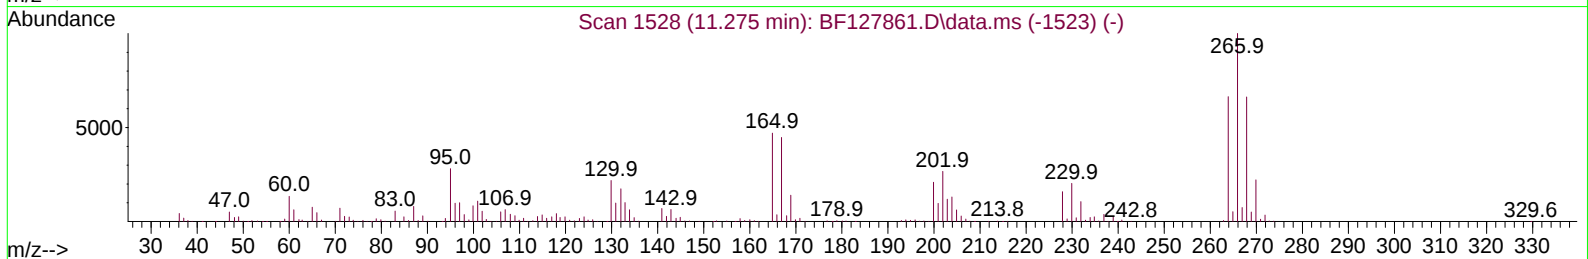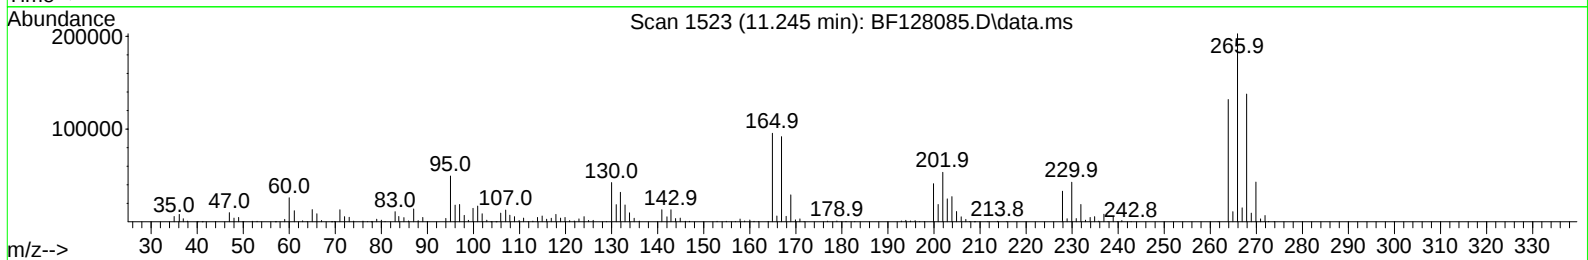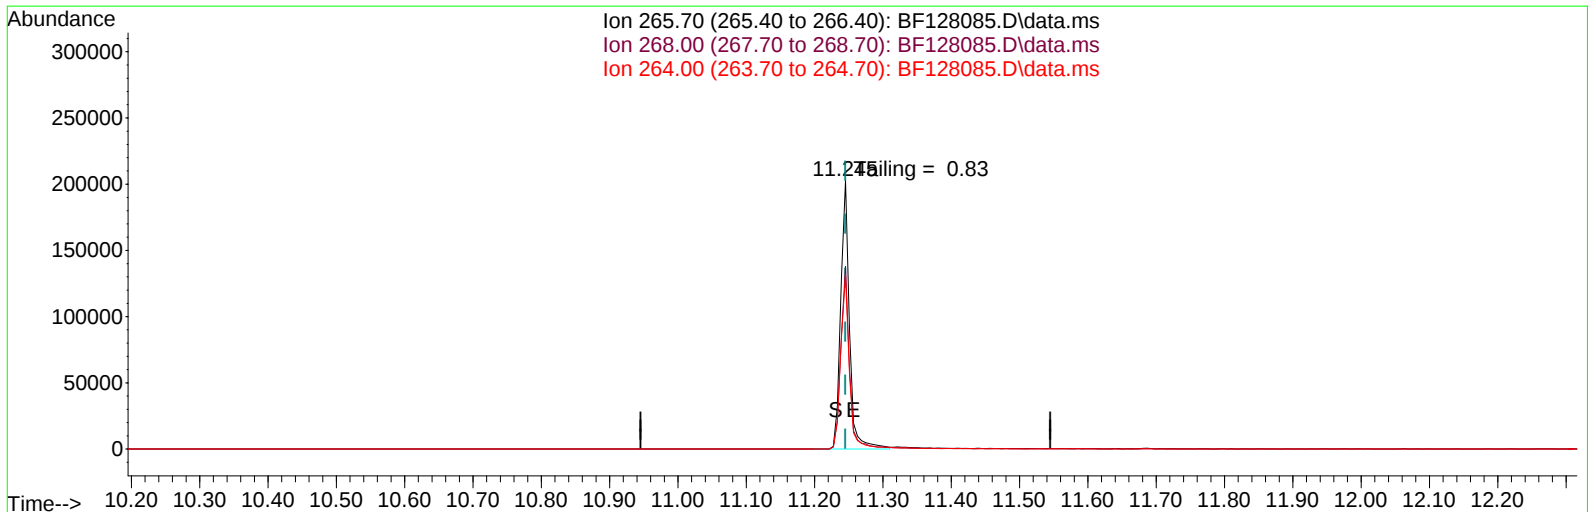

TIC: BF128085.D\data.ms

(70) Pentachlorophenol (C)

11.245min (+ 0.000) 29006.02 ng




response 181766

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	67.95
264.00	66.40	65.01
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050522\  
Data File : BF128085.D  
Acq On    : 05 May 2022  10:04  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 05 18:16:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 17:56:23 2022
Response via : Initial Calibration

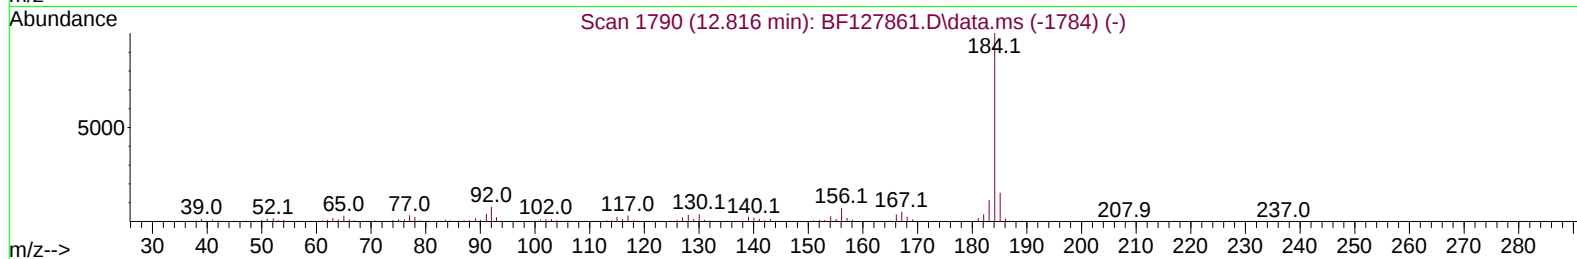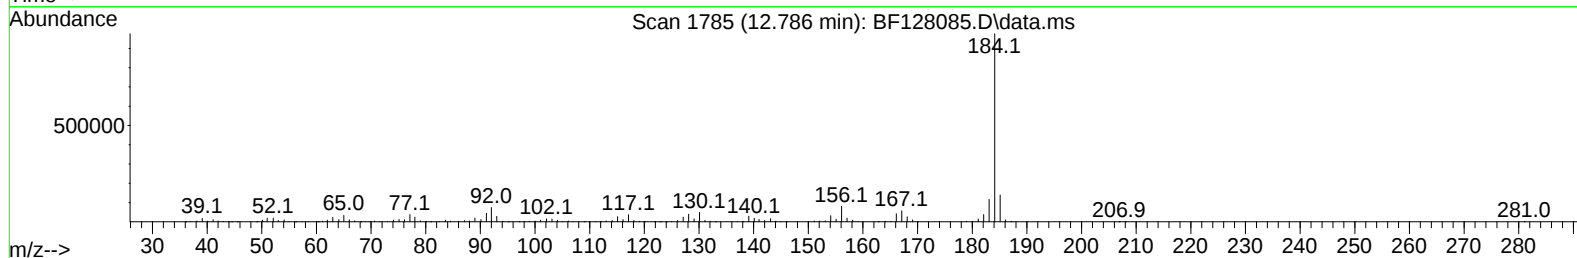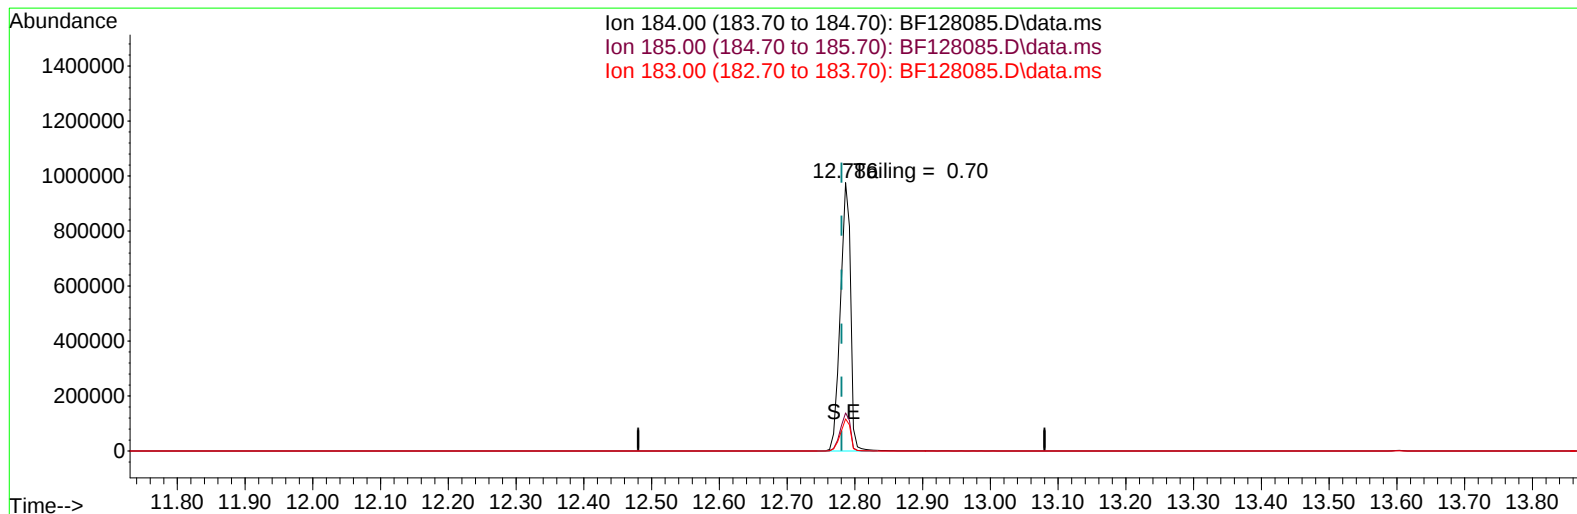

TIC: BF128085.D\data.ms

(77) Benzidine

12.786min (+ 0.006) 0.00 ng

response **1027807**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.21
183.00	11.20	11.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/5/2022	BNA_F	<u>BF128085.D</u>
Compound Name	Response	Retention Time
DDT	503210	13.6
DDD	3614	13.29
DDE	606	12.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4220	507430	0.83

Instrument :
BNA_F
ClientSampleId :
DFTPP