
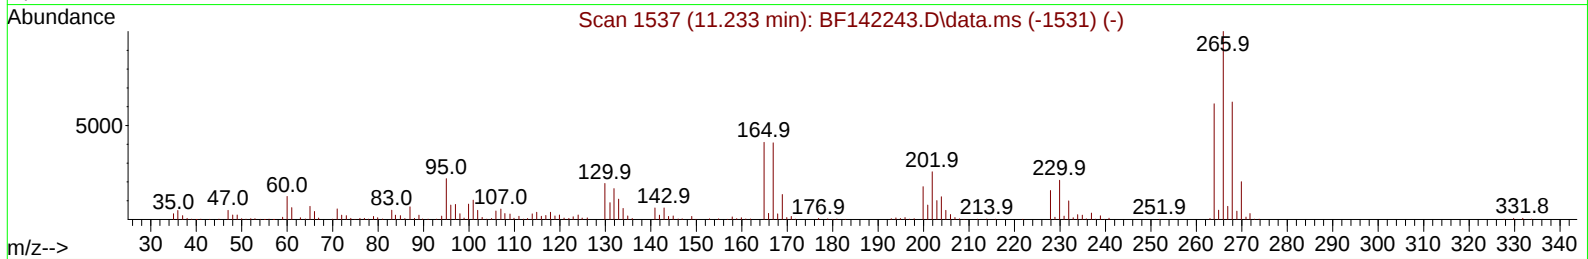
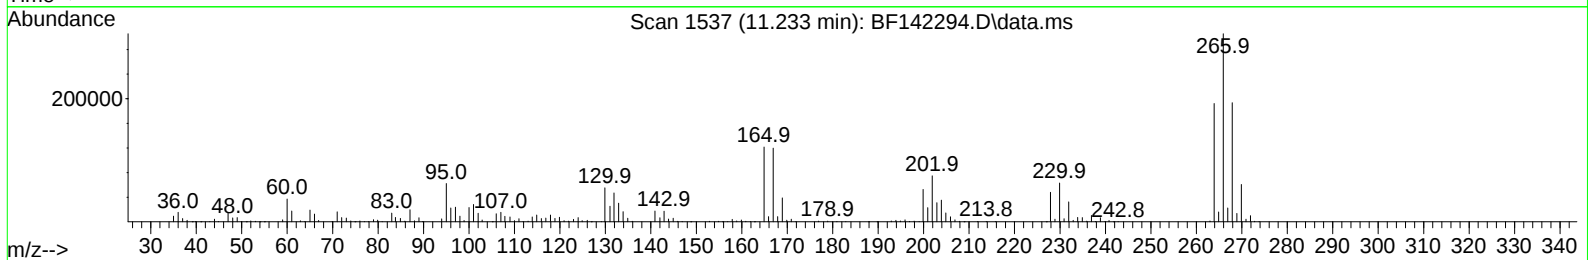


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050525\
Data File : BF142294.D
Acq On : 05 May 2025 13:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 05 15:26:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 15:26:28 2025
Response via : Initial Calibration

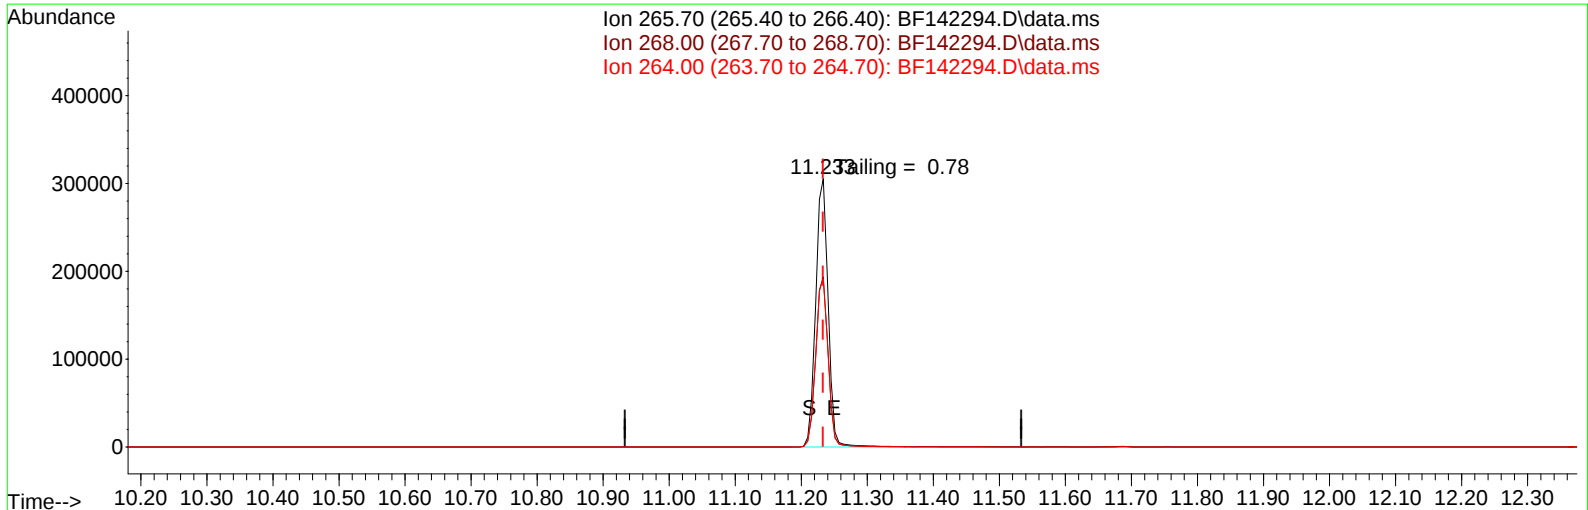

TIC: BF142294.D\data.ms




(70) Pentachlorophenol (C)

11.233min (+ 0.000) 69841.70 ng

response 401301

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	63.35
264.00	61.60	62.89
0.00	0.00	0.00

Quant Time: May 05 15:26:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 15:26:28 2025
Response via : Initial Calibration

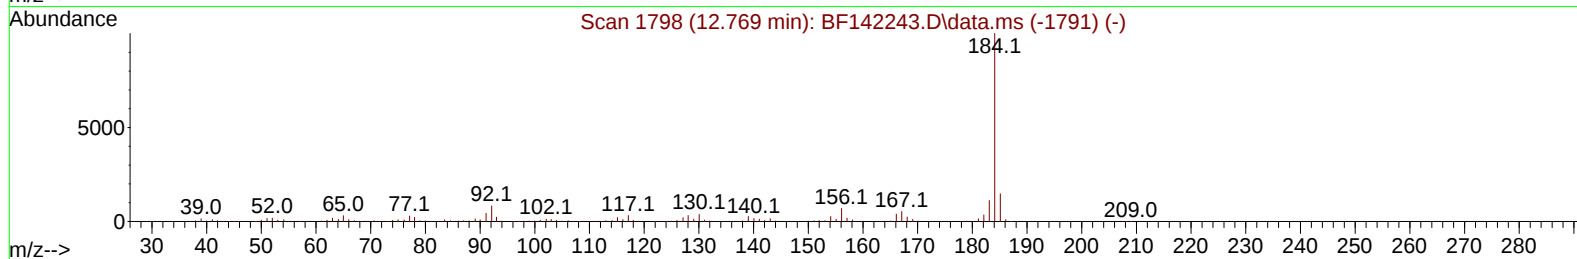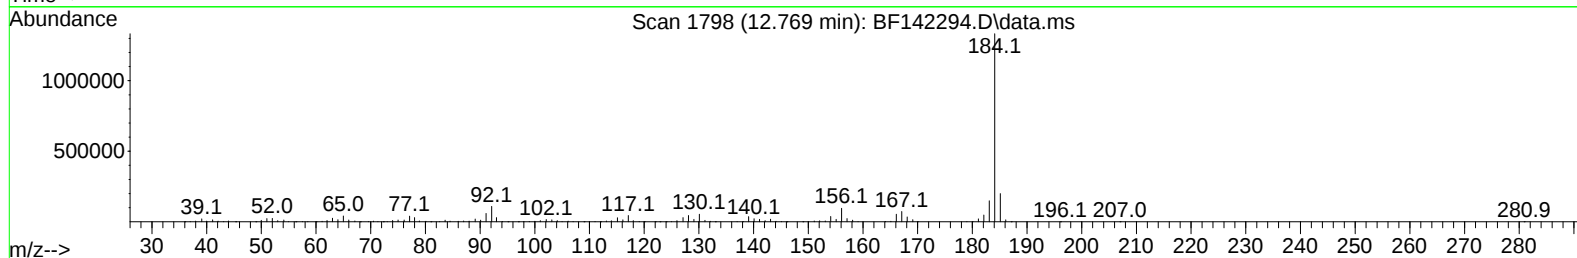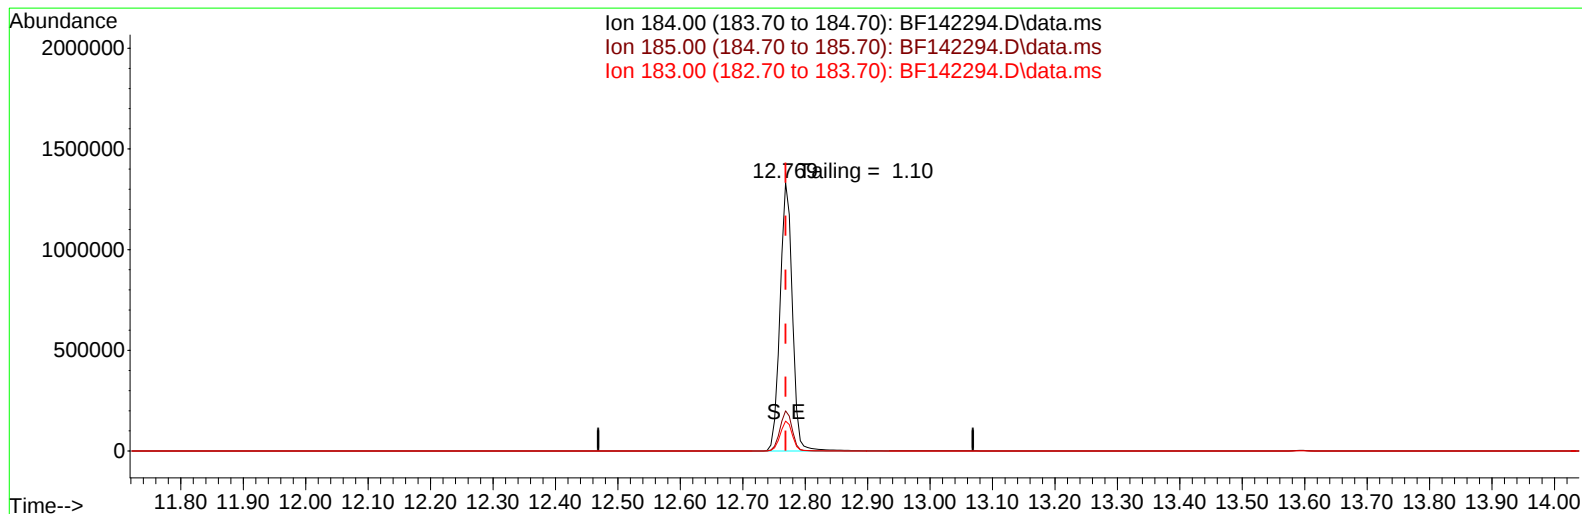

TIC: BF142294.D\data.ms

(77) Benzidine

12.769min (-0.000) 69201.02 ng

response 1834842

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.01
183.00	11.10	11.15
0.00	0.00	0.00