

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050615\
 Data File : BF078965.D
 Acq On : 6 May 2015 17:31
 Operator : TP/IZ
 Sample : G2114-10 2X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 GRID-4(0-6)

Quant Time: May 07 01:10:03 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 07 00:45:56 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.35	152	73253	20.00	ng	0.00
21) Naphthalene-d8	8.92	136	311322	20.00	ng	0.00
38) Acenaphthene-d10	11.10	164	144437	20.00	ng	0.00
63) Phenanthrene-d10	12.95	188	301006	20.00	ng	0.00
75) Chrysene-d12	16.25	240	326070	20.00	ng	-0.06
86) Perylene-d12	18.02	264	353911	20.00	ng	-0.21
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	209788	49.30	ng	0.01
7) Phenol-d6	6.90	99	286334	50.90	ng	0.01
23) Nitrobenzene-d5	8.03	82	158048	29.18	ng	0.00
41) 2,4,6-Tribromophenol	12.08	330	75092	48.06	ng	0.00
44) 2-Fluorobiphenyl	10.27	172	321220	30.98	ng	0.00
78) Terphenyl-d14	0.00	244	0	0.00	ng	
Target Compounds						
70) Phenanthrene	12.98	178	195321	11.60	ng	Qvalue 98
71) Anthracene	13.04	178	43493	2.63	ng	99
74) Fluoranthene	14.46	202	340887	19.43	ng	98
80) Benzo(a)anthracene	16.24	228	179170	10.03	ng	98
82) Chrysene	16.29	228	131281	7.64	ng	96
83) Bis(2-ethylhexyl)phthalate	16.29	149	62998	5.06	ng	# 94
87) Benzo(b)fluoranthene	17.57	252	203385	10.50	ng	100
88) Benzo(k)fluoranthene	17.57	252	287128	15.31	ng	99
89) Benzo(a)pyrene	17.95	252	153157	8.59	ng	# 96
91) Benzo(g,h,i)perylene	19.97	276	106454	5.60	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050615\
Data File : BF078965.D
Acq On : 6 May 2015 17:31
Operator : TP/IZ
Sample : G2114-10 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GRID-4(0-6)

Quant Time: May 07 01:10:03 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 07 00:45:56 2015
Response via : Initial Calibration

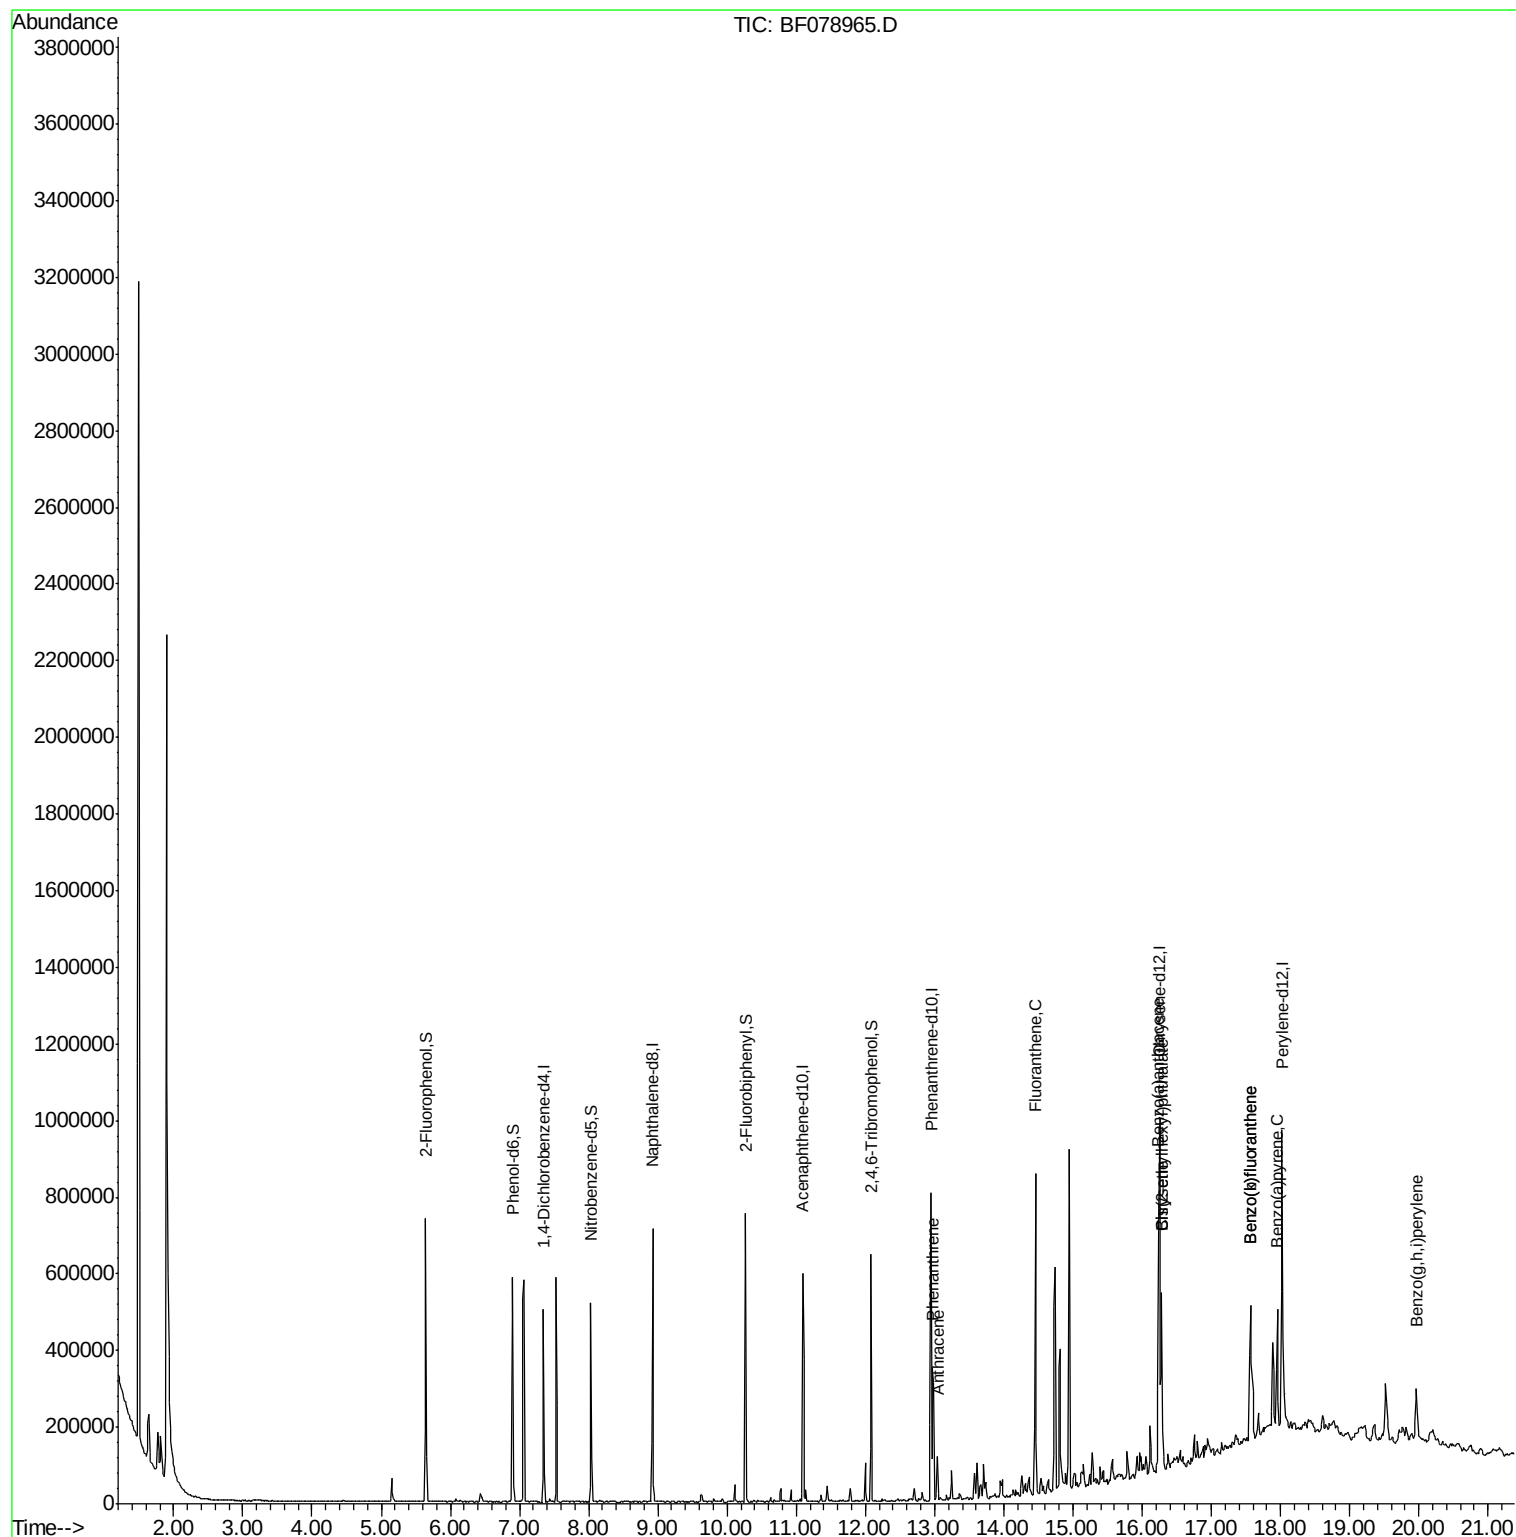




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.35 min Scan# 539
Delta R.T. -0.00 min
Lab File: BF078965.D
Acq: 6 May 2015 17:31

Instrument :
BNA_F
ClientSampleId :
GRID-4(0-6)

Tgt Ion:152 Resp: 73253
Ion Ratio Lower Upper
152 100
150 157.0 122.0 183.0
115 61.6 46.3 69.5

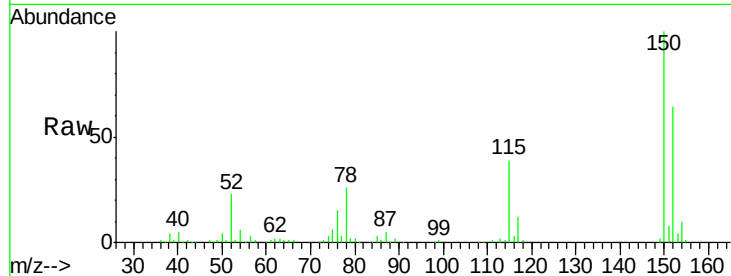


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

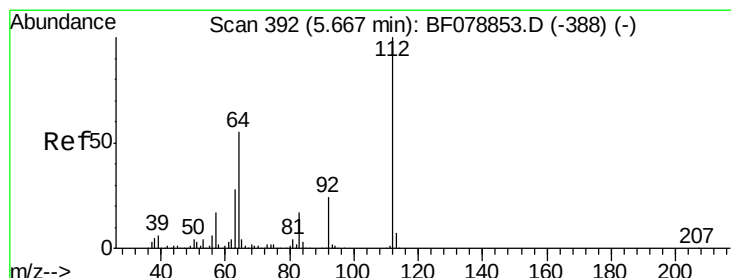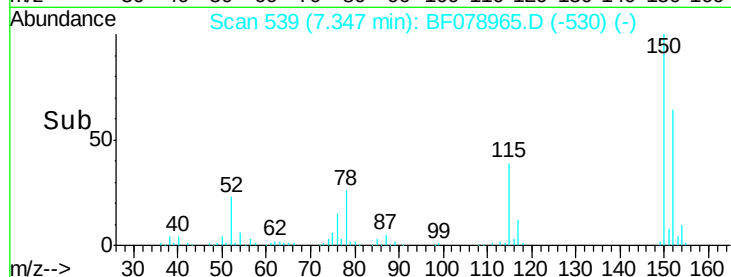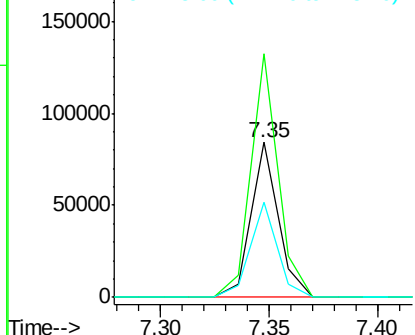



#5


2-Fluorophenol
Concen: 49.30 ng
RT: 5.64 min Scan# 390
Delta R.T. 0.01 min
Lab File: BF078965.D
Acq: 6 May 2015 17:31

Tgt Ion:112 Resp: 209788
Ion Ratio Lower Upper
112 100
64 59.2 53.5 80.3
63 30.2 27.5 41.3

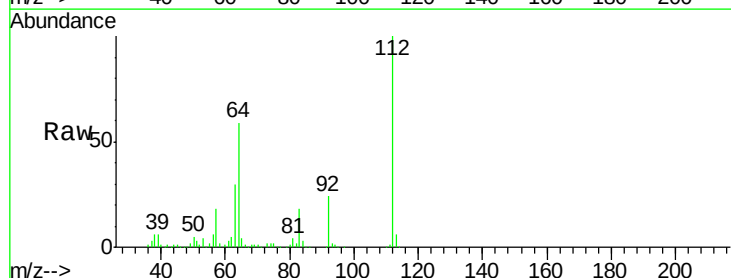

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

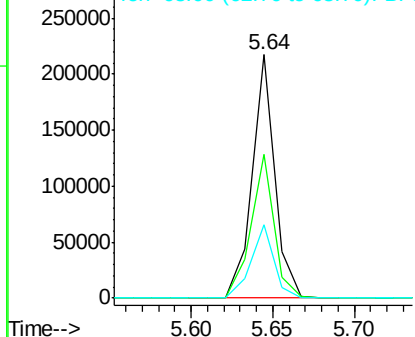

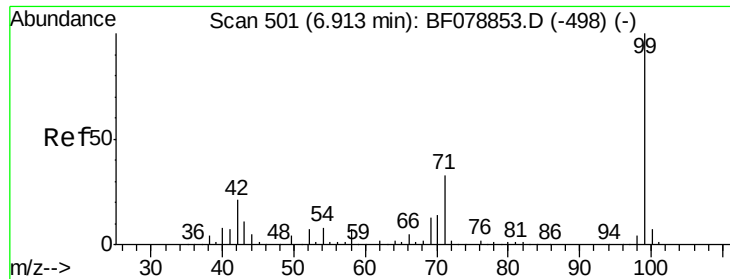

#7

Phenol-d6

Concen: 50.90 ng

RT: 6.90 min Scan# 500

Delta R.T. 0.01 min

Lab File: BF078965.D

Acq: 6 May 2015 17:31

Instrument :

BNA_F

ClientSampleId :

GRID-4(0-6)


Tgt Ion: 99 Resp: 286334

Ion Ratio Lower Upper

99 100

42 14.3 12.8 19.2

71 27.2 23.4 35.2



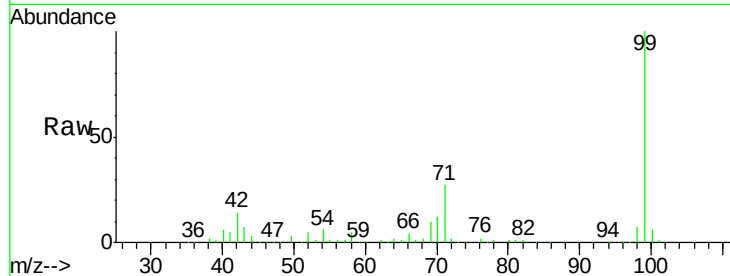


Abundance Ion 99.00 (98.70 to 99.70): BF078853.D (-498) (-)

Ion 42.00 (41.70 to 42.70): BF078853.D (-498) (-)

Ion 71.00 (70.70 to 71.70): BF078853.D (-498) (-)

Time-->

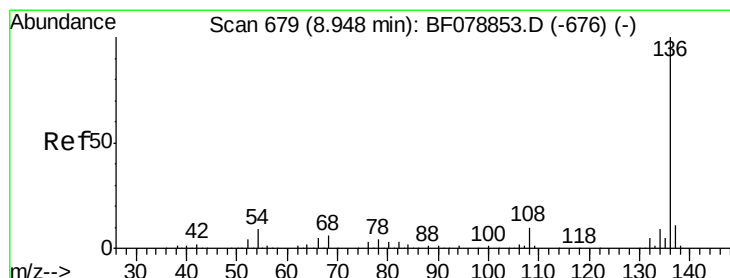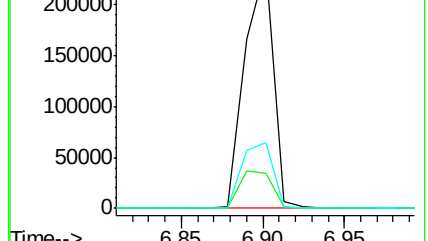

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.92 min Scan# 677

Delta R.T. -0.00 min

Lab File: BF078965.D

Acq: 6 May 2015 17:31

Tgt Ion: 136 Resp: 311322


Ion Ratio Lower Upper

136 100

137 10.6 8.7 13.1

54 7.2 5.8 8.8

68 5.5 4.2 6.4

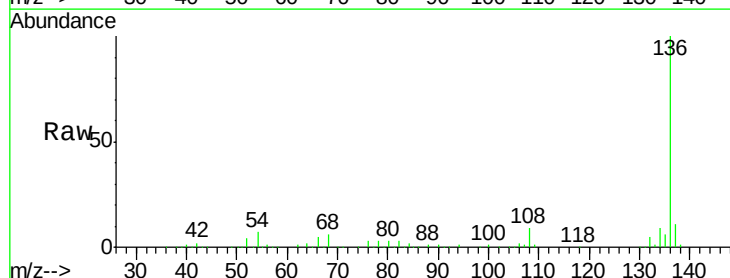



Abundance Ion 136.00 (135.70 to 136.70): BF078853.D (-676) (-)


Ion 137.00 (136.70 to 137.70): BF078853.D (-676) (-)

Ion 54.00 (53.70 to 54.70): BF078853.D (-676) (-)

Ion 68.00 (67.70 to 68.70): BF078853.D (-676) (-)

Time-->

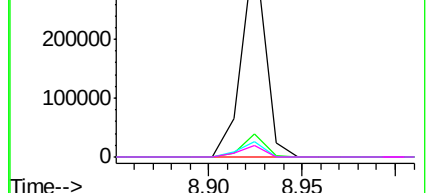







#23
 Nitrobenzene-d5
 Concen: 29.18 ng
 RT: 8.03 min Scan# 599
 Delta R.T. -0.00 min
 Lab File: BF078965.D
 Acq: 6 May 2015 17:31

Instrument :
 BNA_F
 ClientSampleId :
 GRID-4(0-6)

Tgt Ion: 82 Resp: 158048
 Ion Ratio Lower Upper
 82 100
 128 38.8 30.0 45.0
 54 54.0 46.4 69.6

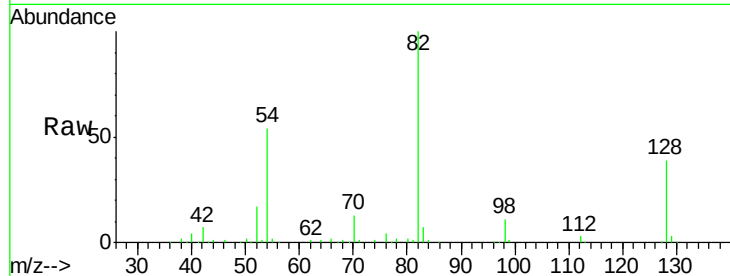


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

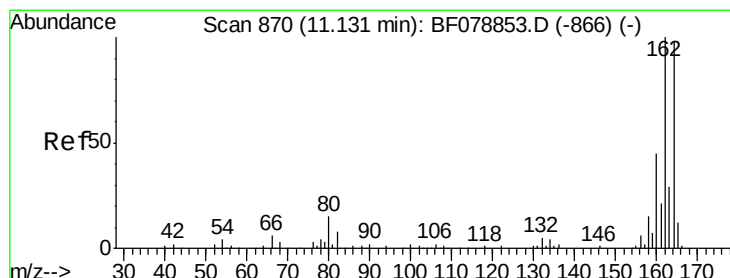
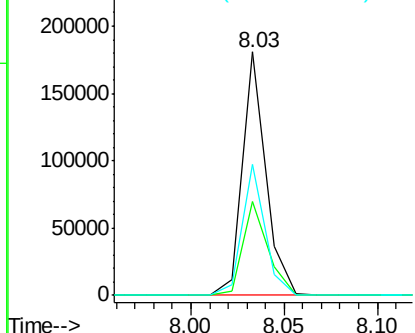



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 11.10 min Scan# 867
 Delta R.T. -0.00 min
 Lab File: BF078965.D
 Acq: 6 May 2015 17:31

Tgt Ion: 164 Resp: 144437
 Ion Ratio Lower Upper
 164 100
 162 101.7 82.7 124.1
 160 45.3 35.8 53.8

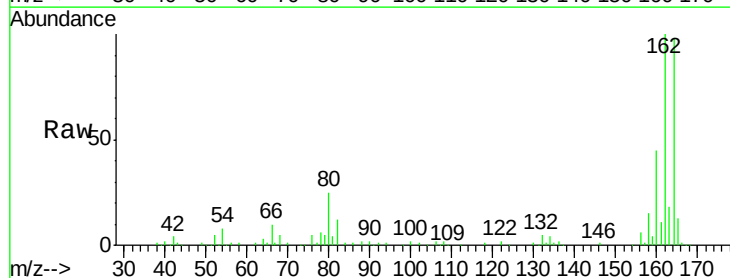

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

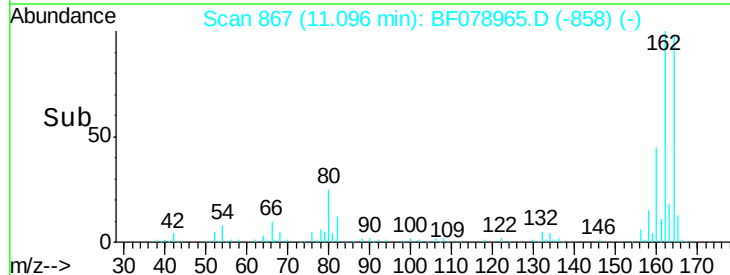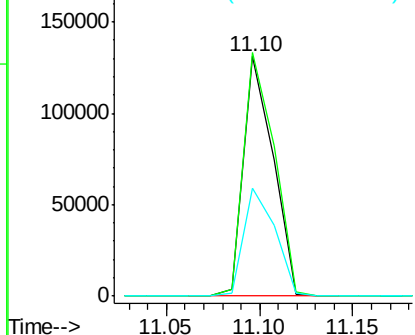







#41
 2,4,6-Tribromophenol
 Concen: 48.06 ng
 RT: 12.08 min Scan# 953
 Delta R.T. -0.00 min
 Lab File: BF078965.D
 Acq: 6 May 2015 17:31

Instrument :
 BNA_F
 ClientSampleId :
 GRID-4(0-6)

Tgt Ion:330 Resp: 75092
 Ion Ratio Lower Upper
 330 100
 332 96.5 0.0 0.0#
 141 37.0 0.0 0.0#

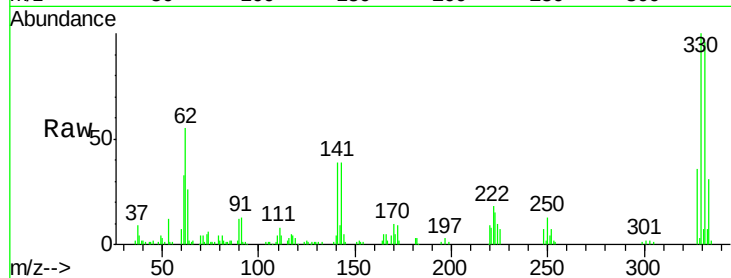


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

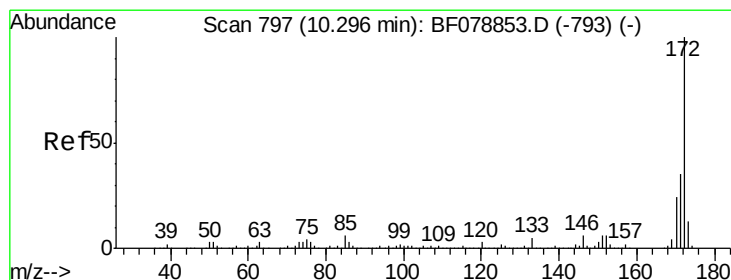
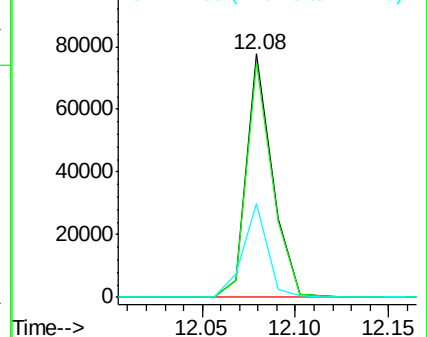



#44
 2-Fluorobiphenyl
 Concen: 30.98 ng
 RT: 10.27 min Scan# 795
 Delta R.T. -0.00 min
 Lab File: BF078965.D
 Acq: 6 May 2015 17:31

Tgt Ion:172 Resp: 321220
 Ion Ratio Lower Upper
 172 100
 171 34.9 27.9 41.9
 170 23.6 19.4 29.0

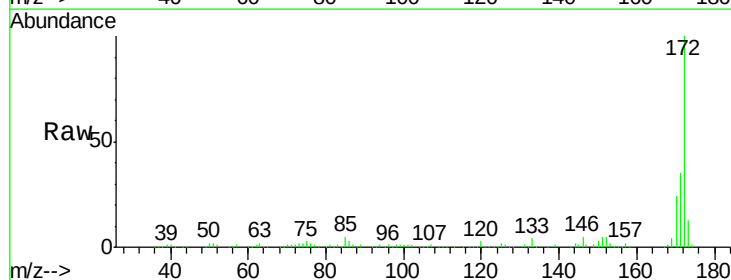

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

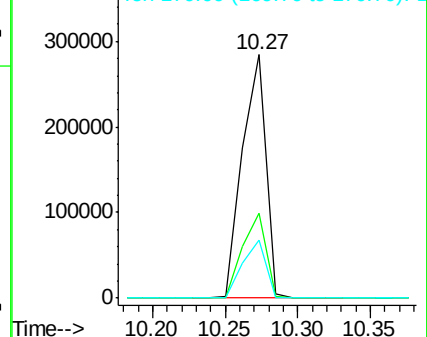







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.95 min Scan# 1029
Delta R.T. -0.00 min
Lab File: BF078965.D
Acq: 6 May 2015 17:31

Instrument :
BNA_F
ClientSampleId :
GRID-4(0-6)

Tgt Ion:188 Resp: 301006
Ion Ratio Lower Upper
188 100
94 10.1 8.2 12.2
80 10.1 8.9 13.3

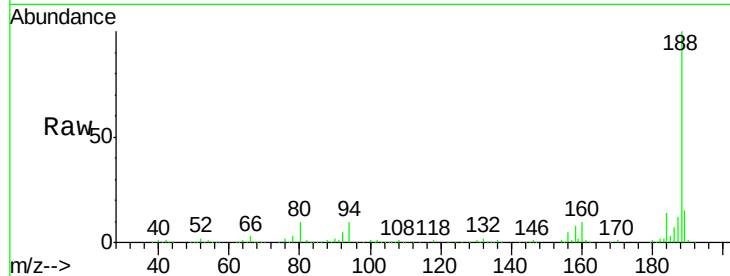


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

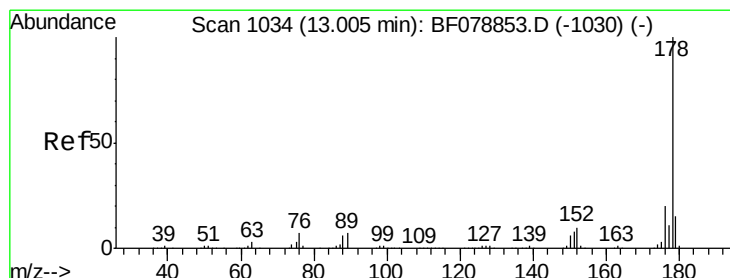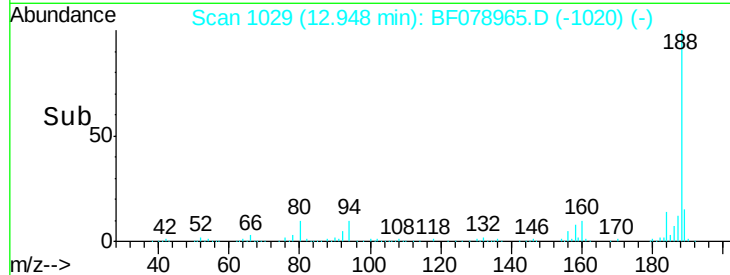
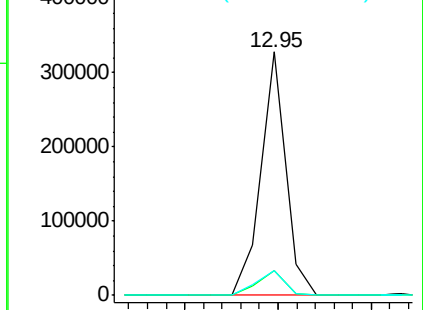



#70
Phenanthrene
Concen: 11.60 ng
RT: 12.98 min Scan# 1032
Delta R.T. -0.00 min
Lab File: BF078965.D
Acq: 6 May 2015 17:31

Tgt Ion:178 Resp: 195321
Ion Ratio Lower Upper
178 100
176 19.0 15.8 23.8
179 14.7 12.5 18.7

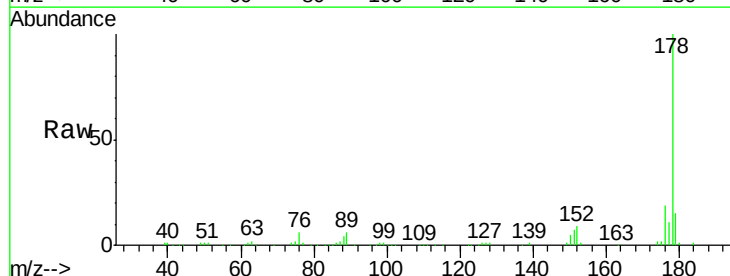

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

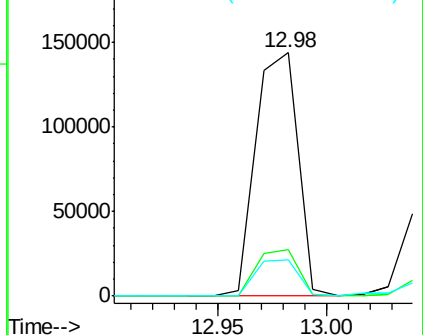


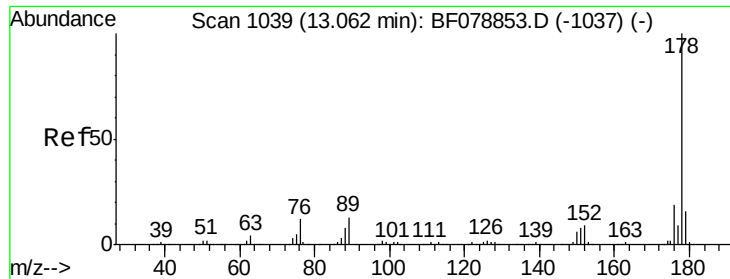




#71
 Anthracene
 Concen: 2.63 ng
 RT: 13.04 min Scan# 1037
 Delta R.T. -0.00 min
 Lab File: BF078965.D
 Acq: 6 May 2015 17:31

Instrument :
 BNA_F
 ClientSampleId :
 GRID-4(0-6)

Tgt Ion:178 Resp: 43493
 Ion Ratio Lower Upper
 178 100
 176 18.8 15.5 23.3
 179 16.2 12.7 19.1

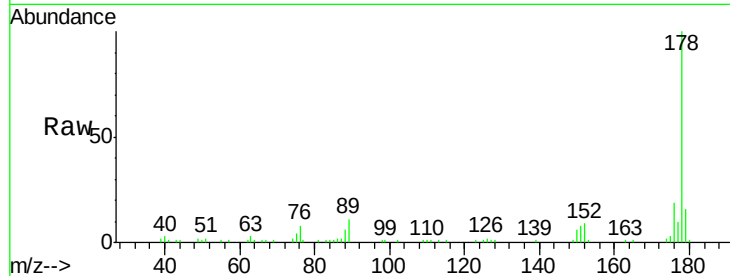


Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 176.00 (175.70 to 176.70): E
 Ion 179.00 (178.70 to 179.70): E

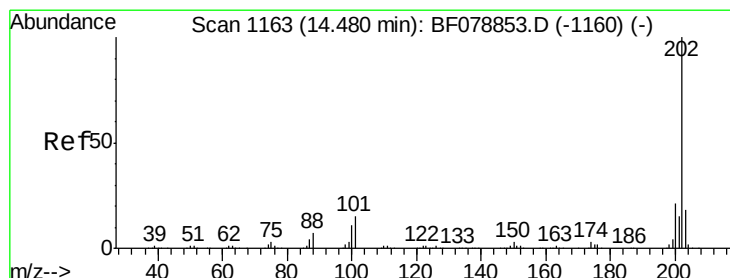
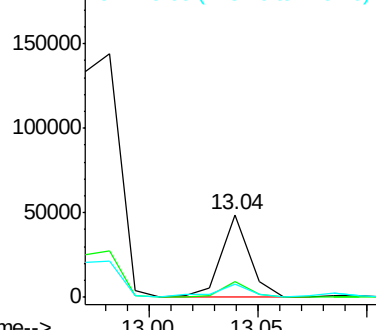



#74
 Fluoranthene
 Concen: 19.43 ng
 RT: 14.46 min Scan# 1161
 Delta R.T. -0.00 min
 Lab File: BF078965.D
 Acq: 6 May 2015 17:31

Tgt Ion:202 Resp: 340887
 Ion Ratio Lower Upper
 202 100
 101 12.7 0.0 34.6
 203 18.2 0.0 38.4

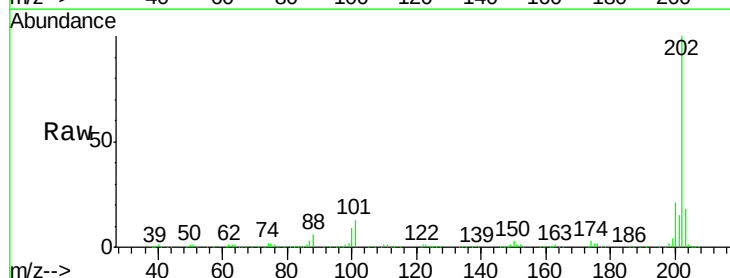

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 203.00 (202.70 to 203.70): E




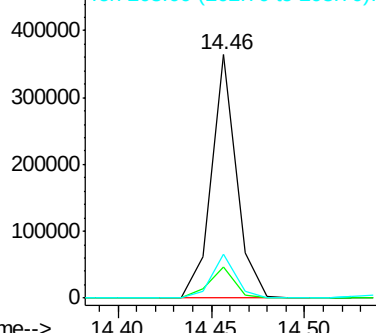




#75
Chrysene-d12
Concen: 20.00 ng
RT: 16.25 min Scan# 1318
Delta R.T. -0.06 min
Lab File: BF078965.D
Acq: 6 May 2015 17:31


Instrument :
BNA_F
ClientSampleId :
GRID-4(0-6)


Tgt Ion: 240 Resp: 326070
Ion Ratio Lower Upper
240 100
120 11.2 9.7 14.5
236 26.1 20.2 30.4

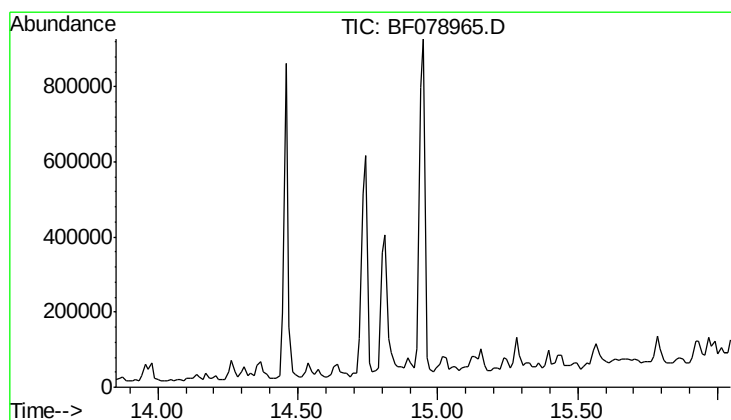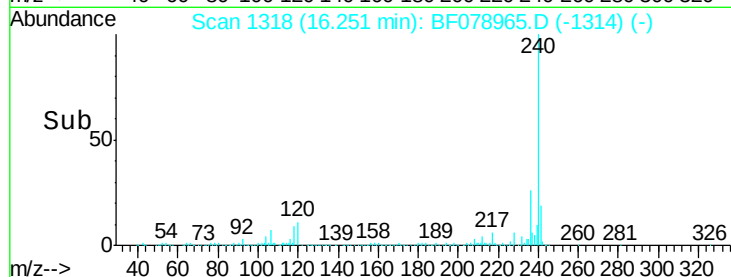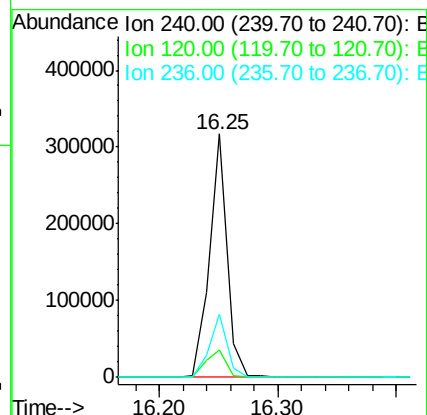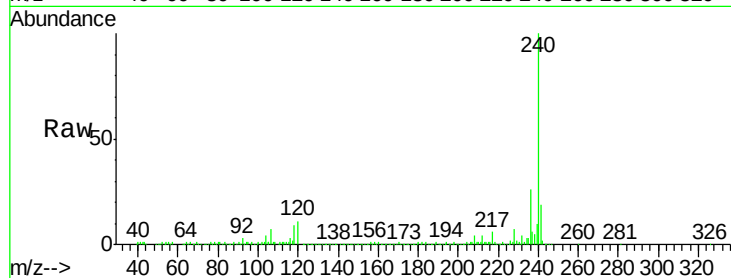

#78
Terphenyl-d14
Concen: 0.00 ng
Expected RT: 14.95 min
Lab File: BF078965.D
Acq: 6 May 2015 17:31

Tgt Ion: 244
Sig Exp Ratio
244 100
212 7.0
122 12.9

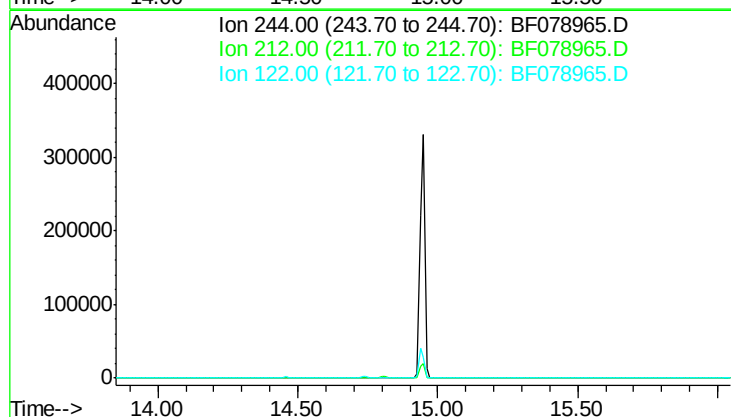



#80

Benzo(a)anthracene

Concen: 10.03 ng

RT: 16.24 min Scan# 1317

Delta R.T. -0.05 min

Lab File: BF078965.D

Acq: 6 May 2015 17:31

Instrument :

BNA_F

ClientSampleId :

GRID-4(0-6)


Tgt Ion:228 Resp: 179170

Ion Ratio Lower Upper

228 100

226 29.5 22.6 33.8




229 20.8 15.9 23.9

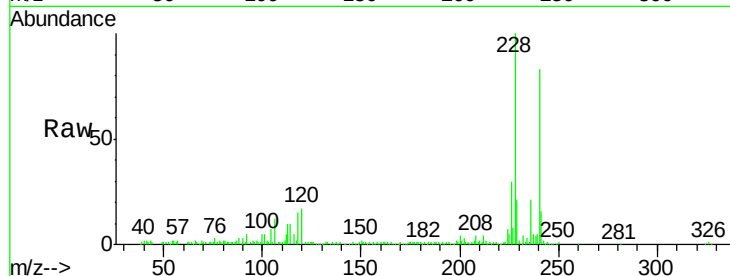

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

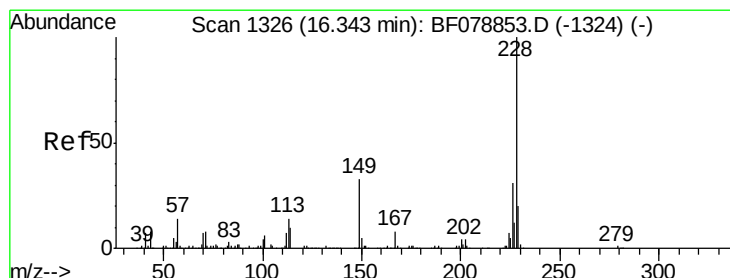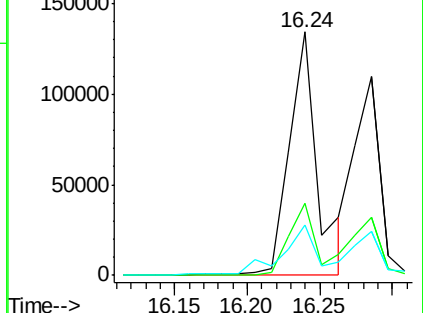

#82

Chrysene

Concen: 7.64 ng

RT: 16.29 min Scan# 1321

Delta R.T. -0.06 min

Lab File: BF078965.D

Acq: 6 May 2015 17:31


Tgt Ion:228 Resp: 131281

Ion Ratio Lower Upper

228 100

226 29.2 24.9 37.3



229 21.9 16.0 24.0

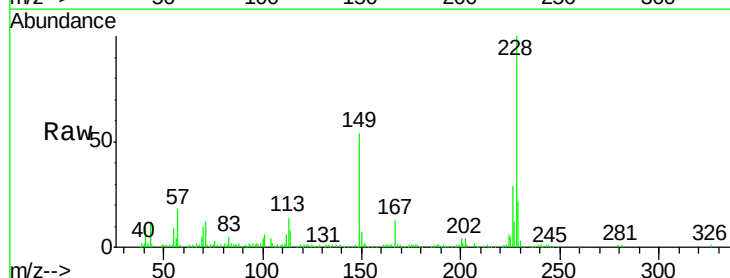


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E



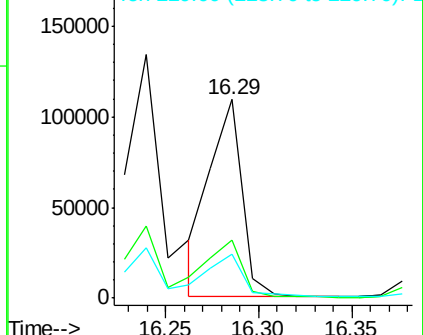





#83
 Bis(2-ethylhexyl)phthalate
 Concen: 5.06 ng
 RT: 16.29 min Scan# 1321
 Delta R.T. -0.07 min
 Lab File: BF078965.D
 Acq: 6 May 2015 17:31




Instrument :
 BNA_F
 ClientSampleId :
 GRID-4(0-6)


Tgt Ion	Ratio	Lower	Upper
149	100		
167	24.2	21.8	32.8
279	2.5	2.9	4.3#

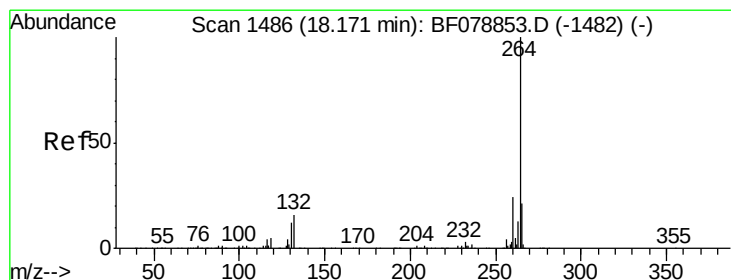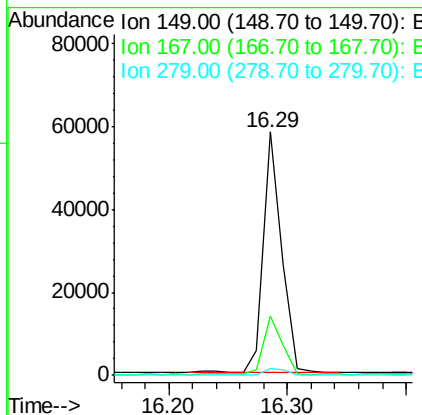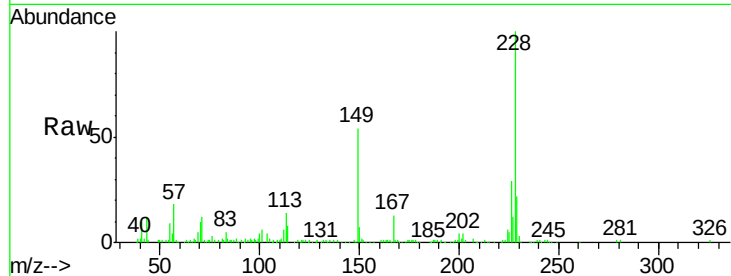

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 18.02 min Scan# 1473
 Delta R.T. -0.21 min
 Lab File: BF078965.D
 Acq: 6 May 2015 17:31

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.5	19.4	29.2
265	22.3	18.3	27.5


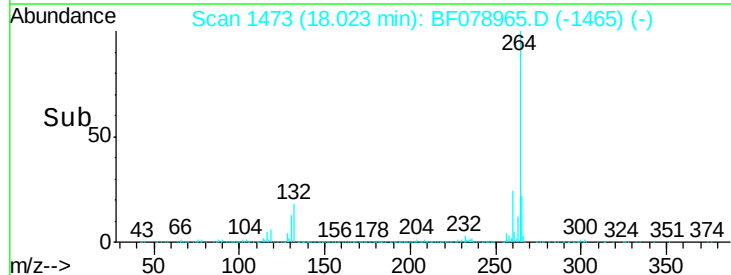
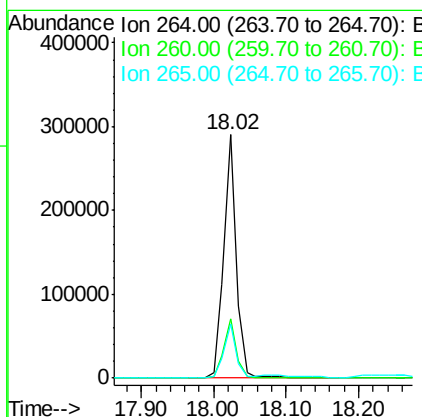
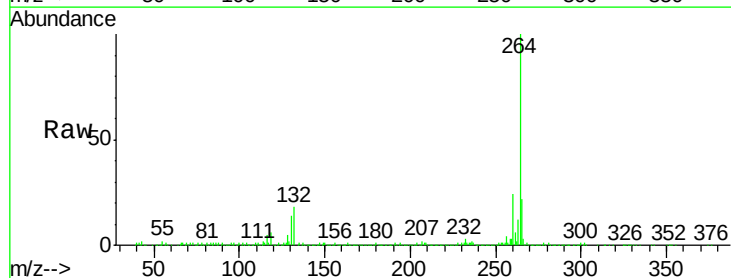




#87
Benzo(b)fluoranthene
Concen: 10.50 ng
RT: 17.57 min Scan# 1433
Delta R.T. -0.16 min
Lab File: BF078965.D
Acq: 6 May 2015 17:31




Instrument :
BNA_F
ClientSampleId :
GRID-4(0-6)


Tgt Ion:252 Resp: 203385
Ion Ratio Lower Upper
252 100
253 22.1 17.7 26.5
125 11.7 9.5 14.3

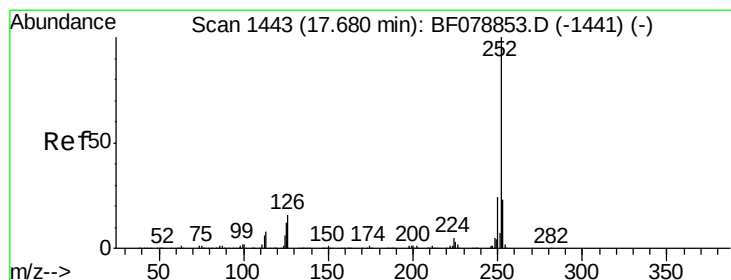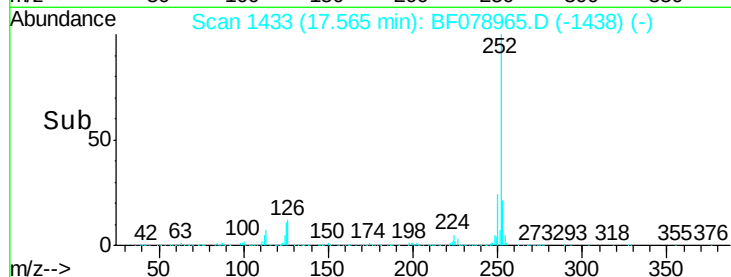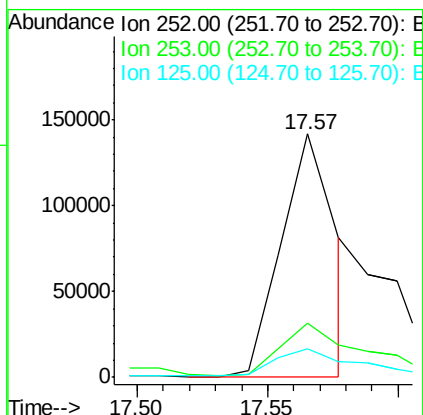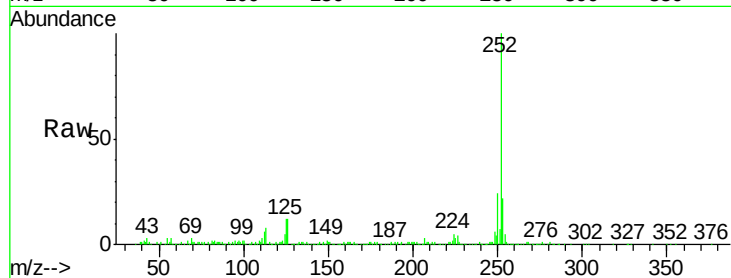

#88
Benzo(k)fluoranthene
Concen: 15.31 ng
RT: 17.57 min Scan# 1433
Delta R.T. -0.19 min
Lab File: BF078965.D
Acq: 6 May 2015 17:31

Tgt Ion:252 Resp: 287128
Ion Ratio Lower Upper
252 100
253 22.1 18.1 27.1
125 11.7 10.0 15.0

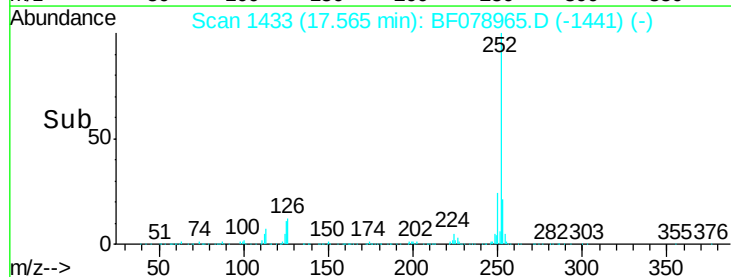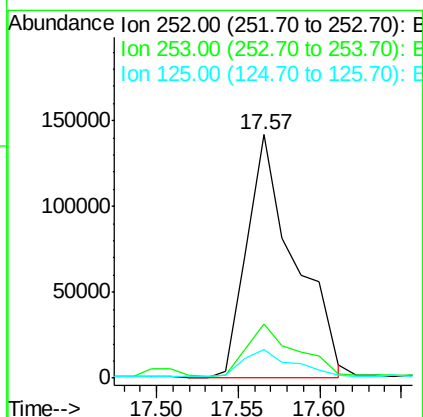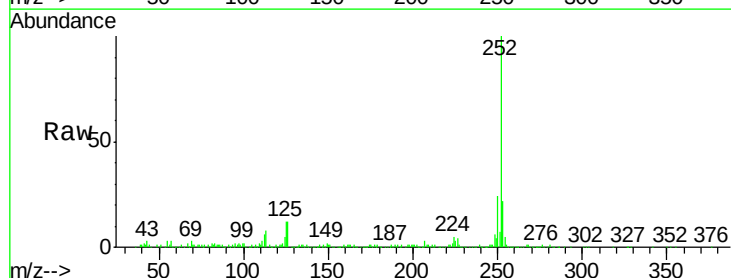



#89

Benzo(a)pyrene

Concen: 8.59 ng

RT: 17.95 min Scan# 1467

Delta R.T. -0.19 min

Lab File: BF078965.D

Acq: 6 May 2015 17:31





Instrument :

BNA_F

ClientSampleId :

GRID-4(0-6)

Tgt Ion:	252	Resp:	153157
Ion	Ratio	Lower	Upper
252	100		
253	23.1	17.3	25.9
125	11.4	7.0	10.6#

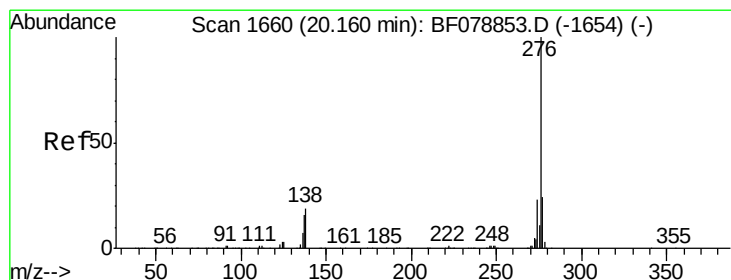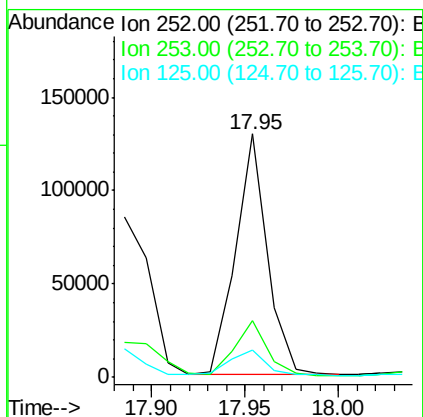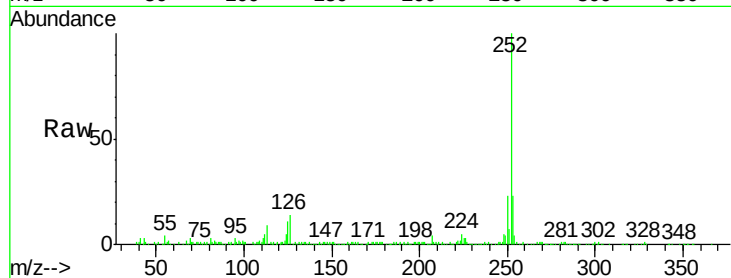

#91

Benzo(g,h,i)perylene

Concen: 5.60 ng

RT: 19.97 min Scan# 1643

Delta R.T. -0.24 min

Lab File: BF078965.D

Acq: 6 May 2015 17:31

Tgt Ion:	276	Resp:	106454
Ion	Ratio	Lower	Upper
276	100		
277	23.5	18.6	28.0
138	24.6	17.4	26.0

