


Data Path : Z:\HPCHEM1\BNA_F\Data\BF050615\
 Data File : BF078951.D
 Acq On : 6 May 2015 10:42
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 30 19:07:47 2015

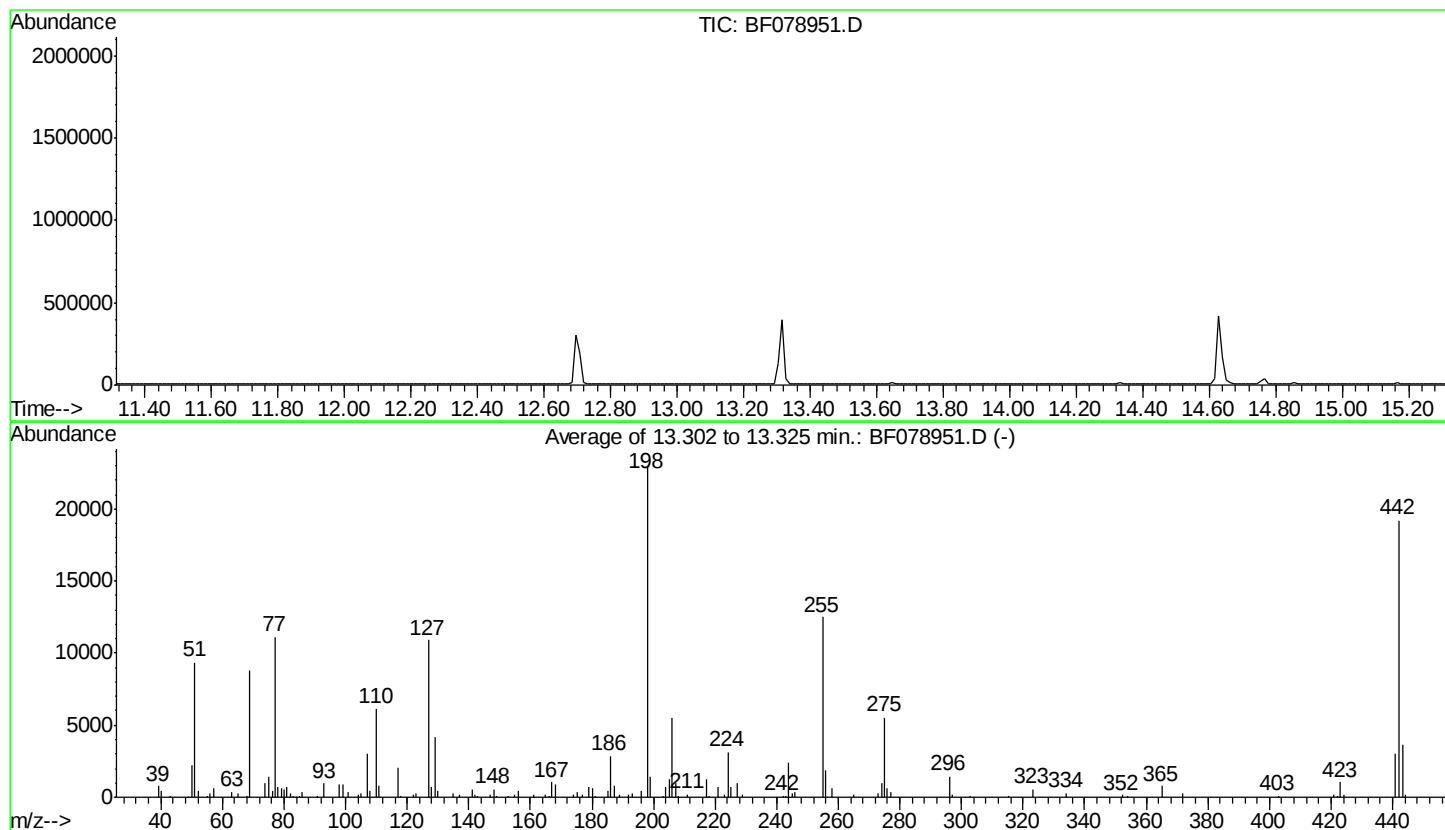

AutoFind: Scans 1060, 1061, 1062; Background Corrected with Scan 1057

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	9344	PASS
68	69	0.00	2	1.2	103	PASS
69	198	0.00	100	38.2	8791	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.4	10905	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	23013	PASS
199	198	5	9	6.2	1437	PASS
275	198	10	60	23.9	5510	PASS
365	198	1	100	3.4	775	PASS
441	442	0.01	24	15.6	3001	PASS
442	198	50	100	83.5	19211	PASS
443	442	15	24	18.9	3638	PASS