
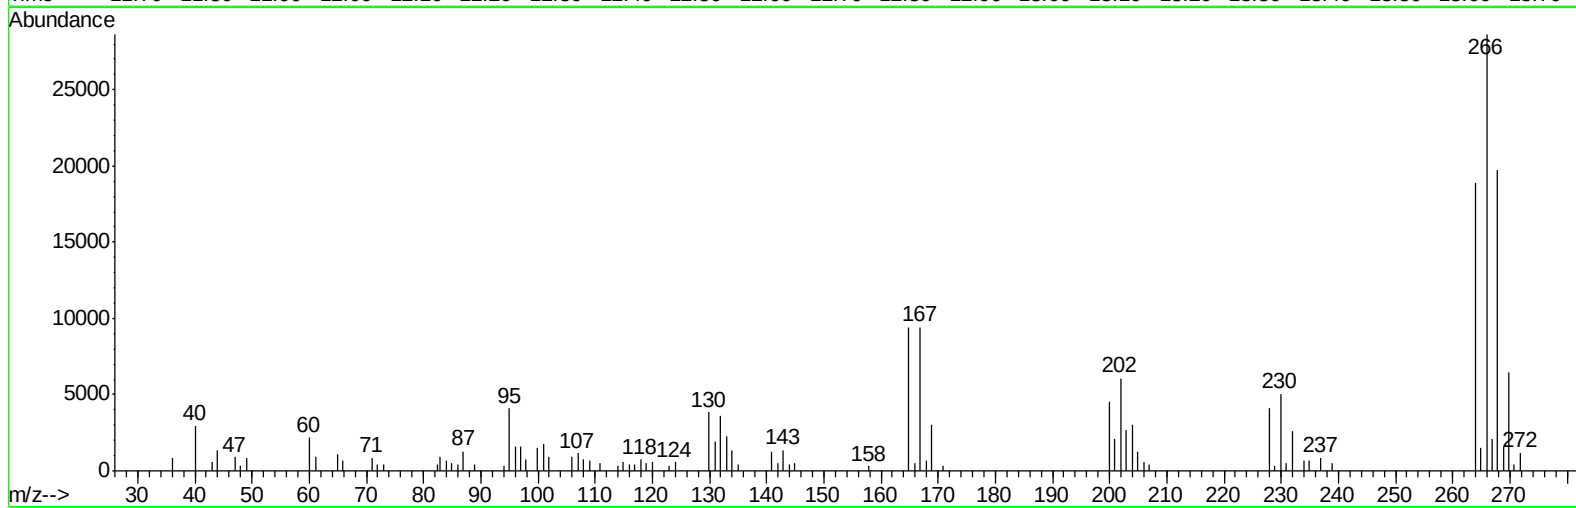


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050615\
Data File : BF078951.D
Acq On : 6 May 2015 10:42
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 07 07:42:27 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 07 05:28:56 2015
Response via : Initial Calibration

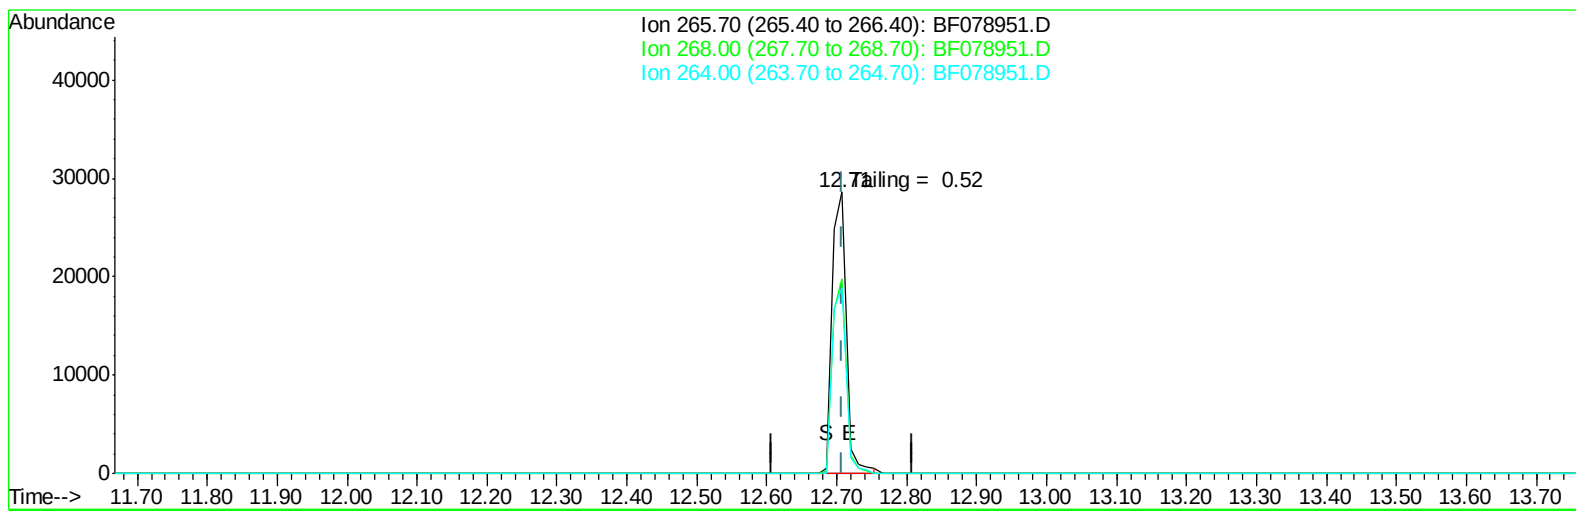

TIC: BF078951.D

(69) Pentachlorophenol (C)



12.708min (-0.000) 0.00ng

response 40187

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	68.93
264.00	60.20	66.14
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050615\
Data File : BF078951.D
Acq On : 6 May 2015 10:42
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 07 07:42:27 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 07 05:28:56 2015
Response via : Initial Calibration

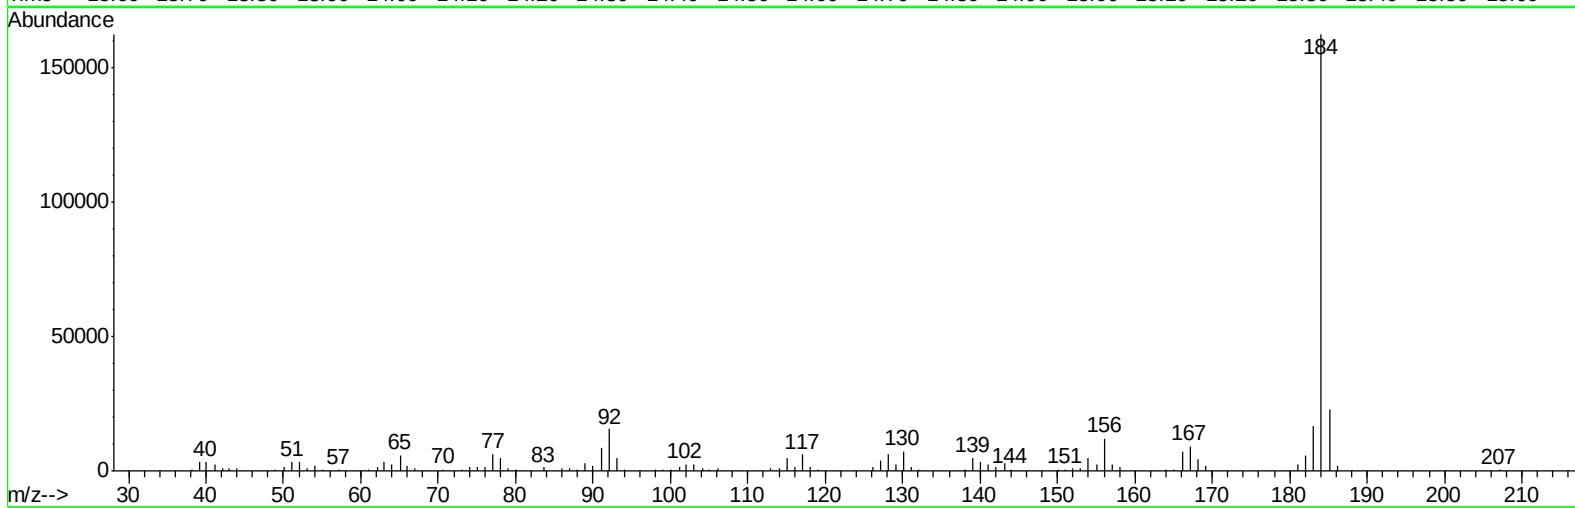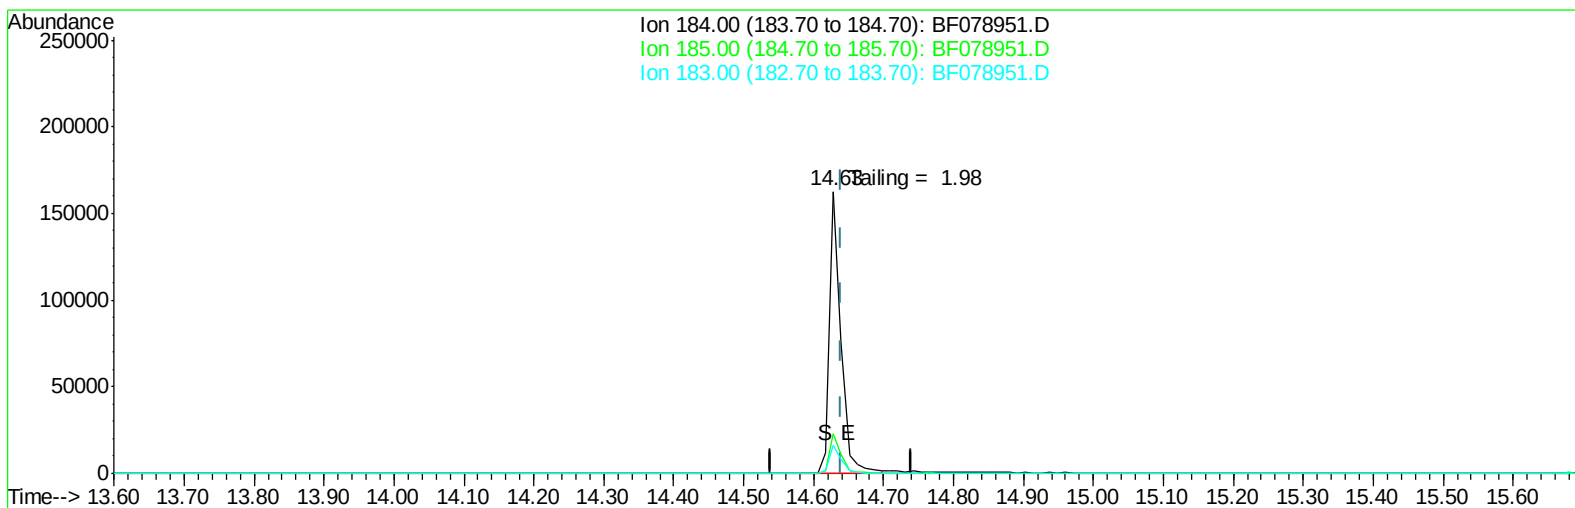

TIC: BF078951.D

(76) Benzidine

14.628min (-0.011) 0.00ng

response 186975

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.13
183.00	10.50	10.19
0.00	0.00	0.00