


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050615\
 Data File : BF078976.D
 Acq On : 7 May 2015 00:10
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 30 19:07:47 2015

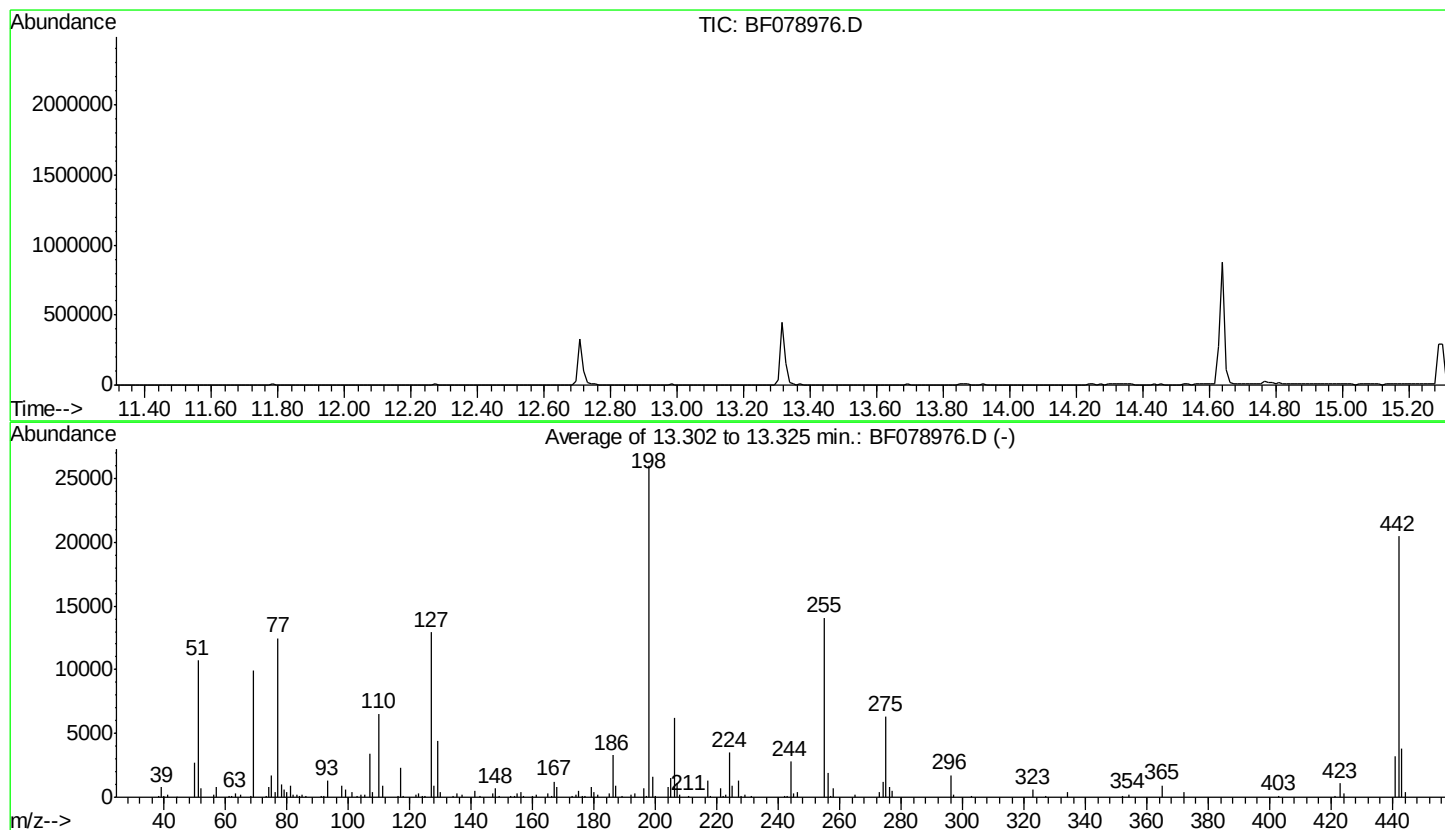

AutoFind: Scans 1060, 1061, 1062; Background Corrected with Scan 1057

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	10705	PASS
68	69	0.00	2	1.3	131	PASS
69	198	0.00	100	38.1	9912	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.7	12935	PASS
197	198	0.00	2	0.4	102	PASS
198	198	100	100	100.0	26002	PASS
199	198	5	9	6.1	1590	PASS
275	198	10	60	24.2	6289	PASS
365	198	1	100	3.5	904	PASS
441	442	0.01	24	15.8	3226	PASS
442	198	50	100	78.6	20448	PASS
443	442	15	24	18.8	3848	PASS