

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050616\
 Data File : BF086738.D
 Acq On : 6 May 2016 21:59
 Operator : UM/SJ
 Sample : H2770-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: May 07 03:27:40 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050416.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 07 03:18:46 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	166445	40.00	ng	0.00
21) Naphthalene-d8	8.00	136	687369	40.00	ng	0.00
38) Acenaphthene-d10	9.74	164	333206	40.00	ng	0.00
63) Phenanthrene-d10	11.22	188	604376	40.00	ng	-0.01
75) Chrysene-d12	13.85	240	423265	40.00	ng	-0.01
86) Perylene-d12	15.23	264	319654	40.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.31	112	541937	53.90	ng	-0.01
7) Phenol-d6	6.36	99	472509	34.89	ng	-0.02
23) Nitrobenzene-d5	7.28	82	1021431	76.36	ng	-0.01
41) 2,4,6-Tribromophenol	10.53	330	421338	129.26	ng	-0.01
44) 2-Fluorobiphenyl	9.07	172	1692487	83.26	ng	-0.01
78) Terphenyl-d14	12.81	244	1421365	67.87	ng	0.00
Target Compounds						
9) Benzaldehyde	6.48	77	26445	3.91	ng	# 69
15) Benzyl Alcohol	6.86	79	19069	2.18	ng	# 38
19) n-Nitroso-di-n-propylamine	7.28	70	141934	15.34	ng	# 72
50) 2,6-Dinitrotoluene	9.74	165	41292	7.75	ng	# 21
56) 2,4-Dinitrotoluene	9.74	165	41287	6.25	ng	# 16
64) 4,6-Dinitro-2-methylphenol	10.53	198	955	5.57	ng	# 1
66) 4-Bromophenyl-phenylether	10.53	248	27099	4.51	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050616\
Data File : BF086738.D
Acq On : 6 May 2016 21:59
Operator : UM/SJ
Sample : H2770-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: May 07 03:27:40 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 07 03:18:46 2016
Response via : Initial Calibration

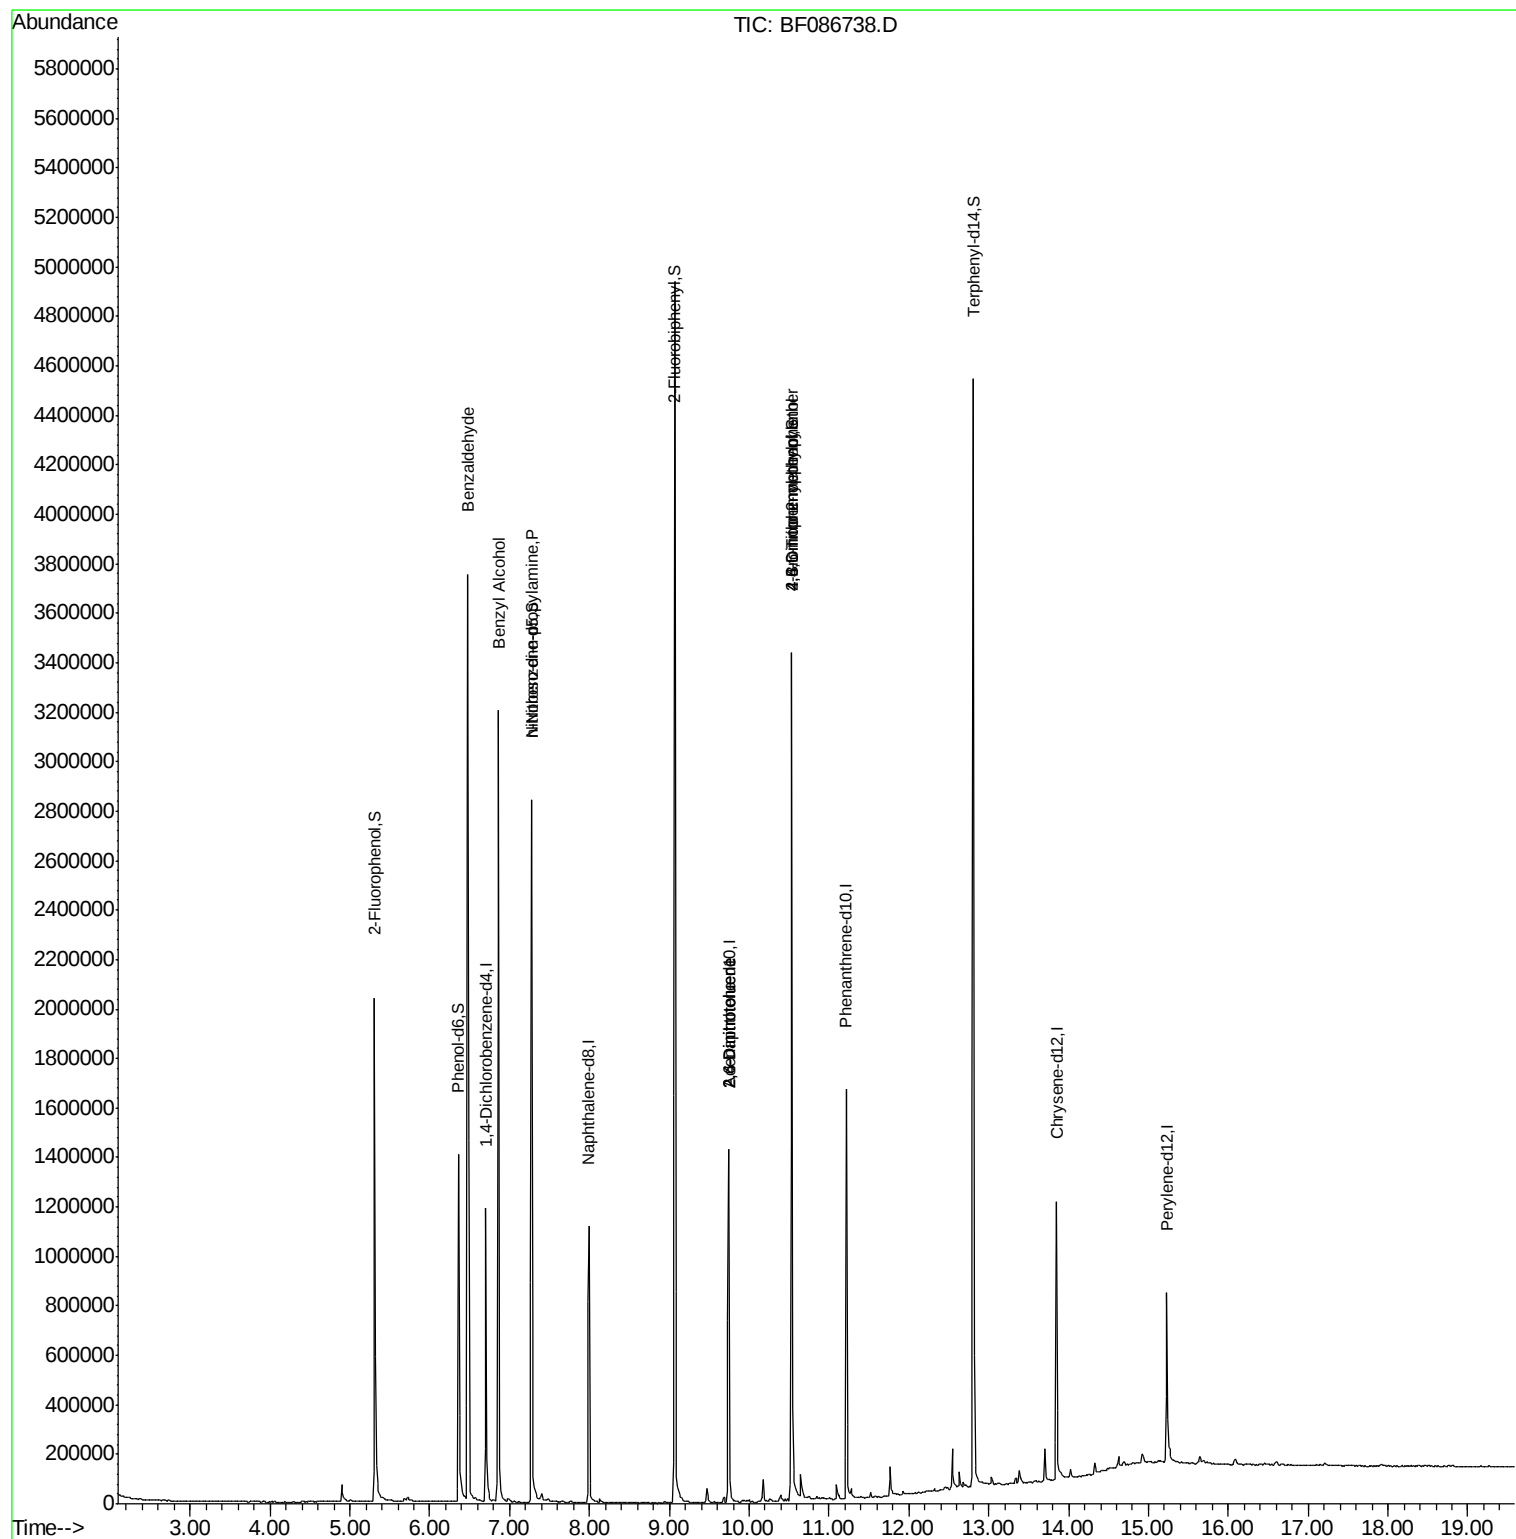



#1

1,4-Dichlorobenzene-d4

Concen: 40.00 ng

RT: 6.70 min Scan# 404

Delta R.T. -0.00 min

Lab File: BF086738.D

Acq: 6 May 2016 21:59

Instrument :

BNA_F

ClientSampleId :


Tot Ion:152 Resp: 166445

Ion Ratio Lower Upper

152 100

150 157.5 125.8 188.6




115 64.6 51.5 77.3



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

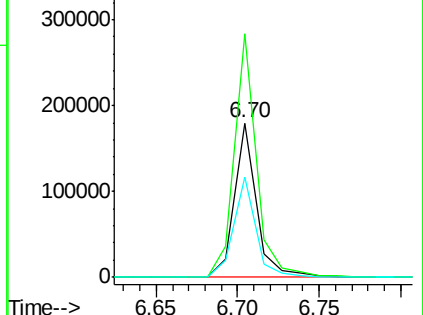

#5

2-Fluorophenol

Concen: 53.90 ng

RT: 5.31 min Scan# 282

Delta R.T. -0.01 min

Lab File: BF086738.D

Acq: 6 May 2016 21:59


Tgt Ion:112 Resp: 541937

Ion Ratio Lower Upper

112 100

64 72.9 52.1 78.1



63 39.6 25.7 38.5#




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

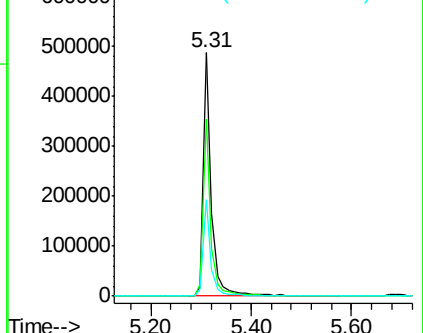

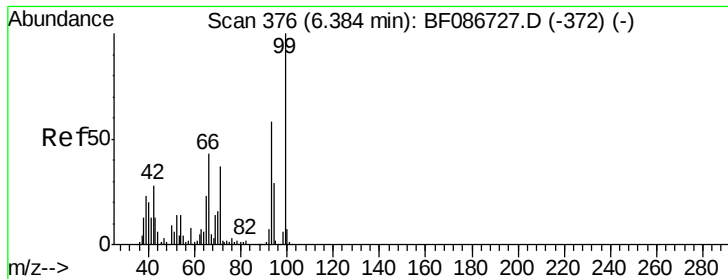

#7

Phenol-d6

Concen: 34.89 ng

RT: 6.36 min Scan# 374

Delta R.T. -0.02 min

Lab File: BF086738.D

Acq: 6 May 2016 21:59

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 472509

Ion Ratio Lower Upper

99 100

42 28.4 13.6 20.4#




71 36.6 24.6 36.8

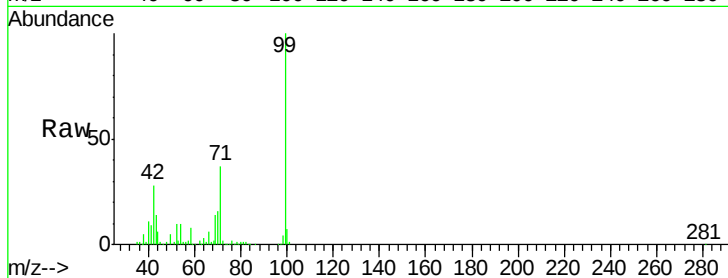

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

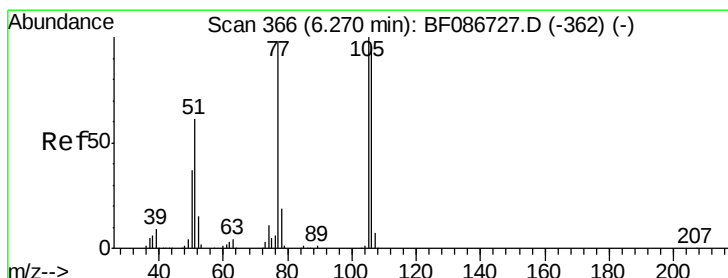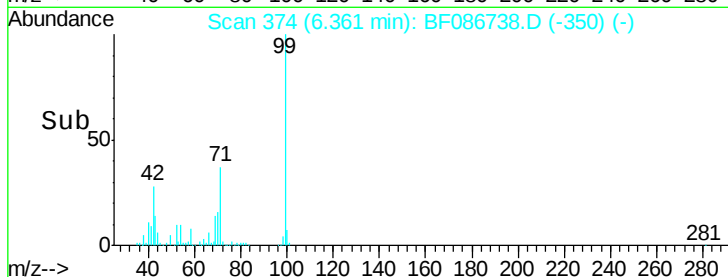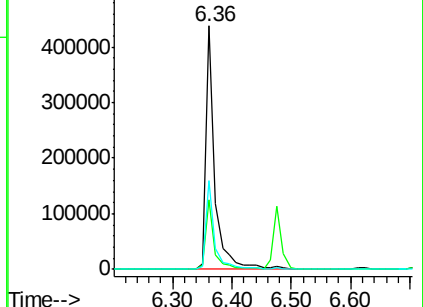

#9

Benzaldehyde

Concen: 3.91 ng

RT: 6.48 min Scan# 384

Delta R.T. 0.21 min

Lab File: BF086738.D

Acq: 6 May 2016 21:59


Tgt Ion: 77 Resp: 26445

Ion Ratio Lower Upper

77 100

105 67.6 72.7 112.7#



106 55.8 70.8 110.8#

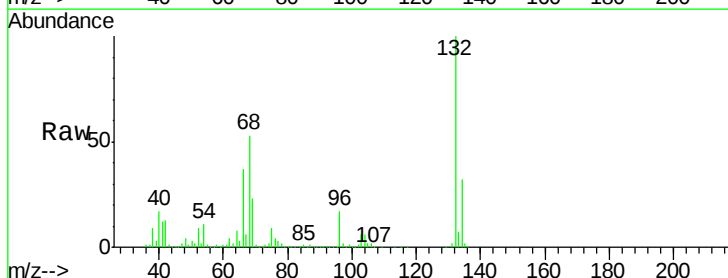


Abundance Ion 77.00 (76.70 to 77.70): BF0

Ion 105.00 (104.70 to 105.70): E

Ion 106.00 (105.70 to 106.70): E

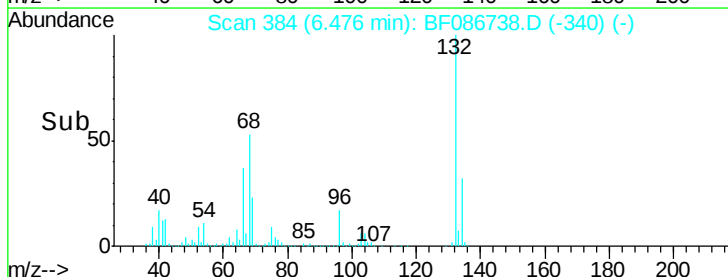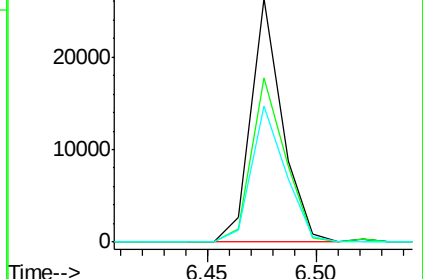

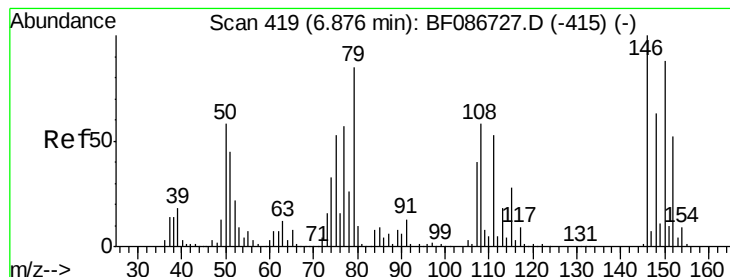

#15

Benzyl Alcohol

Concen: 2.18 ng

RT: 6.86 min Scan# 418

Delta R.T. -0.01 min

Lab File: BF086738.D

Acq: 6 May 2016 21:59

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 79 Resp: 19069

Ion Ratio Lower Upper

79 100

108 36.0 68.4 102.6#




77 119.3 50.6 76.0#

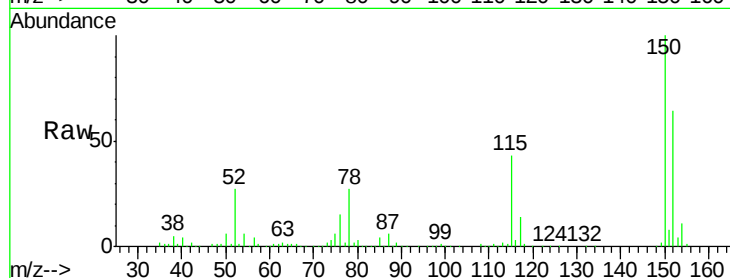

Abundance Ion 79.00 (78.70 to 79.70): BF0

Ion 108.00 (107.70 to 108.70): BF0

Ion 77.00 (76.70 to 77.70): BF0

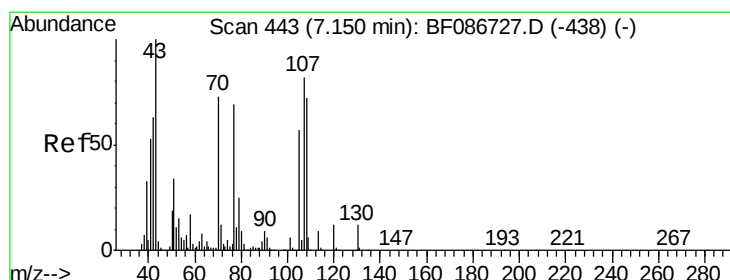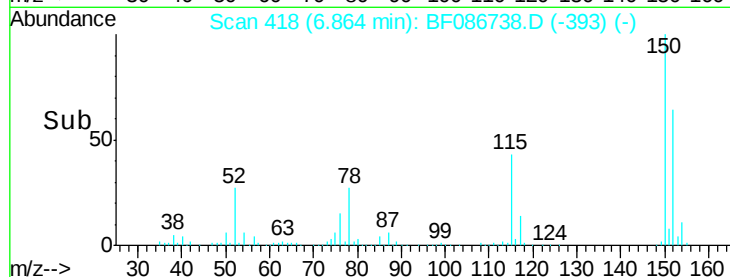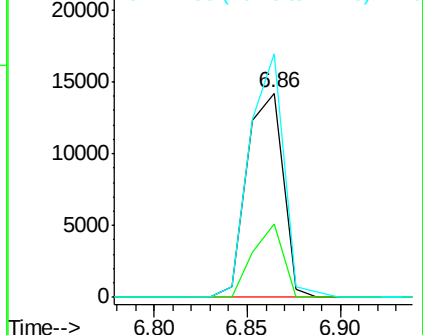

#19

n-Nitroso-di-n-propylamine

Concen: 15.34 ng

RT: 7.28 min Scan# 454

Delta R.T. 0.13 min

Lab File: BF086738.D

Acq: 6 May 2016 21:59

Tgt Ion: 70 Resp: 141934


Ion Ratio Lower Upper

70 100

42 69.3 43.1 64.7#

101 0.0 8.1 12.1#

130 1.6 18.6 28.0#


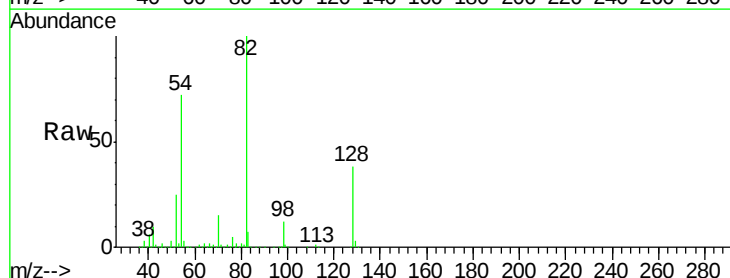



Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

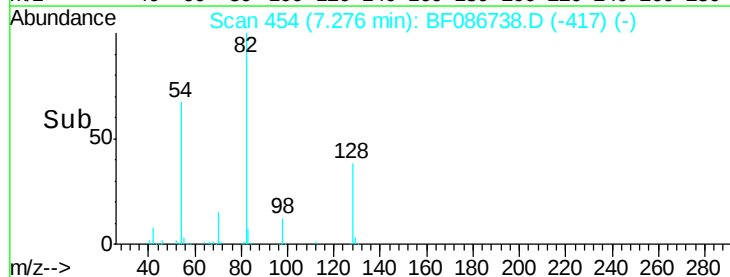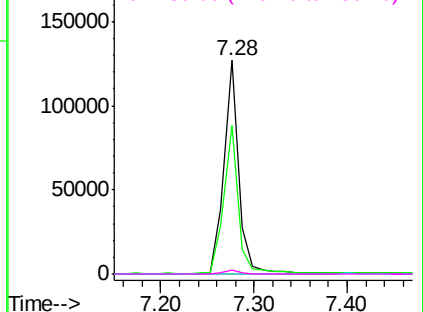



#21

Naphthalene-d8

Concen: 40.00 ng

RT: 8.00 min Scan# 517

Delta R.T. -0.00 min

Lab File: BF086738.D


Acq: 6 May 2016 21:59

Instrument :

BNA_F

ClientSampleId :

Tot Ion:	136	Resp:	687369
Ion	Ratio	Lower	Upper
136	100		
137	10.6	8.8	13.2
54	9.1	5.0	7.4#
68	5.2	4.4	6.6



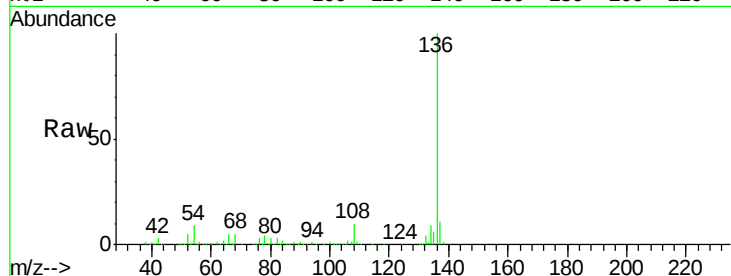


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

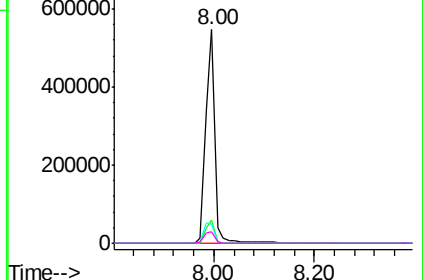

#23

Nitrobenzene-d5

Concen: 76.36 ng


RT: 7.28 min Scan# 454

Delta R.T. -0.01 min

Lab File: BF086738.D

Acq: 6 May 2016 21:59



Tgt Ion:	82	Resp:	1021431
Ion	Ratio	Lower	Upper
82	100		
128	38.3	40.6	61.0#
54	72.2	38.1	57.1#




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

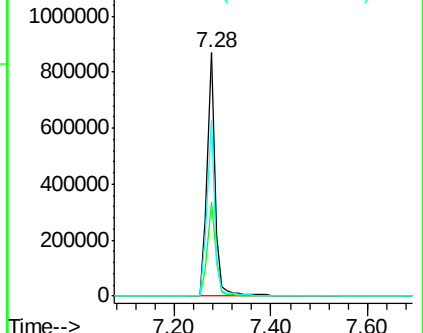

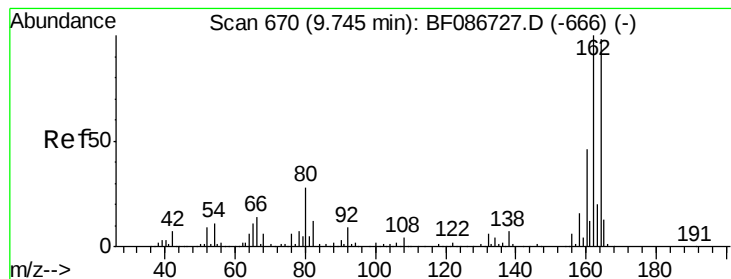

#38

Acenaphthene-d10

Concen: 40.00 ng

RT: 9.74 min Scan# 670

Delta R.T. -0.00 min

Lab File: BF086738.D

Acq: 6 May 2016 21:59

Instrument :

BNA_F

ClientSampleId :


Tot Ion:164 Resp: 333206

Ion Ratio Lower Upper

164 100

162 104.3 82.8 124.2




160 47.1 36.9 55.3



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

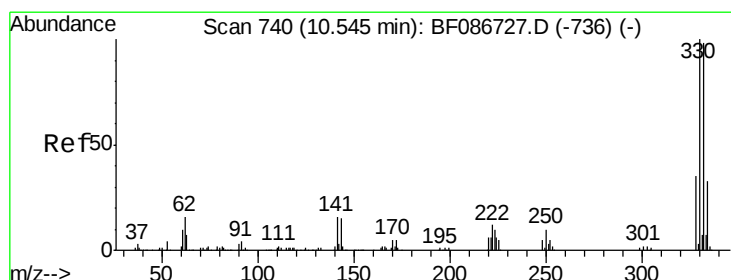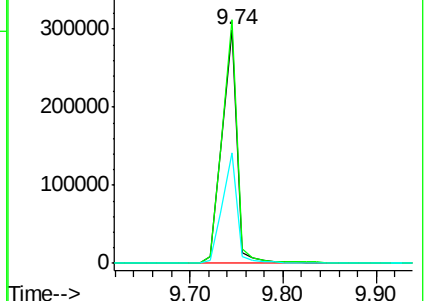

#41

2,4,6-Tribromophenol

Concen: 129.26 ng

RT: 10.53 min Scan# 739

Delta R.T. -0.01 min

Lab File: BF086738.D

Acq: 6 May 2016 21:59


Tgt Ion:330 Resp: 421338

Ion Ratio Lower Upper

330 100

332 96.6 79.0 118.4



141 41.9 31.2 46.8




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

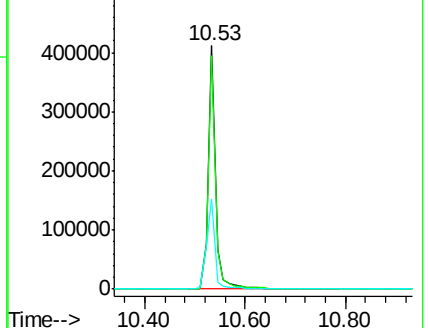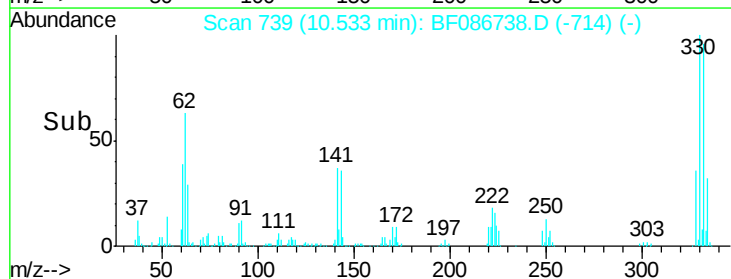

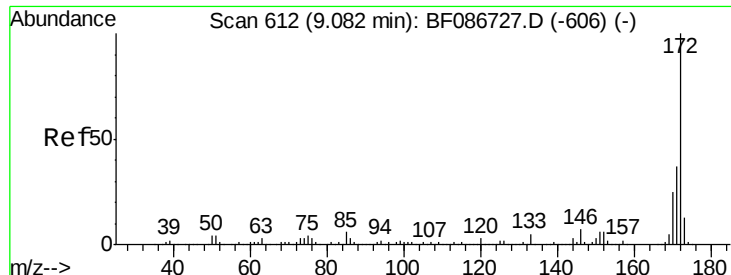


#44
 2-Fluorobiphenyl
 Concen: 83.26 ng
 RT: 9.07 min Scan# 611
 Delta R.T. -0.01 min
 Lab File: BF086738.D
 Acq: 6 May 2016 21:59




Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:172 Resp: 1692487

Ion	Ratio	Lower	Upper
172	100		
171	36.7	29.0	43.6
170	24.8	19.8	29.8

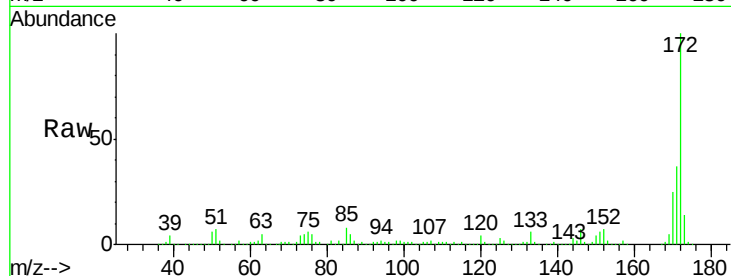


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

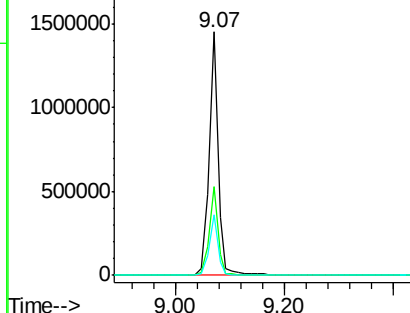



#50
 2,6-Dinitrotoluene
 Concen: 7.75 ng
 RT: 9.74 min Scan# 670
 Delta R.T. 0.19 min
 Lab File: BF086738.D
 Acq: 6 May 2016 21:59


Tgt Ion:165 Resp: 41292

Ion	Ratio	Lower	Upper
165	100		
63	1.9	51.8	77.8#
89	2.0	50.7	76.1#

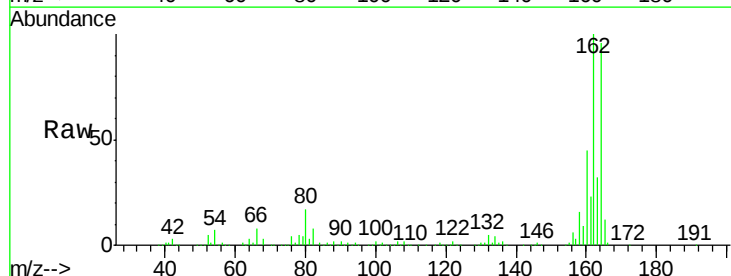

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF0
 Ion 89.00 (88.70 to 89.70): BF0

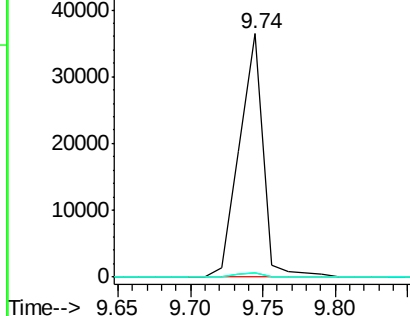







#56
 2,4-Dinitrotoluene
 Concen: 6.25 ng
 RT: 9.74 min Scan# 670
 Delta R.T. -0.21 min
 Lab File: BF086738.D
 Acq: 6 May 2016 21:59

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:165 Resp: 41287
 Ion Ratio Lower Upper
 165 100
 63 1.9 44.3 66.5#
 89 2.0 70.0 105.0#
 182 0.0 1.8 2.6#

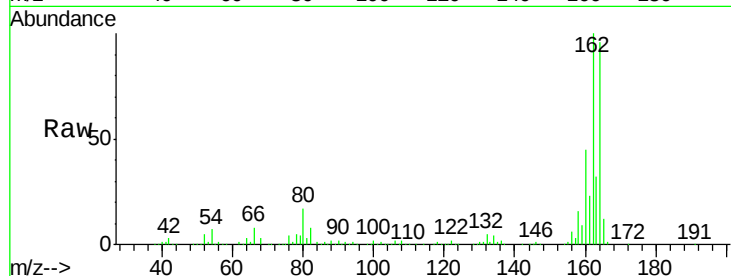


Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF0
 Ion 89.00 (88.70 to 89.70): BF0
 Ion 182.00 (181.70 to 182.70): E

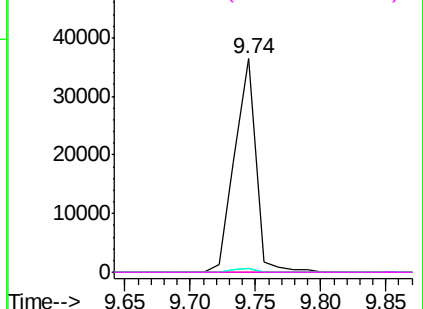




#63
 Phenanthrene-d10
 Concen: 40.00 ng
 RT: 11.22 min Scan# 799
 Delta R.T. -0.01 min
 Lab File: BF086738.D
 Acq: 6 May 2016 21:59

Tgt Ion:188 Resp: 604376
 Ion Ratio Lower Upper
 188 100
 94 11.1 6.8 10.2#
 80 11.7 7.1 10.7#



Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

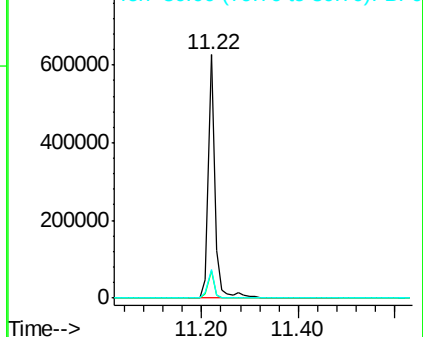


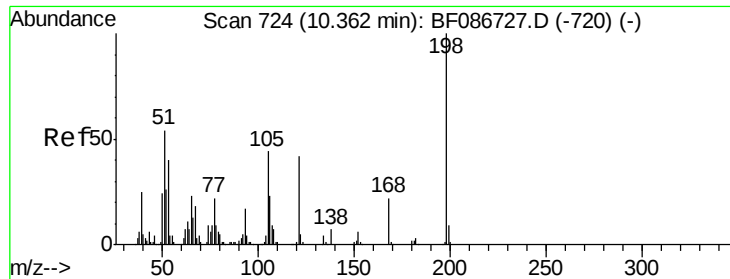




#64
4,6-Dinitro-2-methylphenol
Concen: 5.57 ng
RT: 10.53 min Scan# 739
Delta R.T. 0.17 min
Lab File: BF086738.D
Acq: 6 May 2016 21:59

Instrument :
BNA_F
ClientSampleId :

Tot Ion:198 Resp: 955
Ion Ratio Lower Upper
198 100
51 272.5 20.5 60.5#
105 244.1 24.5 64.5#

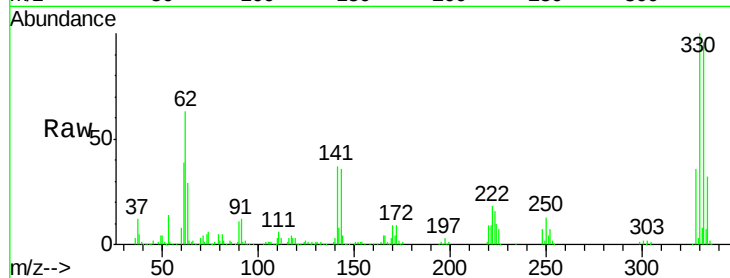


Abundance Ion 198.00 (197.70 to 198.70): E
Ion 51.00 (50.70 to 51.70): BF0
Ion 105.00 (104.70 to 105.70): E

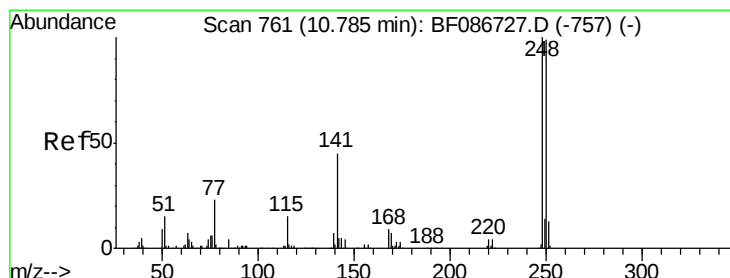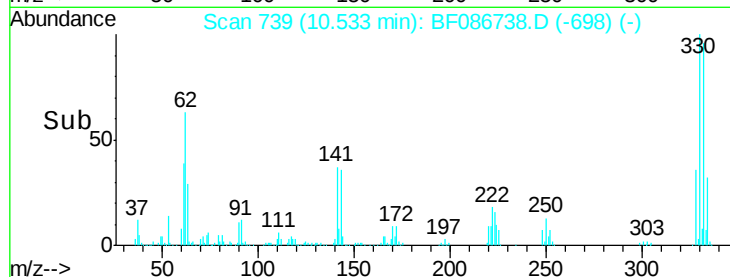
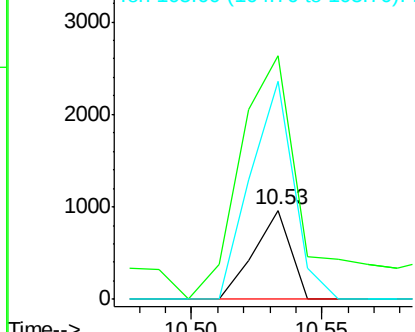



#66
4-Bromophenyl-phenylether
Concen: 4.51 ng
RT: 10.53 min Scan# 739
Delta R.T. -0.25 min
Lab File: BF086738.D
Acq: 6 May 2016 21:59

Tgt Ion:248 Resp: 27099
Ion Ratio Lower Upper
248 100
250 205.3 78.6 117.8#
141 563.9 76.0 114.0#

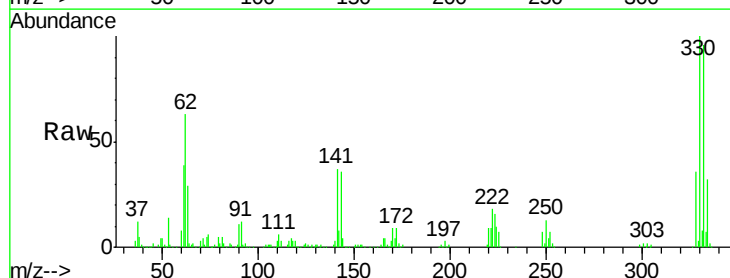

Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

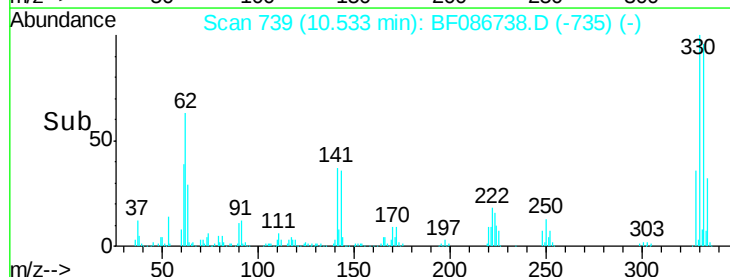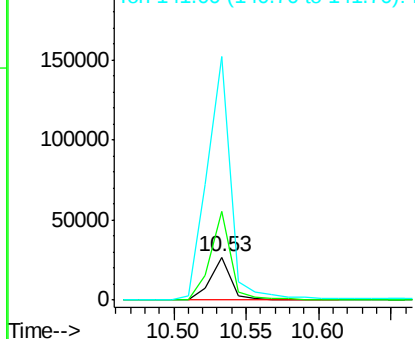



#75

Chrysene-d12

Concen: 40.00 ng

RT: 13.85 min Scan# 1029

Delta R.T. -0.01 min

Lab File: BF086738.D

Acq: 6 May 2016 21:59

Instrument :

BNA_F

ClientSampled :


Tot Ion:240 Resp: 423265

Ion Ratio Lower Upper

240 100

120 13.1 11.2 16.8




236 26.2 21.2 31.8



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

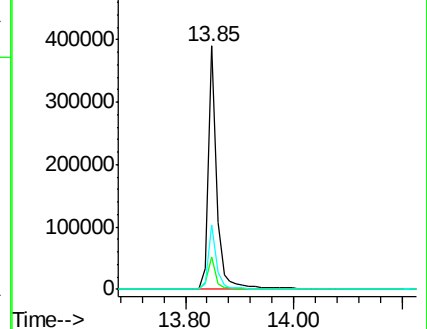

#78

Terphenyl-d14

Concen: 67.87 ng

RT: 12.81 min Scan# 938

Delta R.T. -0.00 min

Lab File: BF086738.D

Acq: 6 May 2016 21:59


Tgt Ion:244 Resp: 1421365

Ion Ratio Lower Upper

244 100

212 8.3 6.2 9.2



122 13.1 12.0 18.0




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

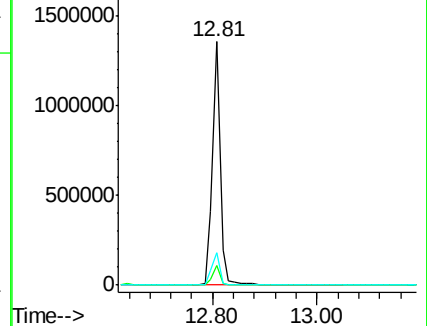

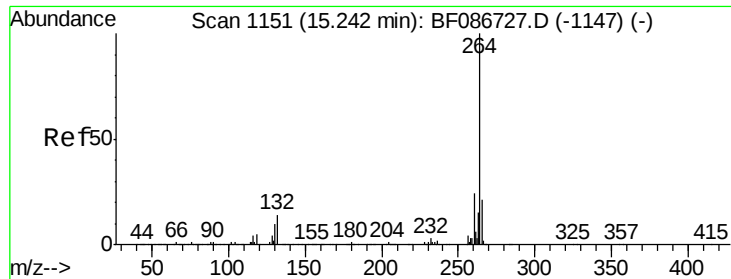

#86
Pervlene-d12
Concen: 40.00 ng
RT: 15.23 min Scan# 1150
Delta R.T. -0.01 min
Lab File: BF086738.D
Acq: 6 May 2016 21:59

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.4	19.5	29.3
265	21.4	17.3	25.9

