

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050616\
 Data File : BF086772.D
 Acq On : 7 May 2016 14:17
 Operator : UM/SJ
 Sample : H2878-02
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MJQUILLFIELD BLANK-1-5-03-16

Quant Time: May 07 23:51:29 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050416.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 04 15:12:53 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	168061	40.00	ng	-0.03
21) Naphthalene-d8	7.98	136	667141	40.00	ng	-0.05
38) Acenaphthene-d10	9.73	164	326642	40.00	ng	-0.05
63) Phenanthrene-d10	11.22	188	623419	40.00	ng	-0.03
75) Chrysene-d12	13.85	240	393554	40.00	ng	-0.03
86) Perylene-d12	15.22	264	301177	40.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.31	112	723641	71.28	ng	-0.01
7) Phenol-d6	6.36	99	568711	41.59	ng	-0.01
23) Nitrobenzene-d5	7.28	82	1311634	101.03	ng	-0.03
41) 2,4,6-Tribromophenol	10.53	330	584510	182.93	ng	-0.03
44) 2-Fluorobiphenyl	9.07	172	2156663	108.23	ng	-0.03
78) Terphenyl-d14	12.81	244	1952942	100.29	ng	-0.03


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050616\
Data File : BF086772.D
Acq On : 7 May 2016 14:17
Operator : UM/SJ
Sample : H2878-02
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MJQUILLFIELD BLANK-1-5-03-16

Quant Time: May 07 23:51:29 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 04 15:12:53 2016
Response via : Initial Calibration

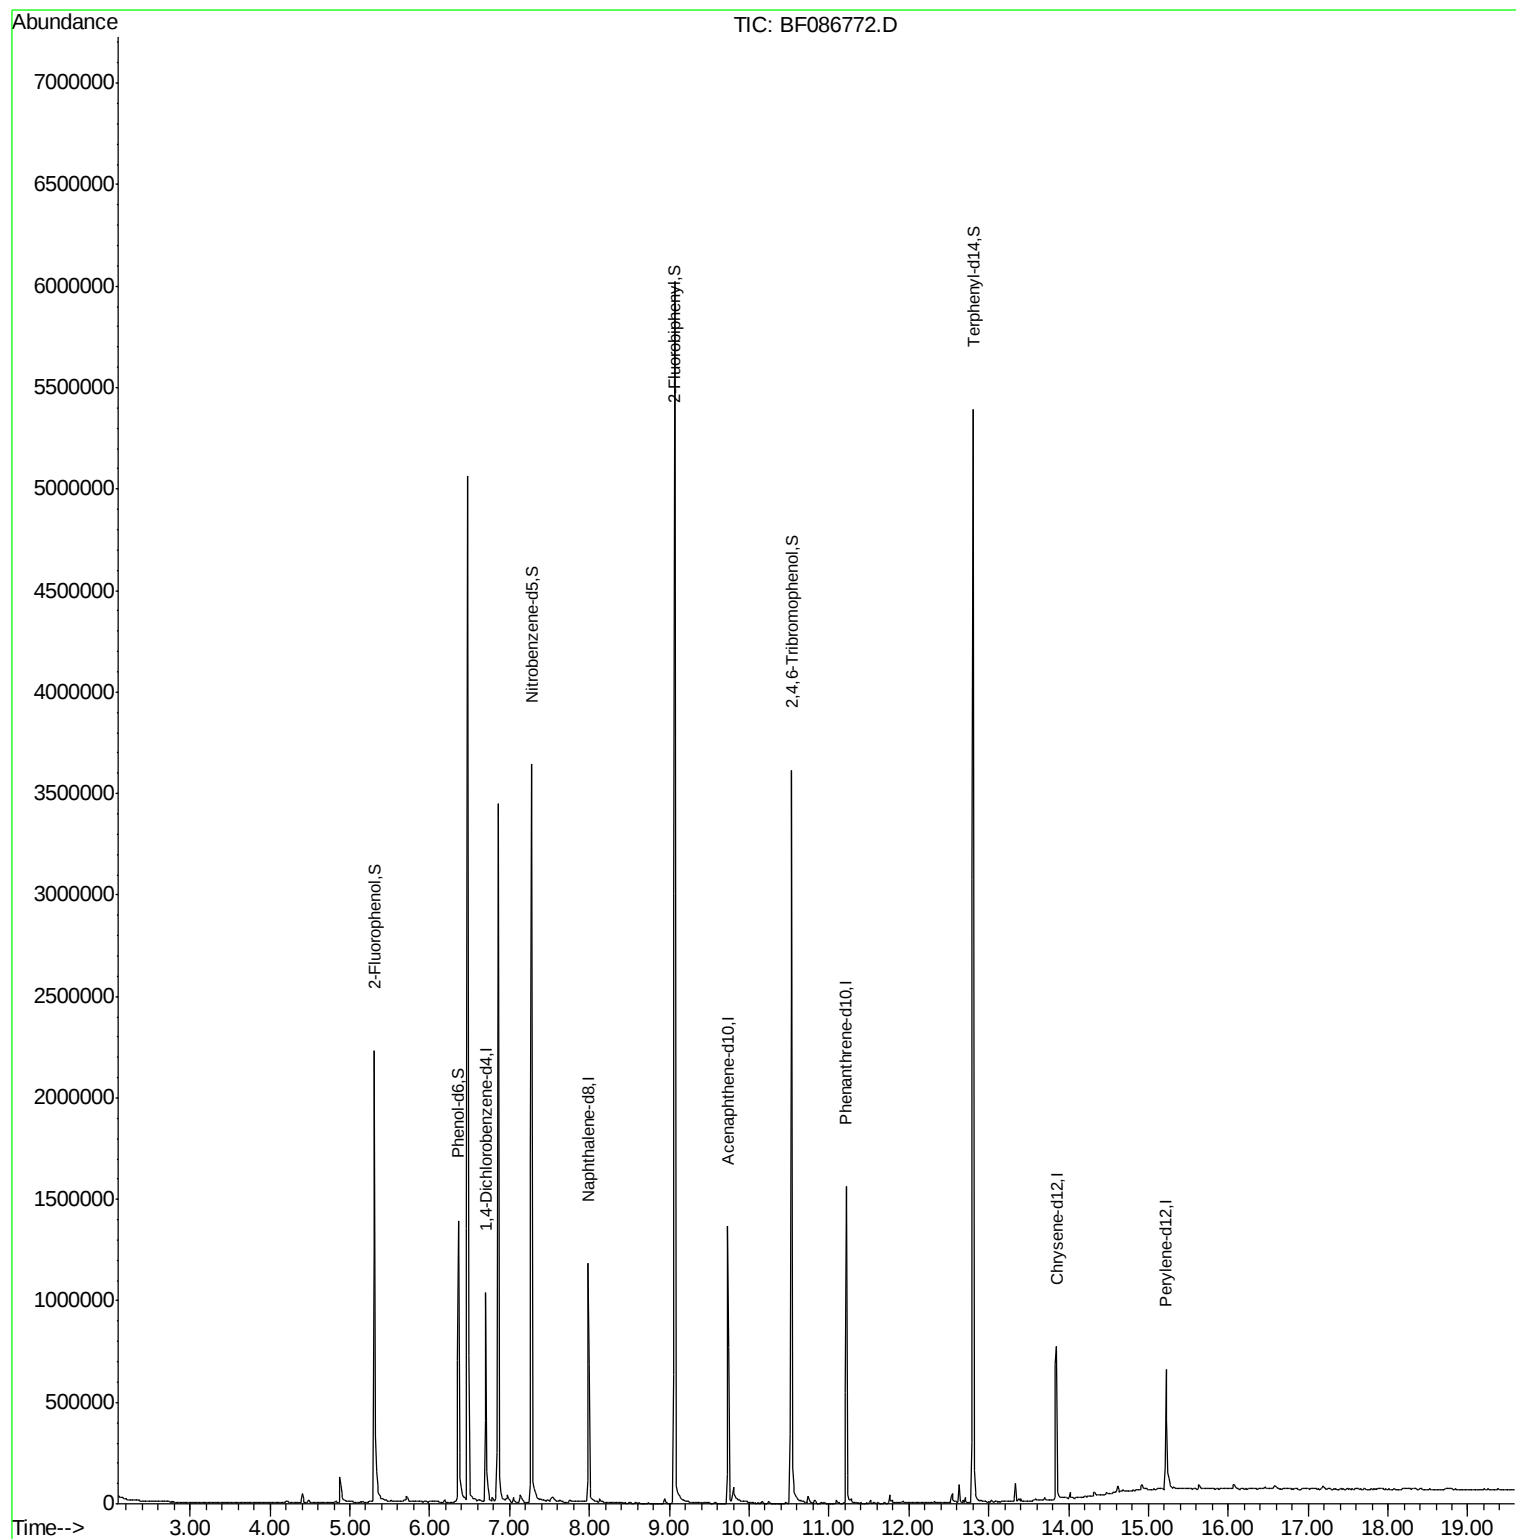

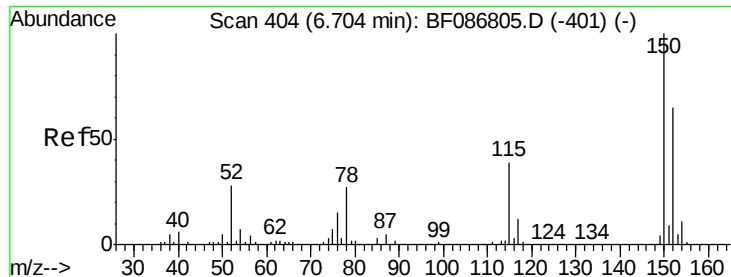


#1




1,4-Dichlorobenzene-d4
Concen: 40.00 ng
RT: 6.70 min Scan# 404
Delta R.T. -0.03 min
Lab File: BF086772.D
Acq: 7 May 2016 14:17

Instrument :
BNA_F
ClientSampleId :
MJQUILLFIELDBLANK-1-5-03-16

Tgt Ion:152 Resp: 168061
Ion Ratio Lower Upper
152 100
150 156.9 125.8 188.6
115 61.6 51.5 77.3

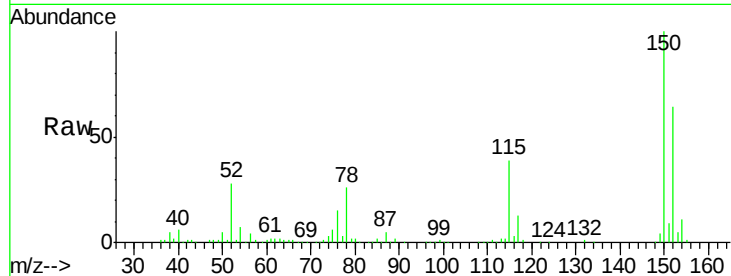


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

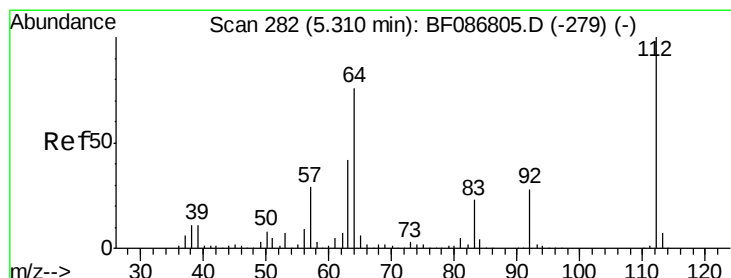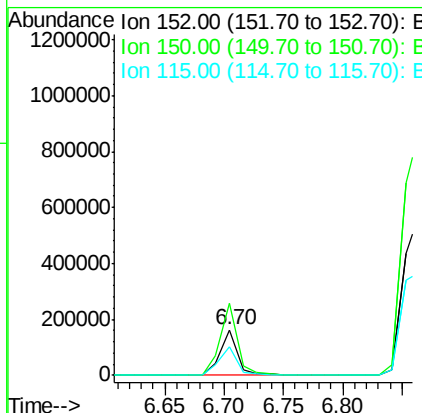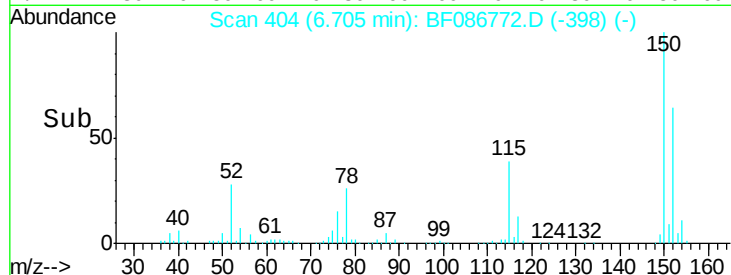



#5


2-Fluorophenol
Concen: 71.28 ng
RT: 5.31 min Scan# 282
Delta R.T. -0.01 min
Lab File: BF086772.D
Acq: 7 May 2016 14:17

Tgt Ion:112 Resp: 723641
Ion Ratio Lower Upper
112 100
64 62.8 52.1 78.1
63 33.5 25.7 38.5

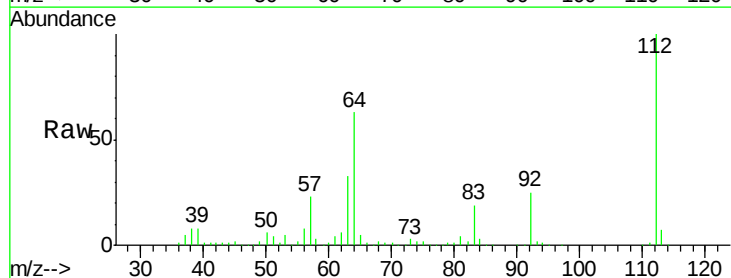

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

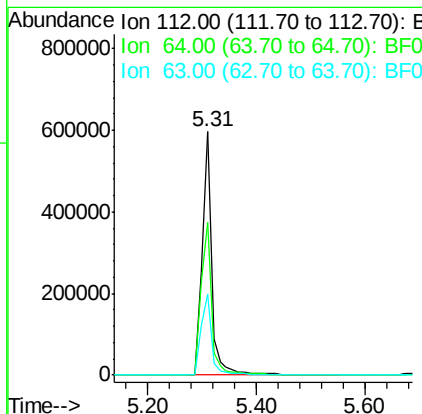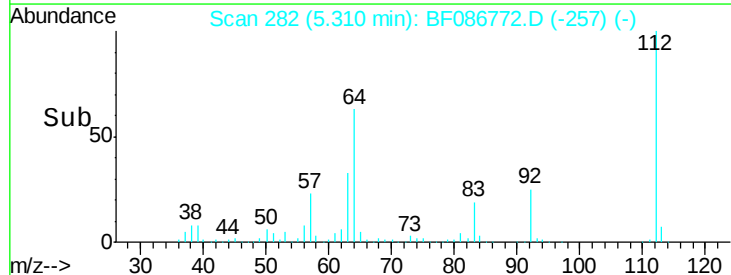

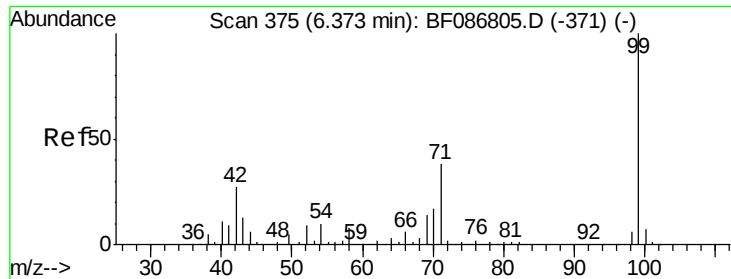

#7

Phenol-d6

Concen: 41.59 ng

RT: 6.36 min Scan# 374

Delta R.T. -0.01 min

Lab File: BF086772.D

Acq: 7 May 2016 14:17

Instrument :





BNA_F

ClientSampleId :

MJQUILLFIELD BLANK-1-5-03-16

Tgt Ion: 99 Resp: 568711

Ion	Ratio	Lower	Upper
99	100		
42	24.5	13.6	20.4#
71	33.4	24.6	36.8

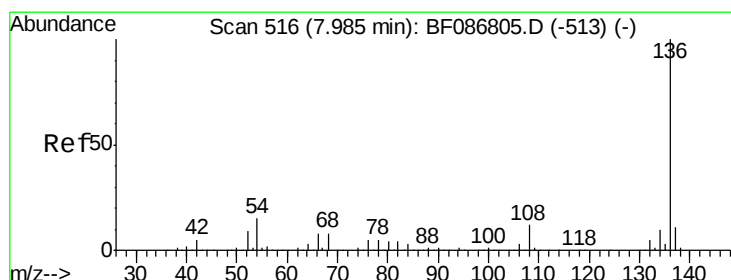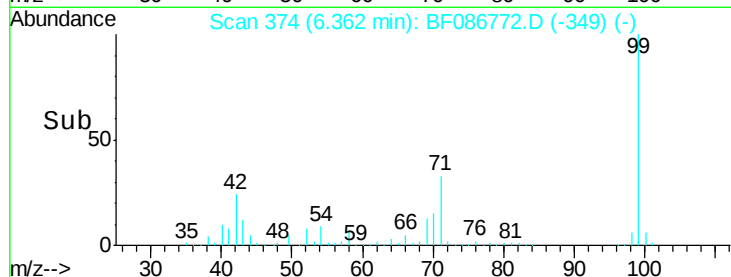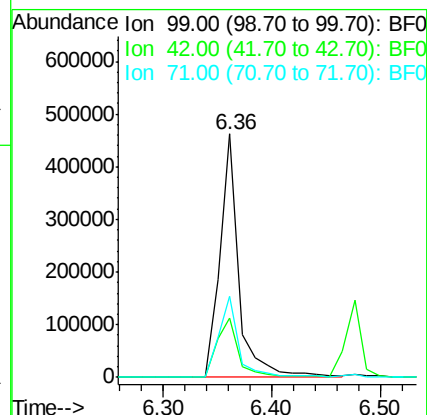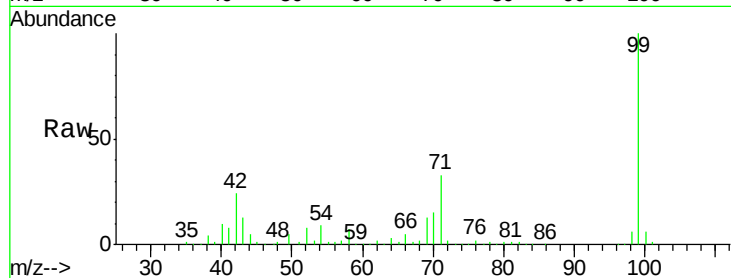

#21

Naphthalene-d8

Concen: 40.00 ng

RT: 7.98 min Scan# 516




Delta R.T. -0.05 min


Lab File: BF086772.D

Acq: 7 May 2016 14:17

Tgt Ion: 136 Resp: 667141

Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.8	13.2
54	14.6	5.0	7.4#
68	7.9	4.4	6.6#


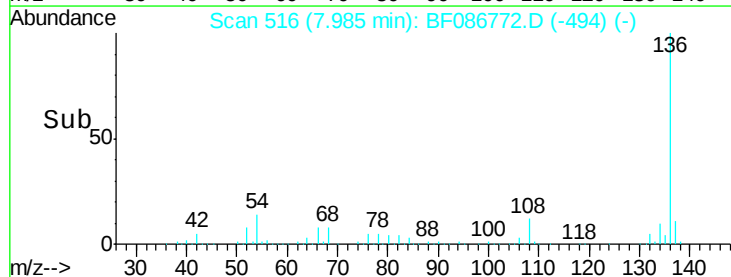
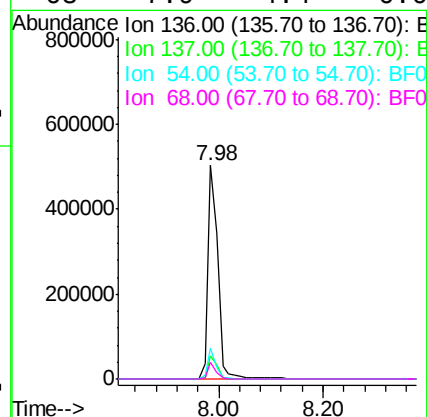
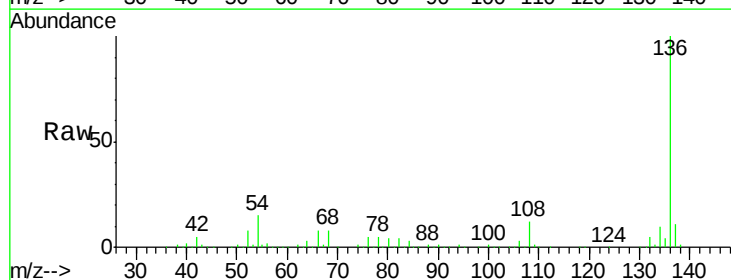


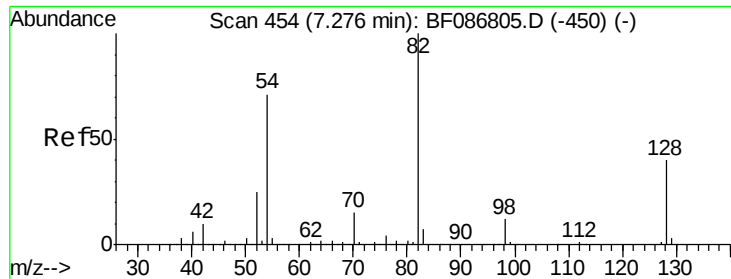

#23
 Nitrobenzene-d5
 Concen: 101.03 ng
 RT: 7.28 min Scan# 454
 Delta R.T. -0.03 min
 Lab File: BF086772.D
 Acq: 7 May 2016 14:17




Instrument :
 BNA_F
 ClientSampleId :
 MJQUILLFIELDBLANK-1-5-03-16


Tgt Ion: 82 Resp: 1311634
 Ion Ratio Lower Upper
 82 100
 128 39.8 40.6 61.0#
 54 72.0 38.1 57.1#

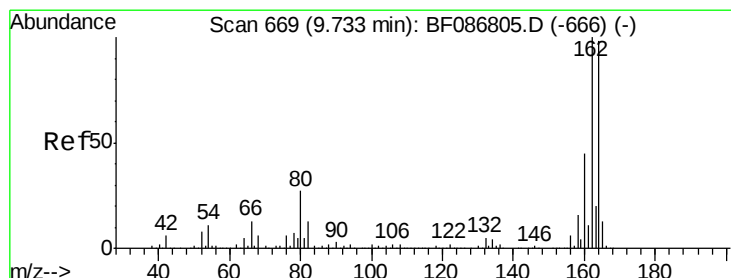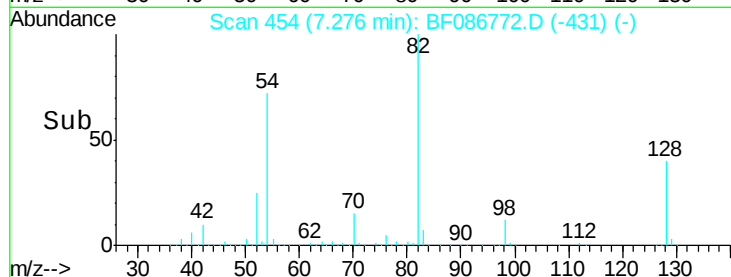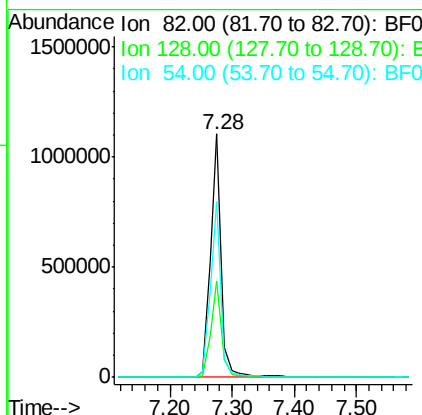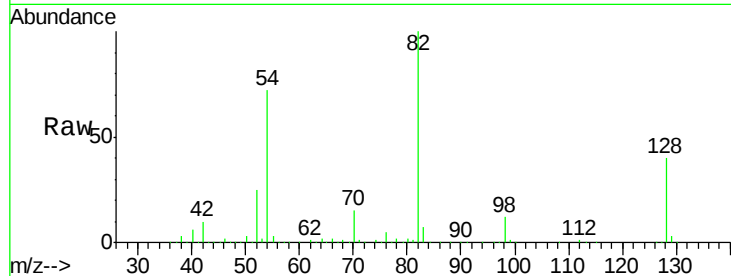

#38
 Acenaphthene-d10
 Concen: 40.00 ng
 RT: 9.73 min Scan# 669
 Delta R.T. -0.05 min
 Lab File: BF086772.D
 Acq: 7 May 2016 14:17

Tgt Ion: 164 Resp: 326642
 Ion Ratio Lower Upper
 164 100
 162 102.0 82.8 124.2
 160 46.2 36.9 55.3

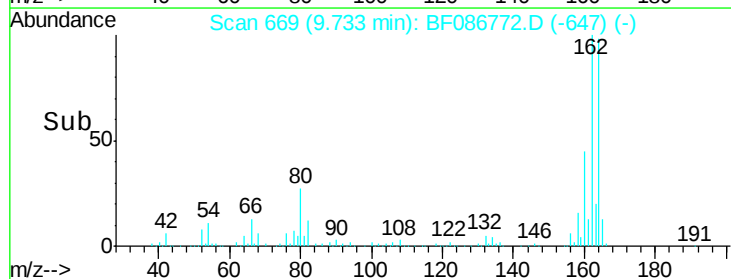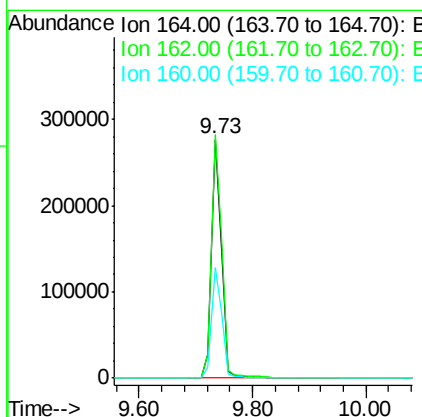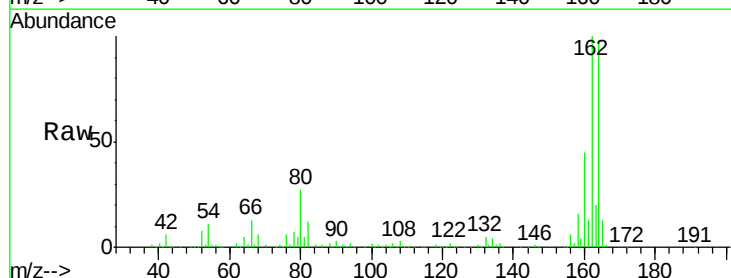


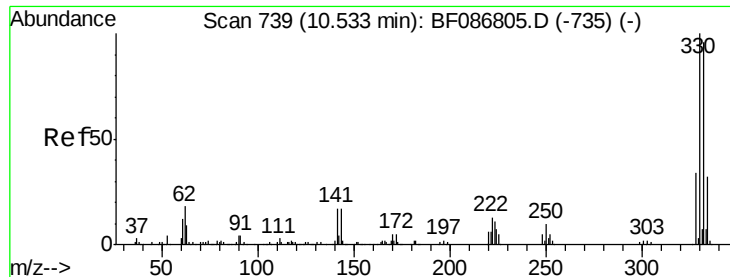




#41
 2,4,6-Tribromophenol
 Concen: 182.93 ng
 RT: 10.53 min Scan# 739
 Delta R.T. -0.03 min
 Lab File: BF086772.D
 Acq: 7 May 2016 14:17

Instrument :
 BNA_F
 ClientSampleId :
 MJQUILLFIELDBLANK-1-5-03-16

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.4	79.0	118.4
141	34.5	31.2	46.8

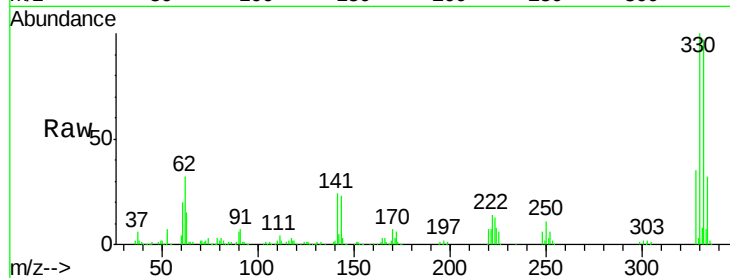


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

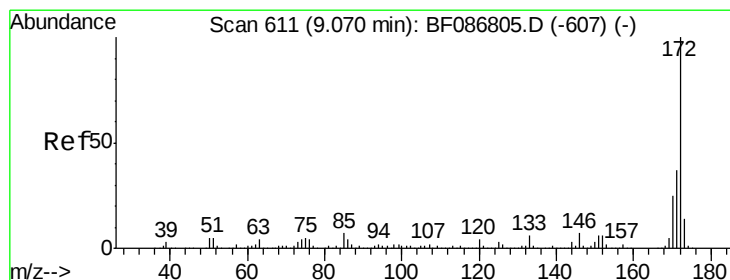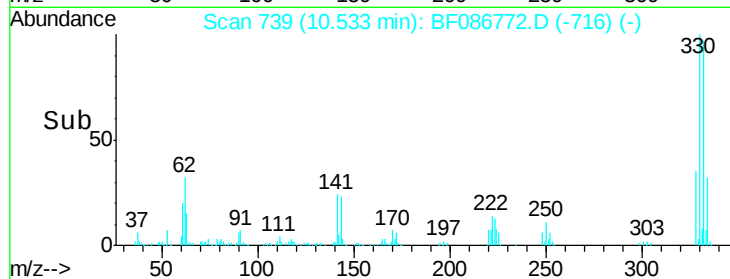
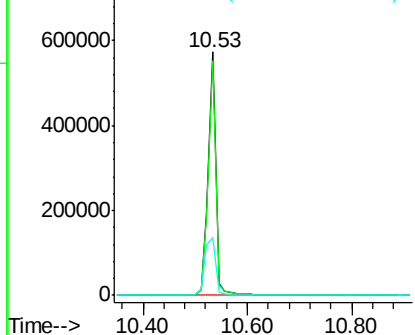



#44
 2-Fluorobiphenyl
 Concen: 108.23 ng
 RT: 9.07 min Scan# 611
 Delta R.T. -0.03 min
 Lab File: BF086772.D
 Acq: 7 May 2016 14:17

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.1	29.0	43.6
170	25.4	19.8	29.8

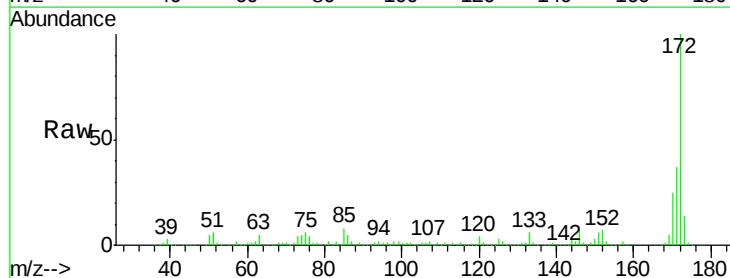

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



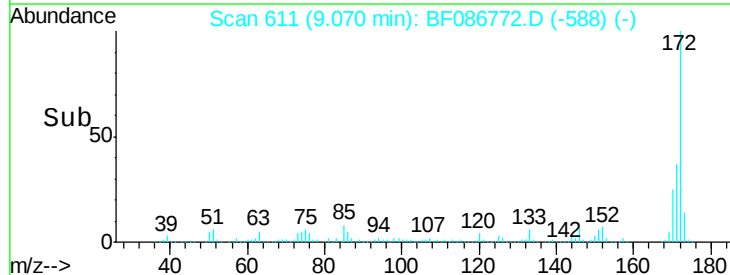
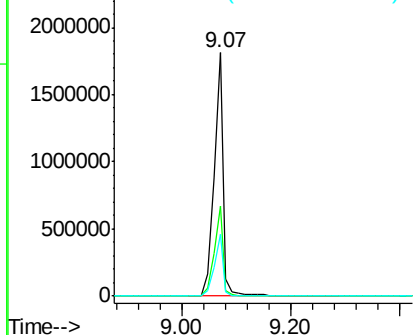


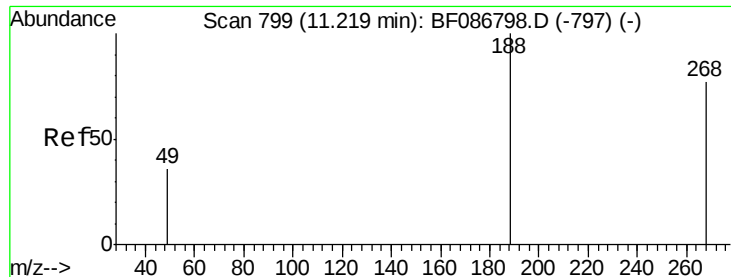

#63
Phenanthrene-d10
Concen: 40.00 ng
RT: 11.22 min Scan# 799
Delta R.T. -0.03 min
Lab File: BF086772.D
Acq: 7 May 2016 14:17




Instrument :
BNA_F
ClientSampleId :
MJQUILLFIELDBLANK-1-5-03-16


Tgt Ion:188 Resp: 623419
Ion Ratio Lower Upper
188 100
94 8.9 6.8 10.2
80 9.7 7.1 10.7

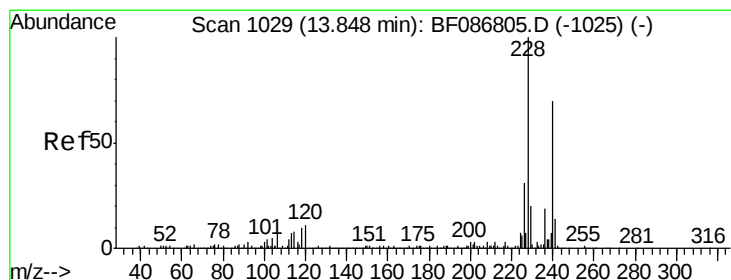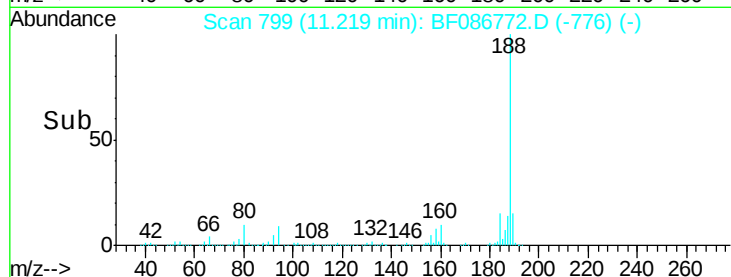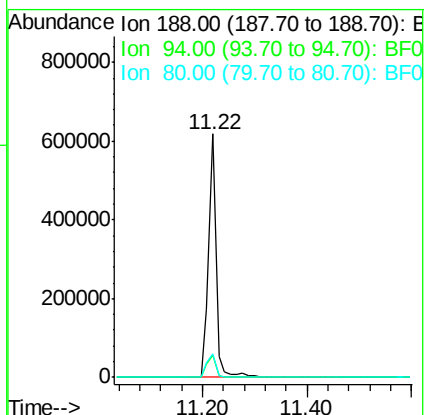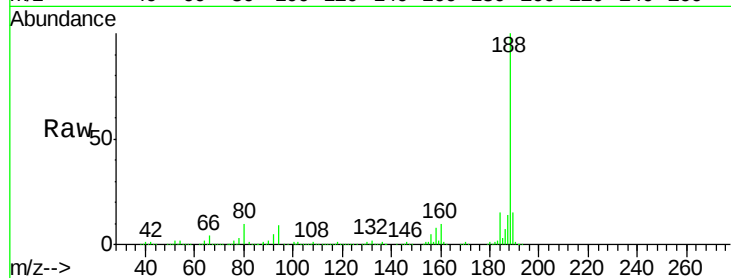

#75
Chrysene-d12
Concen: 40.00 ng
RT: 13.85 min Scan# 1029
Delta R.T. -0.03 min
Lab File: BF086772.D
Acq: 7 May 2016 14:17

Tgt Ion:240 Resp: 393554
Ion Ratio Lower Upper
240 100
120 8.8 11.2 16.8#
236 26.2 21.2 31.8

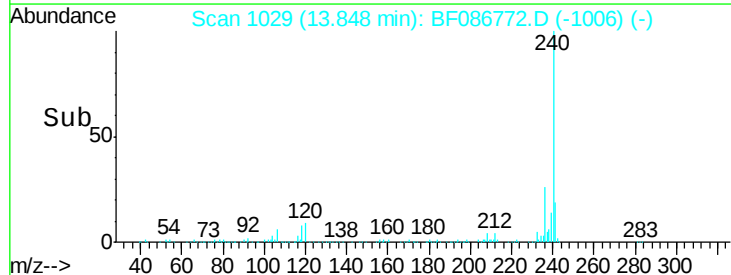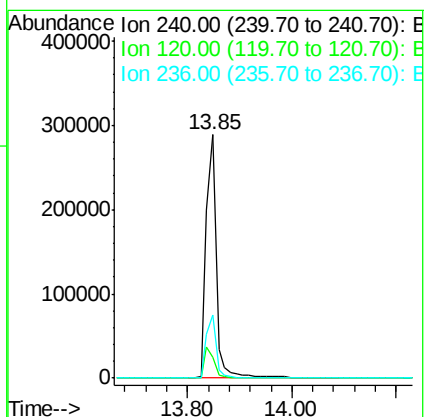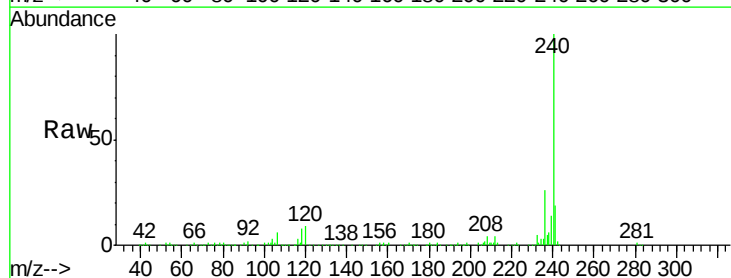

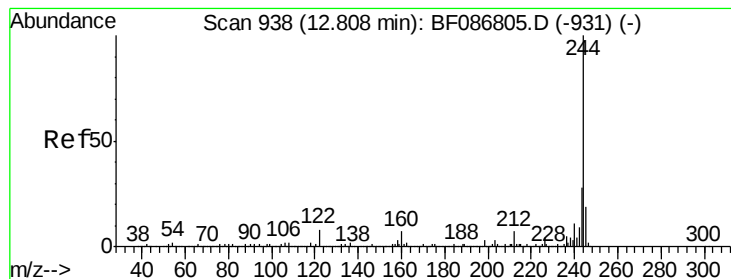

#78

Terphenyl-d14

Concen: 100.29 ng

RT: 12.81 min Scan# 938

Delta R.T. -0.03 min

Lab File: BF086772.D

Acq: 7 May 2016 14:17

Instrument :

BNA_F

ClientSampleId :

MJQUILLFIELD BLANK-1-5-03-16

Tgt Ion: 244 Resp: 1952942

Ion Ratio Lower Upper

244 100

212 7.6


6.2

9.2

122 10.2

12.0




18.0#

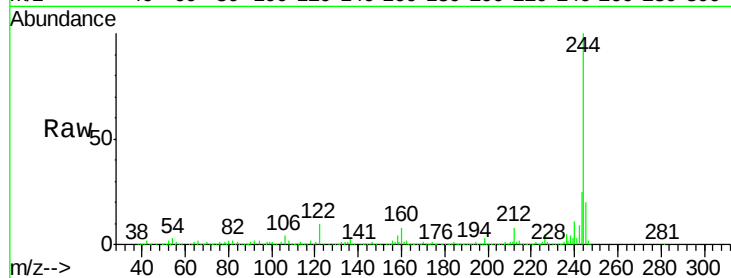

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

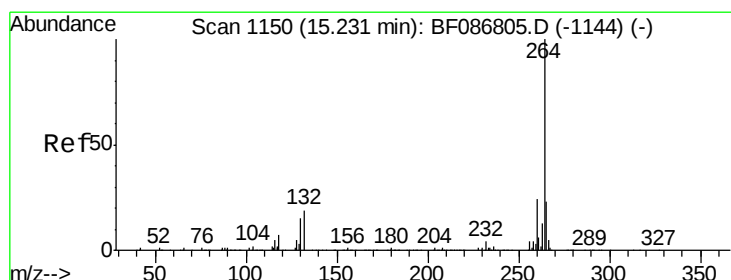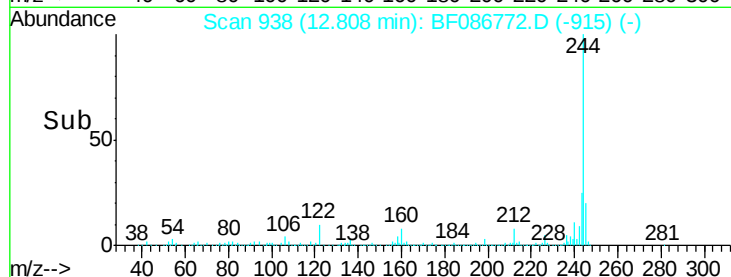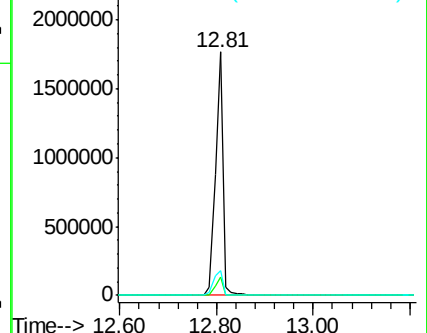

#86

Perylene-d12

Concen: 40.00 ng

RT: 15.22 min Scan# 1149

Delta R.T. -0.05 min

Lab File: BF086772.D

Acq: 7 May 2016 14:17

Tgt Ion: 264 Resp: 301177

Ion Ratio Lower Upper

264 100

260 24.6


19.5

29.3

265 22.0

17.3

25.9

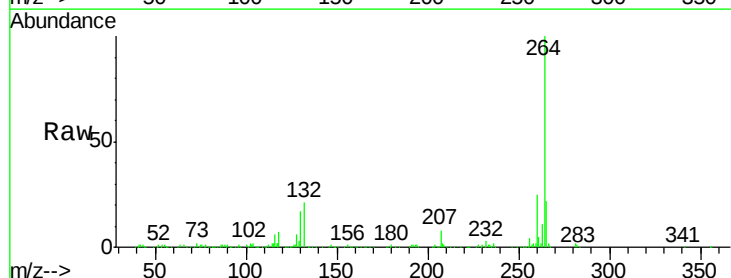

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

