


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050616\
 Data File : BF086726.D
 Acq On : 6 May 2016 16:14
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 04 15:12:53 2016

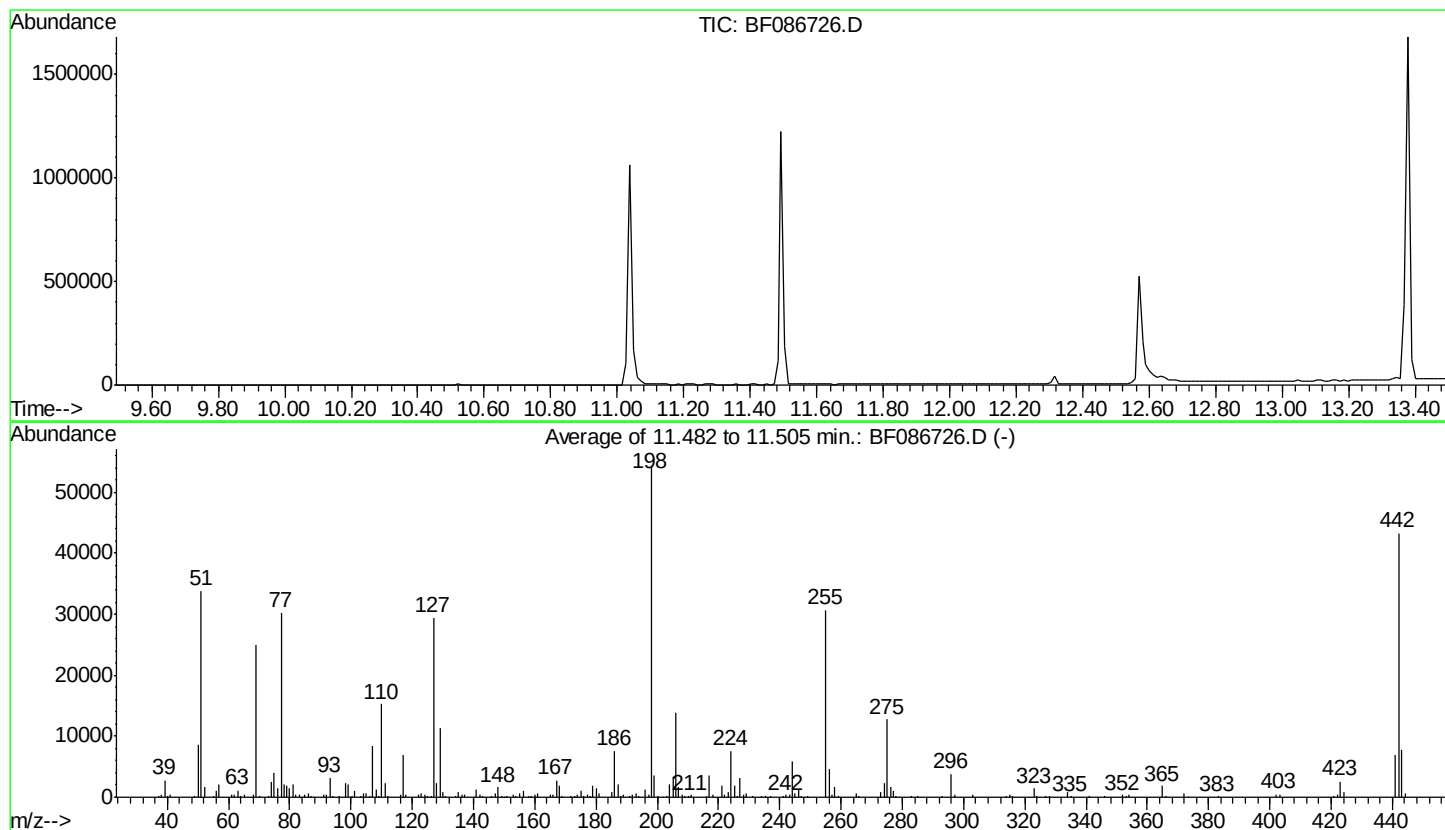

AutoFind: Scans 822, 823, 824; Background Corrected with Scan 819

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.3	33875	PASS
68	69	0.00	2	1.3	336	PASS
69	198	0.00	100	45.9	24947	PASS
70	69	0.00	2	0.5	114	PASS
127	198	10	80	54.1	29399	PASS
197	198	0.00	2	0.7	381	PASS
198	198	100	100	100.0	54356	PASS
199	198	5	9	6.7	3641	PASS
275	198	10	60	23.5	12792	PASS
365	198	1	100	3.4	1852	PASS
441	442	0.01	24	15.9	6866	PASS
442	198	50	100	79.5	43228	PASS
443	442	15	24	18.0	7793	PASS