


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050616\
 Data File : BF086751.D
 Acq On : 7 May 2016 4:13
 Operator : UM/SJ
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTTP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 04 15:12:53 2016

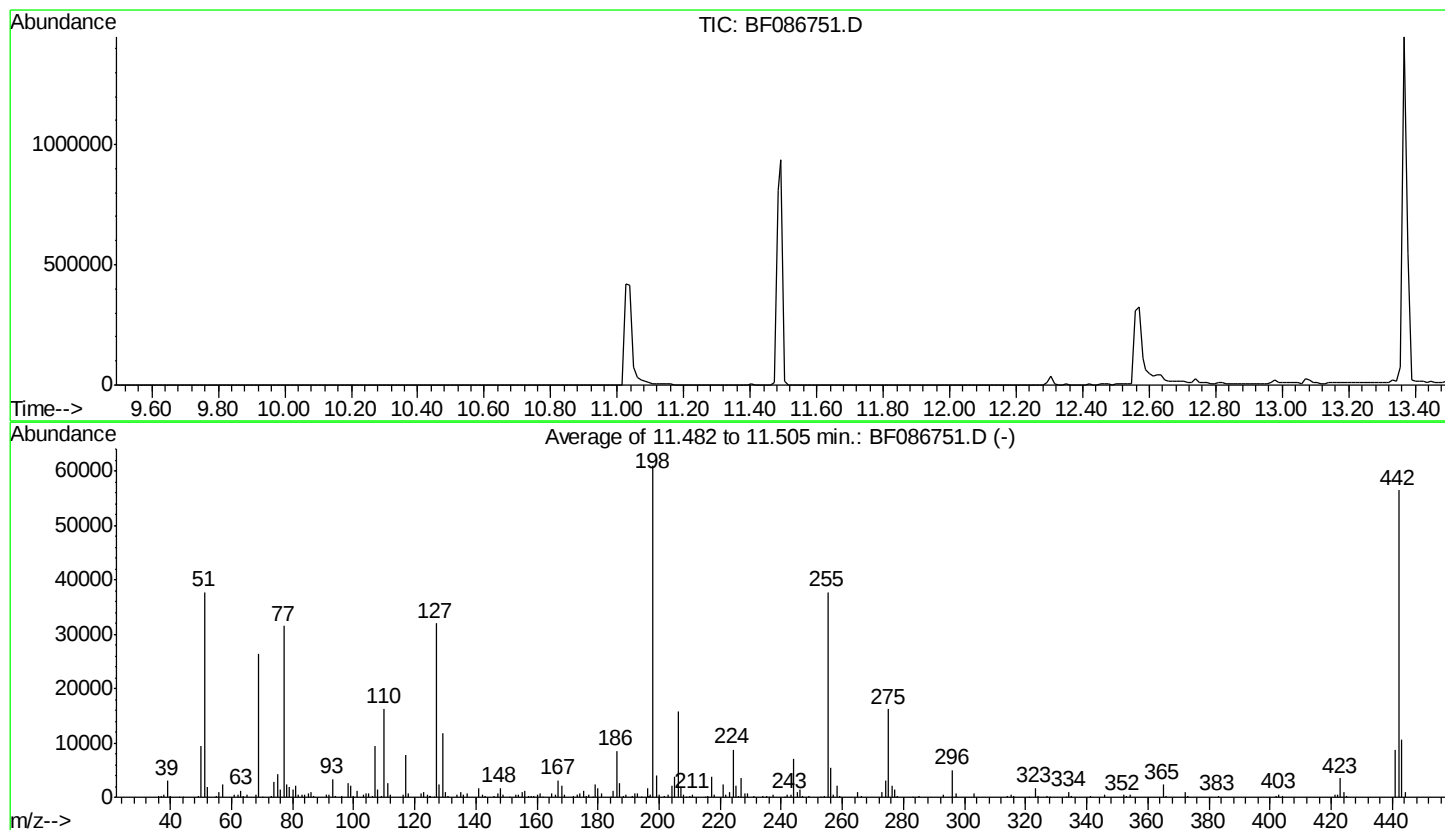

AutoFind: Scans 822, 823, 824; Background Corrected with Scan 818

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.9	37757	PASS
68	69	0.00	2	1.9	503	PASS
69	198	0.00	100	43.1	26280	PASS
70	69	0.00	2	0.5	125	PASS
127	198	10	80	52.4	31941	PASS
197	198	0.00	2	0.9	545	PASS
198	198	100	100	100.0	60990	PASS
199	198	5	9	6.7	4112	PASS
275	198	10	60	26.5	16176	PASS
365	198	1	100	3.8	2343	PASS
441	442	0.01	24	15.7	8832	PASS
442	198	50	100	92.5	56400	PASS
443	442	15	24	18.7	10533	PASS