


Data Path : Z:\HPCHEM1\BNA F\Data\BF050617\
 Data File : BF094952.D
 Acq On : 6 May 2017 10:15
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 03 17:24:51 2017

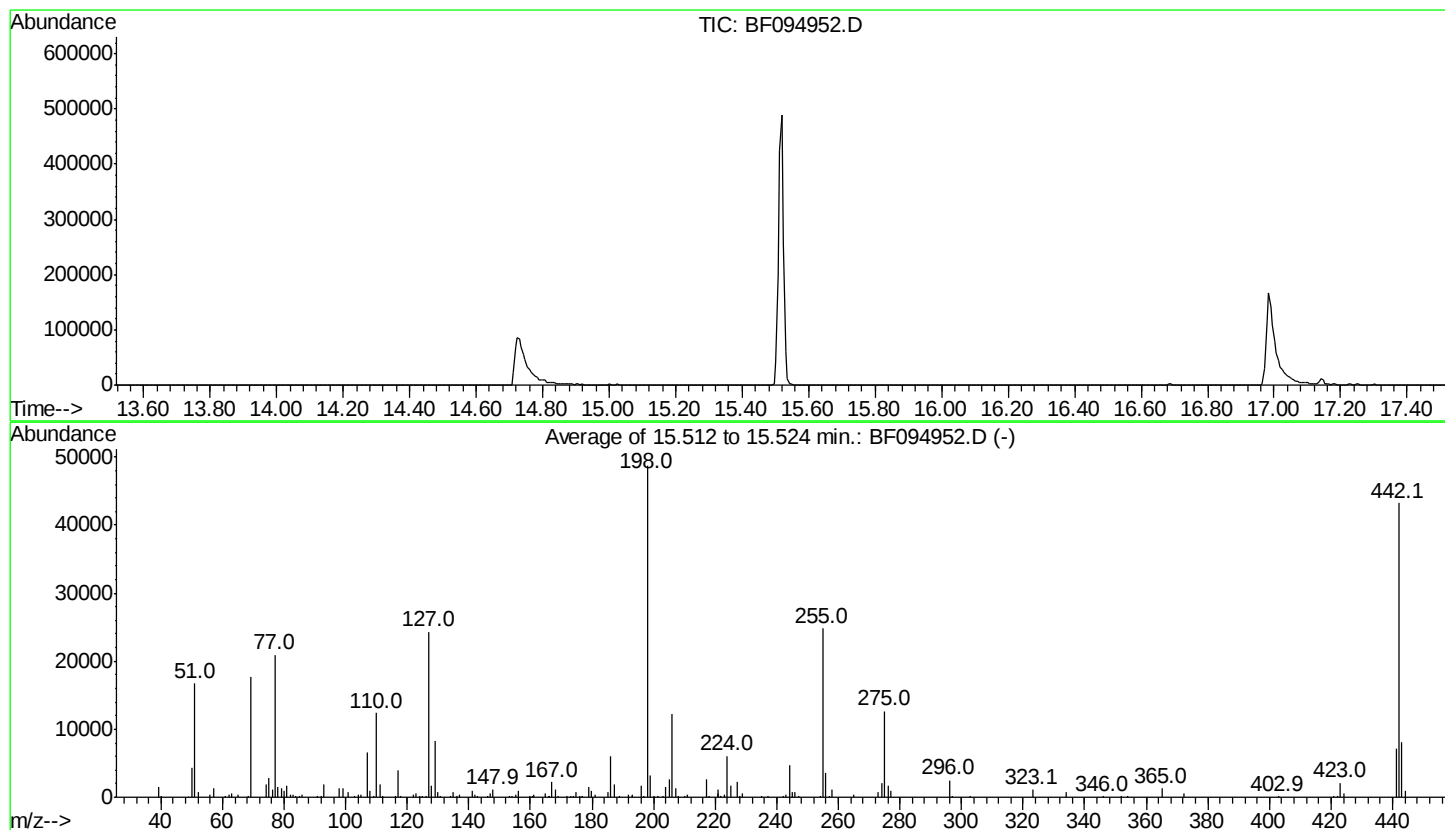

AutoFind: Scans 2308, 2309, 2310; Background Corrected with Scan 2302

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	16673	PASS
68	69	0.00	2	0.8	141	PASS
69	198	0.00	100	36.2	17638	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.8	24290	PASS
197	198	0.00	2	0.4	201	PASS
198	198	100	100	100.0	48738	PASS
199	198	5	9	6.6	3231	PASS
275	198	10	60	25.9	12610	PASS
365	198	1	100	2.6	1250	PASS
441	442	0.01	24	16.4	7094	PASS
442	198	50	100	88.7	43224	PASS
443	442	15	24	18.9	8163	PASS