


Data Path : Z:\HPCHEM1\BNA F\Data\BF050617\  
 Data File : BF094962.D  
 Acq On : 8 May 2017 1:27  
 Operator : SJ/MA  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050217.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed May 03 17:24:51 2017

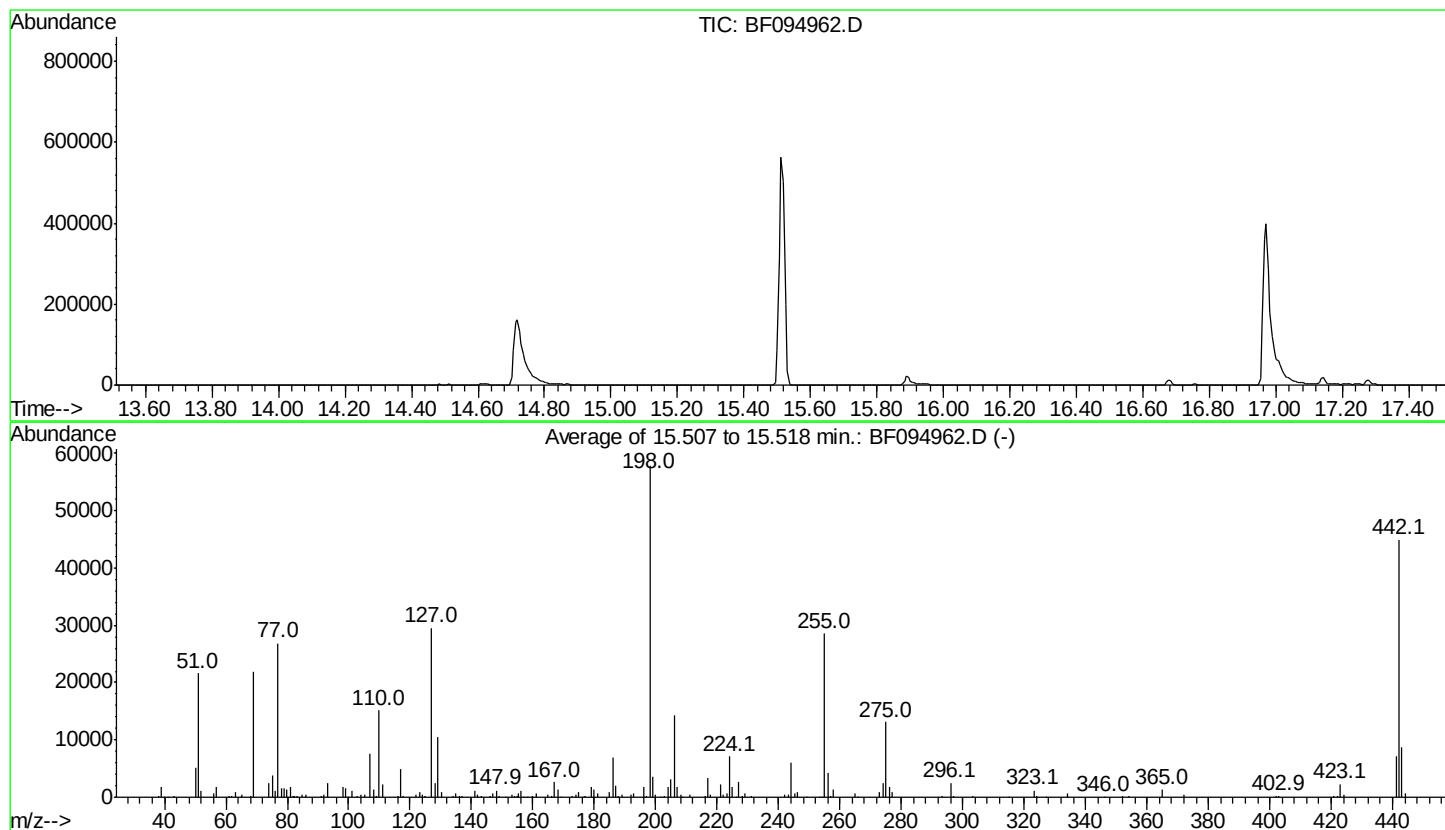

AutoFind: Scans 2307, 2308, 2309; Background Corrected with Scan 2302

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 37.3      | 21608   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.8       | 184     | PASS             |
| 69          | 198          | 0.00         | 100          | 37.8      | 21882   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 51.1      | 29589   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.5       | 304     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 57858   | PASS             |
| 199         | 198          | 5            | 9            | 6.3       | 3656    | PASS             |
| 275         | 198          | 10           | 60           | 22.6      | 13087   | PASS             |
| 365         | 198          | 1            | 100          | 2.2       | 1253    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.7      | 7050    | PASS             |
| 442         | 198          | 50           | 100          | 77.7      | 44933   | PASS             |
| 443         | 442          | 15           | 24           | 19.3      | 8665    | PASS             |