
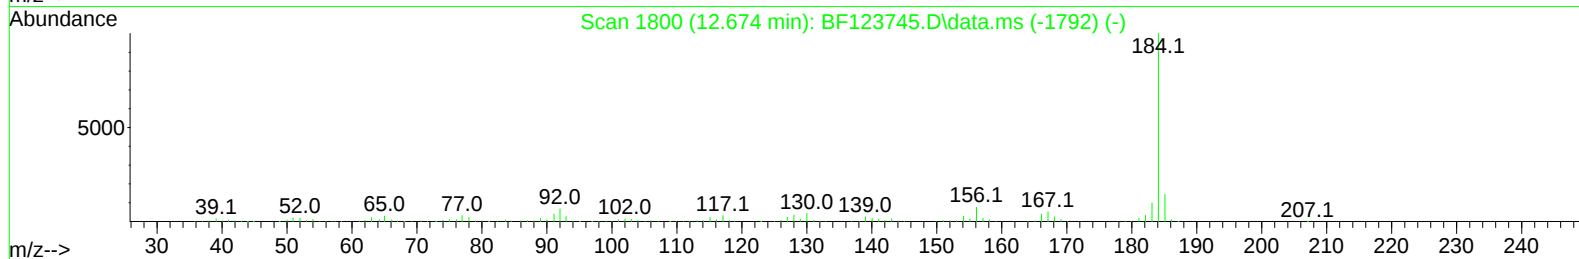
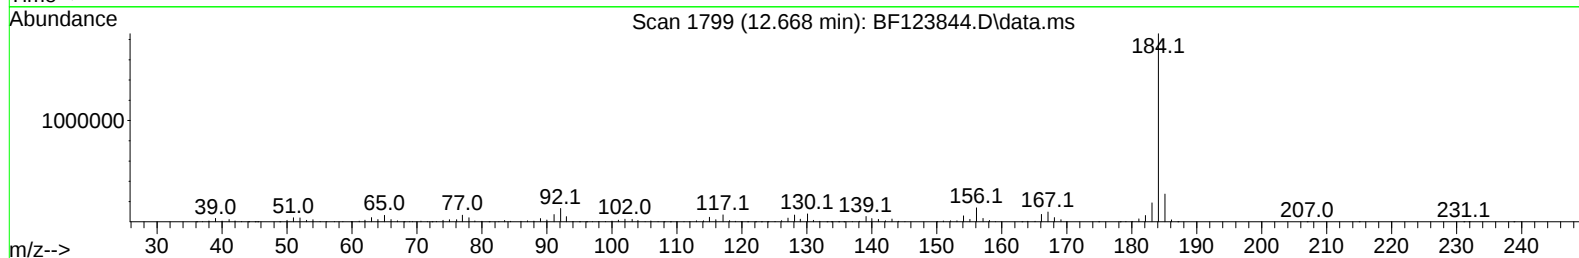


Quant Time: May 06 11:12:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 05 13:09:28 2021
Response via : Initial Calibration

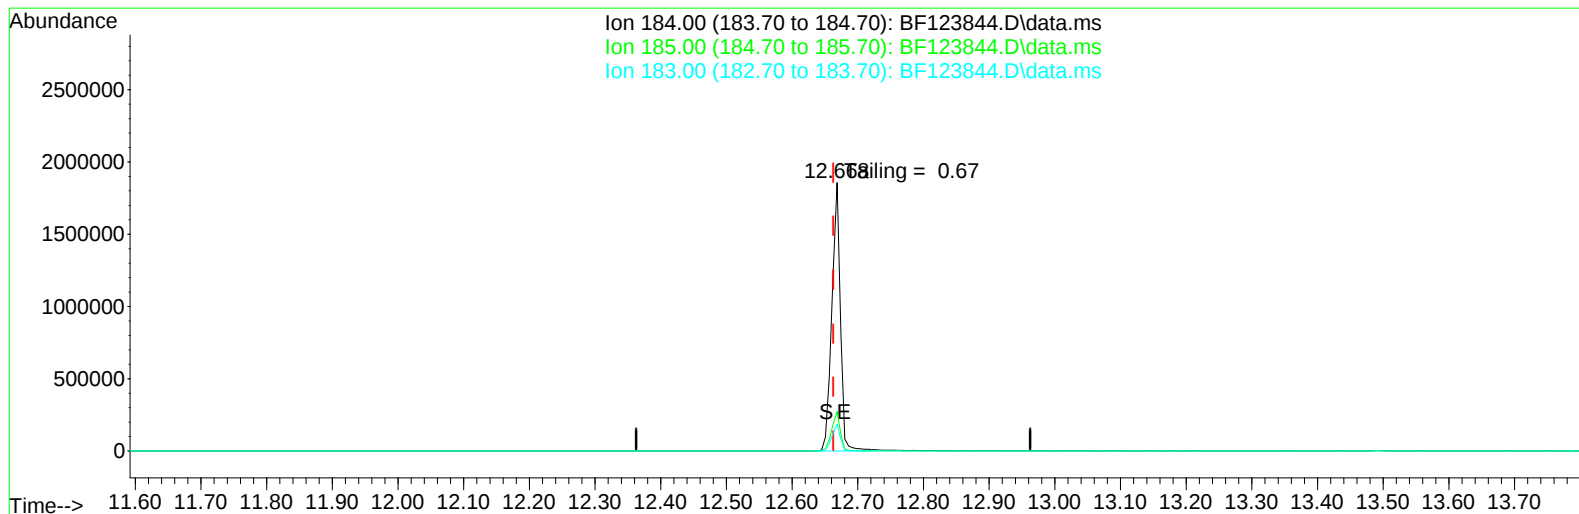

TIC: BF123844.D\data.ms

(77) Benzidine




12.668min (+ 0.006) 272183.91 ng

```
response      1698689
```

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.72
183.00	9.80	10.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050621\
Data File : BF123844.D
Acq On : 6 May 2021 8:57
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 11:12:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 05 13:09:28 2021
Response via : Initial Calibration

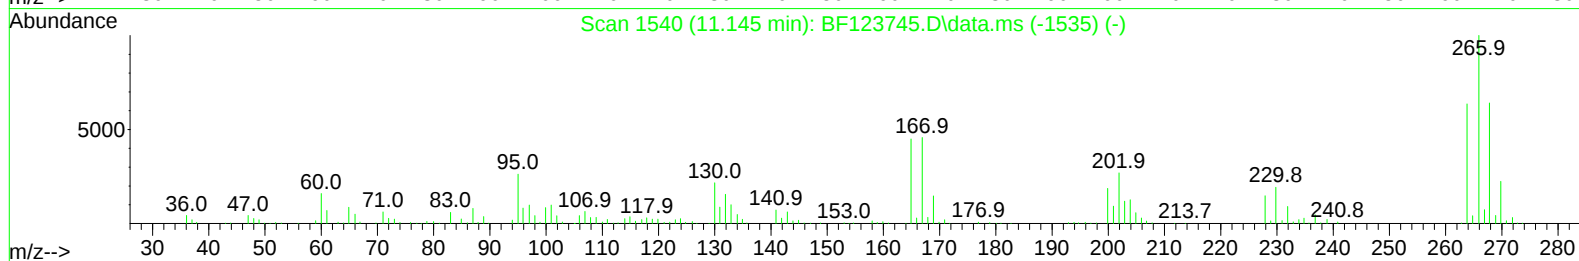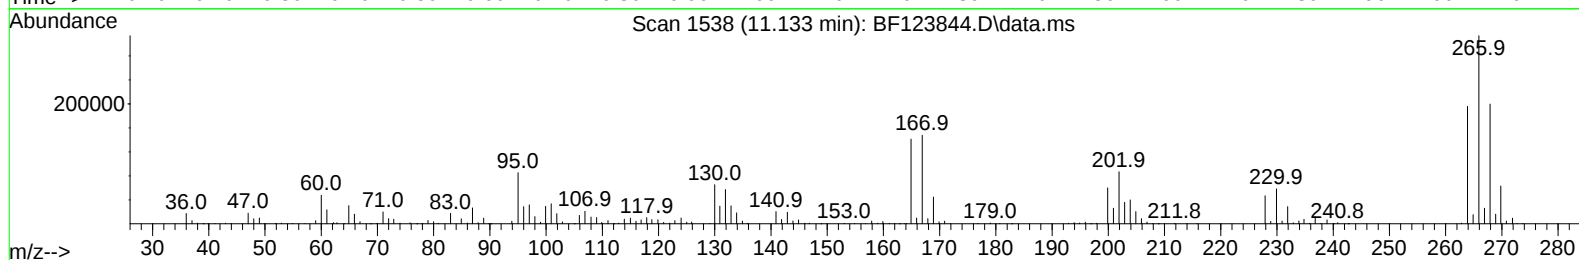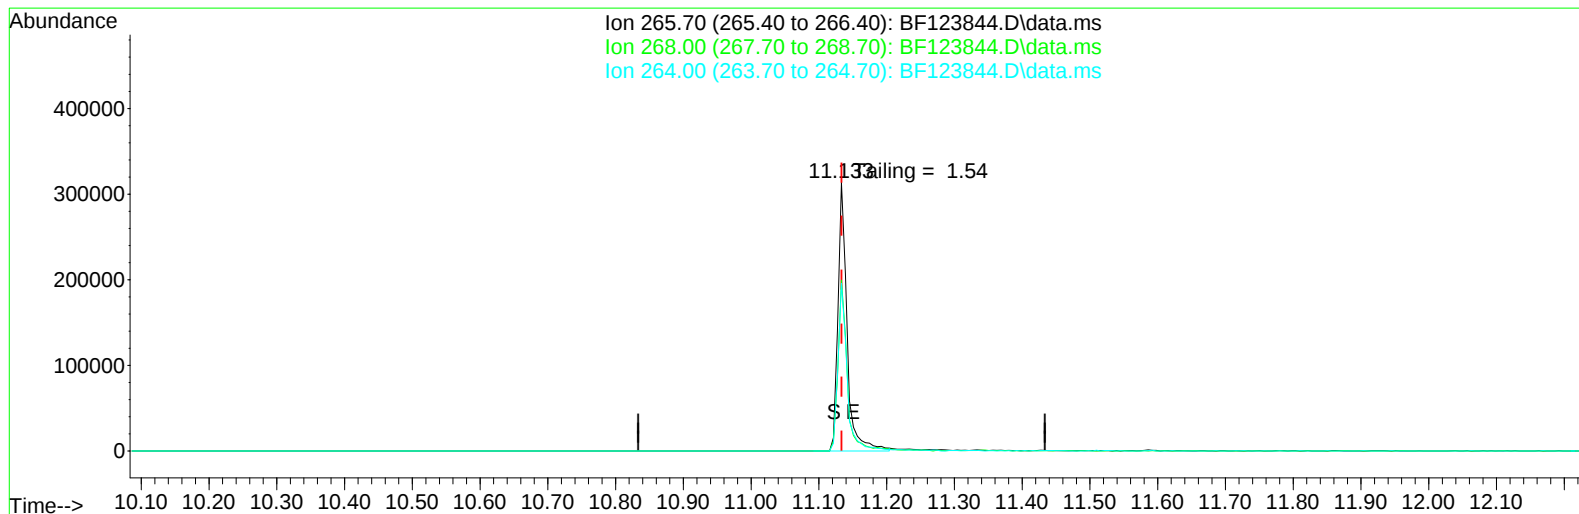

TIC: BF123844.D\data.ms

(70) Pentachlorophenol (C)

11.133min (-0.000) 0.00 ng

response 296940

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.68
264.00	65.70	62.49
0.00	0.00	0.00