
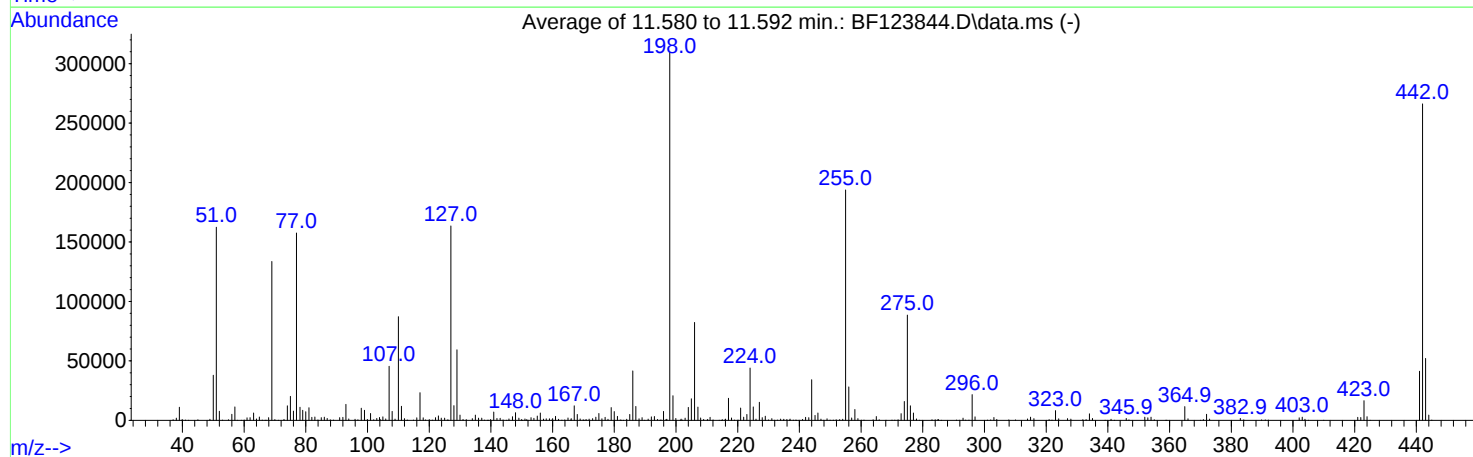


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050621\
 Data File : BF123844.D
 Acq On : 6 May 2021 8:57
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 05 13:09:28 2021

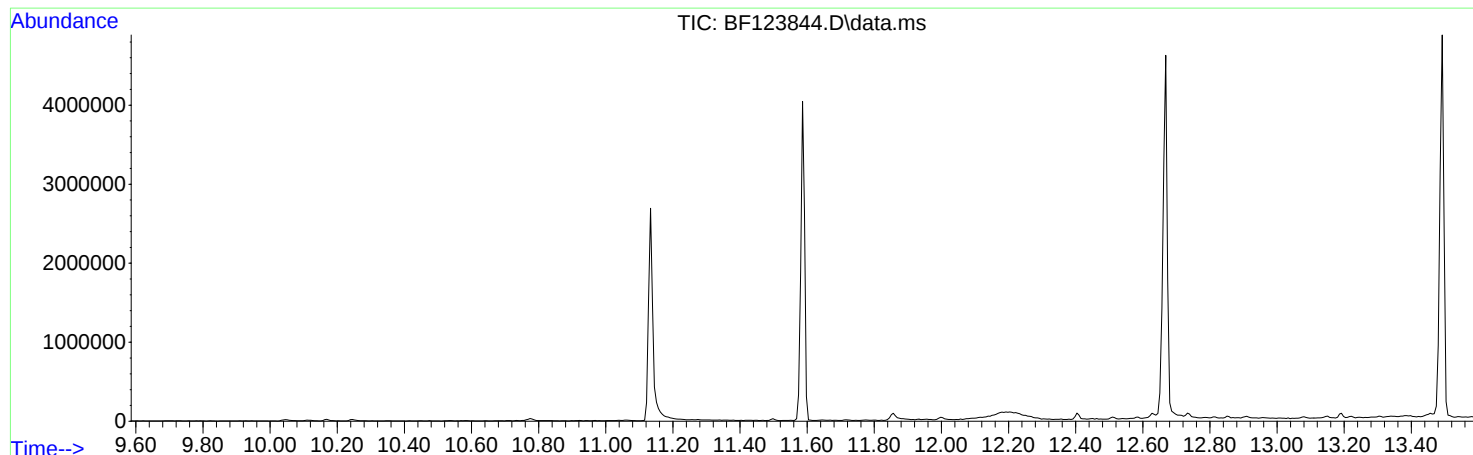




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.5	162429	PASS
68	69	0.00	2	1.7	2304	PASS
69	198	0.00	100	43.2	133660	PASS
70	69	0.00	2	0.5	698	PASS
127	198	10	80	52.8	163440	PASS
197	198	0.00	2	0.3	996	PASS
198	198	100	100	100.0	309376	PASS
199	198	5	9	6.7	20696	PASS
275	198	10	60	28.6	88565	PASS
365	198	1	100	3.7	11542	PASS
441	198	0.01	100	13.4	41311	PASS
442	442	50	100	100.0	266195	PASS
443	442	15	24	19.6	52104	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050621\
Data File : BF123844.D
Acq On : 6 May 2021 8:57
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 06 11:12:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 05 13:09:28 2021
Response via : Initial Calibration

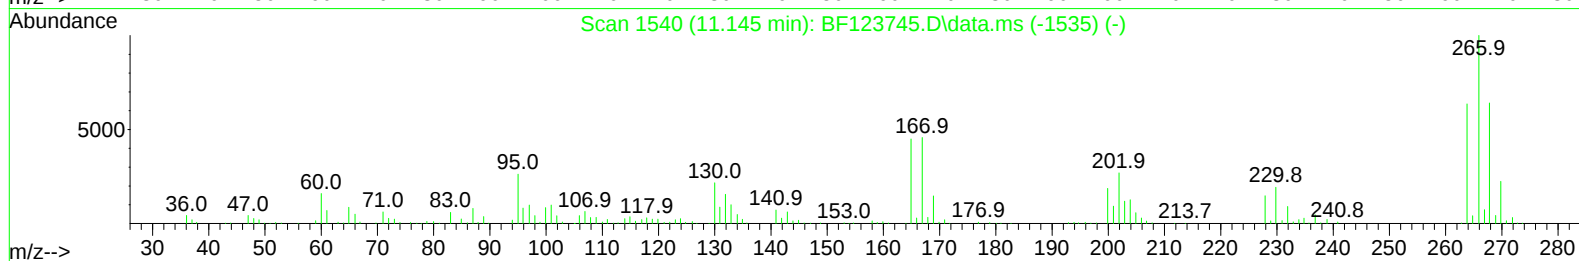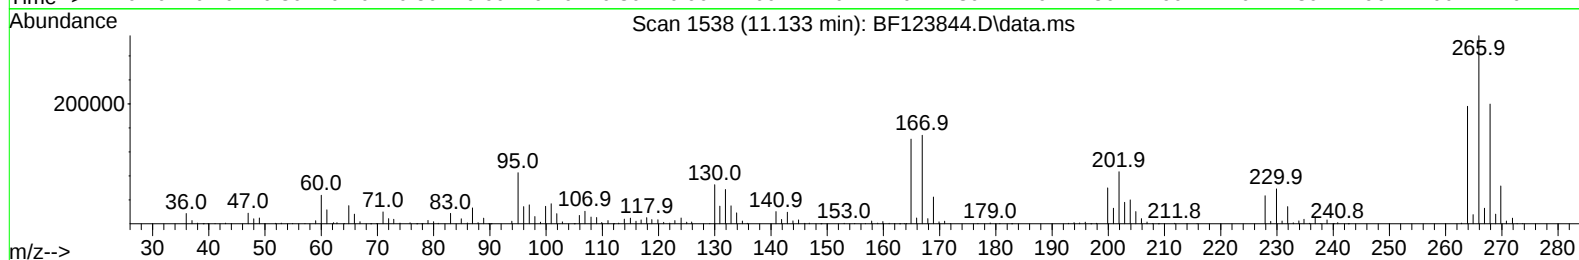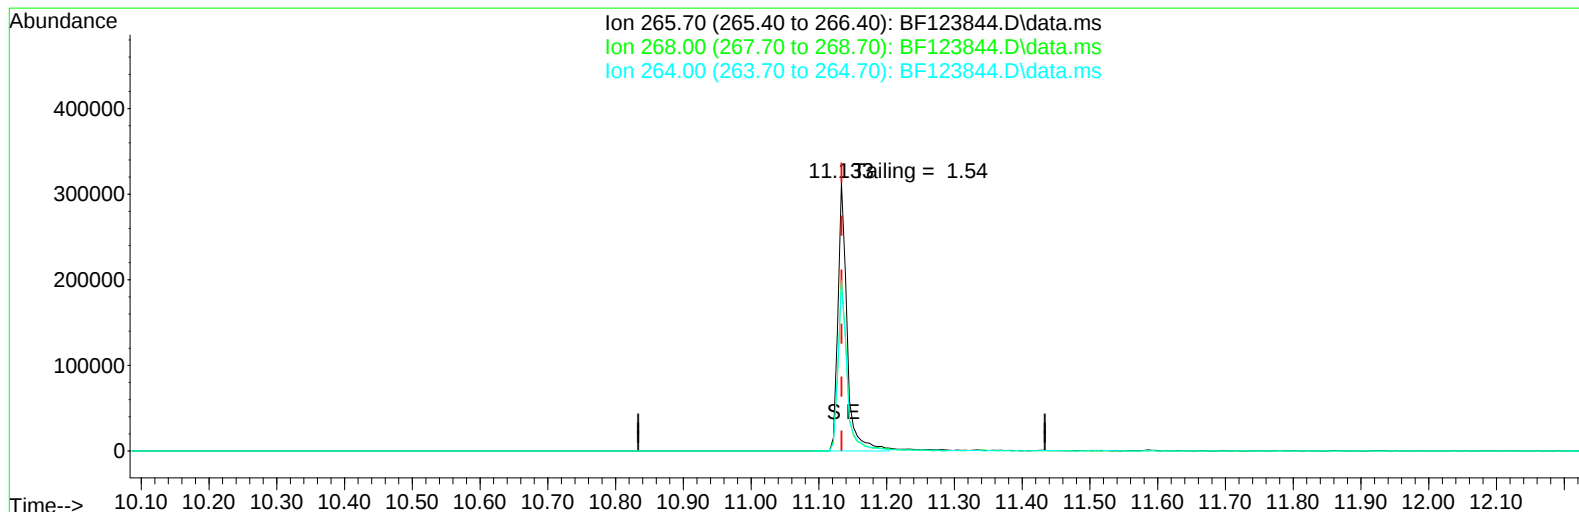

TIC: BF123844.D\data.ms

(70) Pentachlorophenol (C)

11.133min (-0.000) 0.00 ng

response 296940

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.68
264.00	65.70	62.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/6/2021	BNA_F	<u>BF123844.D</u>
Compound Name	Response	Retention Time
DDT	772675	13.49
DDD	10013	13.19
DDE	2939	12.85
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12952	785627	1.65