

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050622\
 Data File : BF128131.D
 Acq On : 06 May 2022 18:30
 Operator : CG\JU
 Sample : N2723-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MMC-PIT2

Quant Time: May 06 23:25:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 05 17:56:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.904	152	75102	20.000	ng	0.00
21) Naphthalene-d8	8.186	136	292579	20.000	ng	-0.01
39) Acenaphthene-d10	9.945	164	166591	20.000	ng	0.00
64) Phenanthrene-d10	11.433	188	321371	20.000	ng	-0.01
76) Chrysene-d12	14.080	240	260745	20.000	ng	-0.01
86) Perylene-d12	15.580	264	193085	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.528	112	470903	99.870	ng	0.00
7) Phenol-d6	6.534	99	624048	101.998	ng	-0.01
23) Nitrobenzene-d5	7.469	82	432434	69.502	ng	-0.01
42) 2,4,6-Tribromophenol	10.739	330	187826	112.000	ng	0.00
45) 2-Fluorobiphenyl	9.263	172	718719	72.986	ng	0.00
79) Terphenyl-d14	13.021	244	899693	63.094	ng	-0.01
Target Compounds						
						Qvalue
19) n-Nitroso-di-n-propyla...	7.469	70	59452	15.874	ng	# 78
25) Isophorone	7.469	82	432428	41.294	ng	# 68
51) 2,6-Dinitrotoluene	9.945	165	21169	8.751	ng	# 22
57) 2,4-Dinitrotoluene	9.945	165	21169	6.607	ng	# 26
67) 4-Bromophenyl-phenylether	10.739	248	11573	3.248	ng	# 1
77) Benzidine	13.021	184	12817	2.598	ng	# 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050622\
Data File : BF128131.D
Acq On : 06 May 2022 18:30
Operator : CG\JU
Sample : N2723-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MMC-PIT2

Quant Time: May 06 23:25:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 17:56:23 2022
Response via : Initial Calibration



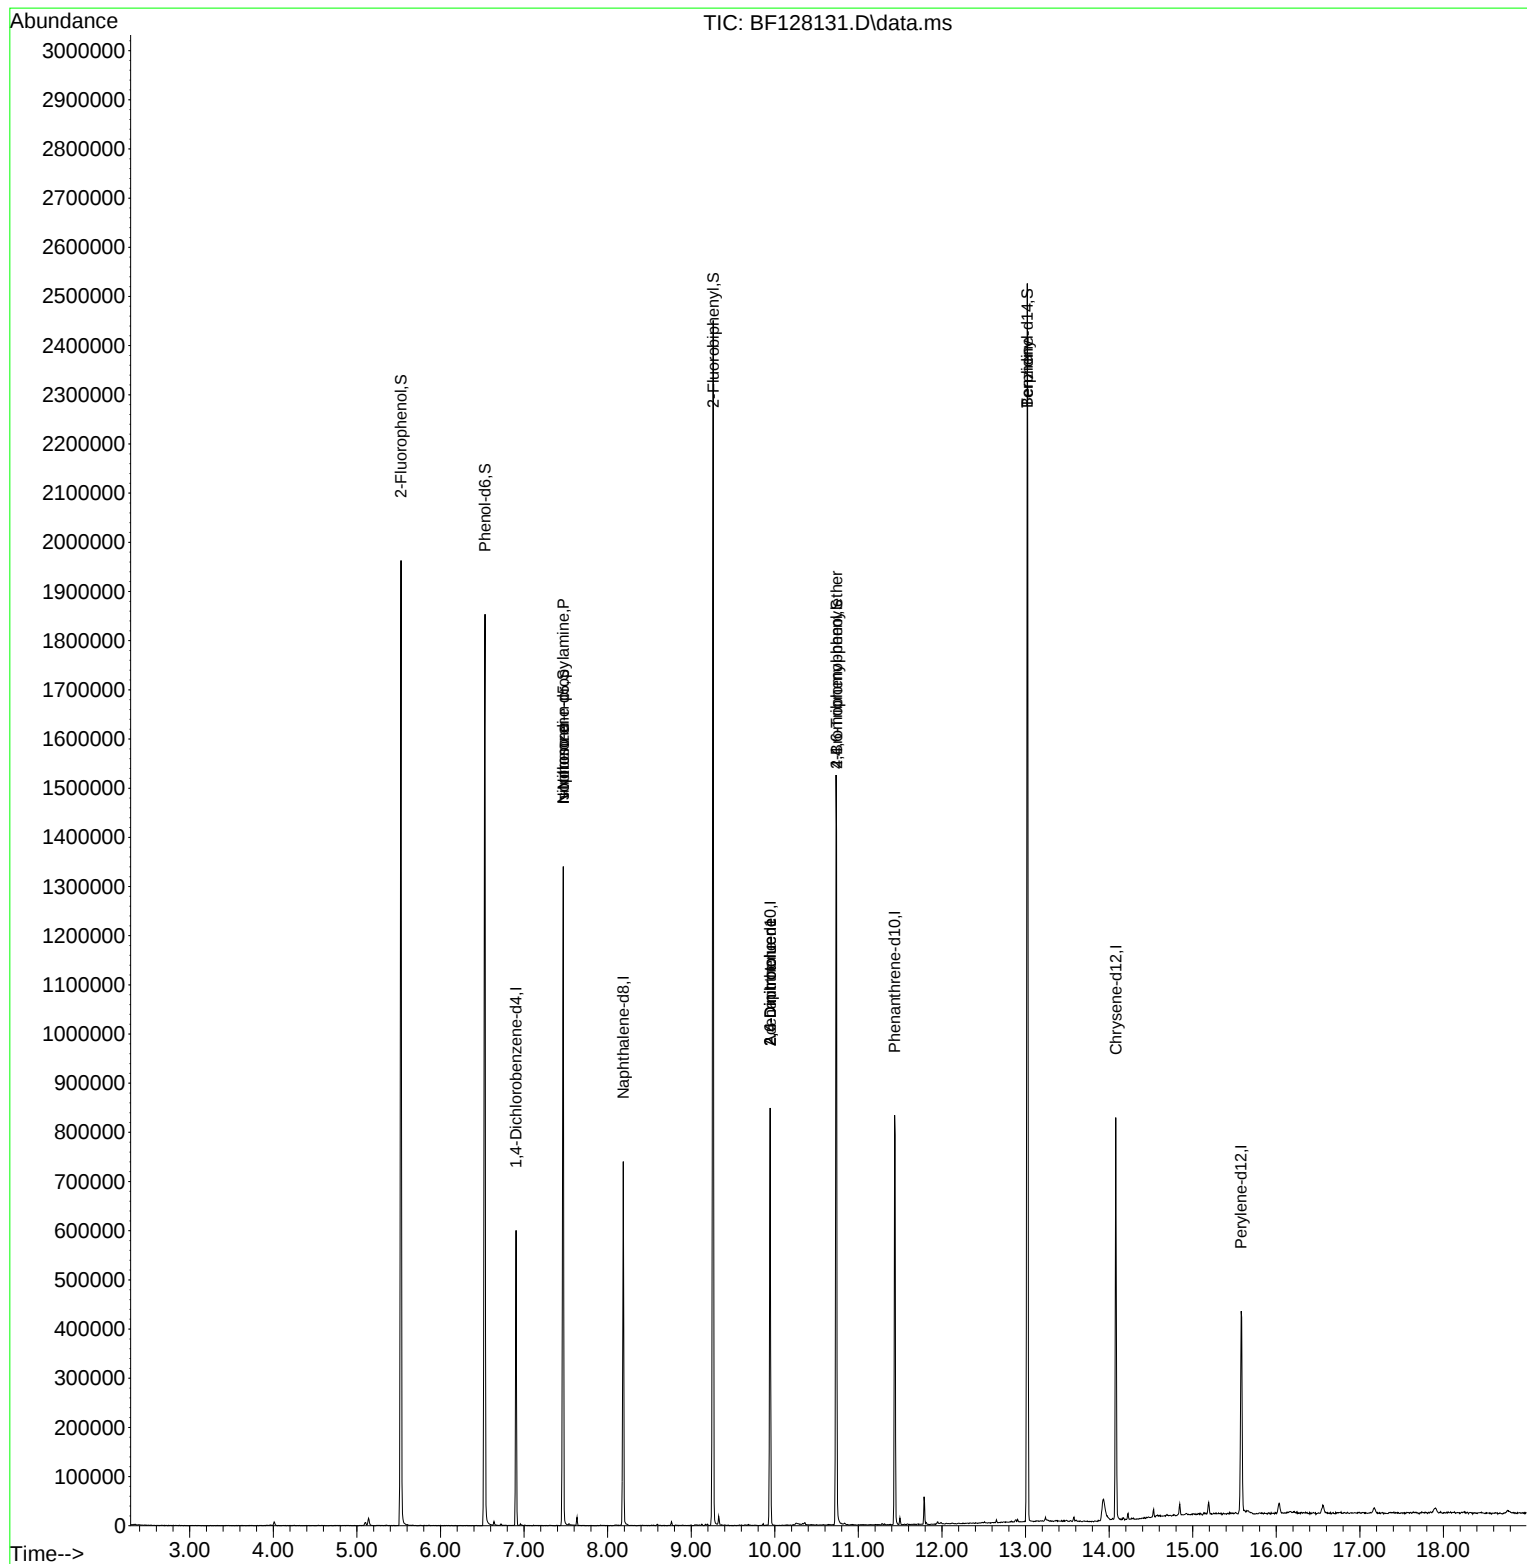


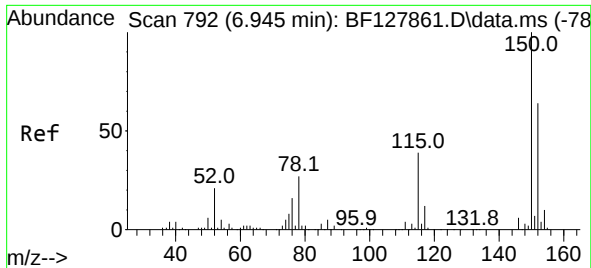

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.904 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF128131.D
Acq: 06 May 2022 18:30




Instrument :
BNA_F
ClientSampleId :
MMC-PIT2


Tgt Ion:152 Resp: 75102
Ion Ratio Lower Upper
152 100
150 155.4 125.3 187.9
115 66.0 48.8 73.2

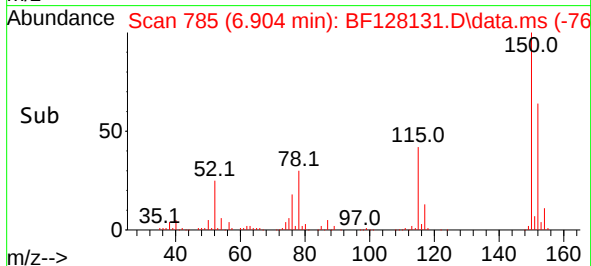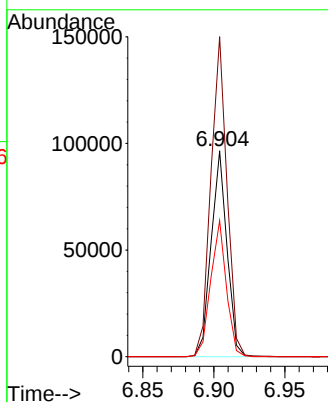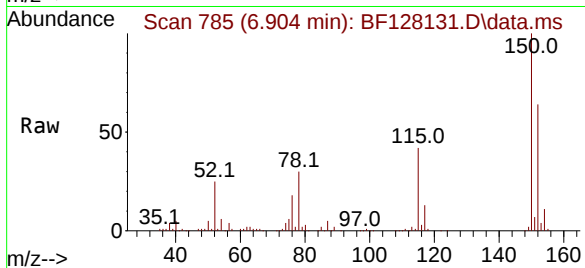

#5
2-Fluorophenol
Concen: 99.870 ng
RT: 5.528 min Scan# 551
Delta R.T. -0.006 min
Lab File: BF128131.D
Acq: 06 May 2022 18:30

Tgt Ion:112 Resp: 470903
Ion Ratio Lower Upper
112 100
64 65.6 49.5 74.3
63 35.7 26.3 39.5

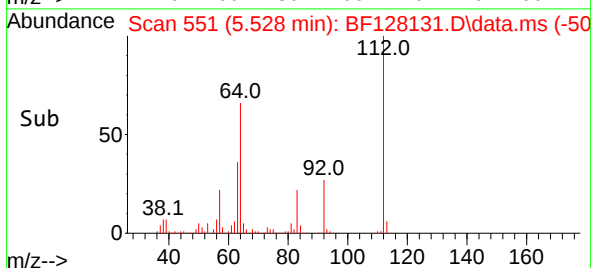
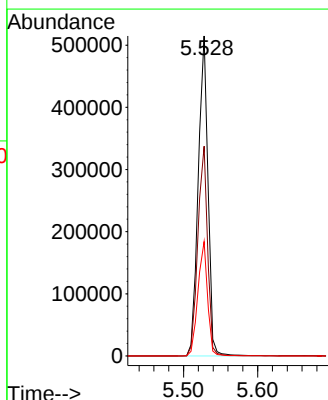
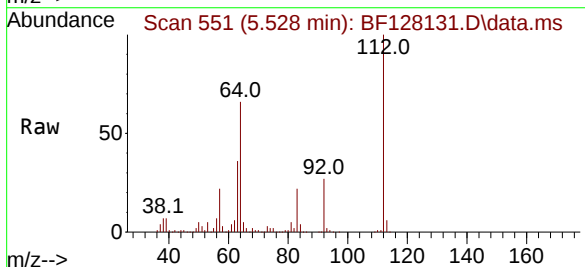


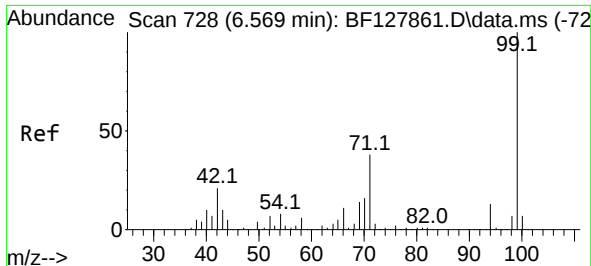

#7
Phenol-d6
Concen: 101.998 ng
RT: 6.534 min Scan# 71
Delta R.T. -0.012 min
Lab File: BF128131.D
Acq: 06 May 2022 18:30




Instrument :
BNA_F
ClientSampleId :
MMC-PIT2

Tgt Ion: 99 Resp: 624048
Ion Ratio Lower Upper
99 100
42 20.6 16.6 24.8
71 39.4 30.0 45.0

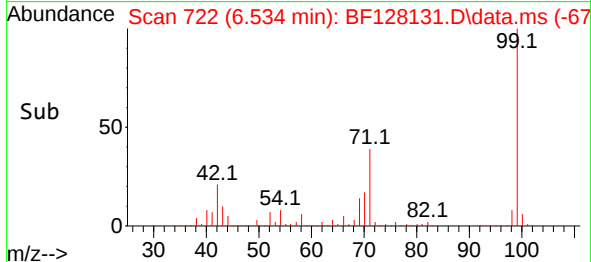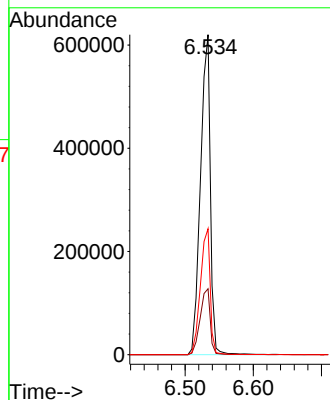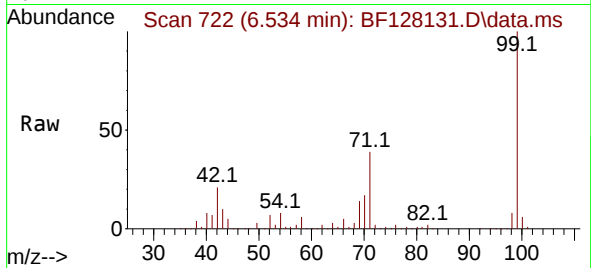

#19
n-Nitroso-di-n-propylamine
Concen: 15.874 ng
RT: 7.469 min Scan# 881
Delta R.T. 0.141 min
Lab File: BF128131.D
Acq: 06 May 2022 18:30

Tgt Ion: 70 Resp: 59452
Ion Ratio Lower Upper
70 100
42 47.4 48.7 73.1#
101 0.0 7.2 10.8#
130 1.8 14.4 21.6#

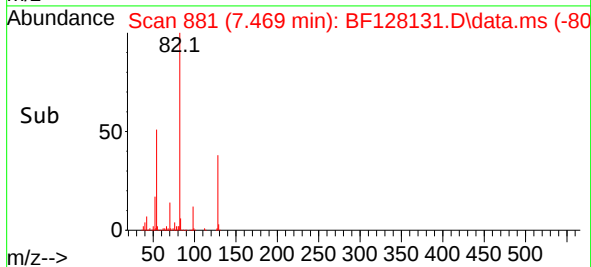
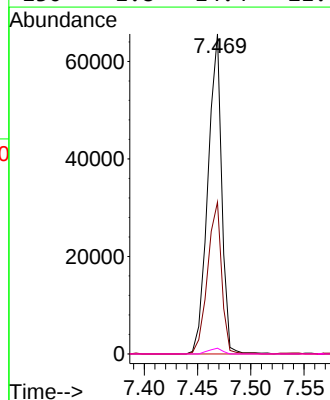
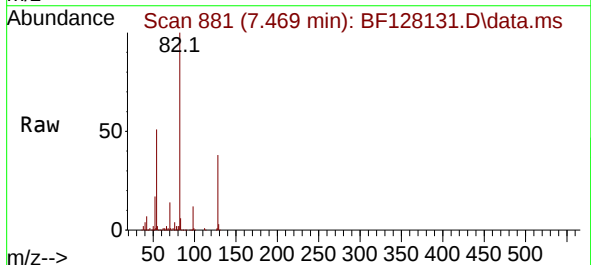




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.186 min Scan# 1010
Delta R.T. -0.012 min
Lab File: BF128131.D
Acq: 06 May 2022 18:30




Instrument :
BNA_F
ClientSampleId :
MMC-PIT2

Tgt Ion:	136	Resp:	292579
Ion	Ratio	Lower	Upper
136	100		
137	10.6	8.6	13.0
54	8.6	6.8	10.2
68	6.4	5.1	7.7

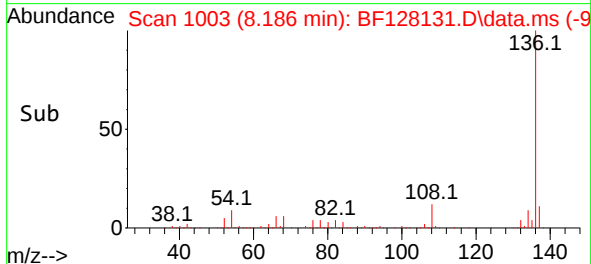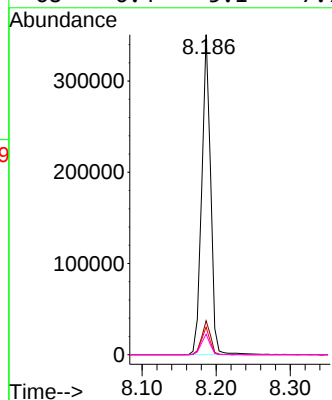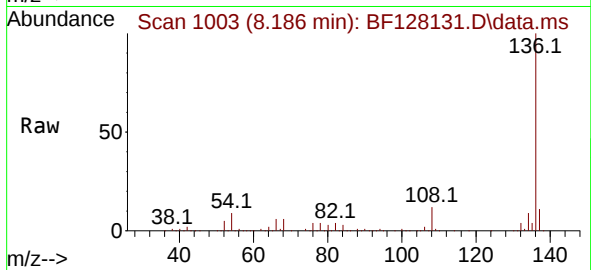

#23
Nitrobenzene-d5
Concen: 69.502 ng
RT: 7.469 min Scan# 881
Delta R.T. -0.012 min
Lab File: BF128131.D
Acq: 06 May 2022 18:30

Tgt Ion:	82	Resp:	432434
Ion	Ratio	Lower	Upper
82	100		
128	38.1	30.0	45.0
54	51.3	41.3	61.9

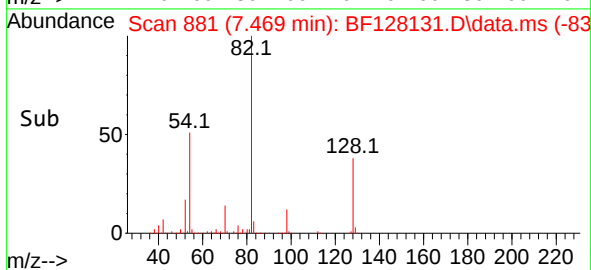
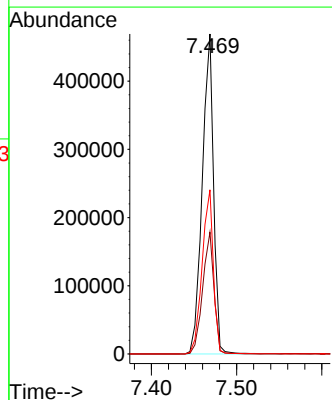
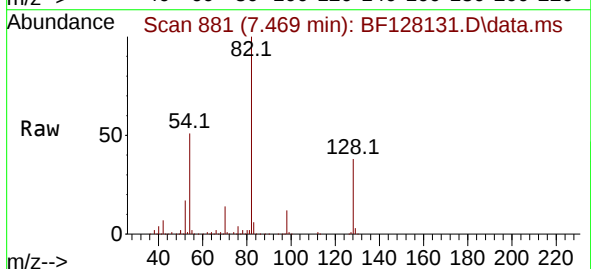




#25
Isophorone
Concen: 41.294 ng
RT: 7.469 min Scan# 81
Delta R.T. -0.271 min
Lab File: BF128131.D
Acq: 06 May 2022 18:30




Instrument :
BNA_F
ClientSampleId :
MMC-PIT2

Tgt Ion: 82 Resp: 432428
Ion Ratio Lower Upper
82 100
95 0.0 5.6 8.4#
138 0.0 12.5 18.7#

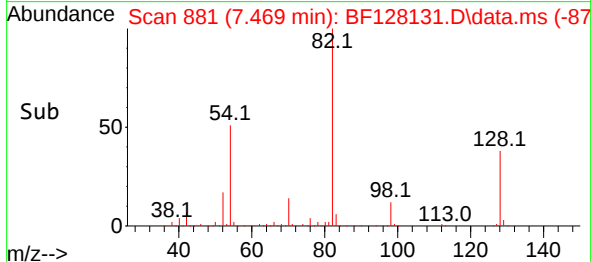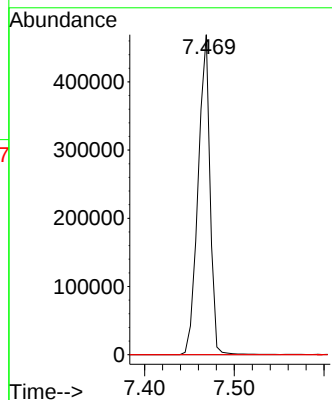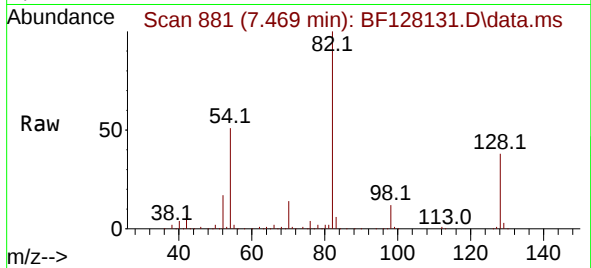

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.945 min Scan# 1302
Delta R.T. -0.006 min
Lab File: BF128131.D
Acq: 06 May 2022 18:30

Tgt Ion:164 Resp: 166591
Ion Ratio Lower Upper
164 100
162 95.4 76.0 114.0
160 42.5 34.8 52.2

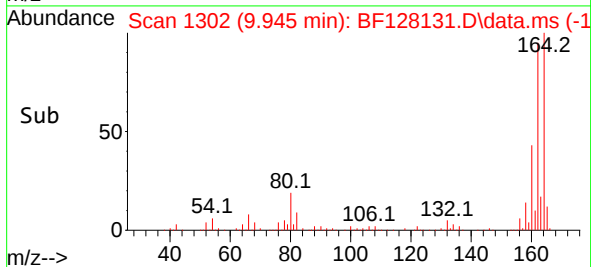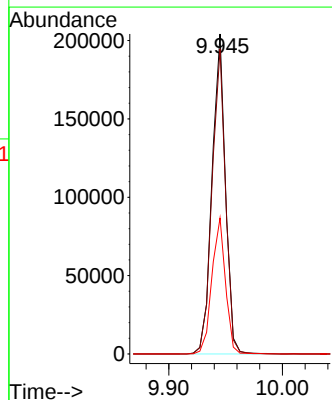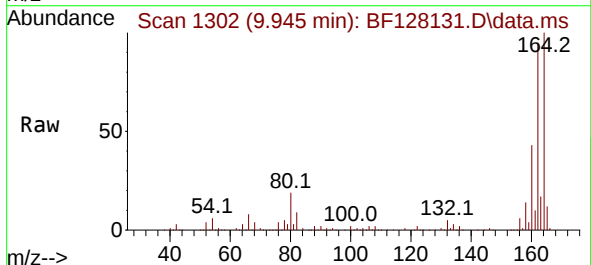



#42

2,4,6-Tribromophenol

Concen: 112.000 ng

RT: 10.739 min Scan# 1444

Delta R.T. -0.006 min

Lab File: BF128131.D

Acq: 06 May 2022 18:30

Instrument :

BNA_F

ClientSampleId :

MMC-PIT2




Tgt Ion:330 Resp: 187826

Ion Ratio Lower Upper

330 100

332 96.0 79.0 118.4

141 33.3 28.9 43.3

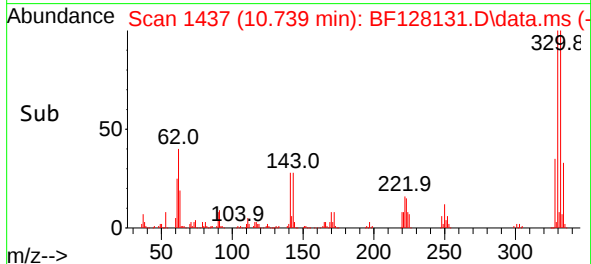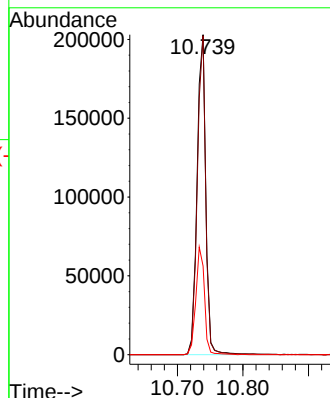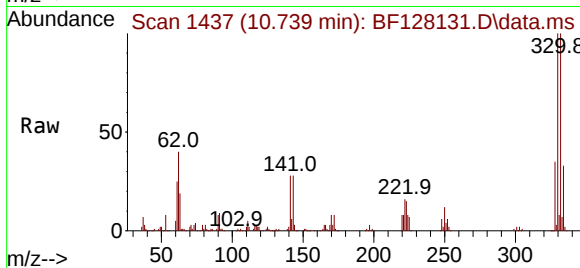

#45

2-Fluorobiphenyl

Concen: 72.986 ng

RT: 9.263 min Scan# 1186

Delta R.T. -0.006 min

Lab File: BF128131.D

Acq: 06 May 2022 18:30




Tgt Ion:172 Resp: 718719

Ion Ratio Lower Upper

172 100

171 34.7 28.6 42.8

170 23.7 19.1 28.7

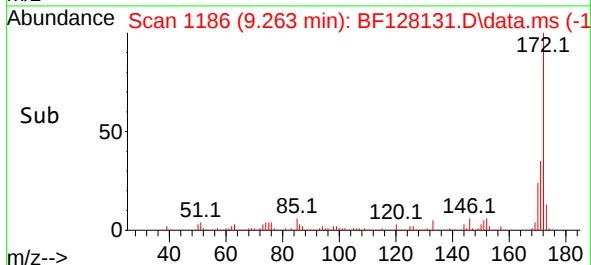
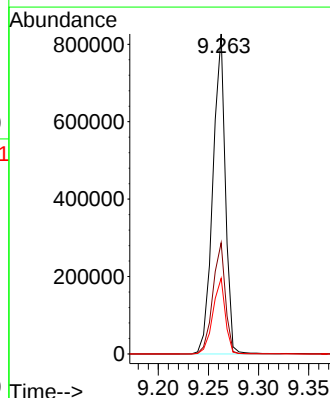
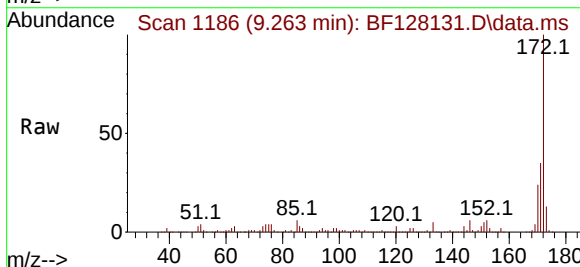




#51
2,6-Dinitrotoluene
Concen: 8.751 ng
RT: 9.945 min Scan# 11
Delta R.T. 0.206 min
Lab File: BF128131.D
Acq: 06 May 2022 18:30




Instrument :
BNA_F
ClientSampleId :
MMC-PIT2

Tgt Ion:165 Resp: 21169
Ion Ratio Lower Upper
165 100
63 1.1 49.5 74.3#
89 1.9 49.0 73.4#

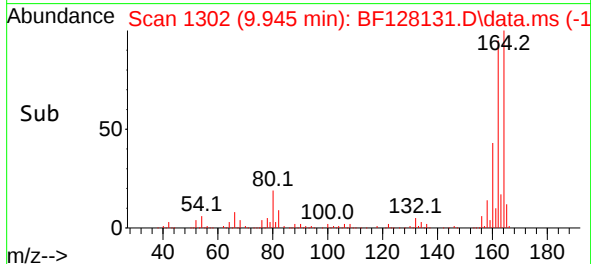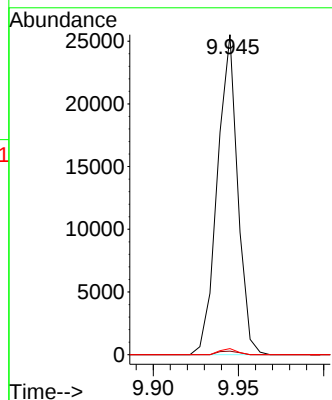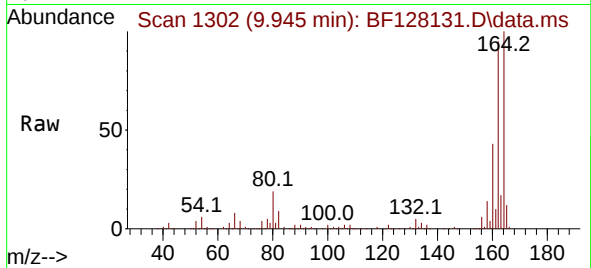

#57
2,4-Dinitrotoluene
Concen: 6.607 ng
RT: 9.945 min Scan# 1302
Delta R.T. -0.200 min
Lab File: BF128131.D
Acq: 06 May 2022 18:30

Tgt Ion:165 Resp: 21169
Ion Ratio Lower Upper
165 100
63 1.1 32.6 49.0#
89 1.9 55.2 82.8#
182 0.0 2.0 3.0#


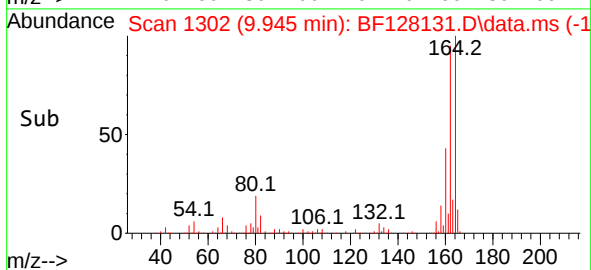
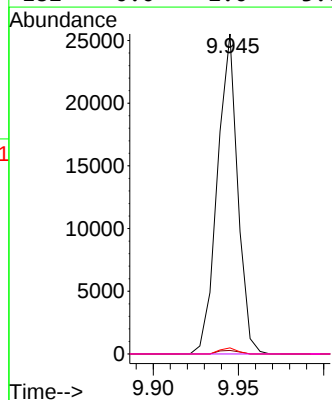
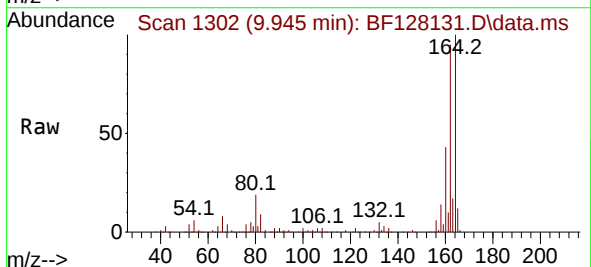




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.433 min Scan# 11
Delta R.T. -0.012 min
Lab File: BF128131.D
Acq: 06 May 2022 18:30




Instrument :
BNA_F
ClientSampleId :
MMC-PIT2


Tgt Ion:188 Resp: 321371
Ion Ratio Lower Upper
188 100
94 9.7 8.0 12.0
80 10.5 8.9 13.3

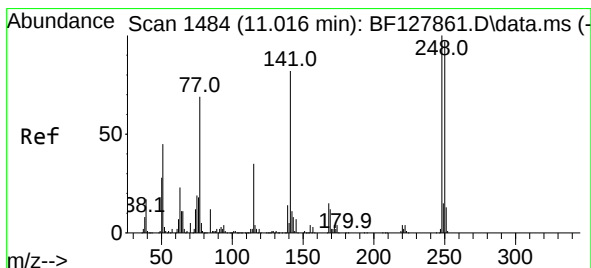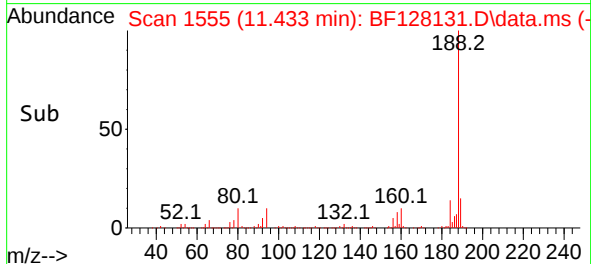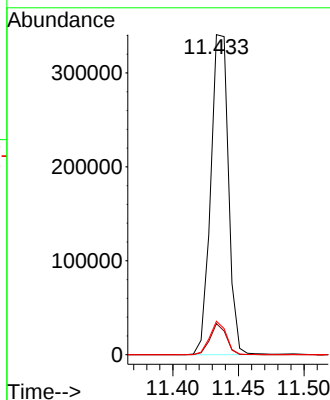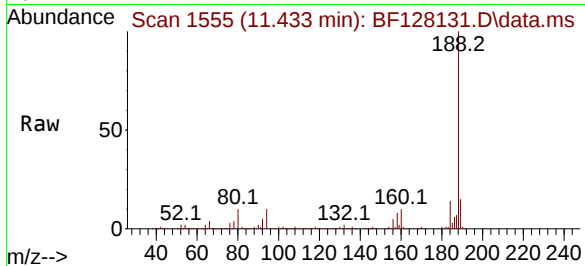

#67
4-Bromophenyl-phenylether
Concen: 3.248 ng
RT: 10.739 min Scan# 1437
Delta R.T. -0.247 min
Lab File: BF128131.D
Acq: 06 May 2022 18:30

Tgt Ion:248 Resp: 11573
Ion Ratio Lower Upper
248 100
250 194.3 77.7 116.5#
141 457.9 65.6 98.4#


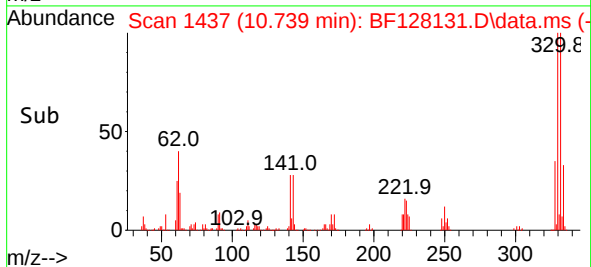
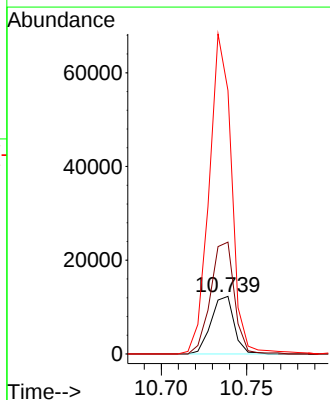
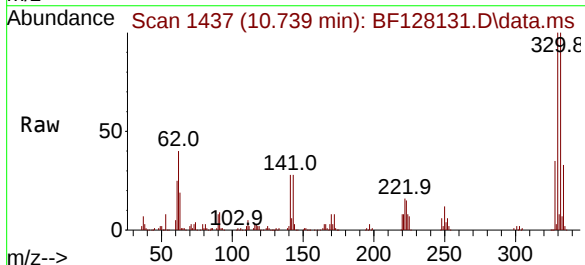


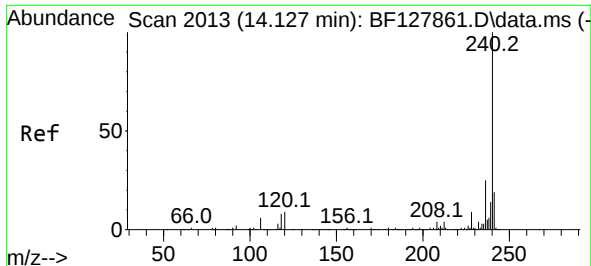

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.080 min Scan# 2013
Delta R.T. -0.012 min
Lab File: BF128131.D
Acq: 06 May 2022 18:30




Instrument :
BNA_F
ClientSampleId :
MMC-PIT2

Tgt Ion:240 Resp: 260745
Ion Ratio Lower Upper
240 100
120 10.3 7.0 10.6
236 25.0 20.3 30.5

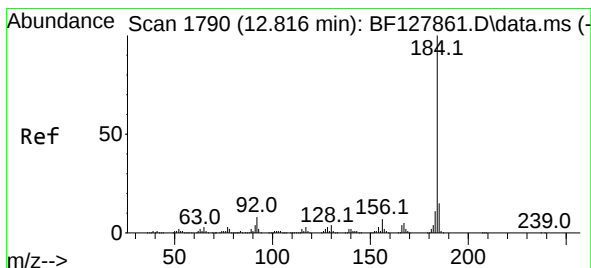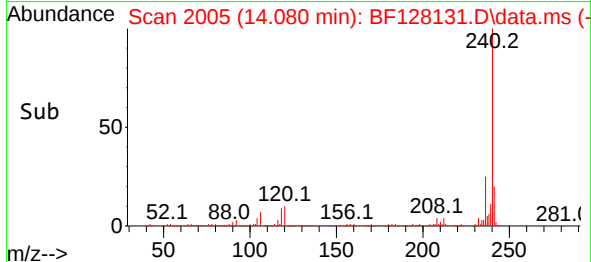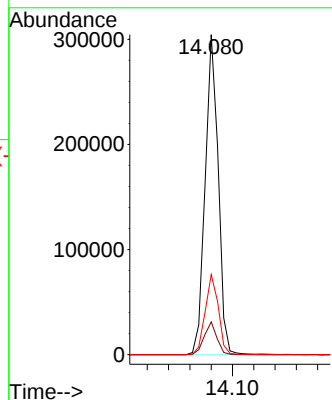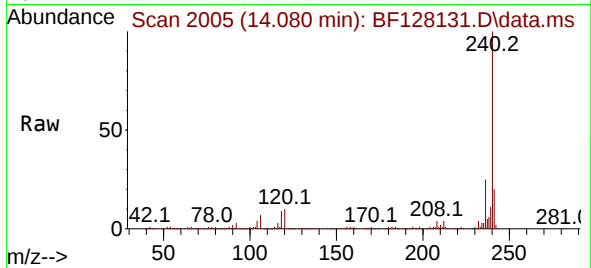

#77
Benzidine
Concen: 2.598 ng
RT: 13.021 min Scan# 1825
Delta R.T. 0.241 min
Lab File: BF128131.D
Acq: 06 May 2022 18:30

Tgt Ion:184 Resp: 12817
Ion Ratio Lower Upper
184 100
185 16.5 12.1 18.1
183 8.1 9.0 13.4#


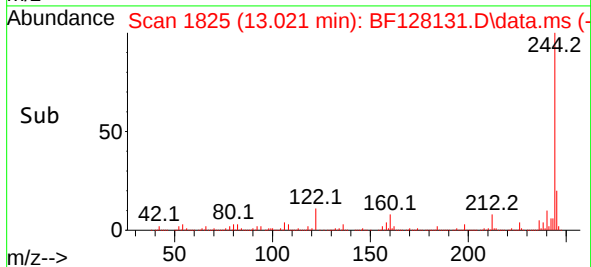
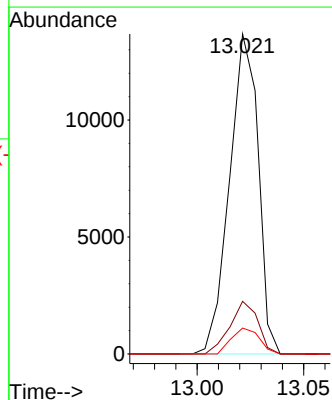
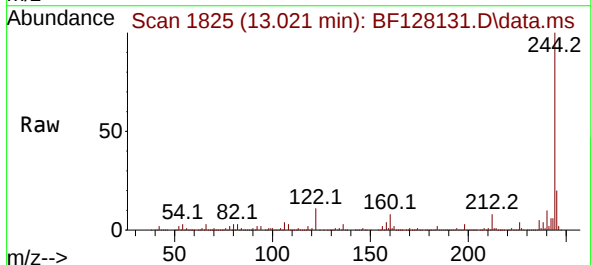




#79
 Terphenyl-d14
 Concen: 63.094 ng
 RT: 13.021 min Scan# 1825
 Delta R.T. -0.012 min
 Lab File: BF128131.D
 Acq: 06 May 2022 18:30

Instrument :
 BNA_F
 ClientSampleId :
 MMC-PIT2

Tgt Ion:244 Resp: 899693
 Ion Ratio Lower Upper
 244 100
 212 7.8 6.2 9.4
 122 10.9 8.6 12.8

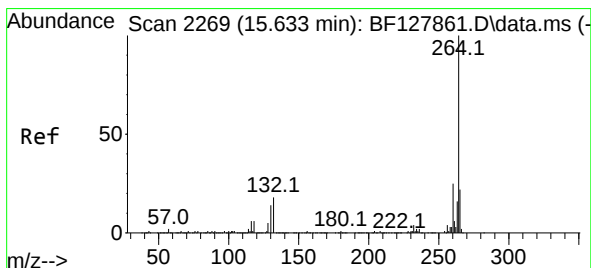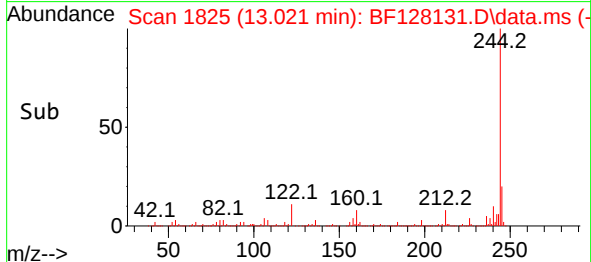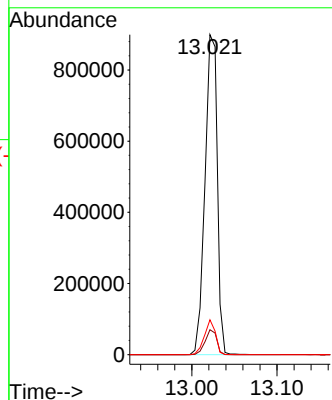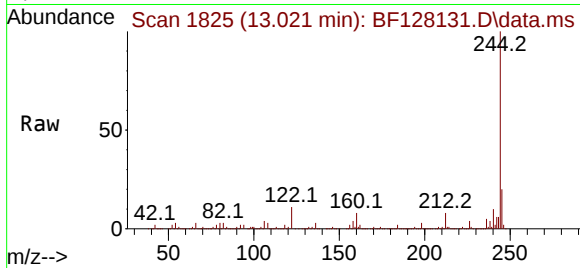

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.580 min Scan# 2260
 Delta R.T. -0.012 min
 Lab File: BF128131.D
 Acq: 06 May 2022 18:30

Tgt Ion:264 Resp: 193085
 Ion Ratio Lower Upper
 264 100
 260 23.4 20.1 30.1
 265 22.1 17.5 26.3

